
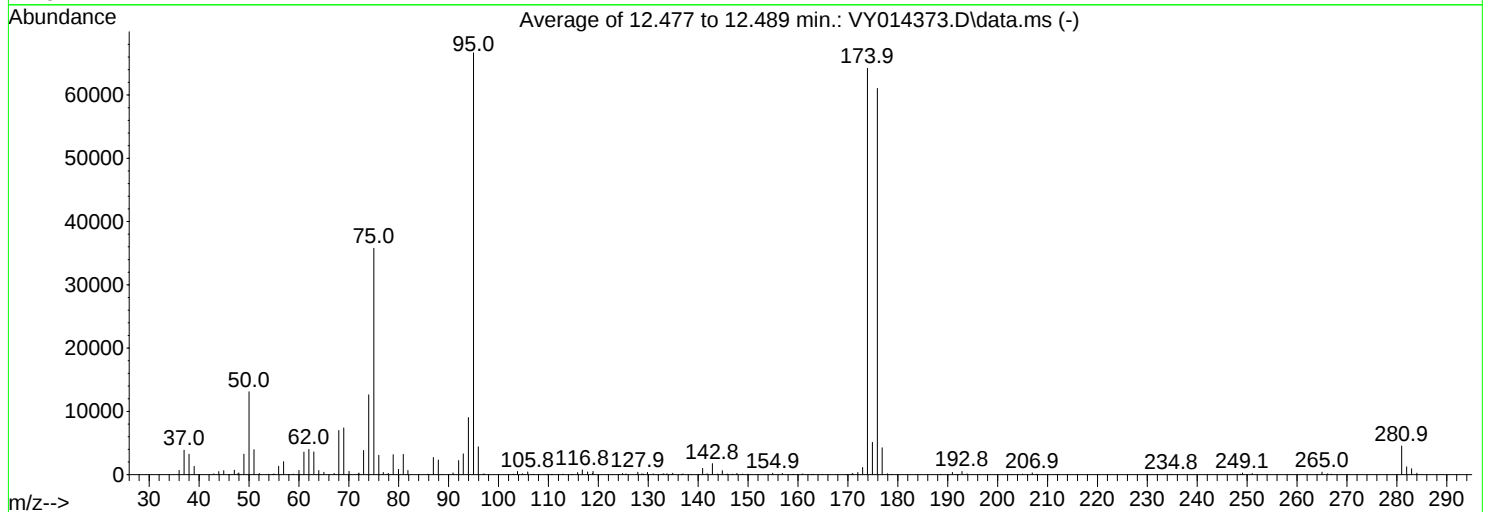


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY062223\
Data File : VY014373.D
Acq On : 22 Jun 2023 10:41
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060923S.M
Title : SW846 8260
Last Update : Fri Jun 09 18:07:13 2023

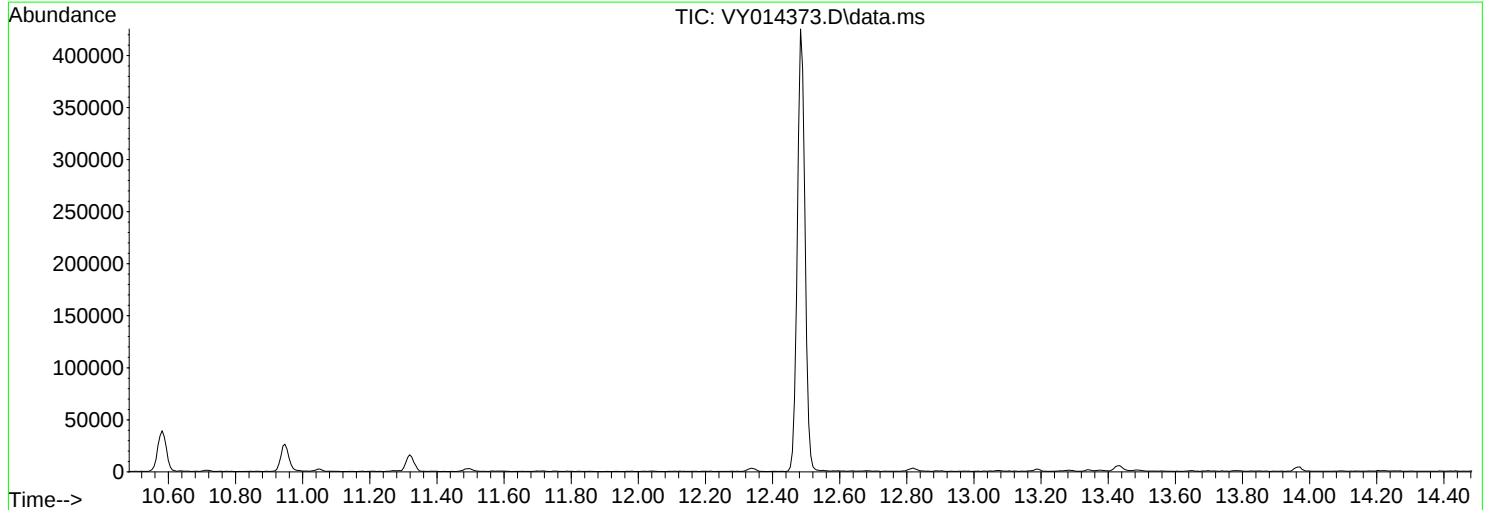

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.7	13105	PASS
75	95	30	60	53.7	35779	PASS
95	95	100	100	100.0	66669	PASS
96	95	5	9	6.6	4405	PASS
173	174	0.00	2	1.8	1130	PASS
174	95	50	100	96.4	64240	PASS
175	174	5	9	8.0	5113	PASS
176	174	95	101	95.0	61053	PASS
177	176	5	9	7.0	4249	PASS