
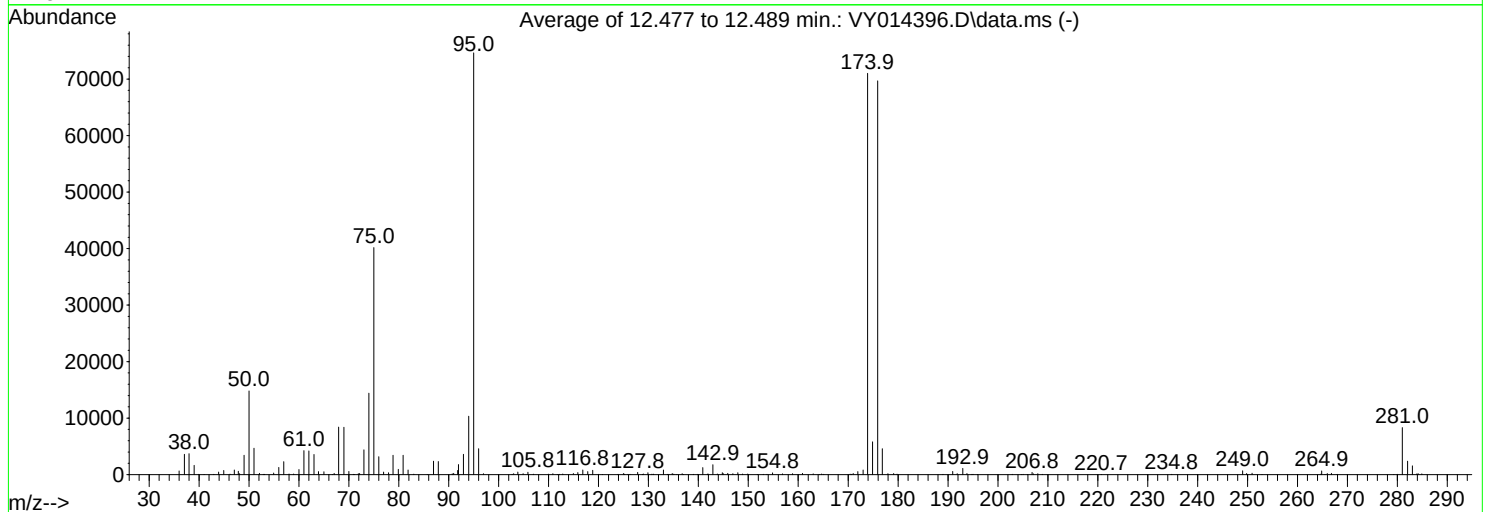


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY062323\
Data File : VY014396.D
Acq On : 23 Jun 2023 09:14
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y062323S.M
Title : SW846 8260
Last Update : Fri Jun 23 17:18:46 2023

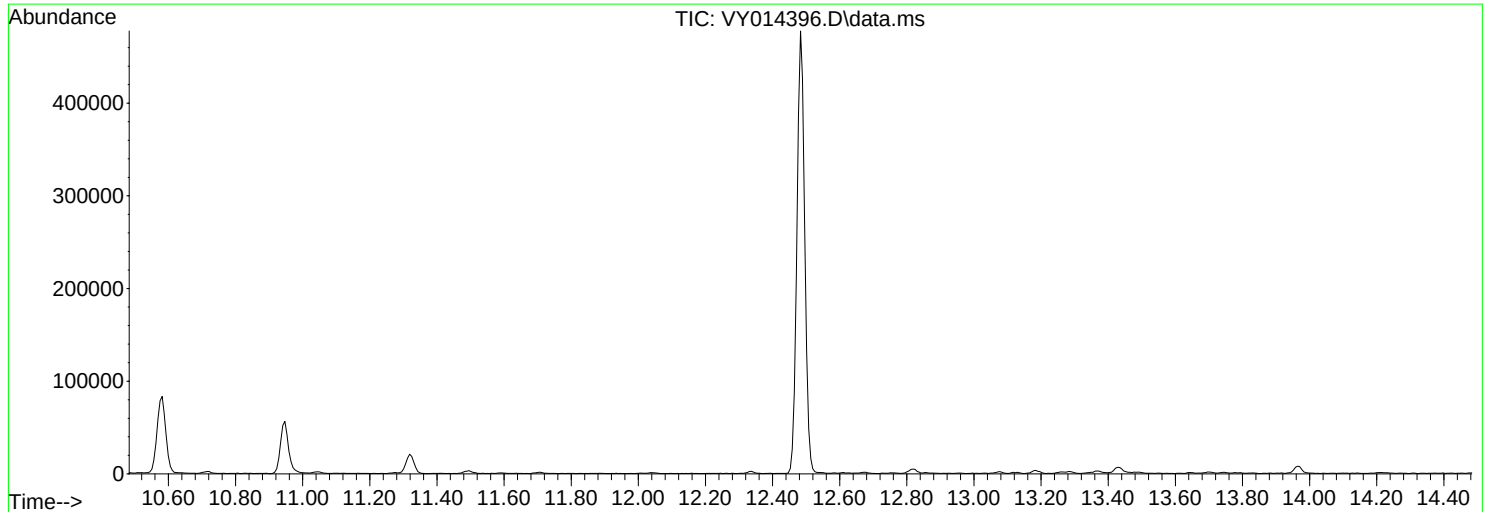

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	14806	PASS
75	95	30	60	53.8	40168	PASS
95	95	100	100	100.0	74640	PASS
96	95	5	9	6.1	4576	PASS
173	174	0.00	2	1.2	832	PASS
174	95	50	100	95.1	71003	PASS
175	174	5	9	8.2	5818	PASS
176	174	95	101	98.1	69685	PASS
177	176	5	9	6.6	4589	PASS