
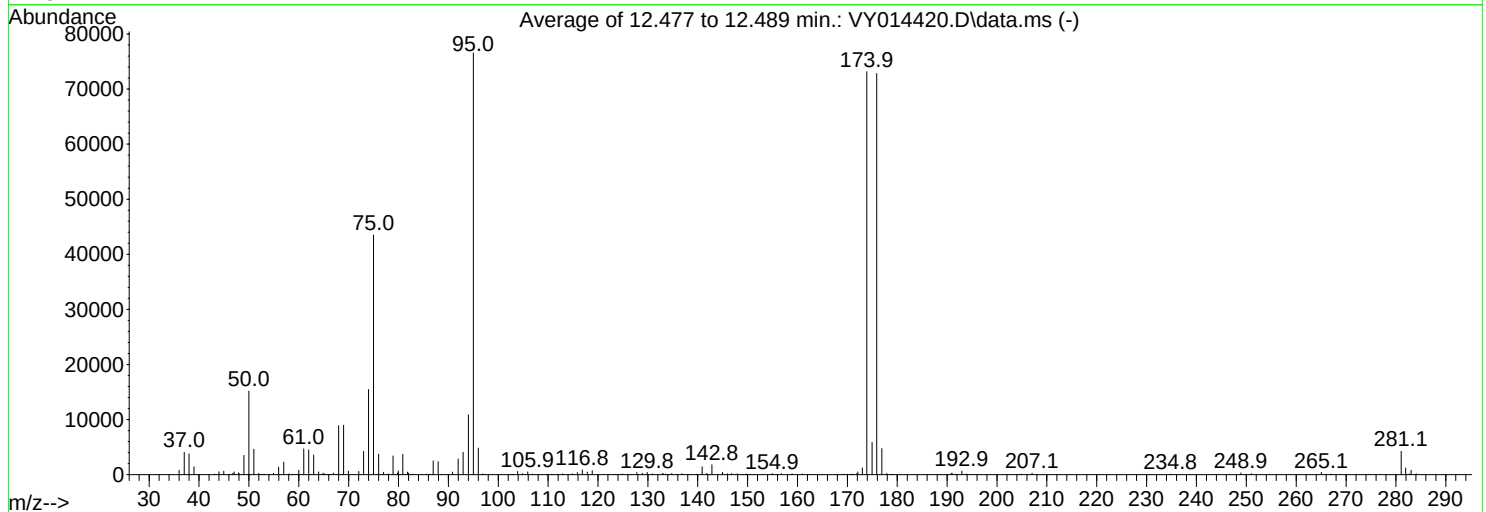


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY062623\
Data File : VY014420.D
Acq On : 26 Jun 2023 09:04
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y062323S.M
Title : SW846 8260
Last Update : Fri Jun 23 17:18:46 2023

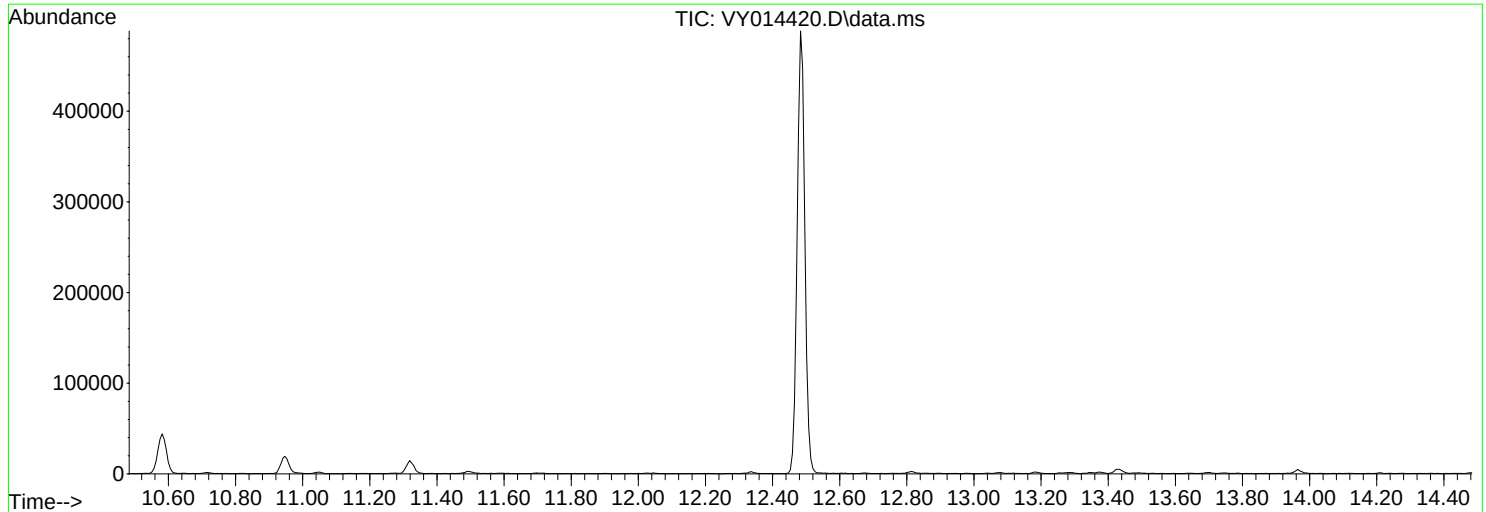

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	15161	PASS
75	95	30	60	56.8	43515	PASS
95	95	100	100	100.0	76576	PASS
96	95	5	9	6.3	4816	PASS
173	174	0.00	2	1.7	1235	PASS
174	95	50	100	95.5	73160	PASS
175	174	5	9	8.0	5843	PASS
176	174	95	101	99.5	72813	PASS
177	176	5	9	6.5	4730	PASS