

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY062624\
 Data File : VY018699.D
 Acq On : 26 Jun 2024 10:53
 Operator : SY/MD
 Sample : VY0626SBL01
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0626SBL01

Quant Time: Jun 27 03:24:25 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y061324S.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 14 07:08:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.777	168	112679	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.679	114	193585	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.483	117	162449	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	58166	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.130	65	61409	54.131	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	108.260%
35) Dibromofluoromethane	7.704	113	59262	50.184	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	100.360%
50) Toluene-d8	10.173	98	220213	48.491	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	96.980%
62) 4-Bromofluorobenzene	12.477	95	58338	40.681	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	81.360%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY062624\
Data File : VY018699.D
Acq On : 26 Jun 2024 10:53
Operator : SY/MD
Sample : VY0626SBL01
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY0626SBL01

Quant Time: Jun 27 03:24:25 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y061324S.M
Quant Title : SW846 8260
QLast Update : Fri Jun 14 07:08:24 2024
Response via : Initial Calibration




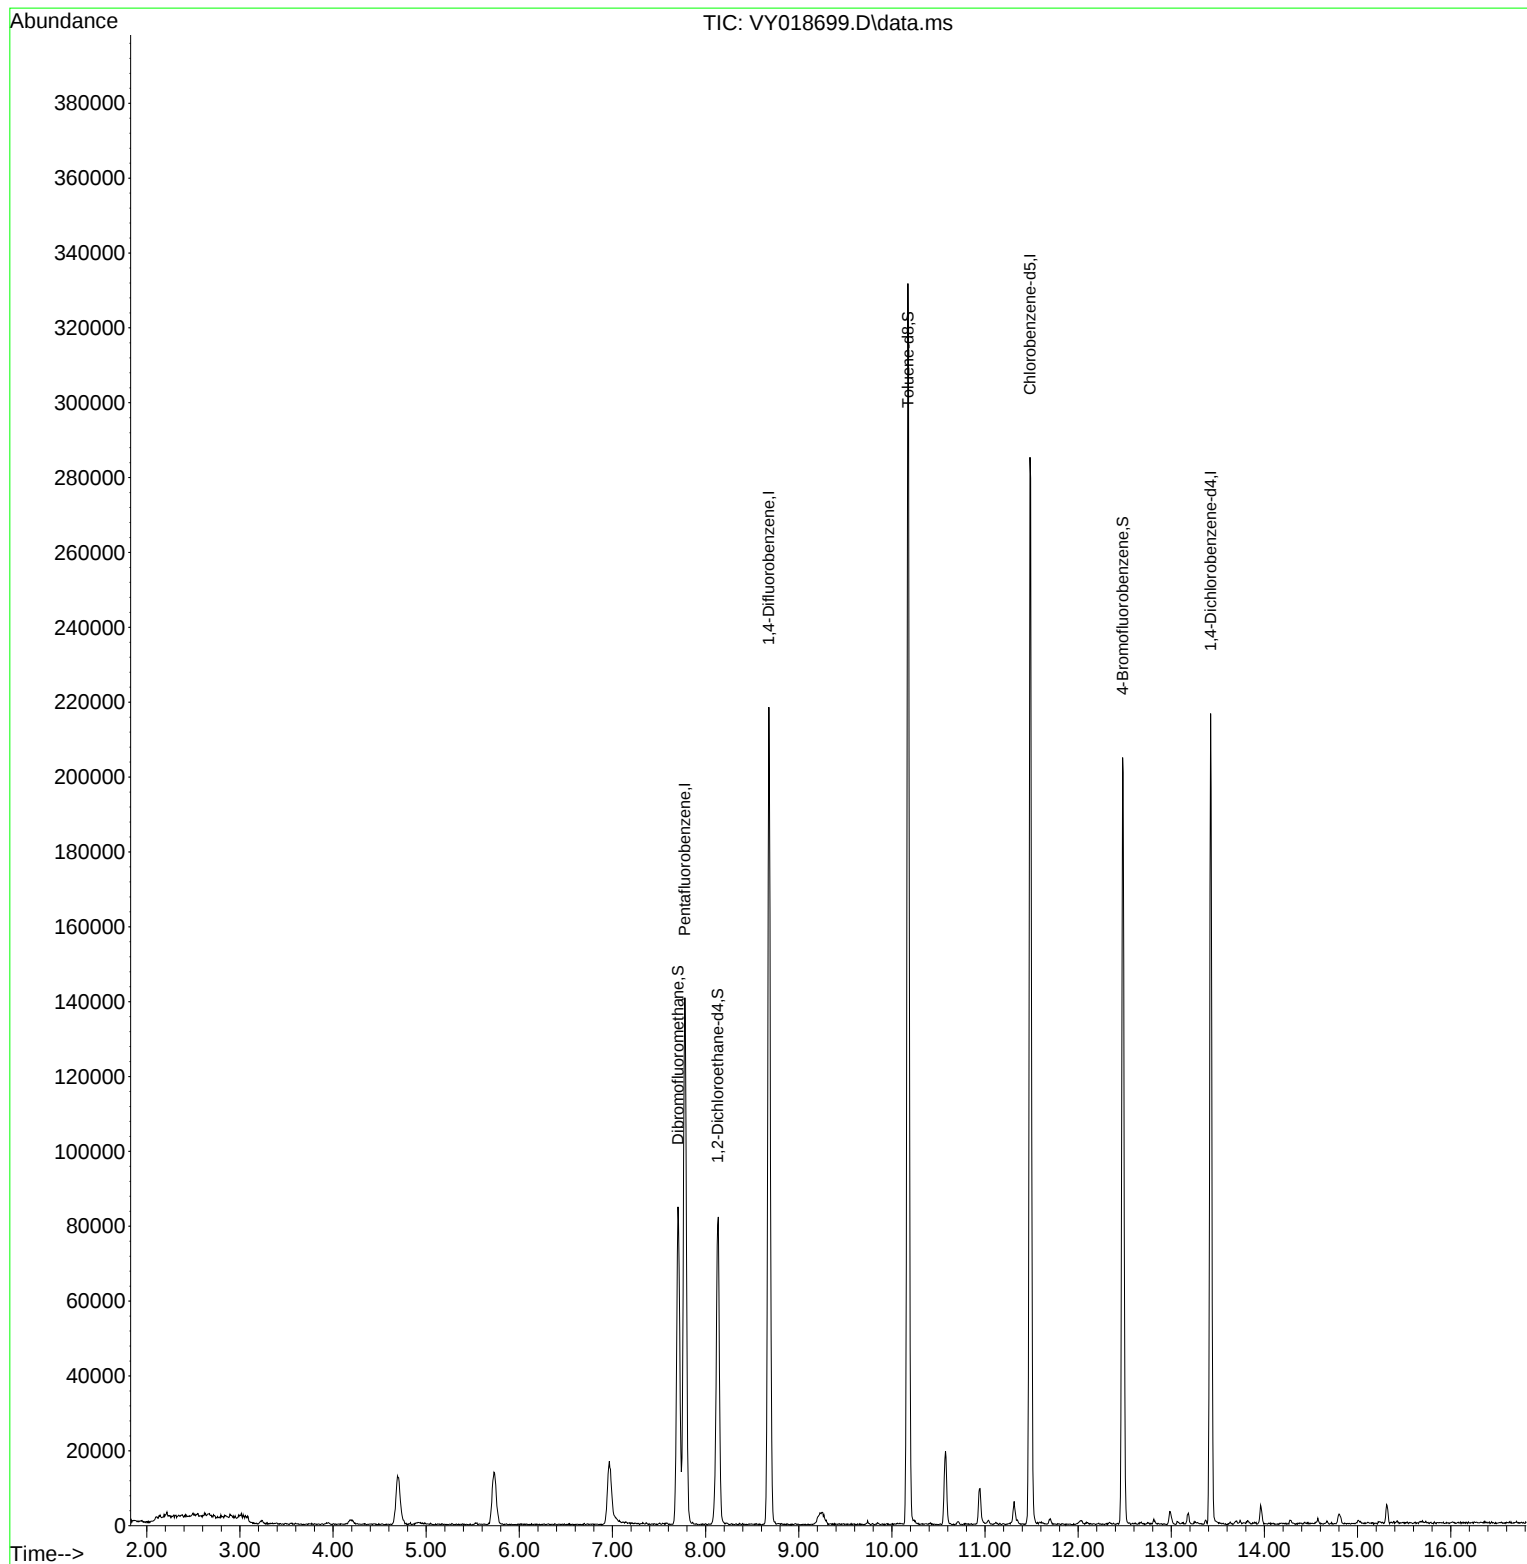


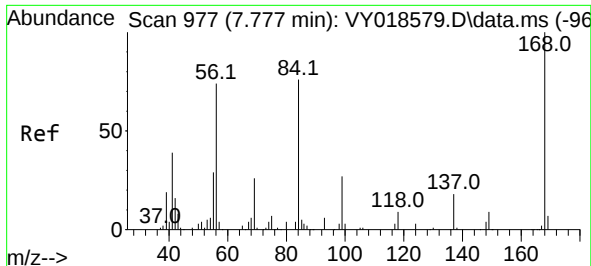

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.777 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY018699.D
Acq: 26 Jun 2024 10:53




Instrument :
MSVOA_Y
ClientSampleId :
VY0626SBL01


Tgt Ion:168 Resp: 112679
Ion Ratio Lower Upper
168 100
99 50.3 39.1 58.7

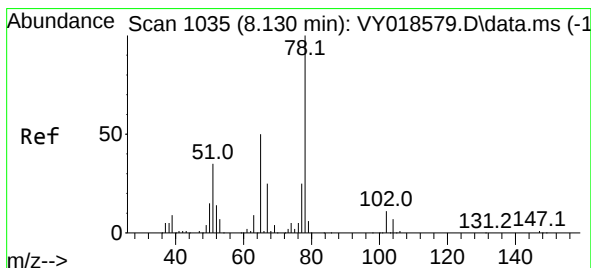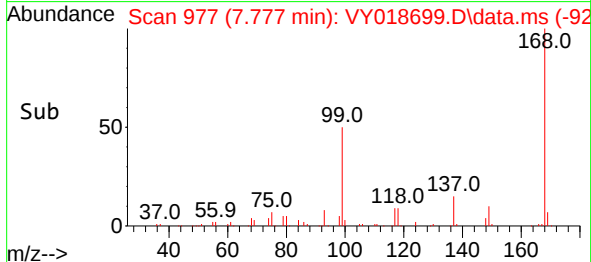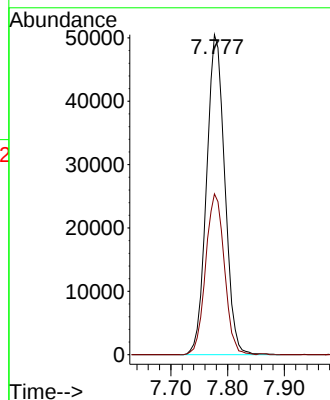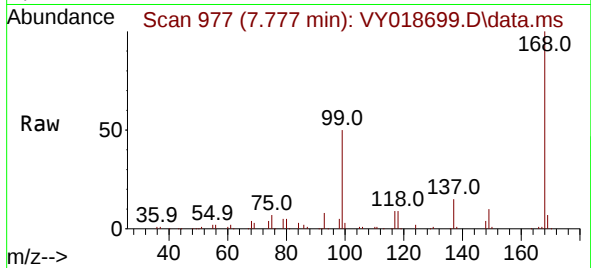

#33
1,2-Dichloroethane-d4
Concen: 54.131 ug/l
RT: 8.130 min Scan# 1035
Delta R.T. 0.000 min
Lab File: VY018699.D
Acq: 26 Jun 2024 10:53

Tgt Ion: 65 Resp: 61409
Ion Ratio Lower Upper
65 100
67 54.5 0.0 109.6

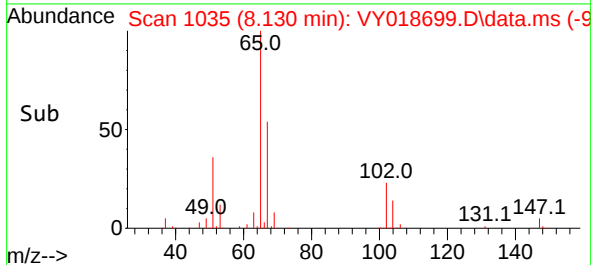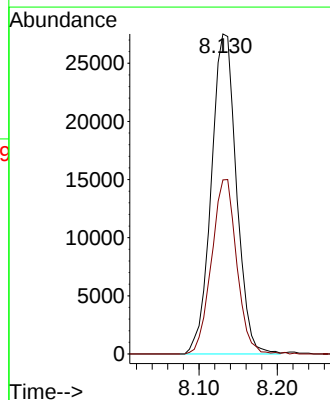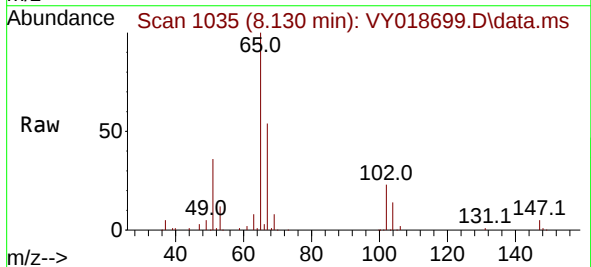

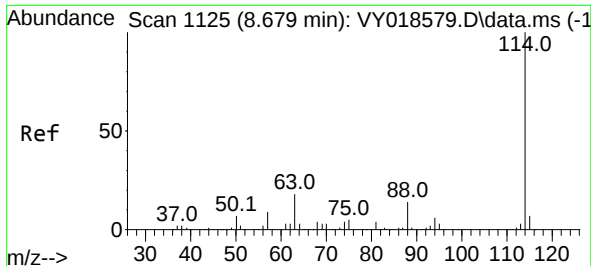

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.679 min Scan# 1125

Delta R.T. 0.000 min

Lab File: VY018699.D

Acq: 26 Jun 2024 10:53

Instrument :

MSVOA_Y

ClientSampleId :

VY0626SBL01





Tgt Ion:114 Resp: 193585

Ion Ratio Lower Upper

114 100

63 17.9 0.0 35.0

88 14.0 0.0 27.2

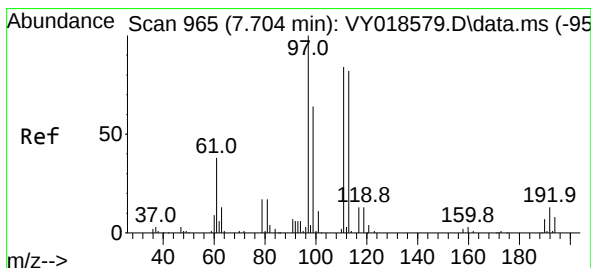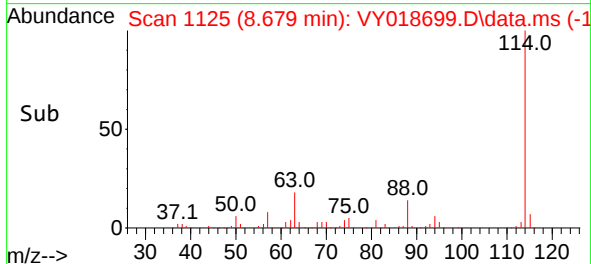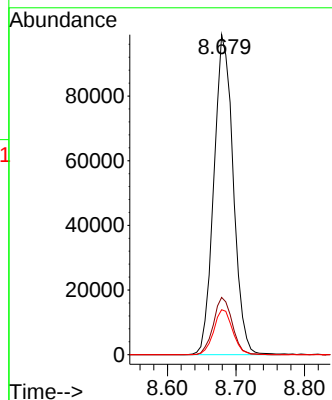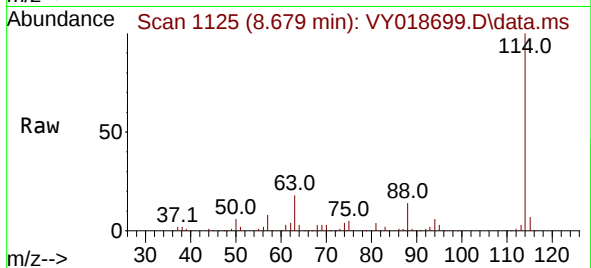

#35

Dibromofluoromethane

Concen: 50.184 ug/l

RT: 7.704 min Scan# 965

Delta R.T. 0.000 min

Lab File: VY018699.D

Acq: 26 Jun 2024 10:53




Tgt Ion:113 Resp: 59262


Ion Ratio Lower Upper

113 100

111 102.7 82.2 123.4

192 20.0 15.9 23.9


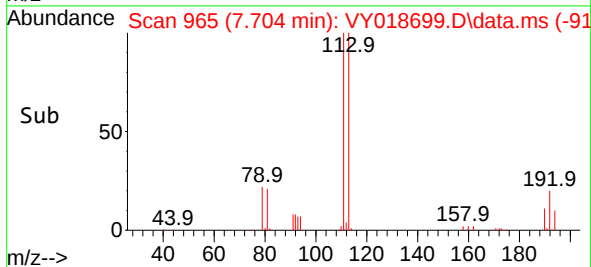
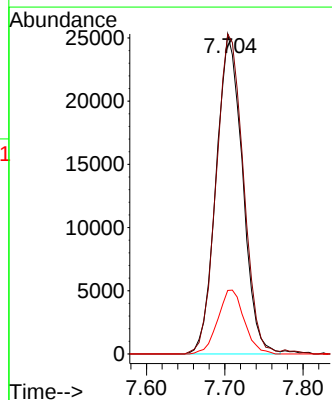
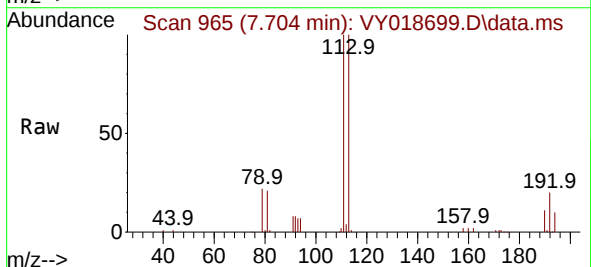


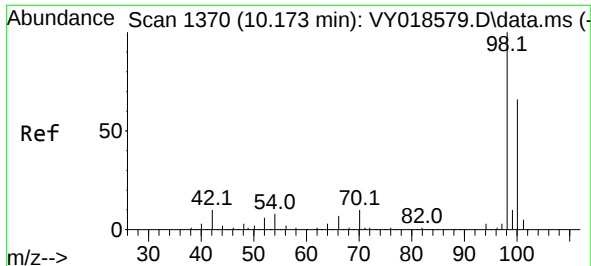

#50
Toluene-d8
Concen: 48.491 ug/l
RT: 10.173 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY018699.D
Acq: 26 Jun 2024 10:53




Instrument :
MSVOA_Y
ClientSampleId :
VY0626SBL01


Tgt Ion: 98 Resp: 220213
Ion Ratio Lower Upper
98 100
100 65.1 52.0 78.0

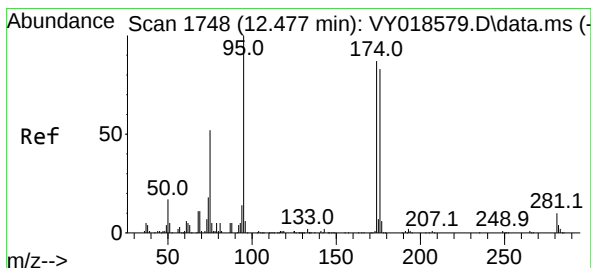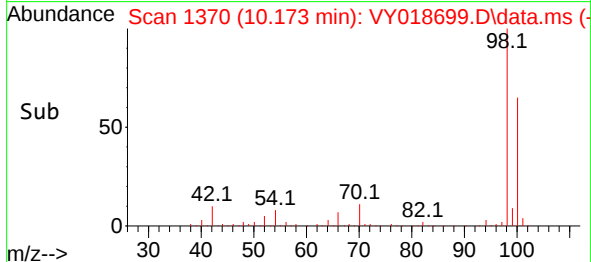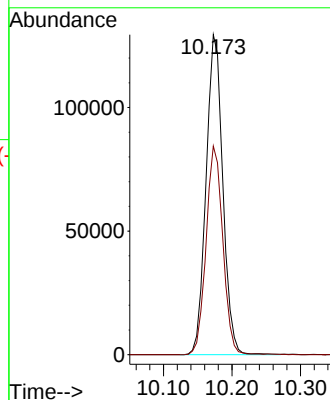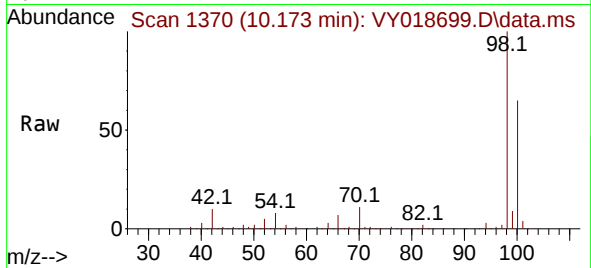

#62
4-Bromofluorobenzene
Concen: 40.681 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. 0.000 min
Lab File: VY018699.D
Acq: 26 Jun 2024 10:53

Tgt Ion: 95 Resp: 58338
Ion Ratio Lower Upper
95 100
174 90.0 0.0 175.6
176 87.4 0.0 171.4


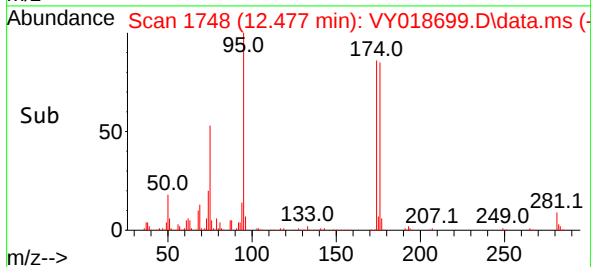
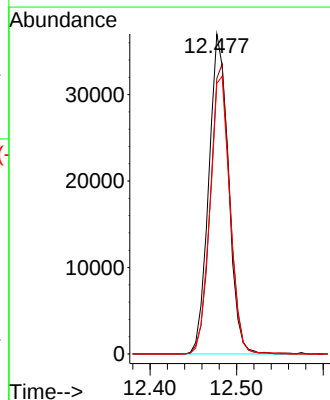
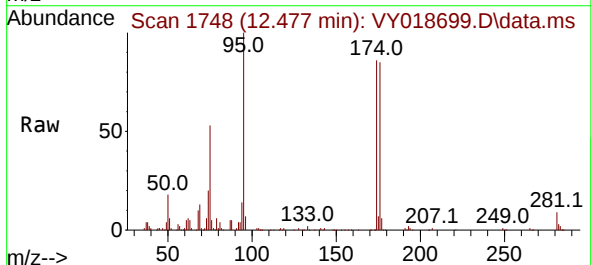


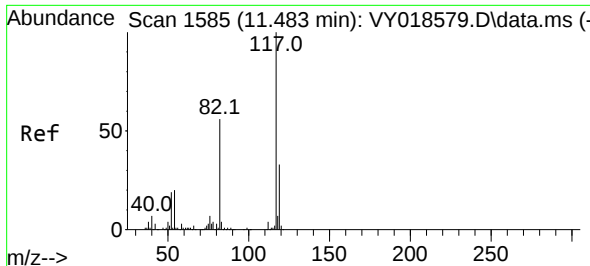

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.483 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY018699.D
Acq: 26 Jun 2024 10:53

Instrument :
MSVOA_Y
ClientSampleId :
VY0626SBL01

Tgt Ion:117 Resp: 162449
Ion Ratio Lower Upper
117 100
82 51.7 42.4 63.6
119 32.5 25.9 38.9

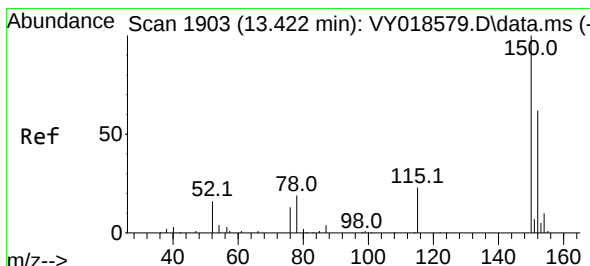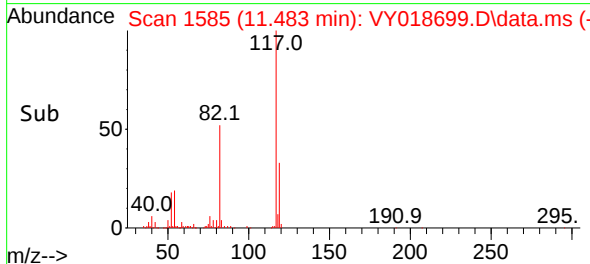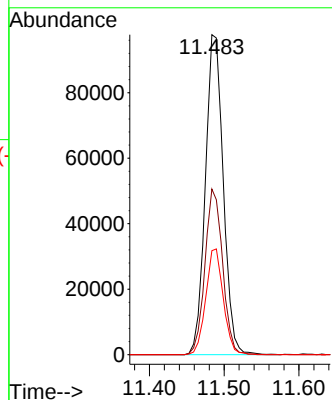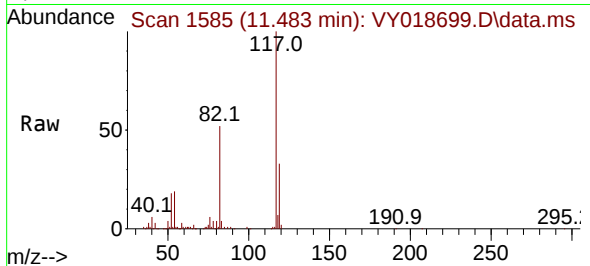

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.422 min Scan# 1903
Delta R.T. 0.000 min
Lab File: VY018699.D
Acq: 26 Jun 2024 10:53

Tgt Ion:152 Resp: 58166
Ion Ratio Lower Upper
152 100
115 55.9 28.2 84.7
150 157.9 0.0 345.6

