

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY062722\
 Data File : VY009348.D
 Acq On : 27 Jun 2022 17:16
 Operator : KP/MD
 Sample : N3434-02
 Misc : 7.29g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 B2203-35

Quant Time: Jun 28 04:31:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y062422S.M
 Quant Title : SW846 8260
 QLast Update : Sat Jun 25 07:08:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.783	168	125623	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	213736	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.483	117	191224	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	88881	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	55028	58.987	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	117.980%
35) Dibromofluoromethane	7.709	113	55249	47.890	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	95.780%
50) Toluene-d8	10.172	98	165834	49.072	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	98.140%
62) 4-Bromofluorobenzene	12.477	95	74009	45.044	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	90.080%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY062722\
Data File : VY009348.D
Acq On : 27 Jun 2022 17:16
Operator : KP/MD
Sample : N3434-02
Misc : 7.29g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
B2203-35

Quant Time: Jun 28 04:31:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y062422S.M
Quant Title : SW846 8260
QLast Update : Sat Jun 25 07:08:46 2022
Response via : Initial Calibration




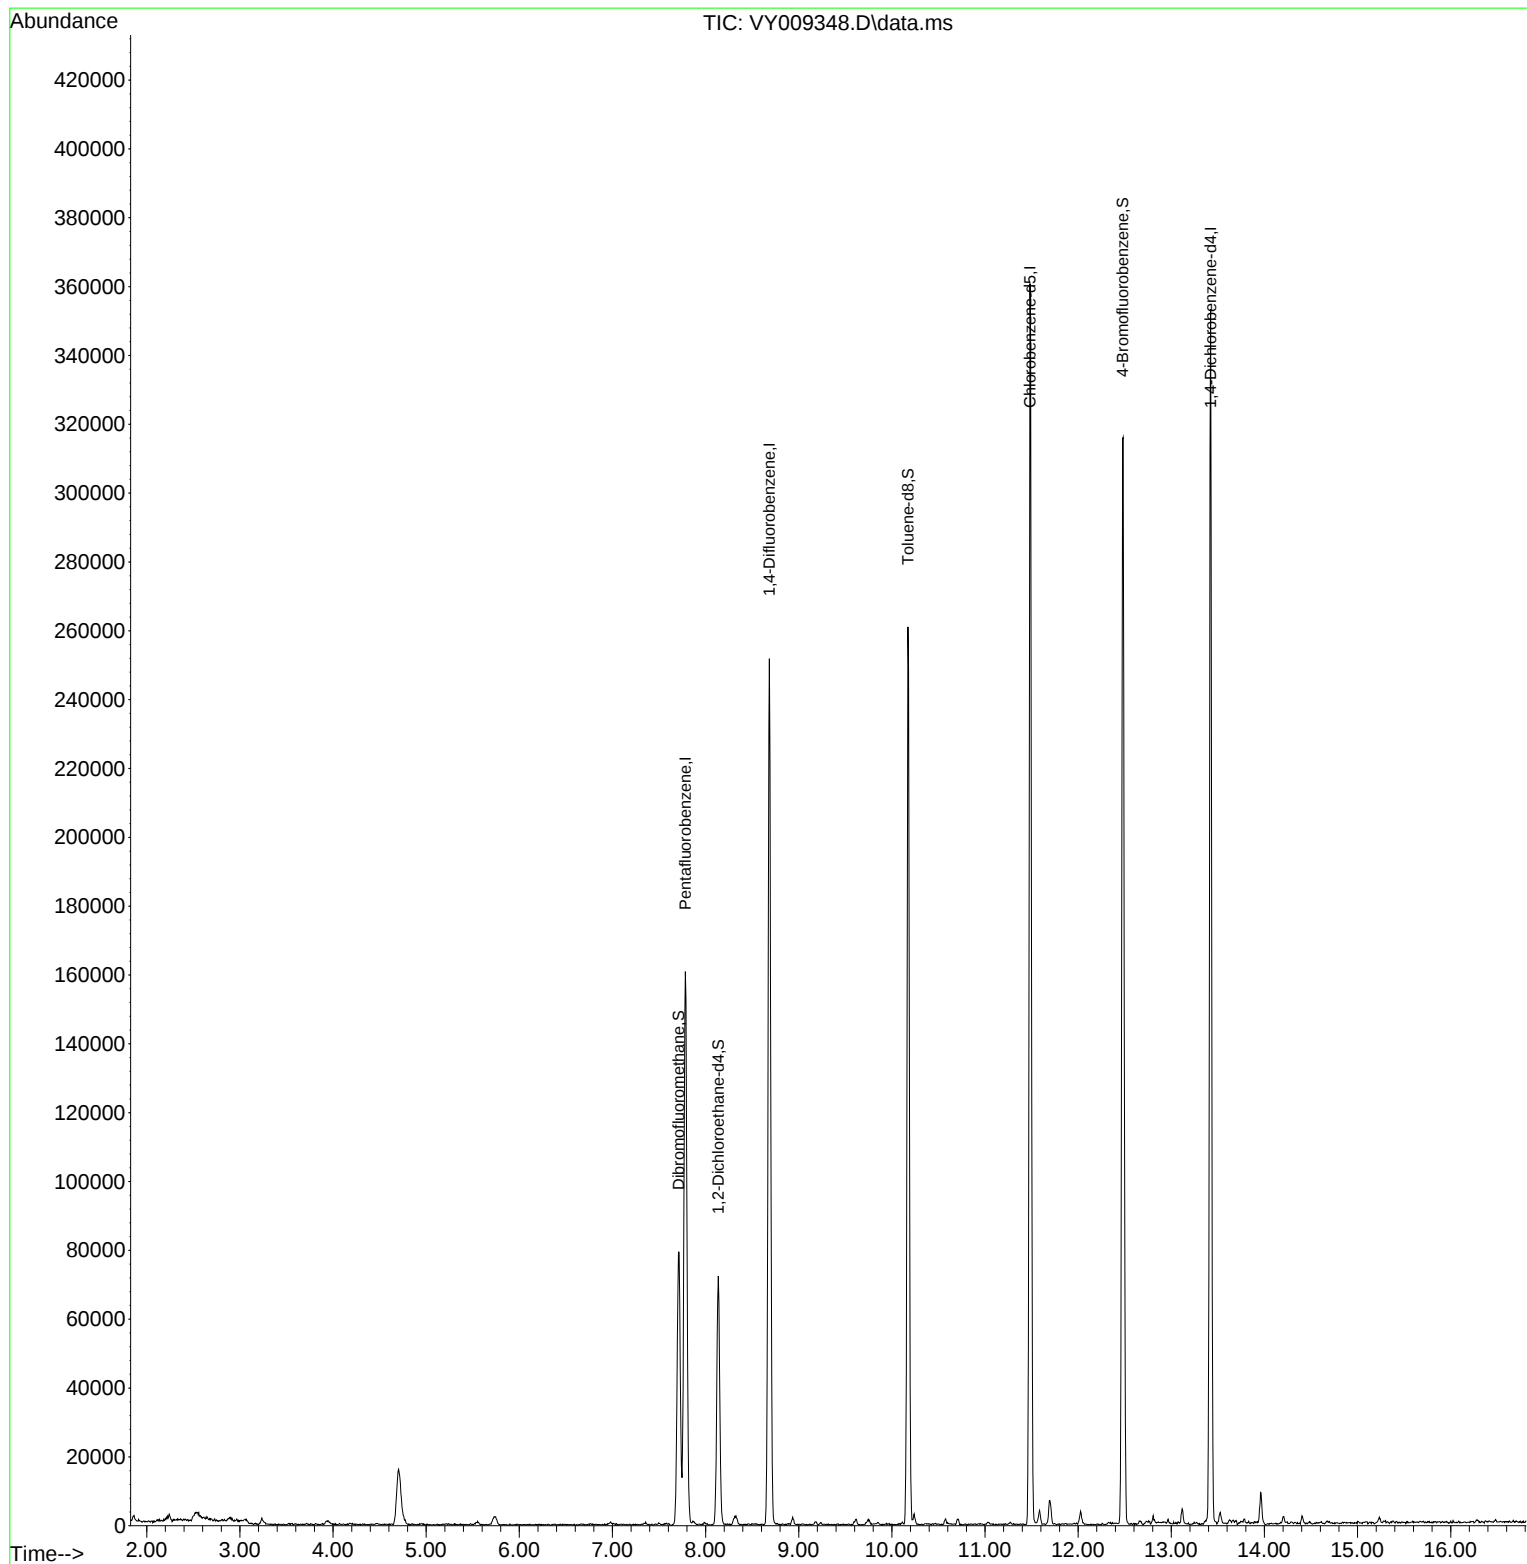


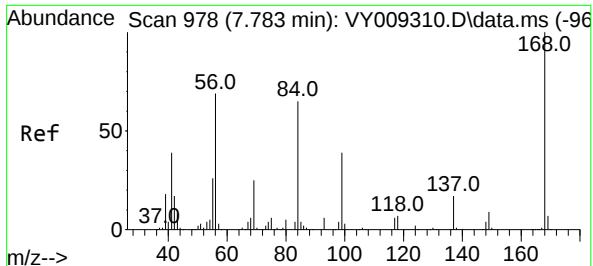

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.783 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY009348.D
Acq: 27 Jun 2022 17:16




Instrument :
MSVOA_Y
ClientSampleId :
B2203-35


Tgt Ion:168 Resp: 125623
Ion Ratio Lower Upper
168 100
99 50.5 42.1 63.1

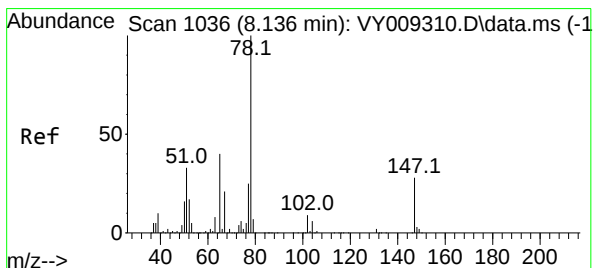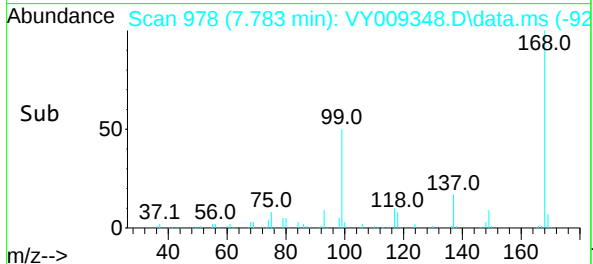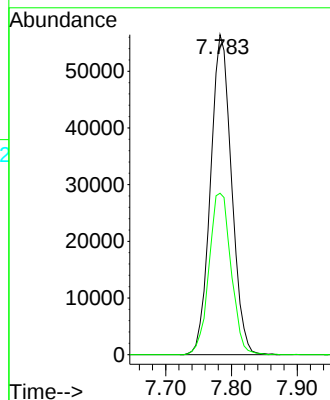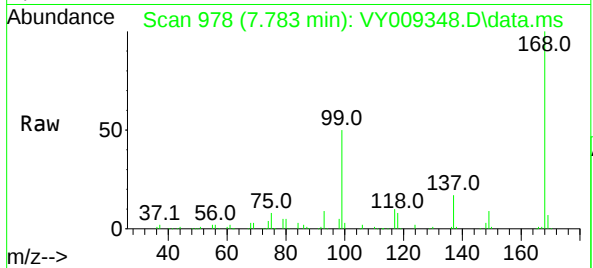

#33
1,2-Dichloroethane-d4
Concen: 58.987 ug/l
RT: 8.136 min Scan# 1036
Delta R.T. 0.000 min
Lab File: VY009348.D
Acq: 27 Jun 2022 17:16

Tgt Ion: 65 Resp: 55028
Ion Ratio Lower Upper
65 100
67 51.7 0.0 108.4

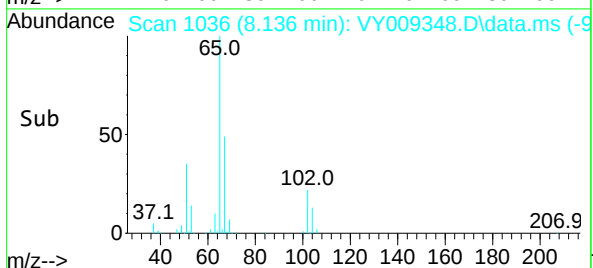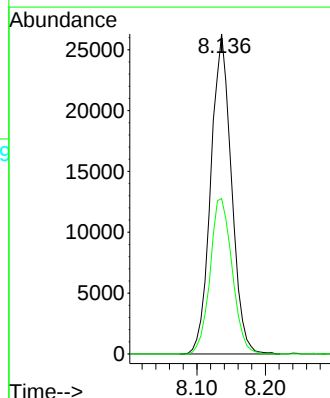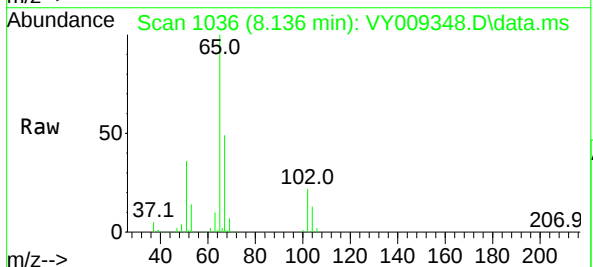

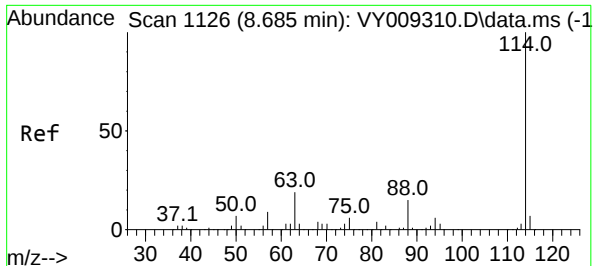

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.685 min Scan# 1126

Delta R.T. -0.000 min

Lab File: VY009348.D

Acq: 27 Jun 2022 17:16

Instrument :

MSVOA_Y

ClientSampleId :

B2203-35





Tgt Ion:114 Resp: 213736

Ion Ratio Lower Upper

114 100

63 19.2 0.0 38.0

88 14.1 0.0 30.0

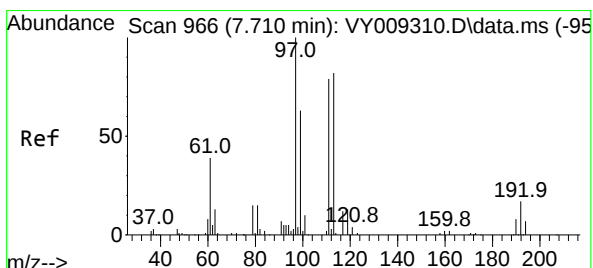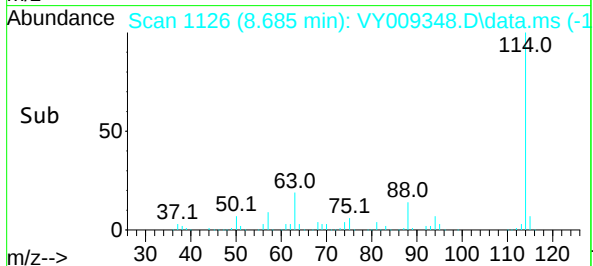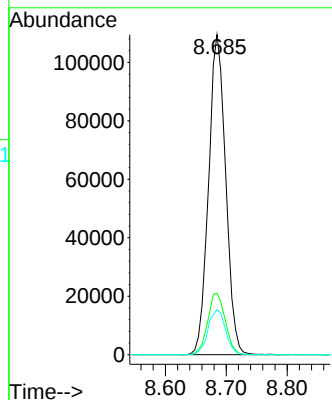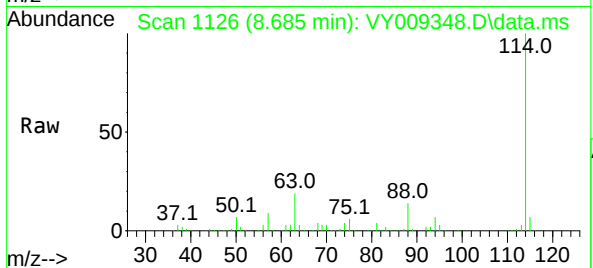

#35

Dibromofluoromethane

Concen: 47.890 ug/l

RT: 7.709 min Scan# 966

Delta R.T. -0.000 min

Lab File: VY009348.D

Acq: 27 Jun 2022 17:16




Tgt Ion:113 Resp: 55249


Ion Ratio Lower Upper

113 100

111 104.1 80.6 120.8

192 20.5 16.2 24.4


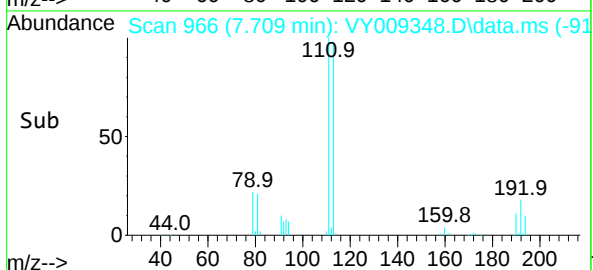
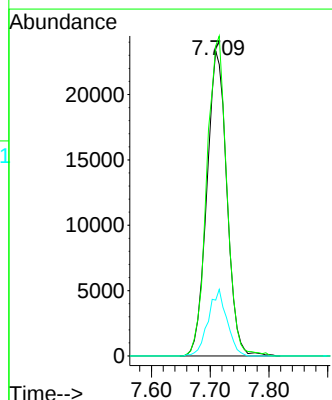
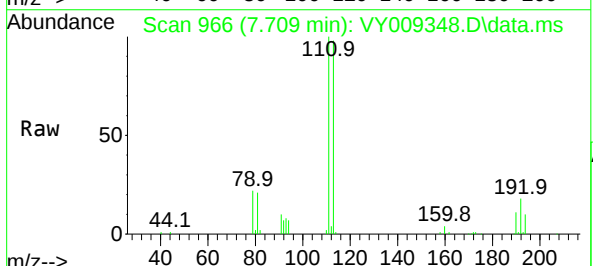


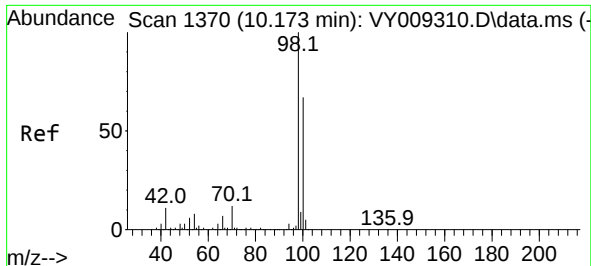

#50
Toluene-d8
Concen: 49.072 ug/l
RT: 10.172 min Scan# 11
Delta R.T. -0.001 min
Lab File: VY009348.D
Acq: 27 Jun 2022 17:16




Instrument :
MSVOA_Y
ClientSampleId :
B2203-35


Tgt Ion: 98 Resp: 165834
Ion Ratio Lower Upper
98 100
100 65.6 52.9 79.3

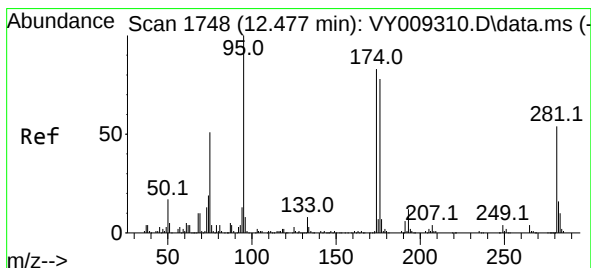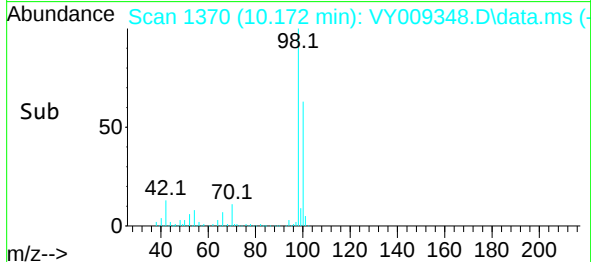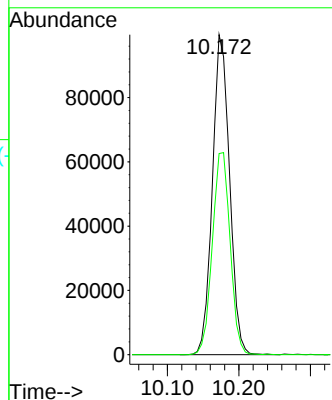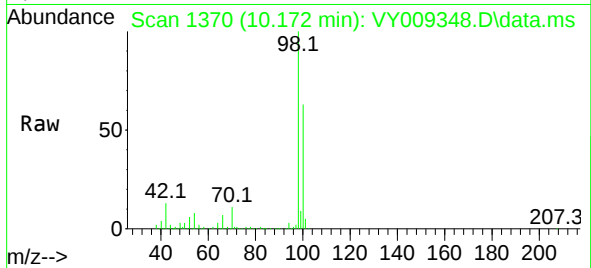

#62
4-Bromofluorobenzene
Concen: 45.044 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. -0.000 min
Lab File: VY009348.D
Acq: 27 Jun 2022 17:16

Tgt Ion: 95 Resp: 74009
Ion Ratio Lower Upper
95 100
174 88.4 0.0 173.8
176 84.8 0.0 167.0

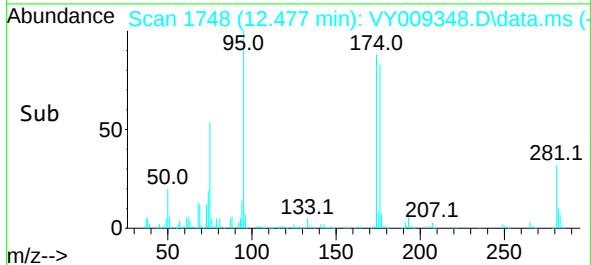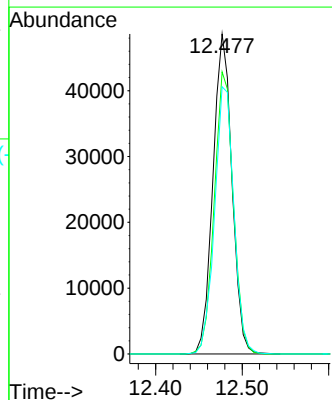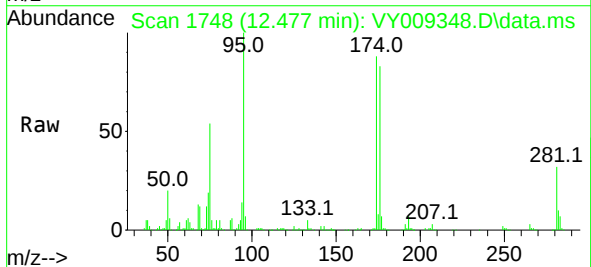

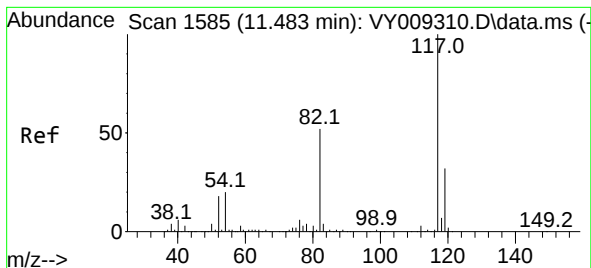

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.483 min Scan# 11

Delta R.T. 0.000 min

Lab File: VY009348.D

Acq: 27 Jun 2022 17:16

Instrument :

MSVOA_Y

ClientSampleId :

B2203-35





Tgt Ion:117 Resp: 191224

Ion Ratio Lower Upper

117 100

82 54.2 41.8 62.6

119 32.3 25.6 38.4

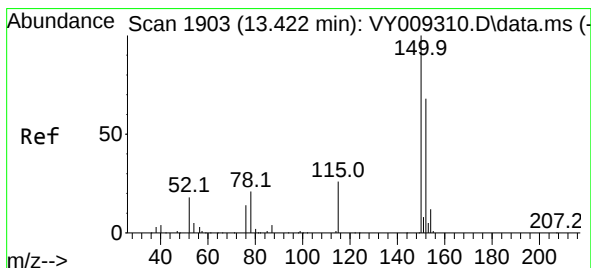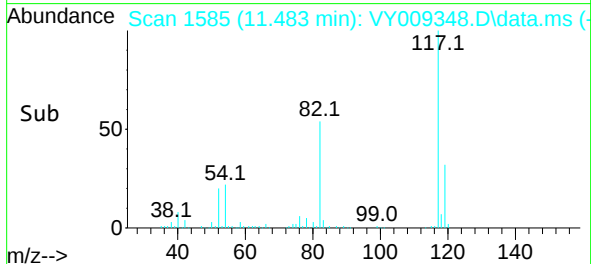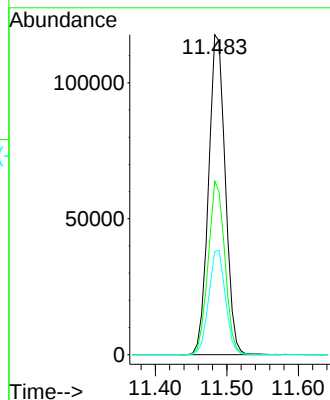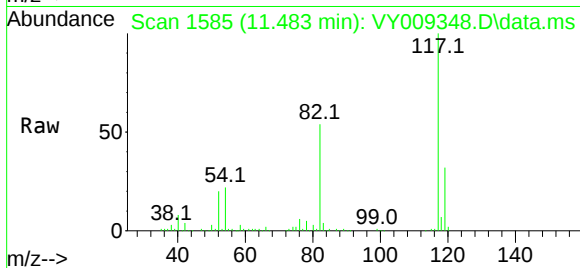

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.422 min Scan# 1903

Delta R.T. -0.000 min

Lab File: VY009348.D

Acq: 27 Jun 2022 17:16

Tgt Ion:152 Resp: 88881

Ion Ratio Lower Upper

152 100

115 56.7 28.6 85.9

150 158.9 0.0 349.8

