
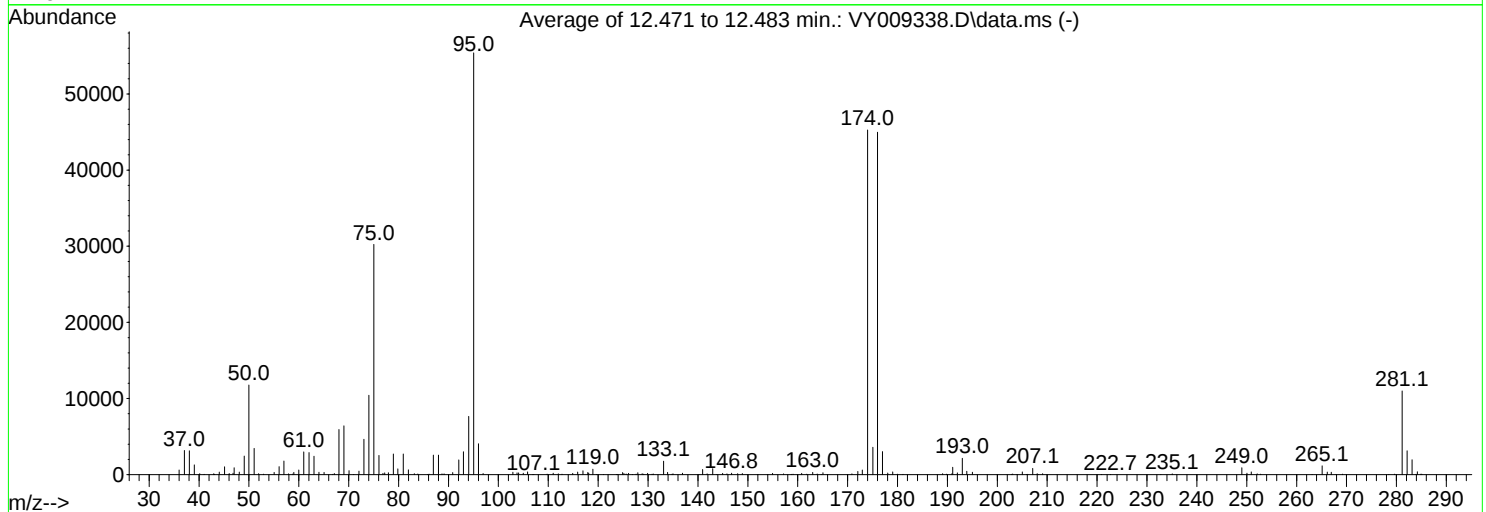


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY062722\
 Data File : VY009338.D
 Acq On : 27 Jun 2022 09:12
 Operator : KP/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y062422S.M
 Title : SW846 8260
 Last Update : Sat Jun 25 07:08:46 2022

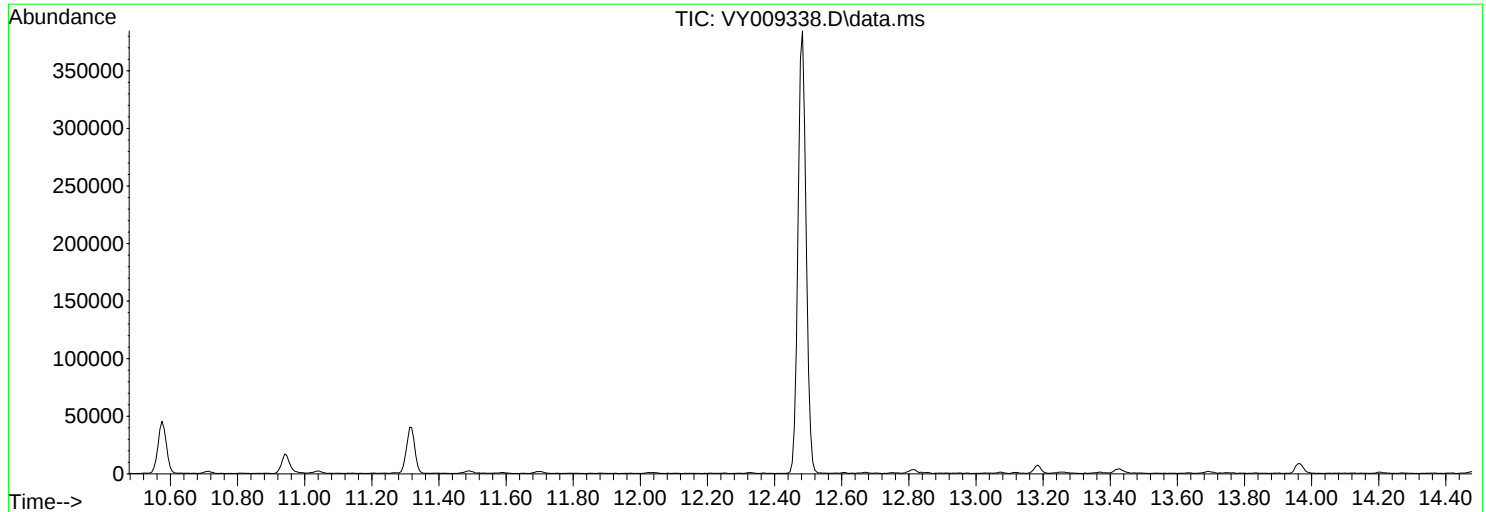

AutoFind: Scans 1747, 1748, 1749; Background Corrected with Scan 1739

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.2	11768	PASS
75	95	30	60	54.6	30235	PASS
95	95	100	100	100.0	55400	PASS
96	95	5	9	7.3	4048	PASS
173	174	0.00	2	1.4	620	PASS
174	95	50	100	81.7	45261	PASS
175	174	5	9	7.9	3584	PASS
176	174	95	101	99.4	44973	PASS
177	176	5	9	6.8	3037	PASS