
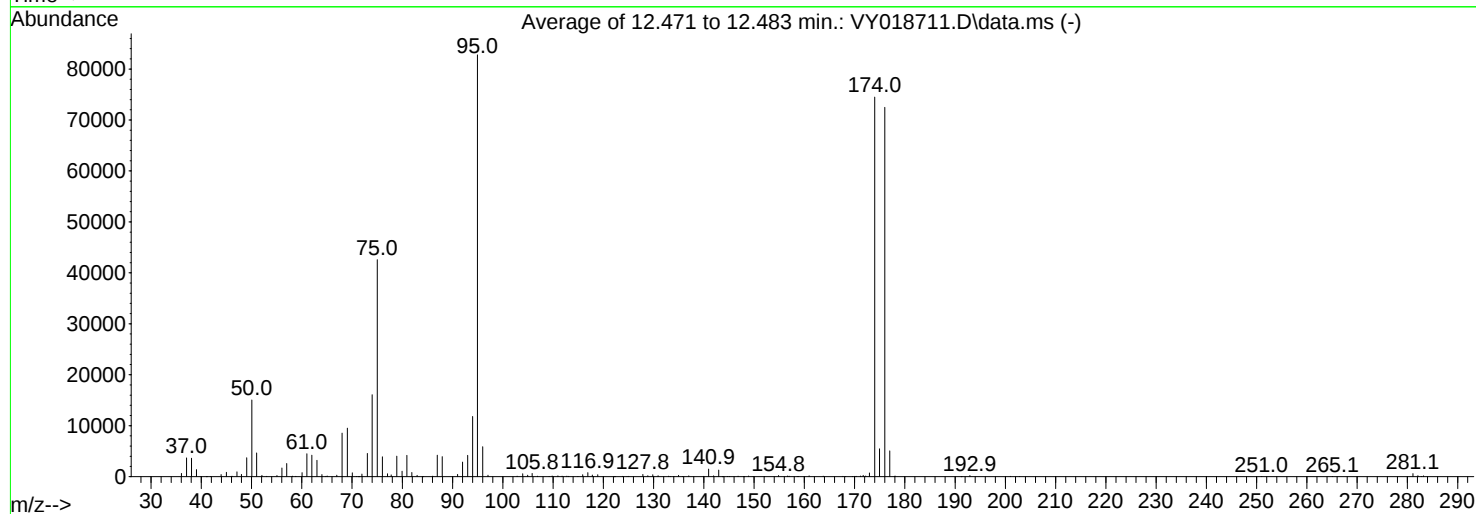


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY062724\
Data File : VY018711.D
Acq On : 27 Jun 2024 09:10
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y061324S.M
Title : SW846 8260
Last Update : Fri Jun 14 07:08:24 2024

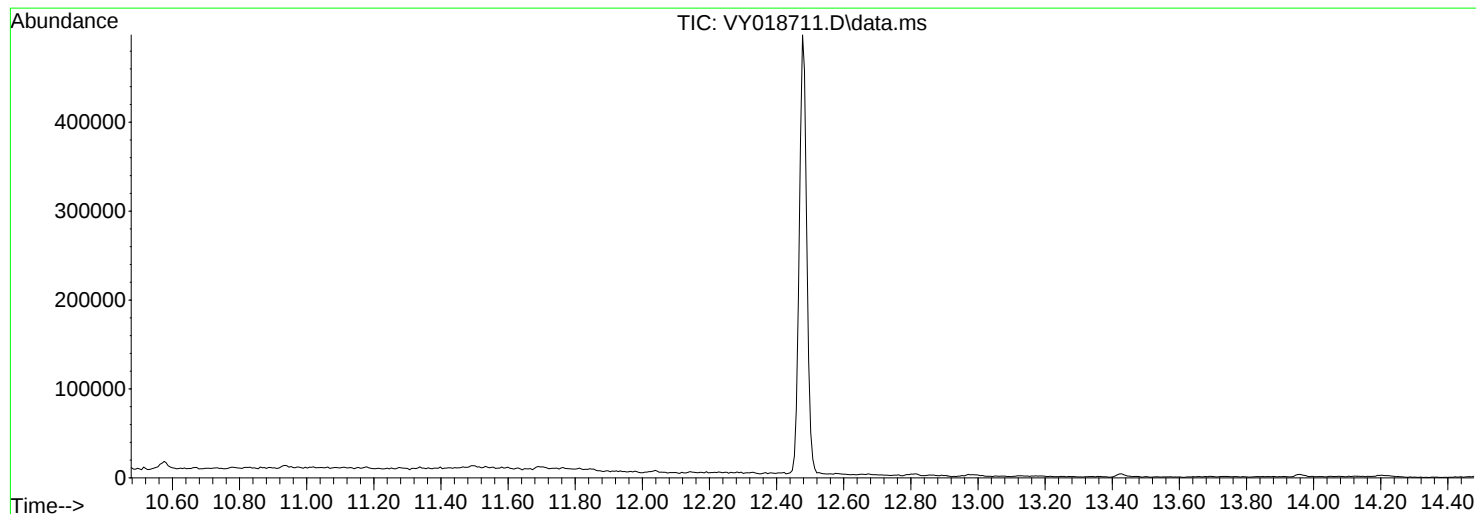

AutoFind: Scans 1747, 1748, 1749; Background Corrected with Scan 1739

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	15059	PASS
75	95	30	60	51.5	42600	PASS
95	95	100	100	100.0	82790	PASS
96	95	5	9	7.1	5890	PASS
173	174	0.00	2	1.0	739	PASS
174	95	50	100	90.0	74480	PASS
175	174	5	9	7.4	5478	PASS
176	174	95	101	97.3	72499	PASS
177	176	5	9	7.0	5058	PASS