
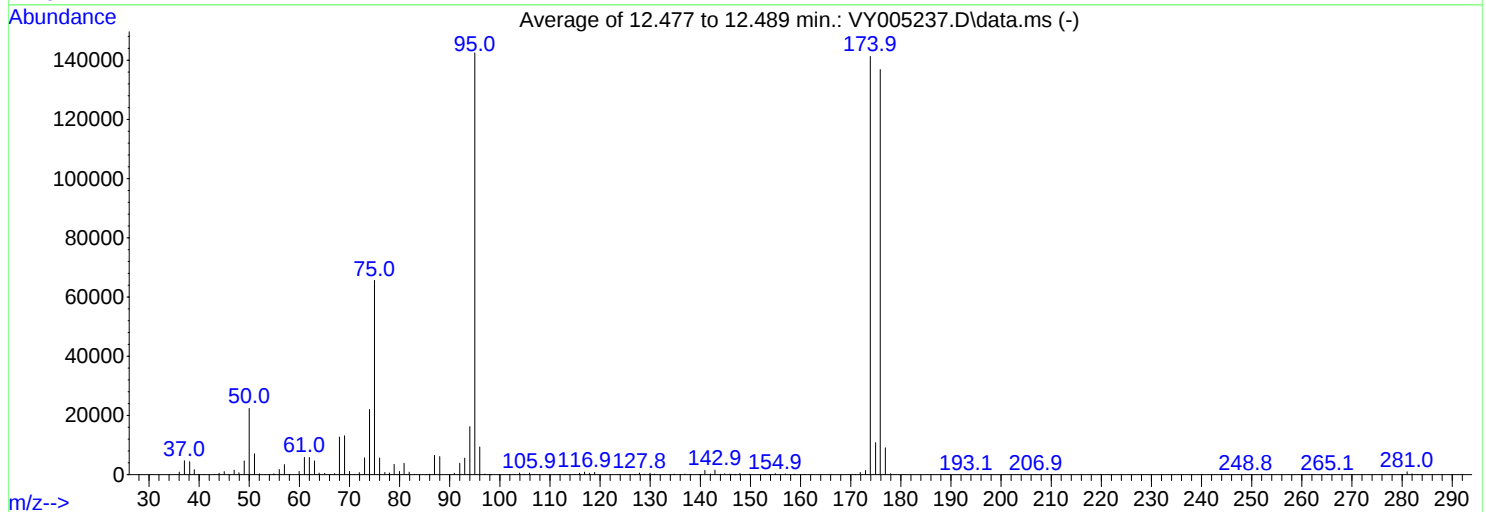


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY062821\  
 Data File : VY005237.D  
 Acq On : 28 Jun 2021 09:50  
 Operator : SY/MD  
 Sample : BFB  
 Misc : 5.00G/5ML/MSVOA\_Y/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_Y  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y062221S.M  
 Title : SW846 8260  
 Last Update : Wed Jun 23 07:57:52 2021

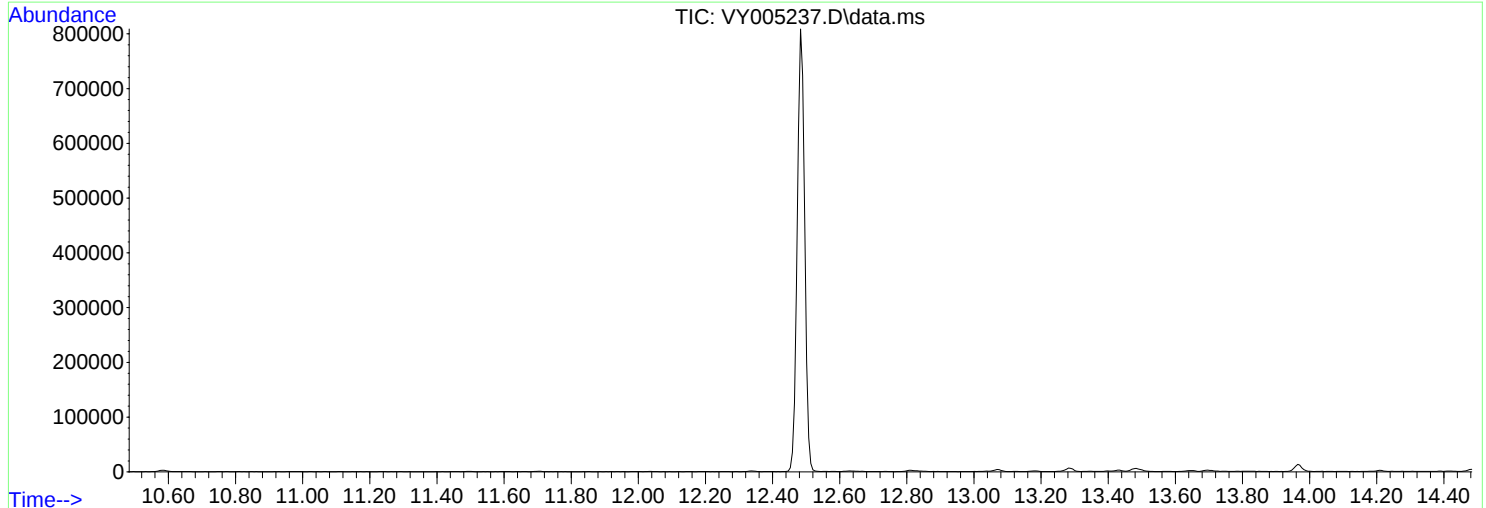

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1739

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 15.7         | 22384      | PASS                |
| 75             | 95              | 30              | 60              | 46.0         | 65608      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 142472     | PASS                |
| 96             | 95              | 5               | 9               | 6.6          | 9346       | PASS                |
| 173            | 174             | 0.00            | 2               | 1.0          | 1401       | PASS                |
| 174            | 95              | 50              | 100             | 99.2         | 141301     | PASS                |
| 175            | 174             | 5               | 9               | 7.7          | 10811      | PASS                |
| 176            | 174             | 95              | 101             | 96.8         | 136845     | PASS                |
| 177            | 176             | 5               | 9               | 6.7          | 9103       | PASS                |