


Tert butylalcohol

Response Ratio

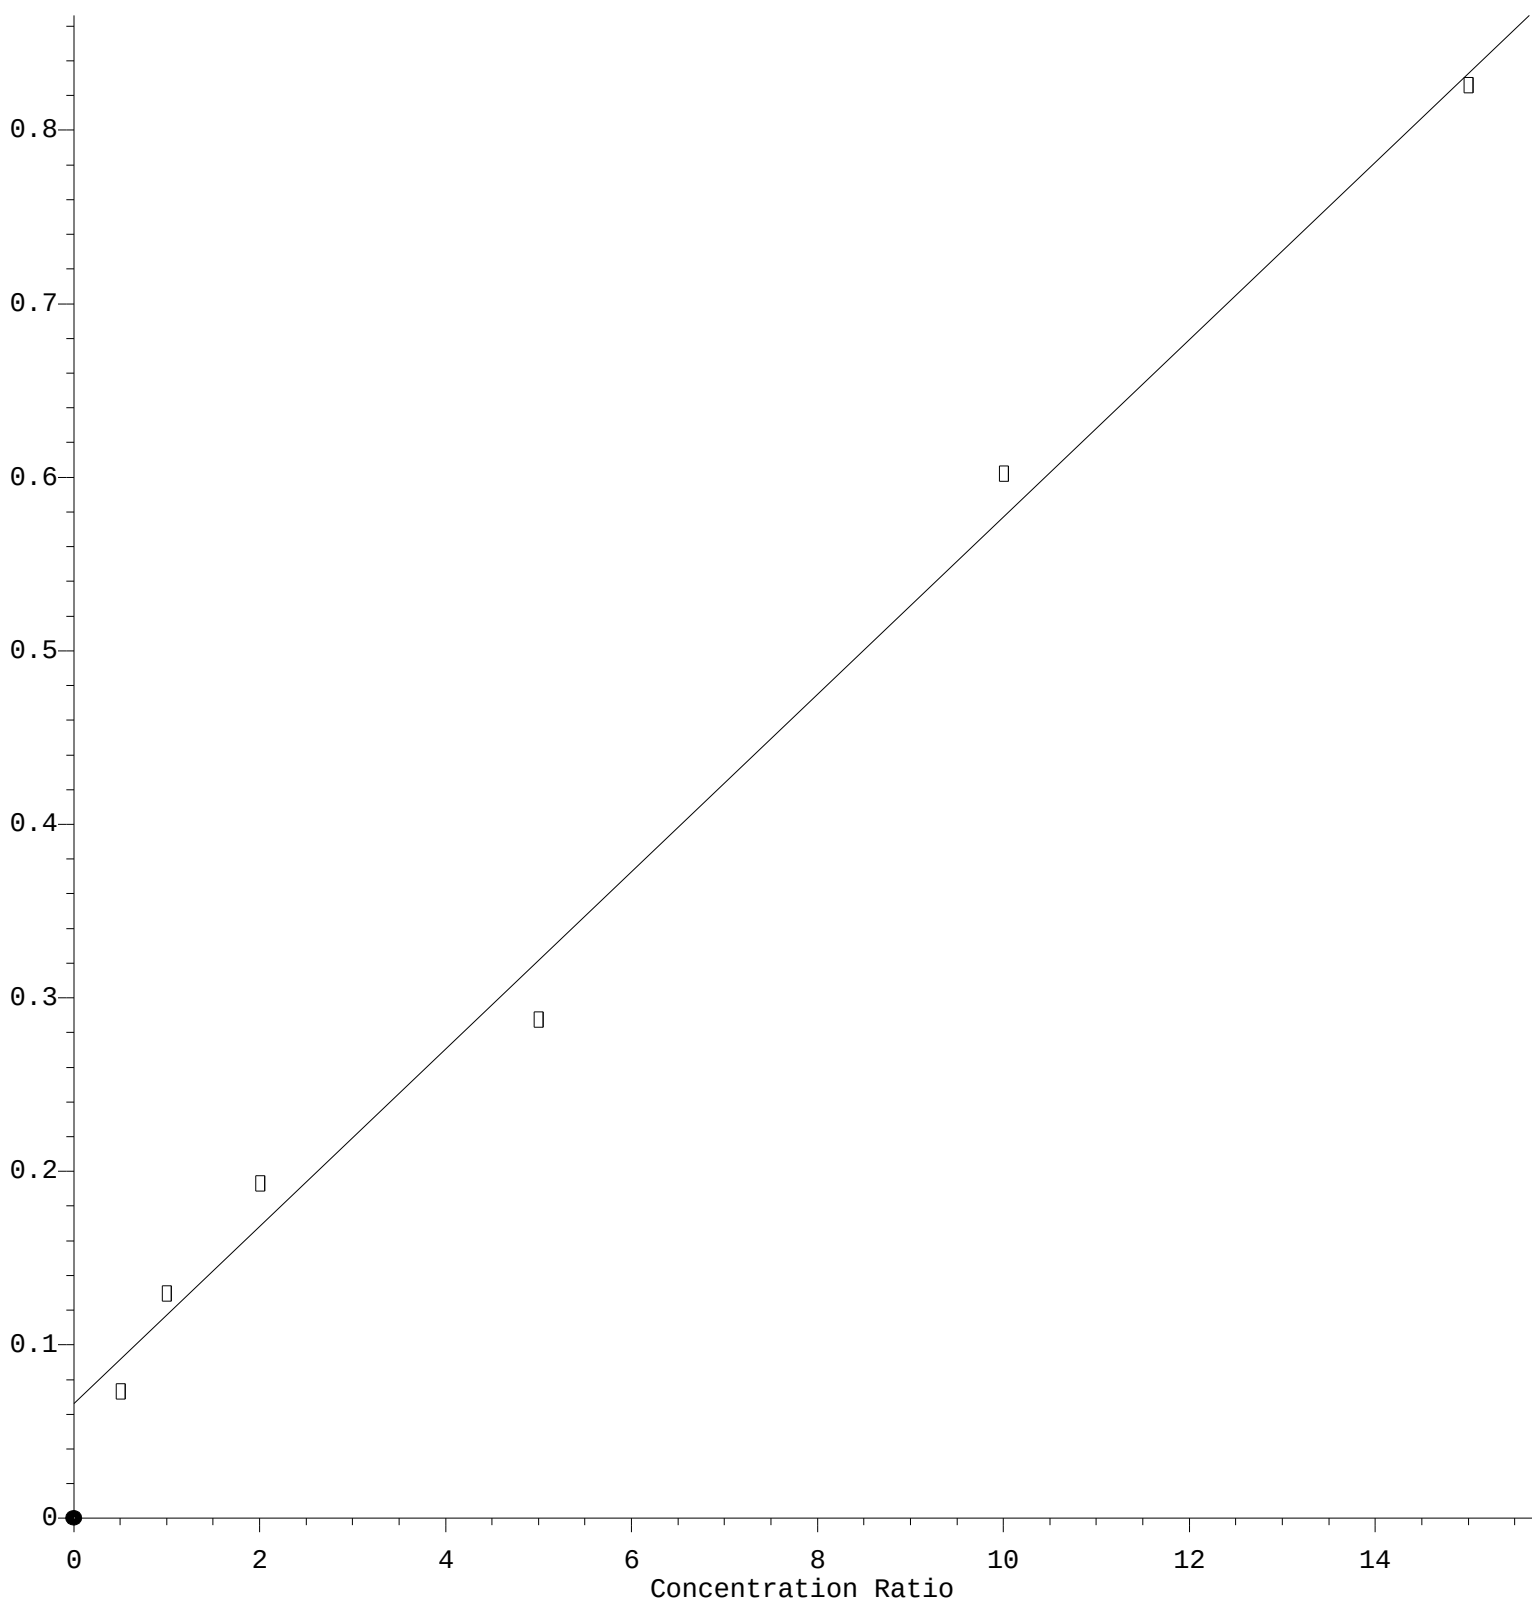

$$\text{Response} = 5.119\text{e-}002 * \text{Amt} + 6.598\text{e-}002$$


Coef of Det (r^2) = 0.993360 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y062822S.M

Calibration Table Last Updated: Wed Jun 29 17:35:34 2022

Methyl Acetate

Response Ratio

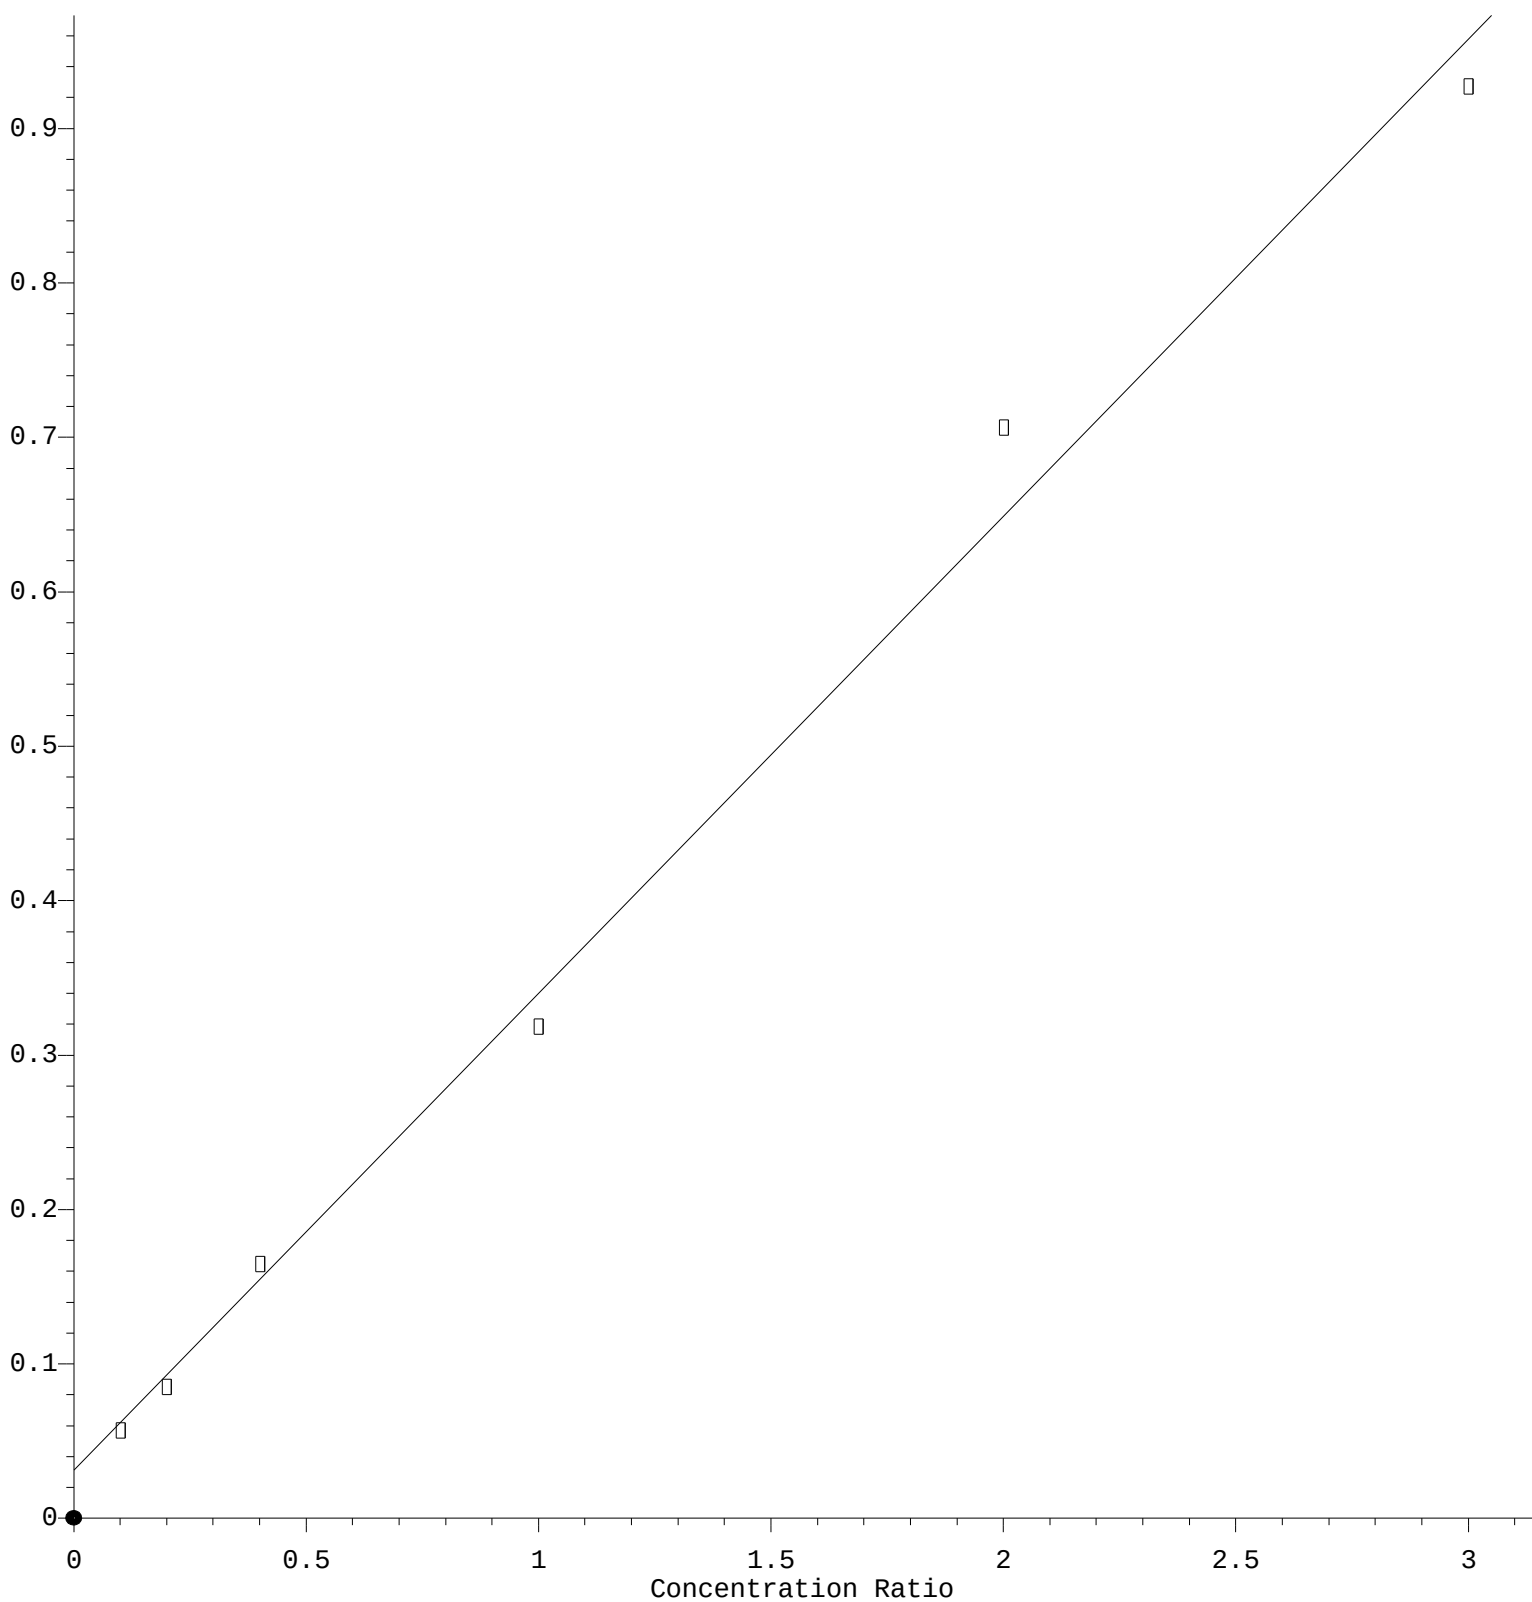

$$\text{Response} = 3.089\text{e-}001 * \text{Amt} + 3.121\text{e-}002$$


Coef of Det (r^2) = 0.992431 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y062822S.M

Calibration Table Last Updated: Wed Jun 29 17:35:34 2022

Methylene Chloride

Response Ratio

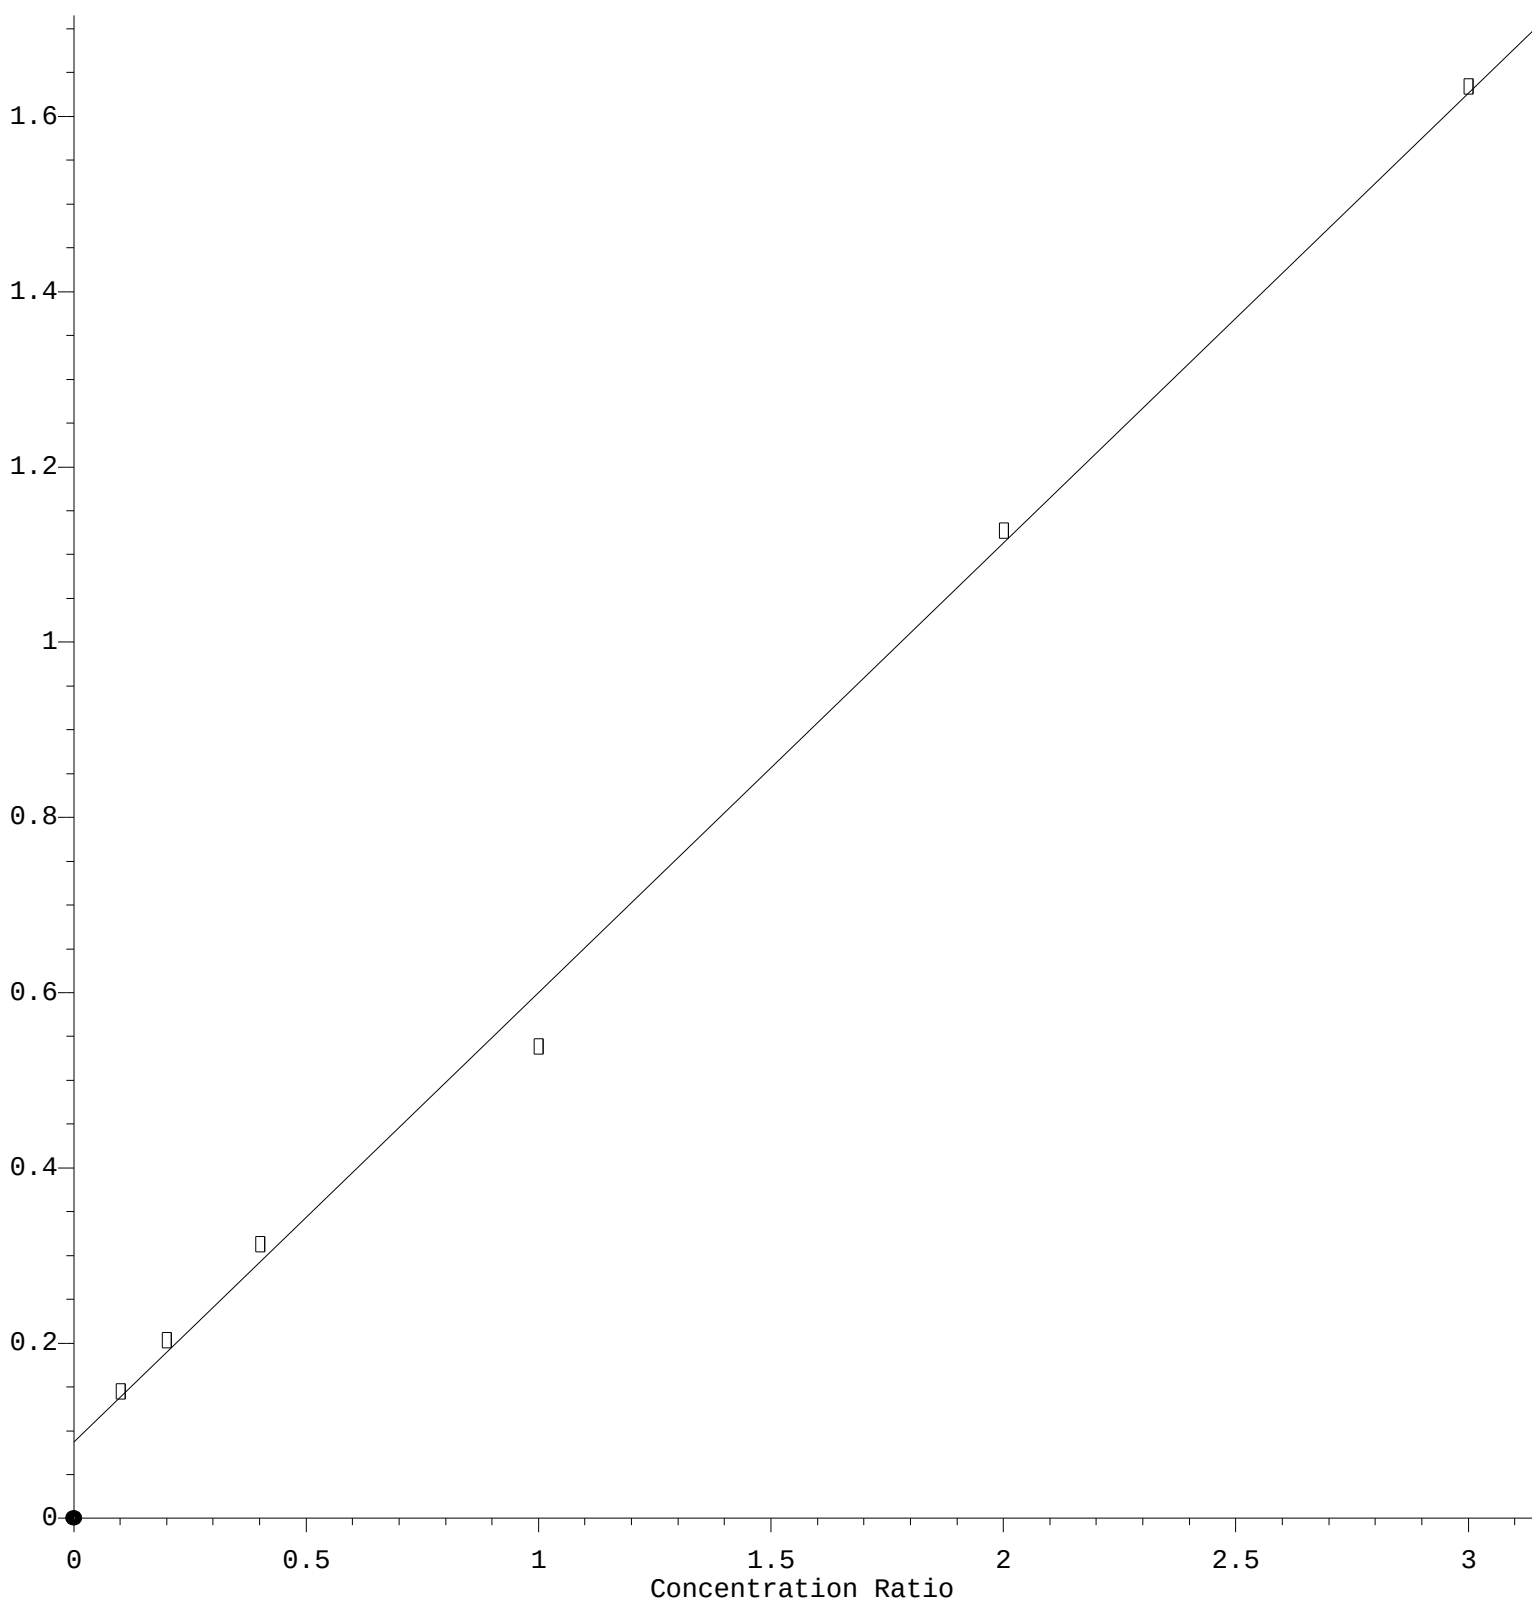

$$\text{Response} = 5.132\text{e-}001 * \text{Amt} + 8.670\text{e-}002$$

Coef of Det (r^2) = 0.997364 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y062822S.M

Calibration Table Last Updated: Wed Jun 29 17:35:34 2022