

Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY062920\
 Data File : VY003006.D
 Acq On : 29 Jun 2020 14:52
 Operator : SY/MD
 Sample : VY0629SBL01
 Misc : 5.00G/5ML/MSVOA Y/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0629SBL01

Quant Time: Jun 30 05:54:03 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y062920S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jun 30 04:11:35 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.80	168	353857	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.69	114	572172	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.49	117	546194	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.42	152	278824	50.00	ug/l	0.00


System Monitoring Compounds

33) 1,2-Dichloroethane-d4	8.14	65	204951	58.32	ug/l	0.00
Spiked Amount	50.000		Recovery	=	116.64%	
35) Dibromofluoromethane	7.72	113	186252	52.18	ug/l	0.00
Spiked Amount	50.000		Recovery	=	104.36%	
50) Toluene-d8	10.18	98	700226	52.66	ug/l	0.00
Spiked Amount	50.000		Recovery	=	105.32%	
62) 4-Bromofluorobenzene	12.48	95	252989	54.05	ug/l	0.00
Spiked Amount	50.000		Recovery	=	108.10%	

Target Compounds

						Qvalue
13) Acrolein	3.74	56	455	1.414	ug/l #	49
15) Acrylonitrile	5.18	53	1129	1.183	ug/l #	89
16) Acetone	3.96	43	3483	4.202	ug/l	99
20) Methylene Chloride	4.72	84	48152	7.027	ug/l	93
25) 2-Butanone	6.99	43	6428	4.882	ug/l #	81
26) 2,2-Dichloropropane	6.99	77	7538	1.322	ug/l #	55
31) Cyclohexane	7.80	56	7165	1.159	ug/l #	1
36) 1,1-Dichloropropene	7.79	75	24781	4.496	ug/l #	51
38) Carbon Tetrachloride	7.80	117	32338	5.639	ug/l #	17
52) Toluene	10.25	92	11667	1.228	ug/l	98
68) m/p-Xylenes	11.70	106	15753	2.148	ug/l	99
76) 1,2,3-Trichloropropane	12.48	75	135042	48.937	ug/l #	100
81) trans-1,4-Dichloro-2-buten	12.48	75	135042	95.211	ug/l #	13
93) 1,2,4-Trichlorobenzene	15.01	180	10047	1.725	ug/l	95
94) Hexachlorobutadiene	15.11	225	3876	1.055	ug/l	96
95) Naphthalene	15.24	128	23444	2.204	ug/l	96
96) 1,2,3-Trichlorobenzene	15.42	180	9654	1.909	ug/l	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

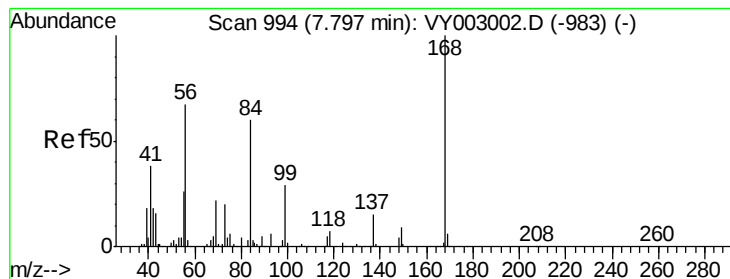

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.80 min Scan# 994

Delta R.T. -0.00 min

Lab File: VY003006.D

Acq: 29 Jun 2020 14:52

Instrument :

MSVOA_Y

ClientSampleId :


VY0629SBL01

Tot Ion:168 Resp: 353857

Ion Ratio Lower Upper

168 100

99 50.0 39.2 58.8



Abundance Ion 167.90 (167.60 to 168.60): VY0

Ion 98.90 (98.60 to 99.60): VY0

7.80



150000

100000

50000

0

Time-->



#13

Acrolein

Concen: 1.414 ug/l

RT: 3.74 min Scan# 328

Delta R.T. -0.00 min

Lab File: VY003006.D


Acq: 29 Jun 2020 14:52

Tgt Ion: 56 Resp: 455

Ion Ratio Lower Upper

56 100

55 112.3 56.4 84.6#



Abundance Ion 56.00 (55.70 to 56.70): VY0

Ion 55.00 (54.70 to 55.70): VY0

3.74

250

200


150


100

50

0

Time-->



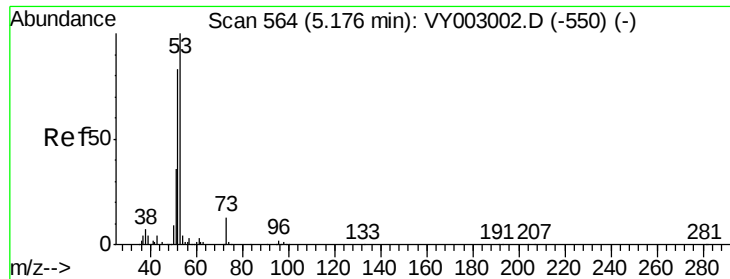

#15

Acrylonitrile

Concen: 1.183 ug/l

RT: 5.18 min Scan# 565

Delta R.T. 0.01 min

Lab File: VY003006.D

Acq: 29 Jun 2020 14:52

Instrument :

MSVOA_Y

ClientSampleId :

VY0629SBL01


Tot Ion: 53 Resp: 1129

Ion Ratio Lower Upper

53 100

52 75.1 66.2 99.2




51 27.5 29.5 44.3#

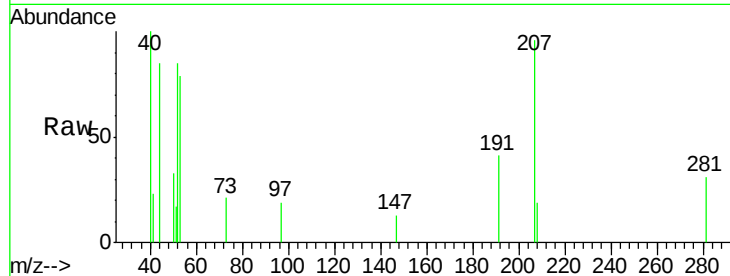

Abundance Ion 53.00 (52.70 to 53.70): VY0

Ion 52.00 (51.70 to 52.70): VY0

Ion 51.00 (50.70 to 51.70): VY0

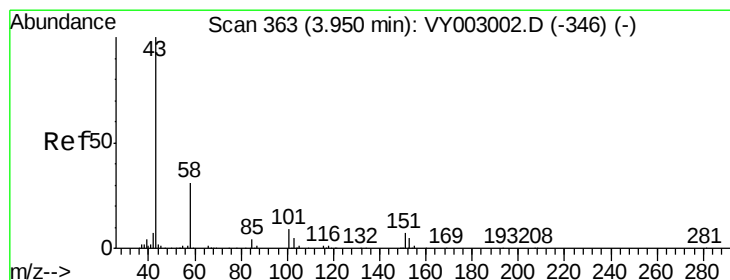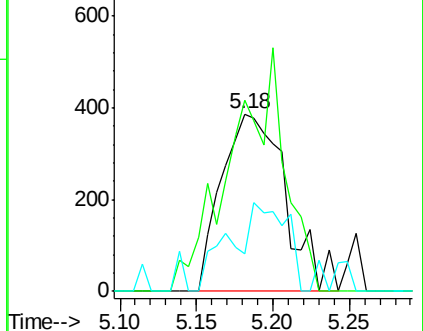

#16

Acetone

Concen: 4.202 ug/l

RT: 3.96 min Scan# 365

Delta R.T. 0.01 min

Lab File: VY003006.D


Acq: 29 Jun 2020 14:52

Tgt Ion: 43 Resp: 3483

Ion Ratio Lower Upper



43 100




58 31.4 24.7 37.1



Abundance Ion 43.00 (42.70 to 43.70): VY0

Ion 58.00 (57.70 to 58.70): VY0



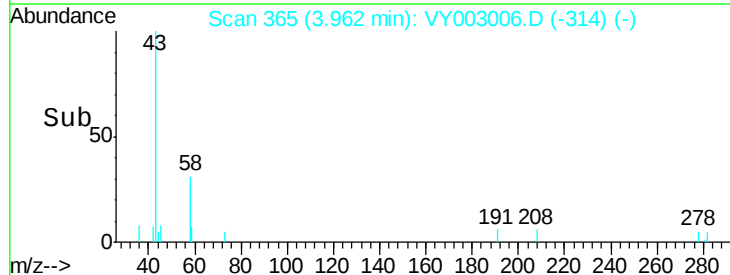
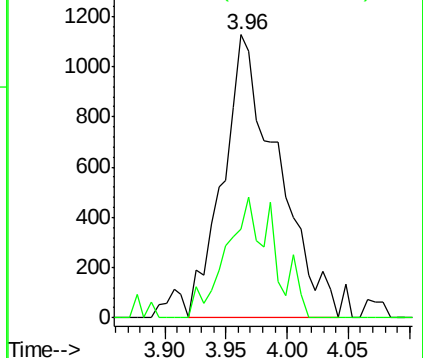


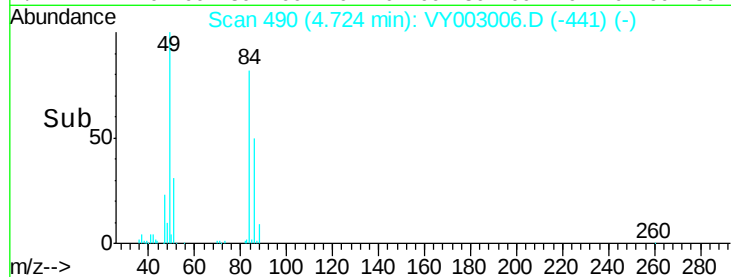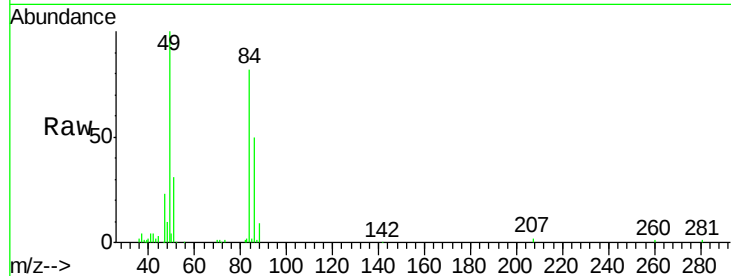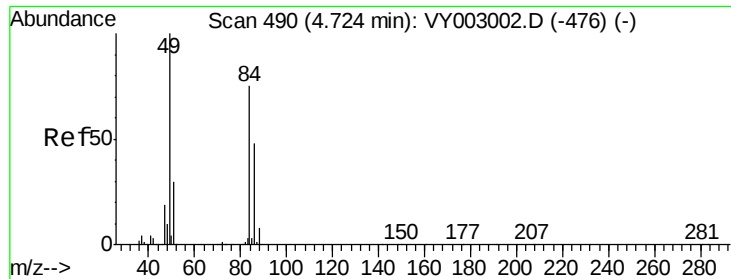

#20
Methvlene Chloride
Concen: 7.027 ug/l
RT: 4.72 min Scan# 490
Delta R.T. 0.00 min
Lab File: VY003006.D
Acq: 29 Jun 2020 14:52


Instrument :
MSVOA_Y
ClientSampleId :
VY0629SBL01


Tot Ion: 84 Resp: 48152
Ion Ratio Lower Upper
84 100
49 122.6 106.8 160.2
51 38.2 32.0 48.0
86 61.7 51.4 77.2

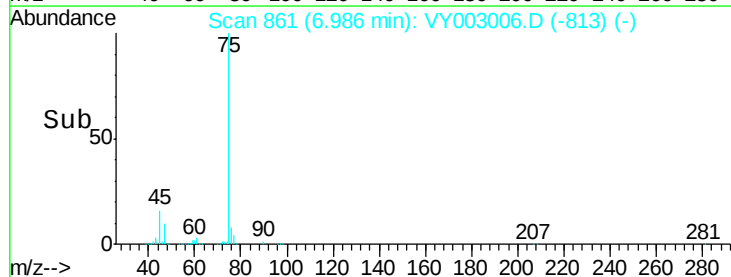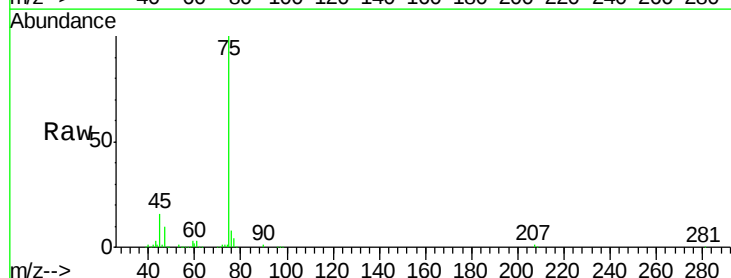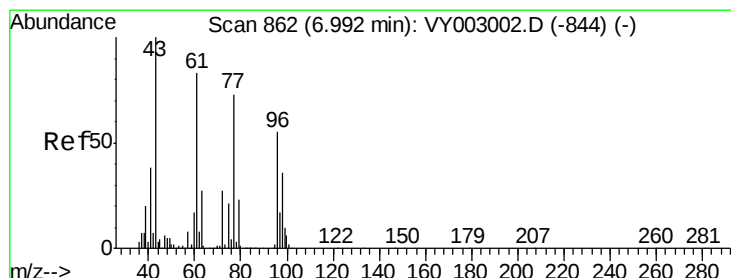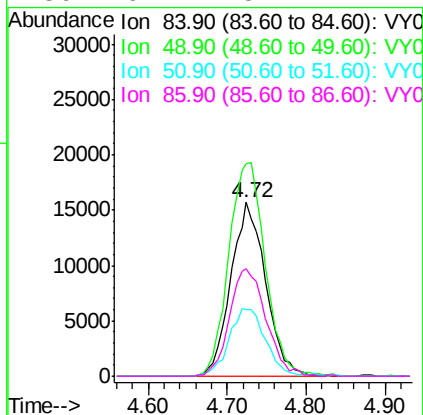

#25
2-Butanone
Concen: 4.882 ug/l
RT: 6.99 min Scan# 861
Delta R.T. -0.01 min
Lab File: VY003006.D
Acq: 29 Jun 2020 14:52

Tgt Ion: 43 Resp: 6428
Ion Ratio Lower Upper
43 100
72 16.8 21.4 32.0#




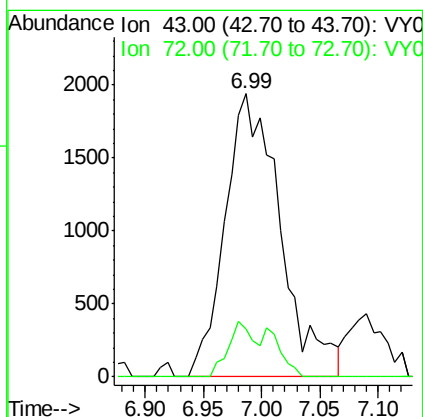


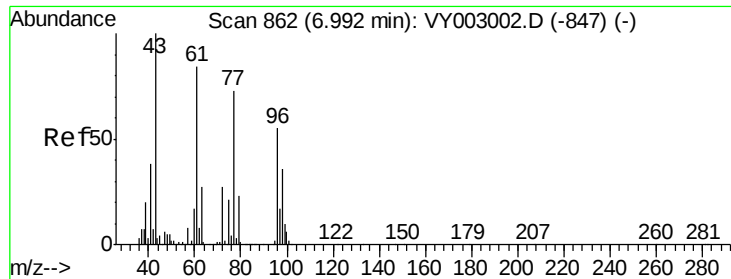

#26
 2,2-Dichloropropane
 Concen: 1.322 ug/l
 RT: 6.99 min Scan# 861
 Delta R.T. -0.01 min
 Lab File: VY003006.D
 Acq: 29 Jun 2020 14:52




Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0629SBL01


Tot Ion: 77 Resp: 7538
 Ion Ratio Lower Upper
 77 100
 97 1.0 11.3 33.9#

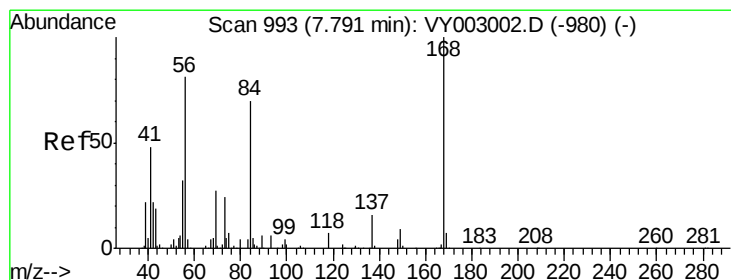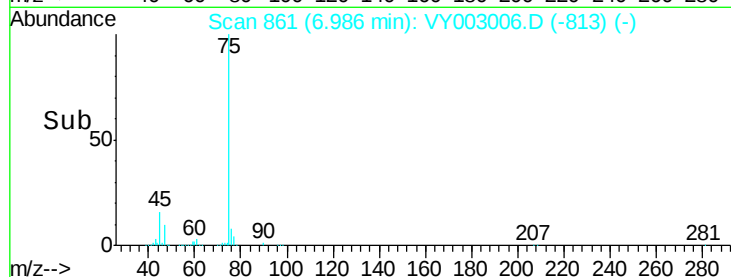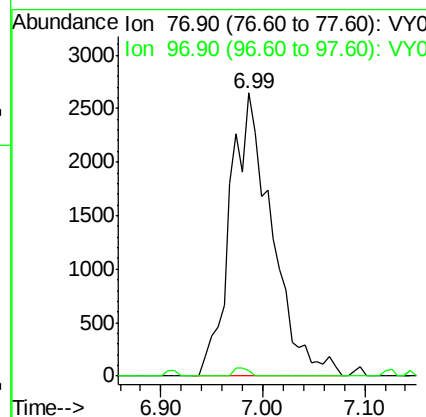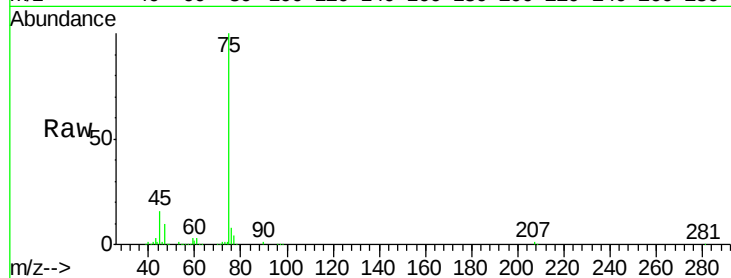

#31
 Cyclohexane
 Concen: 1.159 ug/l
 RT: 7.80 min Scan# 994
 Delta R.T. 0.01 min
 Lab File: VY003006.D
 Acq: 29 Jun 2020 14:52

Tgt Ion: 56 Resp: 7165
 Ion Ratio Lower Upper
 56 100
 69 160.7 27.0 40.4#
 84 153.5 68.1 102.1#


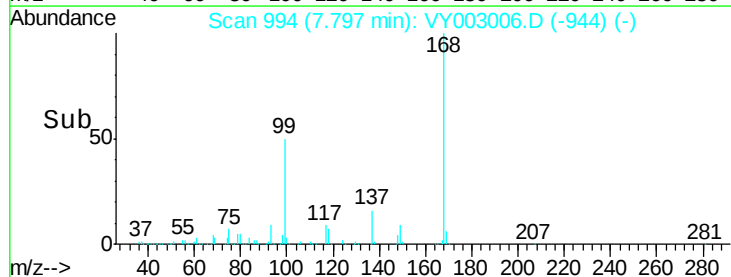
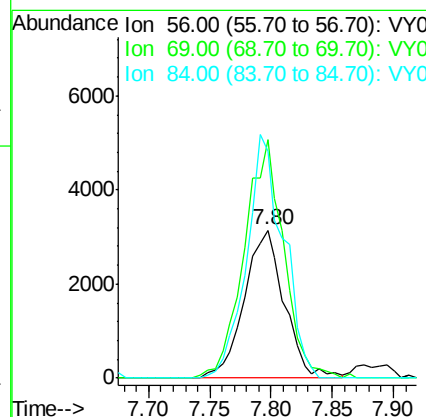
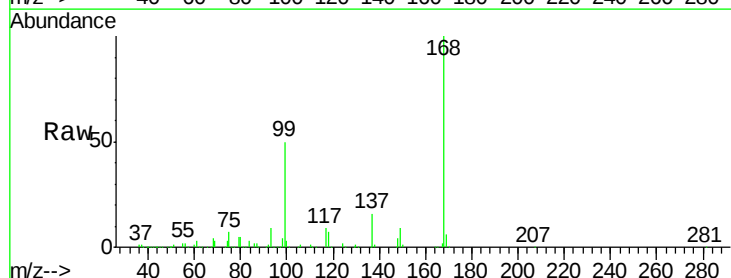




#33
 1,2-Dichloroethane-d4
 Concen: 58.316 ug/l
 RT: 8.14 min Scan# 1051
 Delta R.T. -0.00 min
 Lab File: VY003006.D
 Acq: 29 Jun 2020 14:52




Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0629SBL01


Tot Ion: 65 Resp: 204951
 Ion Ratio Lower Upper
 65 100
 67 52.8 0.0 105.6

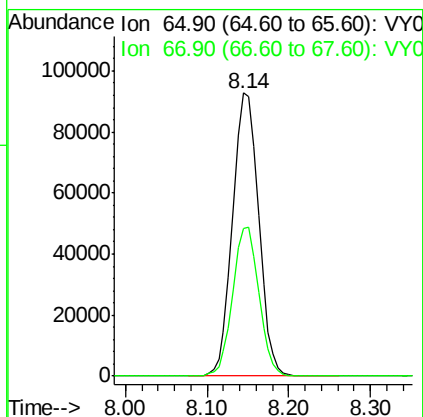

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.69 min Scan# 1141
 Delta R.T. -0.00 min
 Lab File: VY003006.D
 Acq: 29 Jun 2020 14:52

Tgt Ion: 114 Resp: 572172
 Ion Ratio Lower Upper
 114 100
 63 21.4 0.0 40.6
 88 15.8 0.0 30.0



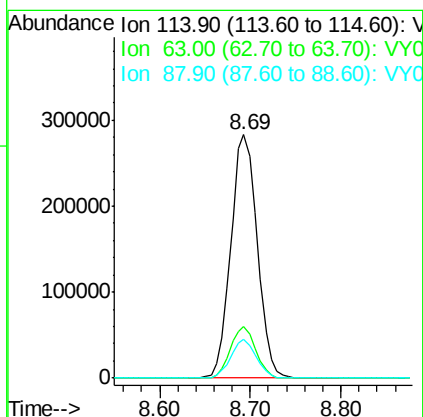





#35
 Dibromofluoromethane
 Concen: 52.182 ug/l
 RT: 7.72 min Scan# 982
 Delta R.T. -0.00 min
 Lab File: VY003006.D
 Acq: 29 Jun 2020 14:52




Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0629SBL01


Tot Ion	Ratio	Lower	Upper
113	100		
111	105.7	82.6	123.8
192	23.2	18.1	27.1

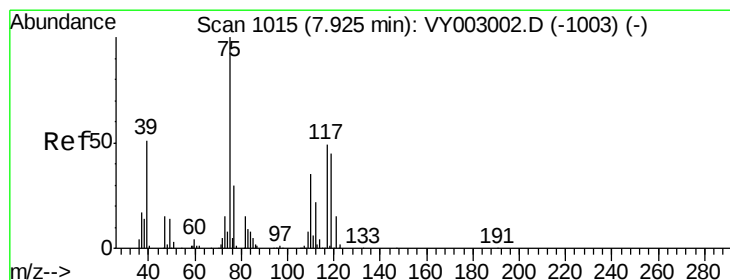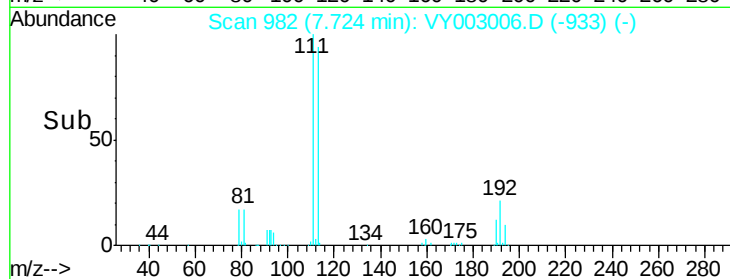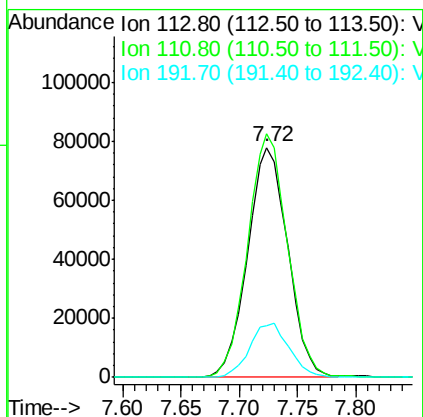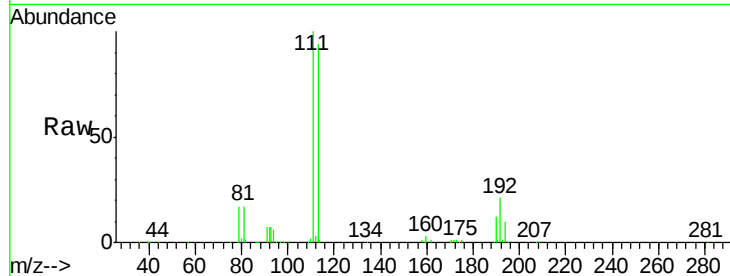

#36
 1,1-Dichloropropene
 Concen: 4.496 ug/l
 RT: 7.79 min Scan# 993
 Delta R.T. -0.13 min
 Lab File: VY003006.D
 Acq: 29 Jun 2020 14:52

Tgt Ion	Ratio	Lower	Upper
75	100		
110	9.7	17.1	51.2#
77	0.3	24.9	37.3#

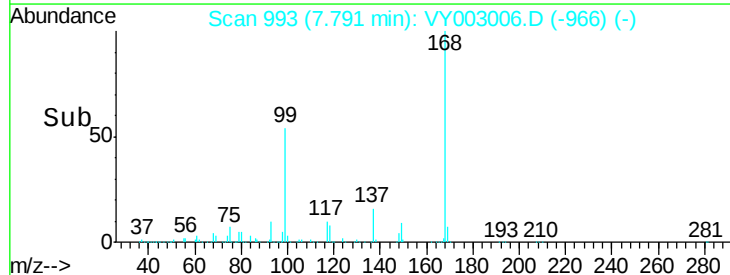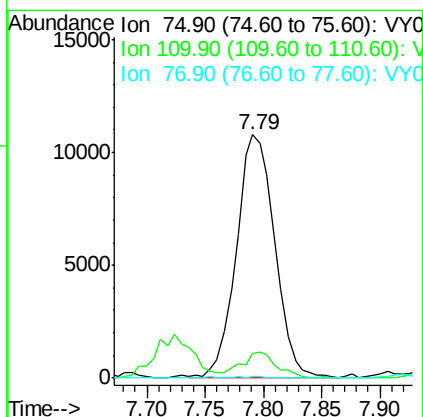



#38

Carbon Tetrachloride

Concen: 5.639 ug/l

RT: 7.80 min Scan# 994

Delta R.T. -0.11 min

Lab File: VY003006.D

Acq: 29 Jun 2020 14:52

Instrument :

MSVOA_Y

ClientSampleId :

VY0629SBL01


Tot Ion:117 Resp: 32338

Ion Ratio Lower Upper

117 100

119 5.1 75.7 113.5#




121 0.0 23.9 35.9#



Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

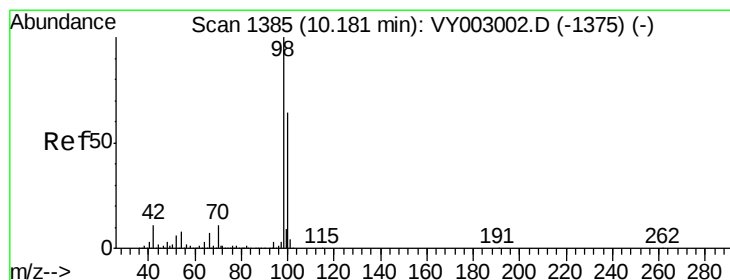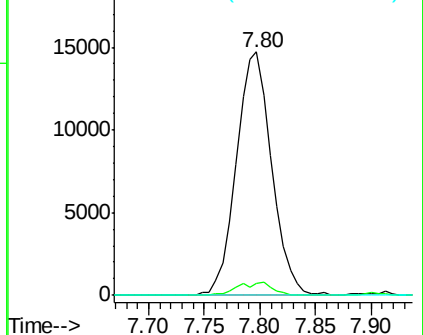

#50

Toluene-d8

Concen: 52.659 ug/l

RT: 10.18 min Scan# 1385

Delta R.T. -0.00 min

Lab File: VY003006.D


Acq: 29 Jun 2020 14:52

Tgt Ion: 98 Resp: 700226

Ion Ratio Lower Upper



98 100


100 63.7 51.1 76.7



Abundance Ion 98.00 (97.70 to 98.70): VY0

Ion 100.00 (99.70 to 100.70): VY

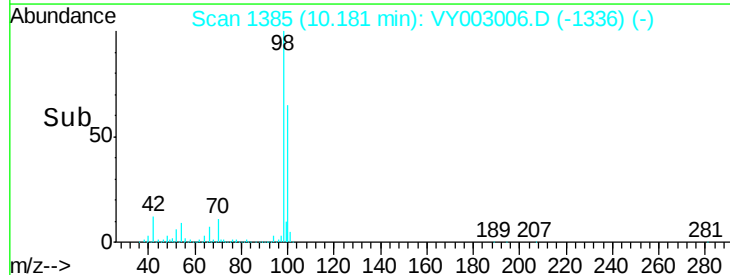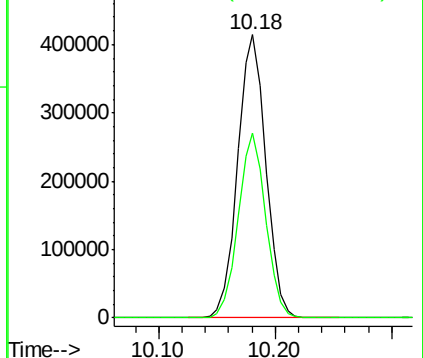



#52

Toluene

Concen: 1.228 ug/l

RT: 10.25 min Scan# 1396

Delta R.T. 0.01 min

Lab File: VY003006.D

Acq: 29 Jun 2020 14:52

Instrument :

MSVOA_Y

ClientSampleId :





VY0629SBL01

Tot Ion: 92 Resp: 11667

Ion Ratio Lower Upper

92 100

91 177.4 139.6 209.4

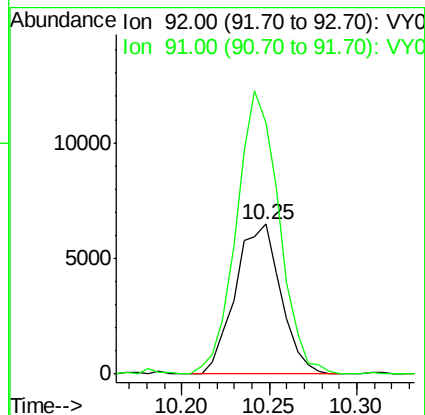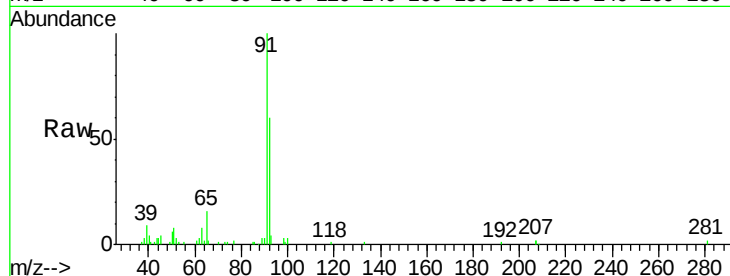

#62

4-Bromofluorobenzene

Concen: 54.050 ug/l

RT: 12.48 min Scan# 1762

Delta R.T. -0.00 min

Lab File: VY003006.D

Acq: 29 Jun 2020 14:52




Tgt Ion: 95 Resp: 252989


Ion Ratio Lower Upper

95 100

174 92.7 0.0 184.8

176 89.6 0.0 183.0



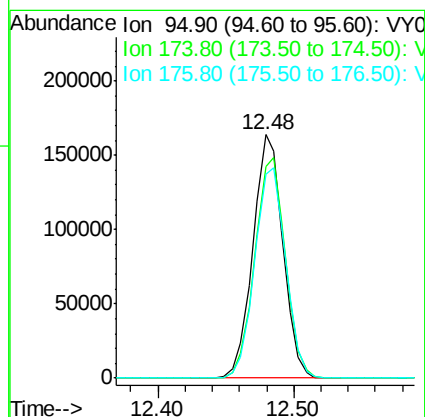





#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.49 min Scan# 1600
Delta R.T. -0.00 min
Lab File: VY003006.D
Acq: 29 Jun 2020 14:52




Instrument :
MSVOA_Y
ClientSampleId :
VY0629SBL01


Tot Ion:117 Resp: 546194
Ion Ratio Lower Upper
117 100
82 55.5 43.0 64.6
119 32.6 25.8 38.8

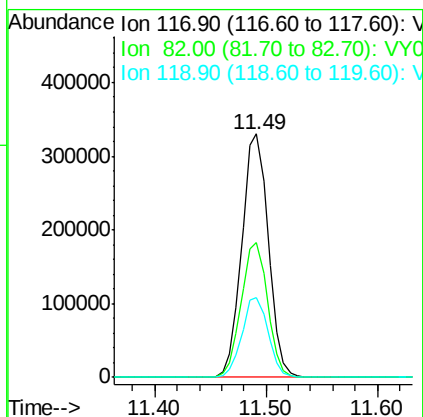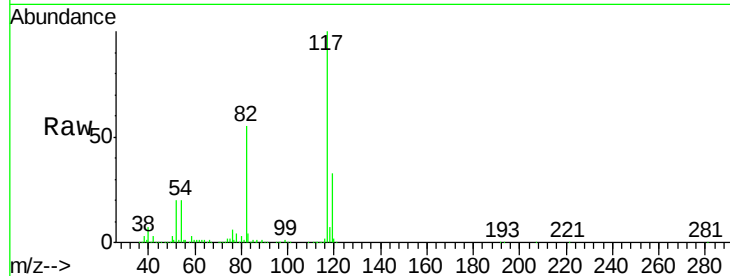

#68
m/p-Xylenes
Concen: 2.148 ug/l
RT: 11.70 min Scan# 1634
Delta R.T. -0.00 min
Lab File: VY003006.D
Acq: 29 Jun 2020 14:52

Tgt Ion:106 Resp: 15753
Ion Ratio Lower Upper
106 100
91 204.1 161.9 242.9

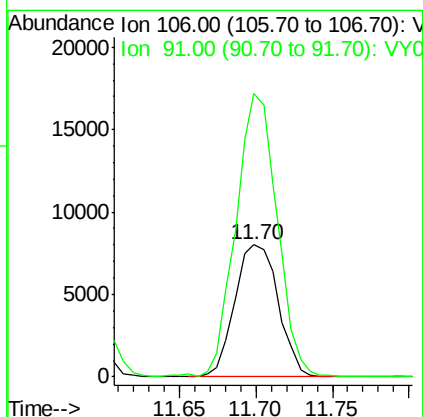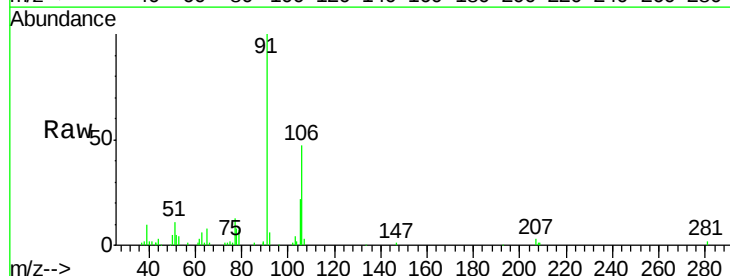




#72


1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.42 min Scan# 1917
Delta R.T. -0.00 min
Lab File: VY003006.D
Acq: 29 Jun 2020 14:52

Instrument :
MSVOA_Y
ClientSampleId :
VY0629SBL01



Tot Ion	Ratio	Lower	Upper
152	100		
115	54.8	27.3	81.9
150	155.5	0.0	343.4



Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

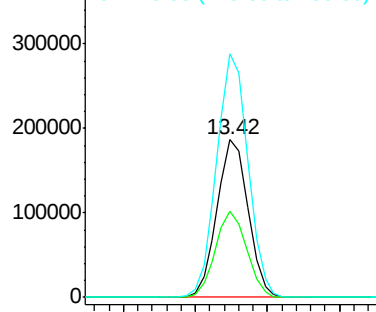


Time-->




#76

1,2,3-Trichloropropane
Concen: 48.937 ug/l
RT: 12.48 min Scan# 1762
Delta R.T. -0.15 min
Lab File: VY003006.D
Acq: 29 Jun 2020 14:52


Tgt Ion	Ratio	Lower	Upper
75	100		
77	1.3	0.0	0.0#




Abundance Ion 74.90 (74.60 to 75.60): VY0
Ion 77.00 (76.70 to 77.70): VY0

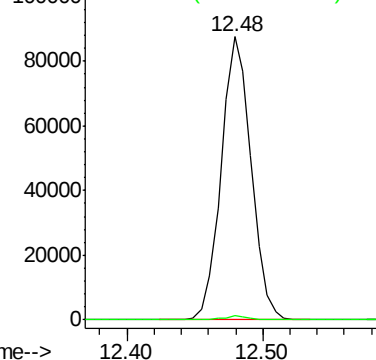

Time-->







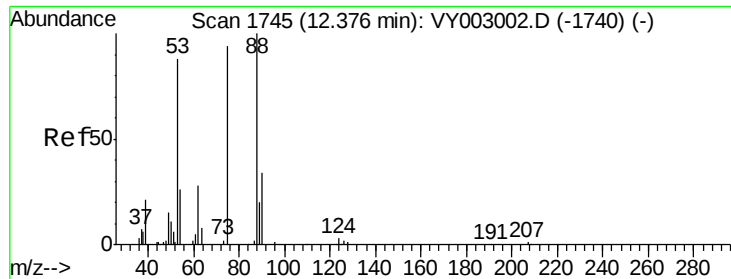

#81
trans-1,4-Dichloro-2-butene
Concen: 95.211 ug/l
RT: 12.48 min Scan# 1762
Delta R.T. 0.10 min
Lab File: VY003006.D
Acq: 29 Jun 2020 14:52




Instrument :
MSVOA_Y
ClientSampleId :
VY0629SBL01


Tot Ion: 75 Resp: 135042
Ion Ratio Lower Upper
75 100
53 0.0 73.9 110.9#
89 1.1 37.5 56.3#

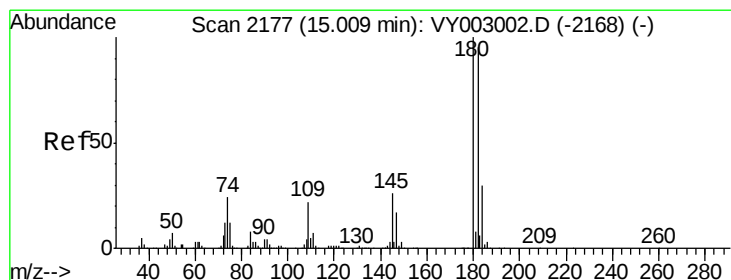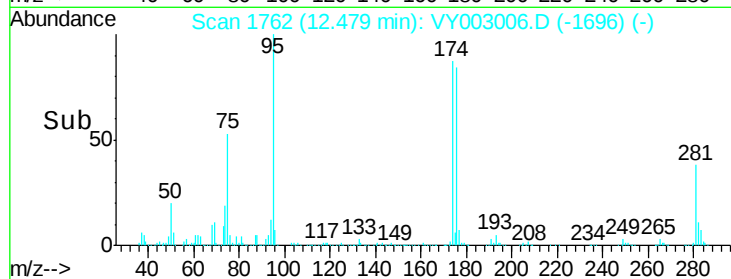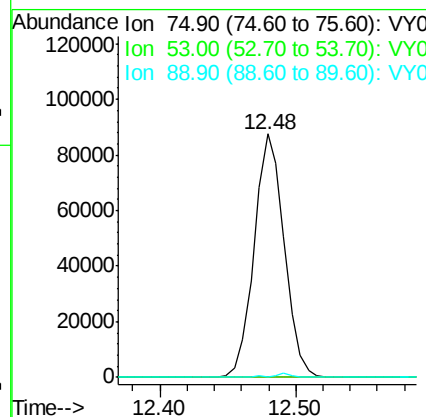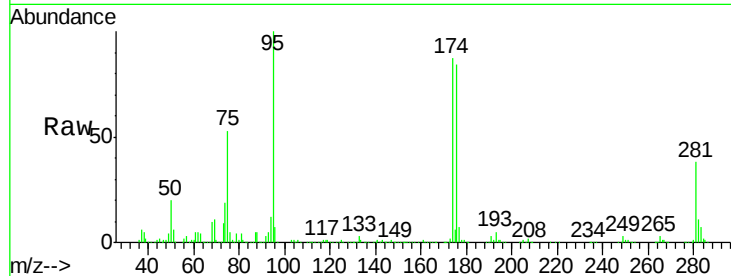

#93
1,2,4-Trichlorobenzene
Concen: 1.725 ug/l
RT: 15.01 min Scan# 2177
Delta R.T. -0.00 min
Lab File: VY003006.D
Acq: 29 Jun 2020 14:52

Tgt Ion:180 Resp: 10047
Ion Ratio Lower Upper
180 100
182 90.9 48.1 144.3
145 29.7 13.9 41.6

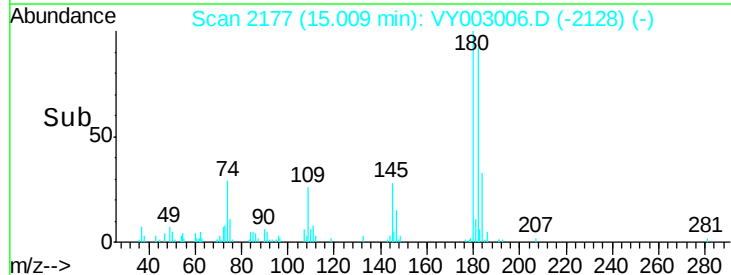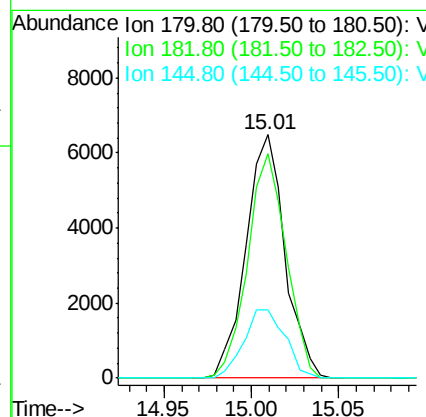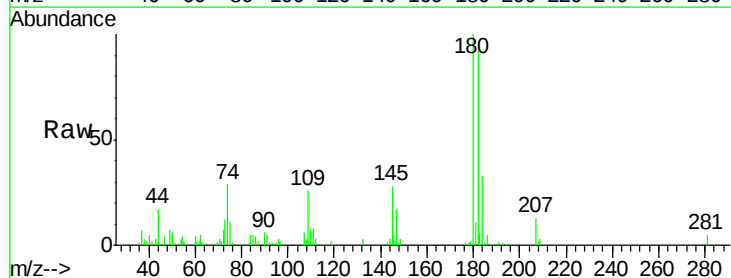


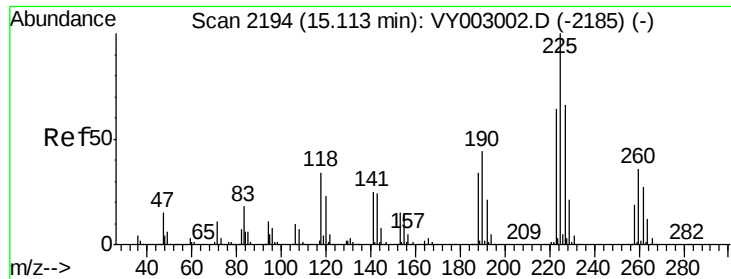




#94
Hexachlorobutadiene
Concen: 1.055 ug/l
RT: 15.11 min Scan# 2194
Delta R.T. -0.00 min
Lab File: VY003006.D
Acq: 29 Jun 2020 14:52

Instrument :
MSVOA_Y
ClientSampleId :
VY0629SBL01

Tot Ion:225 Resp: 3876
Ion Ratio Lower Upper
225 100
223 69.3 32.4 97.0
227 62.7 32.4 97.2

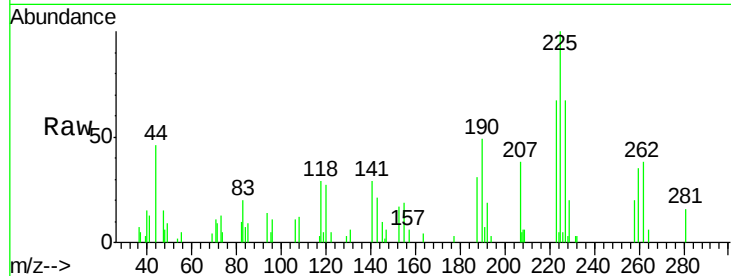


Abundance Ion 224.70 (224.40 to 225.40): V
Ion 222.70 (222.40 to 223.40): V
Ion 226.70 (226.40 to 227.40): V

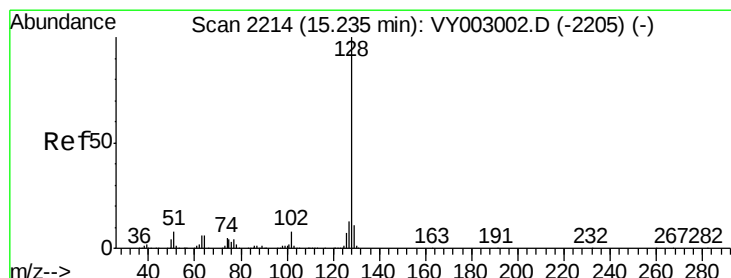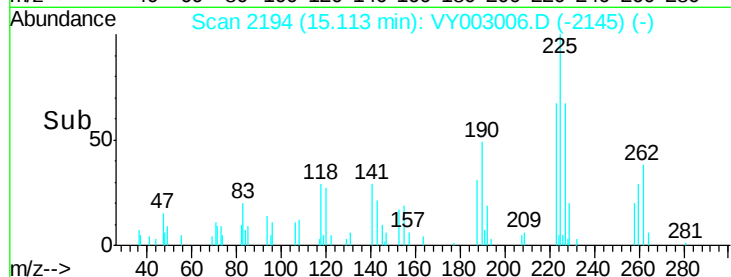
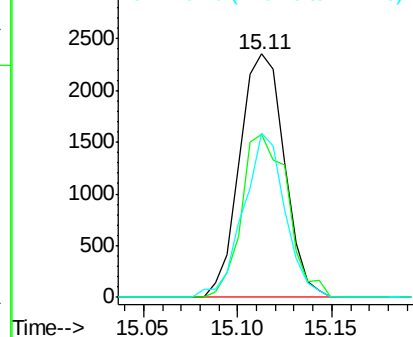



#95
Naphthalene
Concen: 2.204 ug/l
RT: 15.24 min Scan# 2215
Delta R.T. 0.01 min
Lab File: VY003006.D
Acq: 29 Jun 2020 14:52

Tgt Ion:128 Resp: 23444
Ion Ratio Lower Upper
128 100
127 15.5 10.8 16.2
129 12.3 8.8 13.2

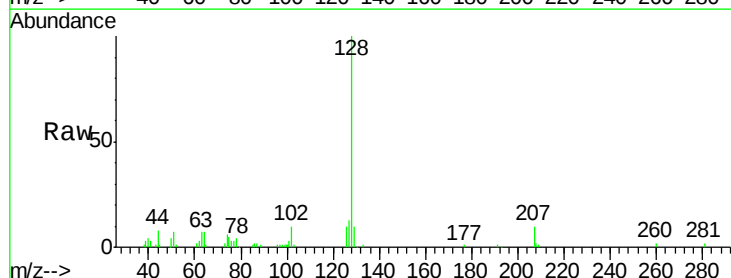

Abundance Ion 128.00 (127.70 to 128.70): V
Ion 127.00 (126.70 to 127.70): V
Ion 129.00 (128.70 to 129.70): V

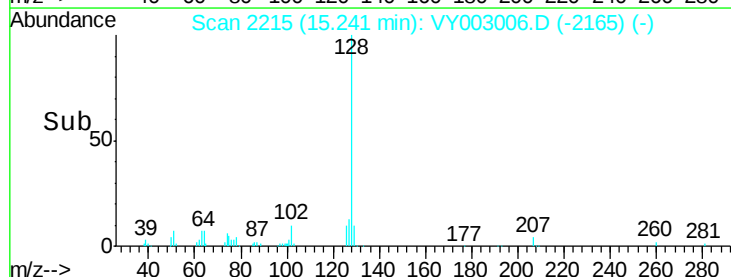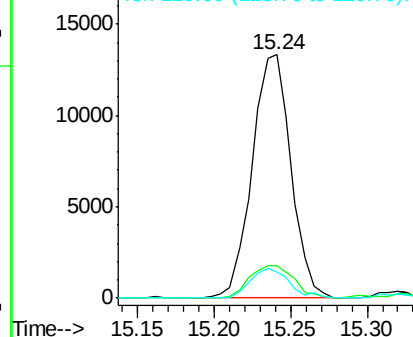


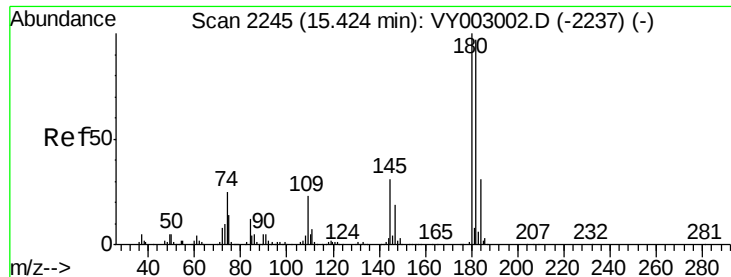

#96
 1,2,3-Trichlorobenzene
 Concen: 1.909 ug/l
 RT: 15.42 min Scan# 2245
 Delta R.T. -0.00 min
 Lab File: VY003006.D
 Acq: 29 Jun 2020 14:52

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0629SBL01

Tot Ion	Ratio	Lower	Upper
180	100		
182	91.9	47.8	143.3
145	29.0	14.7	44.1

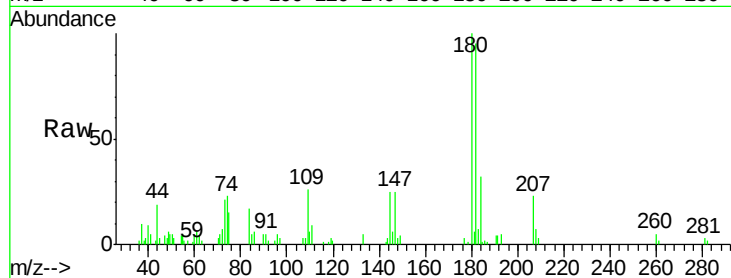

Abundance Ion 179.80 (179.50 to 180.50): V
 Ion 181.80 (181.50 to 182.50): V
 Ion 144.90 (144.60 to 145.60): V

