
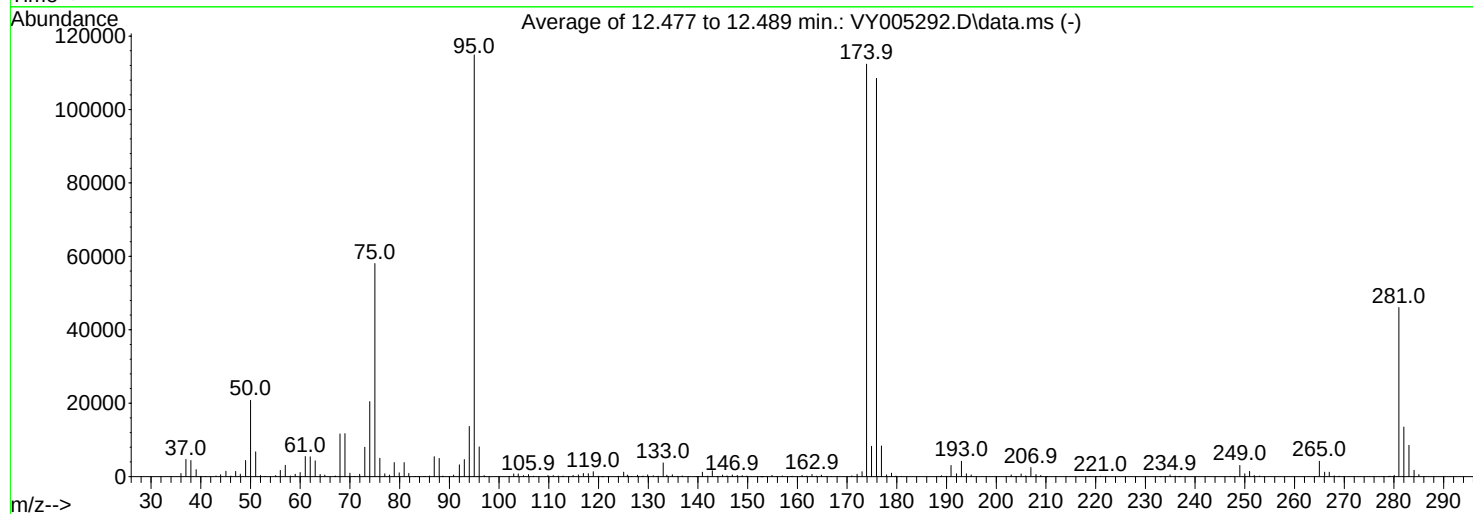


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY063021\
Data File : VY005292.D
Acq On : 30 Jun 2021 09:46
Operator : SY/MD
Sample : BFB
Misc : 5.00G/5ML/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y062221S.M
Title : SW846 8260
Last Update : Wed Jun 23 07:57:52 2021

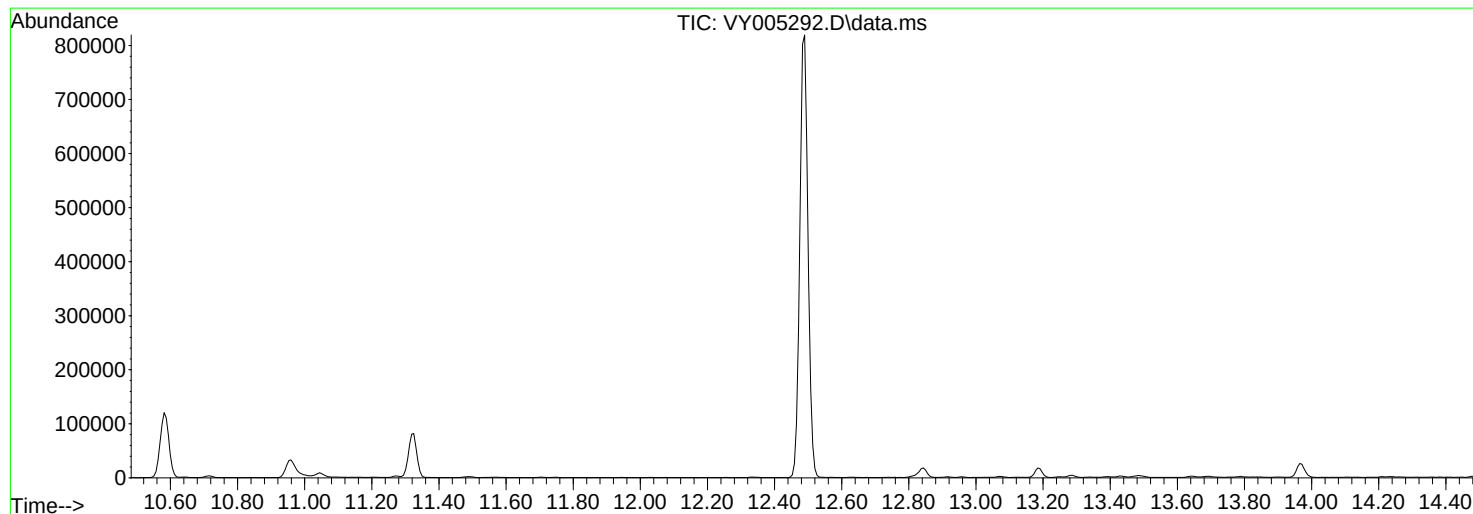

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.1	20795	PASS
75	95	30	60	50.5	58077	PASS
95	95	100	100	100.0	114896	PASS
96	95	5	9	7.1	8115	PASS
173	174	0.00	2	1.2	1345	PASS
174	95	50	100	97.8	112352	PASS
175	174	5	9	7.4	8305	PASS
176	174	95	101	96.5	108467	PASS
177	176	5	9	7.7	8355	PASS