

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY070121\
 Data File : VY005313.D
 Acq On : 01 Jul 2021 14:52
 Operator : SY/MD
 Sample : M2896-05
 Misc : 9.26G/5ML/MSVOA_Y/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 FS-03

Quant Time: Jul 02 05:15:40 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y062221S.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 23 07:57:52 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.795	168	204048	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.697	114	336219	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.496	117	338392	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	172497	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.149	65	115501	68.210	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 136.420%	
35) Dibromofluoromethane	7.728	113	103143	52.017	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 104.040%	
50) Toluene-d8	10.185	98	416154	52.481	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	= 104.960%	
62) 4-Bromofluorobenzene	12.483	95	162590	61.532	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	= 123.060%	


Target Compounds				Qvalue		
11) Tert butyl alcohol	4.966	59	370	Below Cal	#	77
16) Acetone	3.960	43	137220	350.788	ug/l	96
17) Carbon Disulfide	4.204	76	6897	1.298	ug/l	97
20) Methylene Chloride	4.728	84	8169	Below Cal		94
25) 2-Butanone	7.002	43	8048	14.110	ug/l #	83
31) Cyclohexane	7.795	56	4239	1.402	ug/l #	1
36) 1,1-Dichloropropene	7.795	75	13593	4.591	ug/l #	47
37) Ethyl Acetate	7.002	43	8048	5.271	ug/l #	65
38) Carbon Tetrachloride	7.795	117	17143	5.531	ug/l #	17
43) Isopropyl Acetate	8.551	43	18978	6.763	ug/l #	49
48) Methyl methacrylate	9.356	41	4984	4.048	ug/l #	89
51) 4-Methyl-2-Pentanone	9.965	43	3793	2.582	ug/l #	32
59) 2-Hexanone	10.801	43	3306	3.273	ug/l #	22
67) Ethyl Benzene	11.593	91	25440	2.200	ug/l	95
68) m/p-Xylenes	11.703	106	27071	5.842	ug/l	98
69) o-Xylene	12.032	106	16540	3.770	ug/l	93
73) Isopropylbenzene	12.331	105	20386	1.822	ug/l	100
74) N-amyl acetate	12.123	43	4194	1.584	ug/l #	50
75) 1,1,2,2-Tetrachloroethane	12.568	83	2711	1.230	ug/l #	26
76) 1,2,3-Trichloropropane	12.483	75	78515	51.322	ug/l #	100
78) n-propylbenzene	12.672	91	115547	8.758	ug/l	99
79) 2-Chlorotoluene	12.770	91	8953	1.203	ug/l #	40
80) 1,3,5-Trimethylbenzene	12.812	105	71892	7.768	ug/l	99
81) trans-1,4-Dichloro-2-b...	12.483	75	78515	95.755	ug/l #	24
83) tert-Butylbenzene	13.123	119	26923	3.263	ug/l #	71
84) 1,2,4-Trimethylbenzene	13.123	105	203295	22.217	ug/l	99
85) sec-Butylbenzene	13.251	105	22245	1.853	ug/l #	61
86) p-Isopropyltoluene	13.318	119	43237	4.174	ug/l	92
89) n-Butylbenzene	13.696	91	196855	21.636	ug/l #	76
90) Hexachloroethane	13.971	117	20545	10.981	ug/l #	1
92) 1,2-Dibromo-3-Chloropr...	14.385	75	6593	17.954	ug/l #	1
95) Naphthalene	15.239	128	145595	22.275	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY070121\
Data File : VY005313.D
Acq On : 01 Jul 2021 14:52
Operator : SY/MD
Sample : M2896-05
Misc : 9.26G/5ML/MSVOA_Y/SOIL
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
FS-03

Quant Time: Jul 02 05:15:40 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y062221S.M
Quant Title : SW846 8260
QLast Update : Wed Jun 23 07:57:52 2021
Response via : Initial Calibration




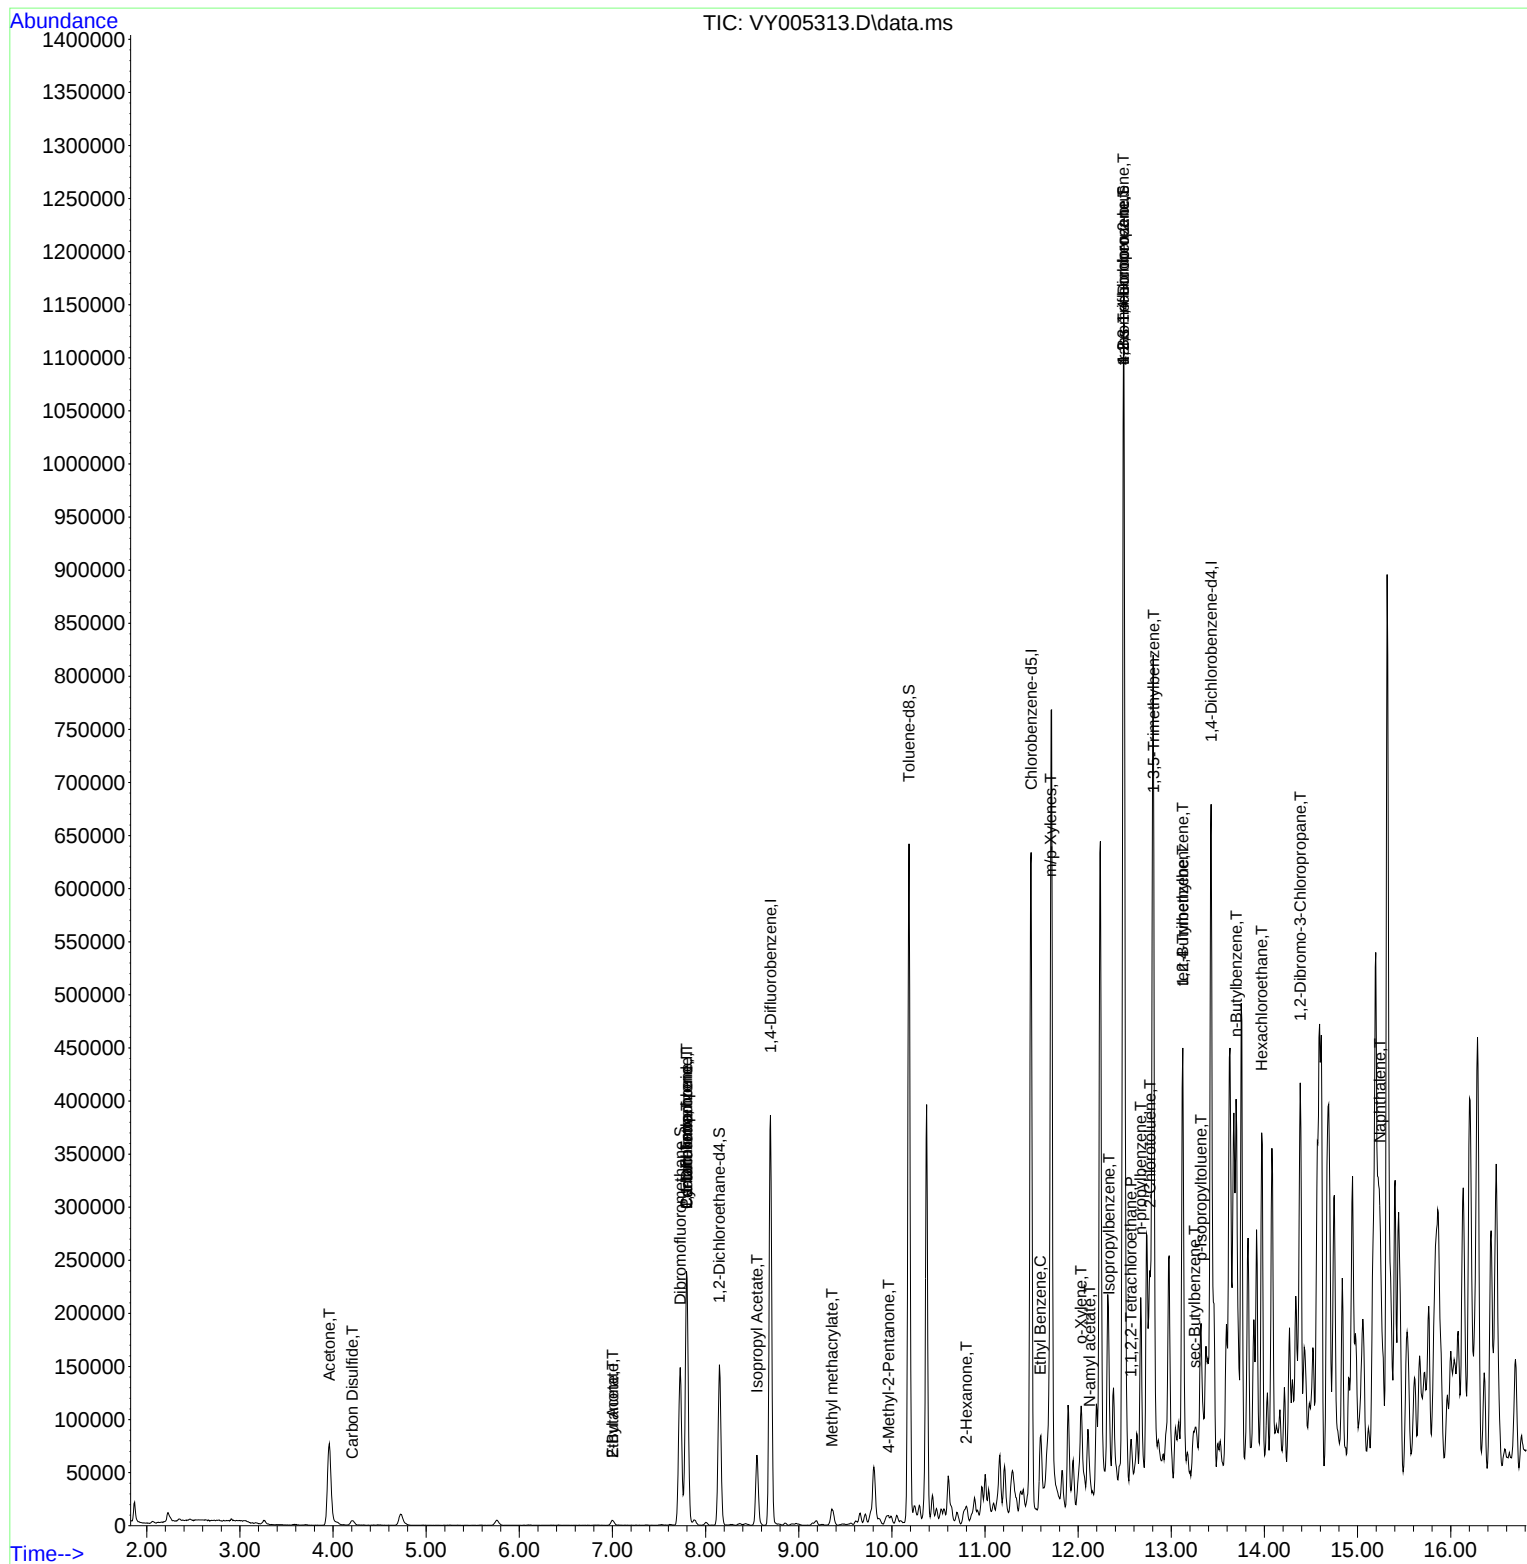


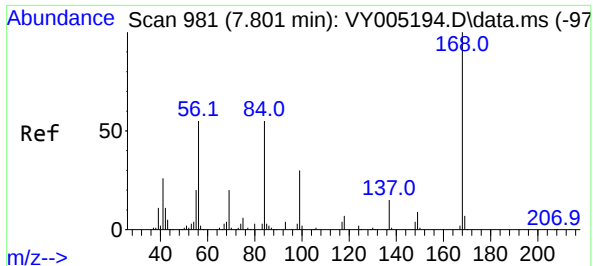

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.795 min Scan# 980
Delta R.T. -0.006 min
Lab File: VY005313.D
Acq: 01 Jul 2021 14:52




Instrument :
MSVOA_Y
ClientSampleId :
FS-03


Tgt Ion:168 Resp: 204048
Ion Ratio Lower Upper
168 100
99 47.6 36.2 54.4

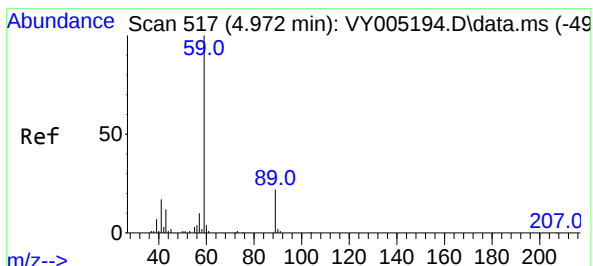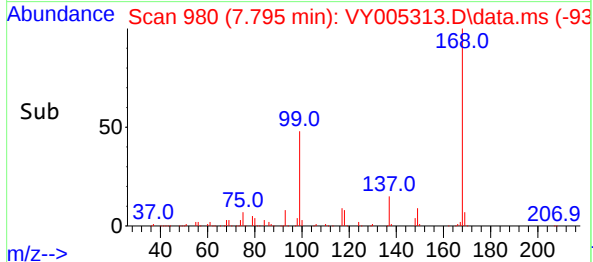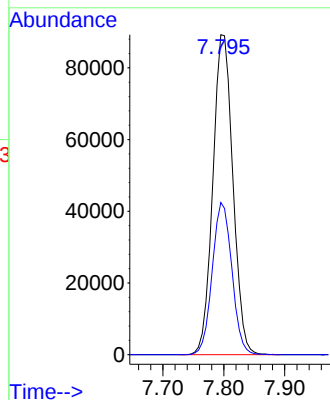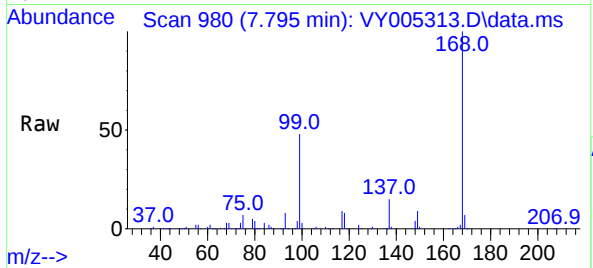

#11
Tert butyl alcohol
Concen: Below Cal
RT: 4.966 min Scan# 516
Delta R.T. -0.006 min
Lab File: VY005313.D
Acq: 01 Jul 2021 14:52

Tgt Ion: 59 Resp: 370
Ion Ratio Lower Upper
59 100
57 0.0 6.5 9.7#


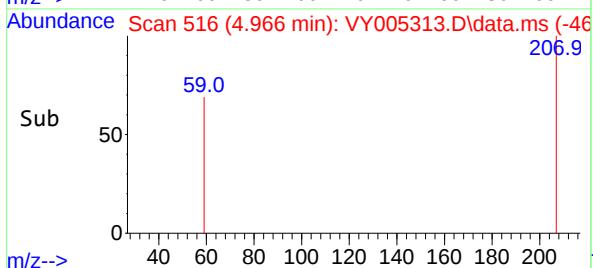
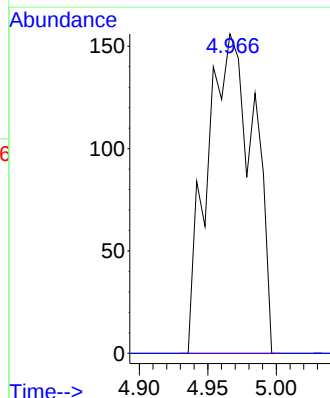
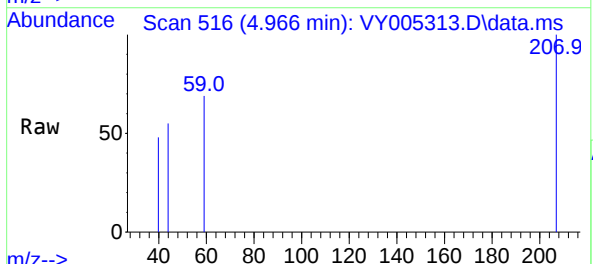




#16
Acetone
Concen: 350.788 ug/l
RT: 3.960 min Scan# 351
Delta R.T. -0.000 min
Lab File: VY005313.D
Acq: 01 Jul 2021 14:52




Instrument :
MSVOA_Y
ClientSampleId :
FS-03


Tgt Ion: 43 Resp: 137220
Ion Ratio Lower Upper
43 100
58 32.7 28.2 42.2



#17
Carbon Disulfide
Concen: 1.298 ug/l
RT: 4.204 min Scan# 391
Delta R.T. -0.000 min
Lab File: VY005313.D
Acq: 01 Jul 2021 14:52

Tgt Ion: 76 Resp: 6897
Ion Ratio Lower Upper
76 100
78 8.0 7.3 10.9

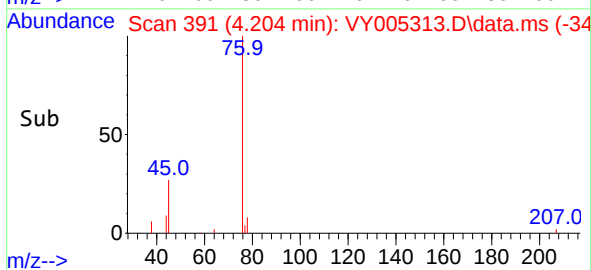




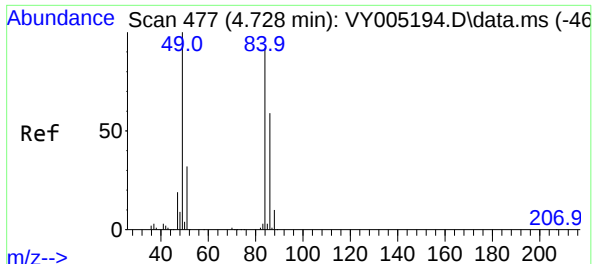


#20
Methylene Chloride
Concen: Below Cal
RT: 4.728 min Scan# 477
Delta R.T. 0.000 min
Lab File: VY005313.D
Acq: 01 Jul 2021 14:52

Instrument :
MSVOA_Y
ClientSampleId :
FS-03

Tgt Ion: 84 Resp: 8169




Ion	Ratio	Lower	Upper
84	100		
49	115.6	86.9	130.3
51	36.4	27.4	41.2
86	58.1	51.0	76.6

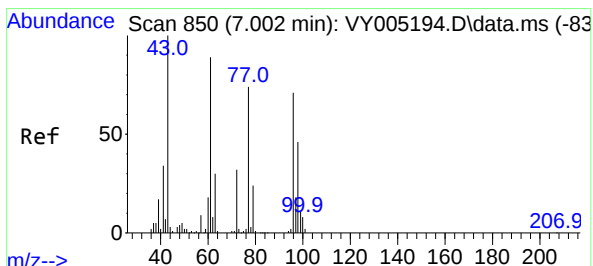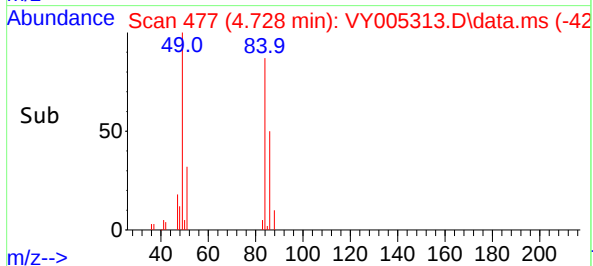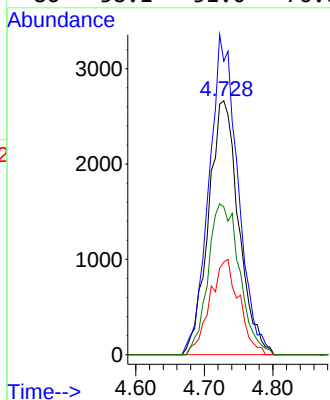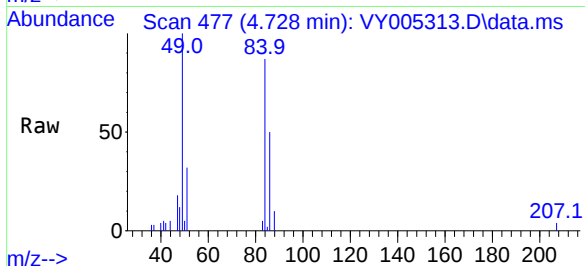


#25
2-Butanone
Concen: 14.110 ug/l
RT: 7.002 min Scan# 850
Delta R.T. -0.000 min
Lab File: VY005313.D
Acq: 01 Jul 2021 14:52

Tgt Ion: 43 Resp: 8048

Ion	Ratio	Lower	Upper
43	100		
72	22.2	25.3	37.9#


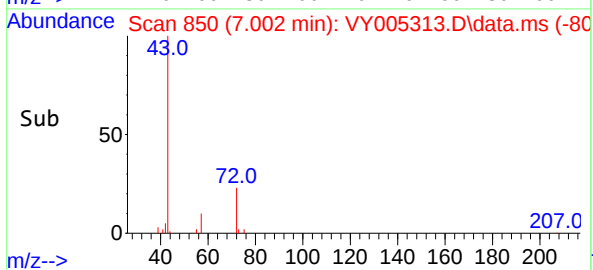
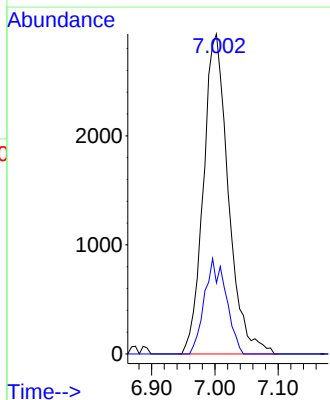
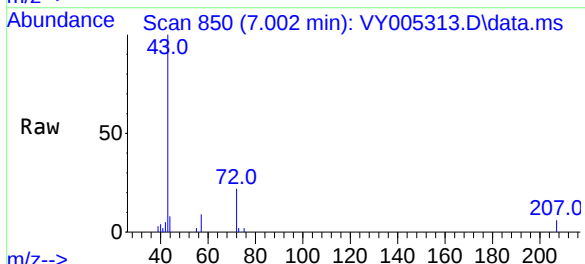




#31
Cyclohexane
Concen: 1.402 ug/l
RT: 7.795 min Scan# 980
Delta R.T. -0.000 min
Lab File: VY005313.D
Acq: 01 Jul 2021 14:52




Instrument :
MSVOA_Y
ClientSampleId :
FS-03


Tgt Ion: 56 Resp: 4239
Ion Ratio Lower Upper
56 100
69 179.0 29.6 44.4#
84 148.2 76.4 114.6#



#33
1,2-Dichloroethane-d4
Concen: 68.210 ug/l
RT: 8.149 min Scan# 1038
Delta R.T. -0.000 min
Lab File: VY005313.D
Acq: 01 Jul 2021 14:52

Tgt Ion: 65 Resp: 115501
Ion Ratio Lower Upper
65 100
67 53.4 0.0 110.6


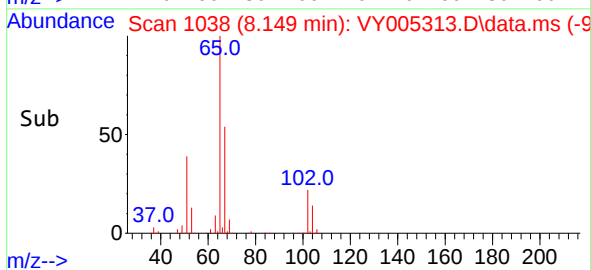






#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.697 min Scan# 1128
Delta R.T. -0.000 min
Lab File: VY005313.D
Acq: 01 Jul 2021 14:52




Instrument :
MSVOA_Y
ClientSampled :
FS-03


Tgt Ion:114 Resp: 336219
Ion Ratio Lower Upper
114 100
63 18.7 0.0 35.2
88 14.7 0.0 29.4



#35
Dibromofluoromethane
Concen: 52.017 ug/l
RT: 7.728 min Scan# 969
Delta R.T. -0.000 min
Lab File: VY005313.D
Acq: 01 Jul 2021 14:52

Tgt Ion:113 Resp: 103143
Ion Ratio Lower Upper
113 100
111 102.5 82.6 124.0
192 24.7 20.2 30.2


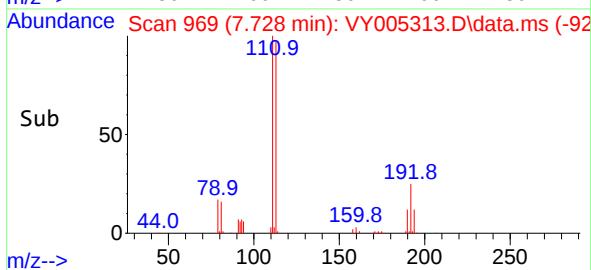




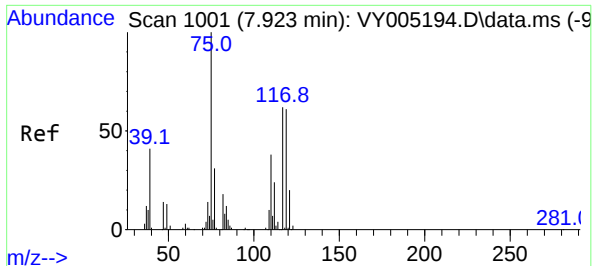

#36
1,1-Dichloropropene
Concen: 4.591 ug/l
RT: 7.795 min Scan# 980
Delta R.T. -0.128 min
Lab File: VY005313.D
Acq: 01 Jul 2021 14:52




Instrument :
MSVOA_Y
ClientSampleId :
FS-03


Tgt Ion: 75 Resp: 13593
Ion Ratio Lower Upper
75 100
110 8.3 19.1 57.5#
77 0.0 25.2 37.8#

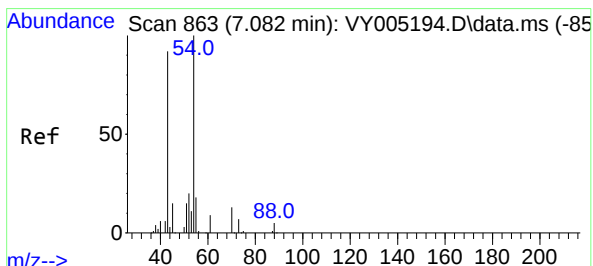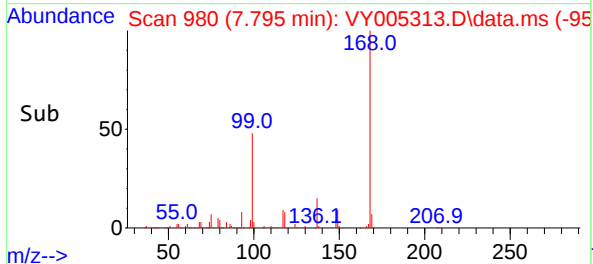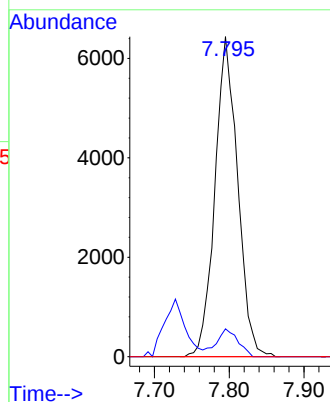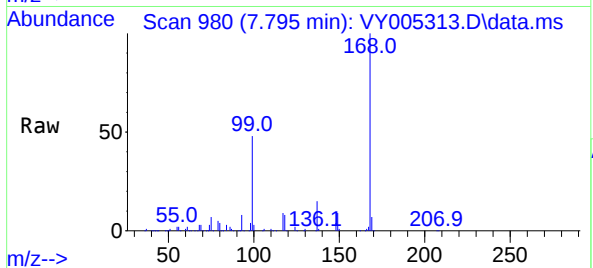

#37
Ethyl Acetate
Concen: 5.271 ug/l
RT: 7.002 min Scan# 850
Delta R.T. -0.079 min
Lab File: VY005313.D
Acq: 01 Jul 2021 14:52

Tgt Ion: 43 Resp: 8048
Ion Ratio Lower Upper
43 100
61 0.0 12.8 19.2#
70 0.0 9.7 14.5#


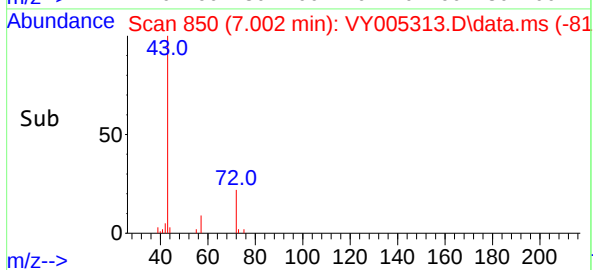
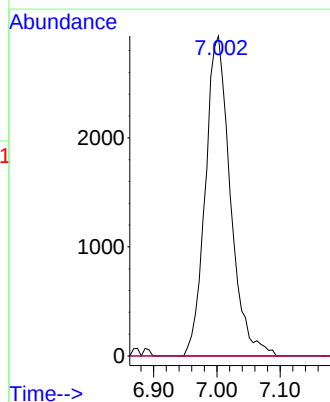
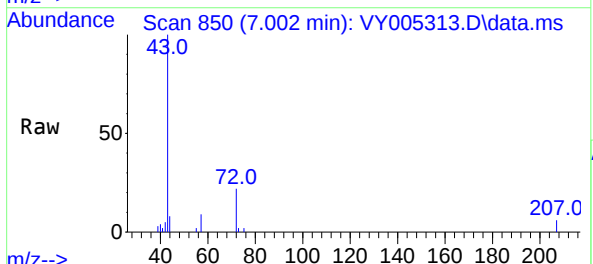




#38
Carbon Tetrachloride
Concen: 5.531 ug/l
RT: 7.795 min Scan# 980
Delta R.T. -0.116 min
Lab File: VY005313.D
Acq: 01 Jul 2021 14:52




Instrument :
MSVOA_Y
ClientSampleId :
FS-03


Tgt Ion:117 Resp: 17143
Ion Ratio Lower Upper
117 100
119 5.6 76.2 114.4#
121 0.0 24.7 37.1#

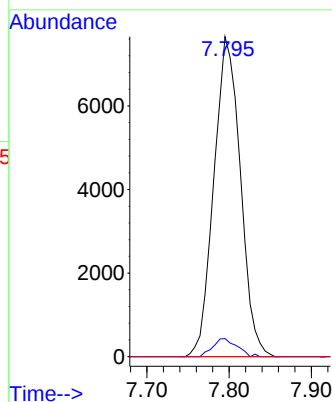

#43
Isopropyl Acetate
Concen: 6.763 ug/l
RT: 8.551 min Scan# 1104
Delta R.T. 0.268 min
Lab File: VY005313.D
Acq: 01 Jul 2021 14:52

Tgt Ion: 43 Resp: 18978
Ion Ratio Lower Upper
43 100
61 0.0 25.5 38.3#
87 0.0 12.9 19.3#









#48
Methyl methacrylate
Concen: 4.048 ug/l
RT: 9.356 min Scan# 1236
Delta R.T. 0.055 min
Lab File: VY005313.D
Acq: 01 Jul 2021 14:52




Instrument :
MSVOA_Y
ClientSampled :
FS-03


Tgt Ion: 41 Resp: 4984
Ion Ratio Lower Upper
41 100
69 96.7 83.3 124.9
39 39.6 42.3 63.5#

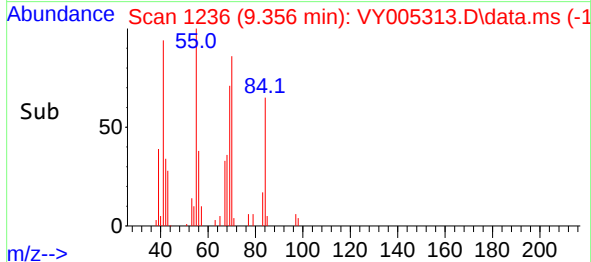

#50
Toluene-d8
Concen: 52.481 ug/l
RT: 10.185 min Scan# 1372
Delta R.T. -0.000 min
Lab File: VY005313.D
Acq: 01 Jul 2021 14:52

Tgt Ion: 98 Resp: 416154
Ion Ratio Lower Upper
98 100
100 64.3 51.9 77.9


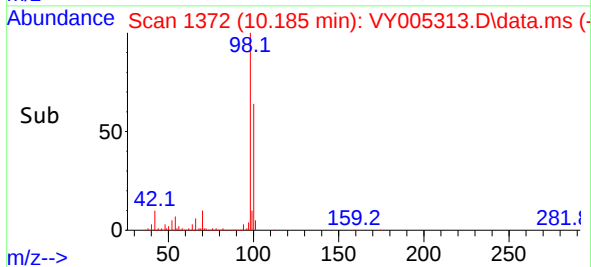

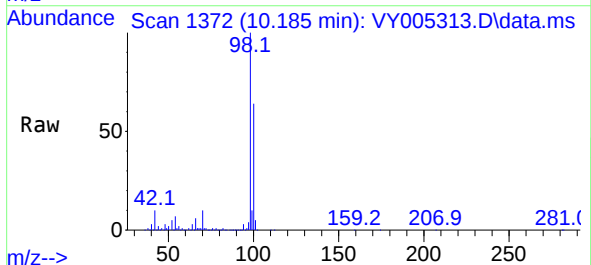




#51
4-Methyl-2-Pentanone
Concen: 2.582 ug/l
RT: 9.965 min Scan# 1336
Delta R.T. -0.110 min
Lab File: VY005313.D
Acq: 01 Jul 2021 14:52




Instrument :
MSVOA_Y
ClientSampled :
FS-03


Tgt Ion: 43 Resp: 3793
Ion Ratio Lower Upper
43 100
58 0.0 35.3 52.9#

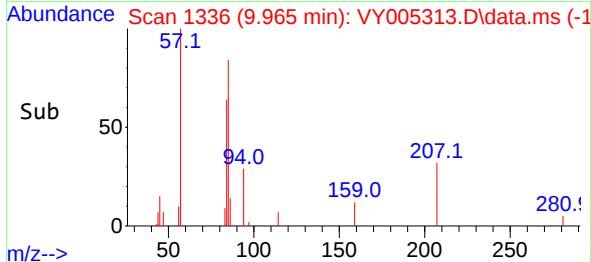

#59
2-Hexanone
Concen: 3.273 ug/l
RT: 10.801 min Scan# 1473
Delta R.T. -0.037 min
Lab File: VY005313.D
Acq: 01 Jul 2021 14:52

Tgt Ion: 43 Resp: 3306
Ion Ratio Lower Upper
43 100
58 1.5 30.8 92.4#


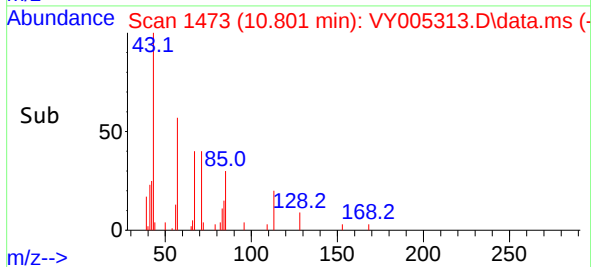

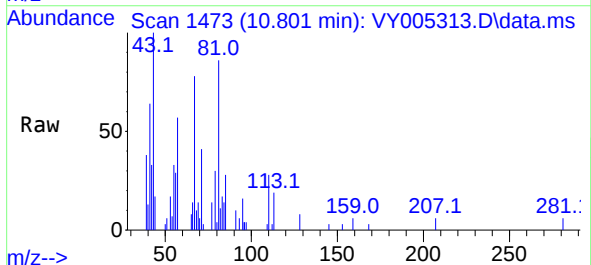




#62
4-Bromofluorobenzene
Concen: 61.532 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. -0.000 min
Lab File: VY005313.D
Acq: 01 Jul 2021 14:52




Instrument :
MSVOA_Y
ClientSampleId :
FS-03


Tgt Ion: 95 Resp: 162590
Ion Ratio Lower Upper
95 100
174 91.0 0.0 201.6
176 89.0 0.0 197.4

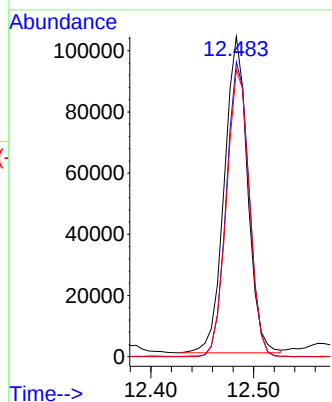

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.496 min Scan# 1587
Delta R.T. -0.000 min
Lab File: VY005313.D
Acq: 01 Jul 2021 14:52

Tgt Ion: 117 Resp: 338392
Ion Ratio Lower Upper
117 100
82 51.8 40.6 60.8
119 32.4 26.1 39.1


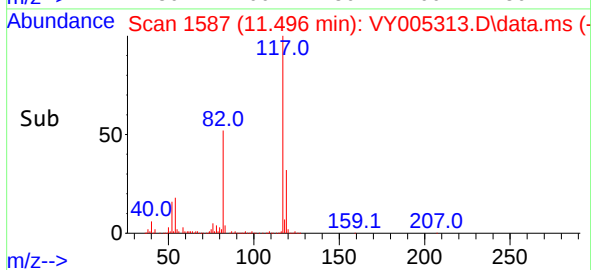






#67
Ethyl Benzene
Concen: 2.200 ug/l
RT: 11.593 min Scan# 1603
Delta R.T. -0.000 min
Lab File: VY005313.D
Acq: 01 Jul 2021 14:52




Instrument :
MSVOA_Y
ClientSampleId :
FS-03


Tgt Ion: 91 Resp: 25440
Ion Ratio Lower Upper
91 100
106 29.3 25.8 38.6

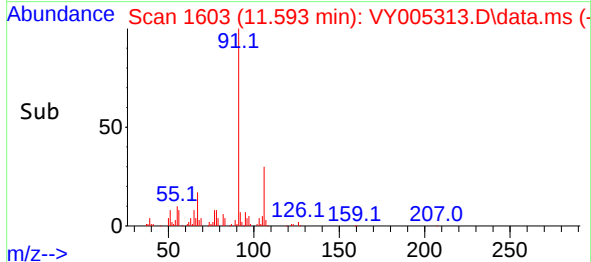

#68
m/p-Xylenes
Concen: 5.842 ug/l
RT: 11.703 min Scan# 1621
Delta R.T. -0.000 min
Lab File: VY005313.D
Acq: 01 Jul 2021 14:52

Tgt Ion:106 Resp: 27071
Ion Ratio Lower Upper
106 100
91 196.9 154.8 232.2


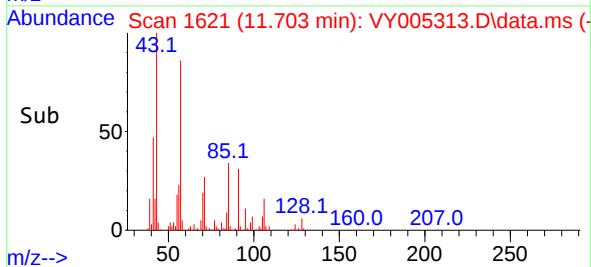

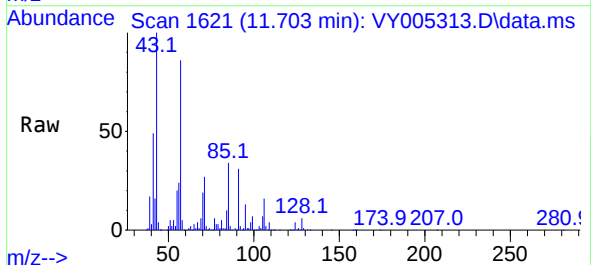




#69
o-Xylene
Concen: 3.770 ug/l
RT: 12.032 min Scan# 1675
Delta R.T. -0.000 min
Lab File: VY005313.D
Acq: 01 Jul 2021 14:52




Instrument :
MSVOA_Y
ClientSampleId :
FS-03


Tgt Ion:106 Resp: 16540
Ion Ratio Lower Upper
106 100
91 213.9 101.6 304.8



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. -0.000 min
Lab File: VY005313.D
Acq: 01 Jul 2021 14:52

Tgt Ion:152 Resp: 172497
Ion Ratio Lower Upper
152 100
115 51.0 26.3 78.8
150 149.9 0.0 344.2


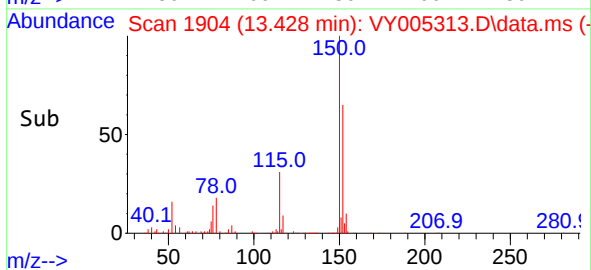






#73
Isopropylbenzene
Concen: 1.822 ug/l
RT: 12.331 min Scan# 1724
Delta R.T. -0.000 min
Lab File: VY005313.D
Acq: 01 Jul 2021 14:52




Instrument :
MSVOA_Y
ClientSampleId :
FS-03


Tgt Ion:105 Resp: 20386
Ion Ratio Lower Upper
105 100
120 28.2 14.0 42.0

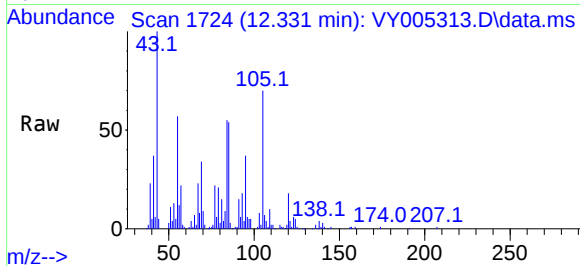

#74
N-ethyl acetate
Concen: 1.584 ug/l
RT: 12.123 min Scan# 1690
Delta R.T. -0.024 min
Lab File: VY005313.D
Acq: 01 Jul 2021 14:52

Tgt Ion: 43 Resp: 4194
Ion Ratio Lower Upper
43 100
70 42.8 40.6 61.0
55 88.4 21.5 32.3#
61 0.0 22.6 33.8#


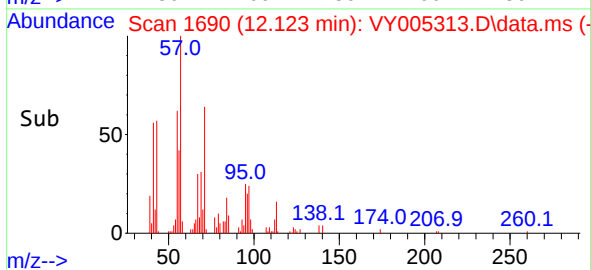

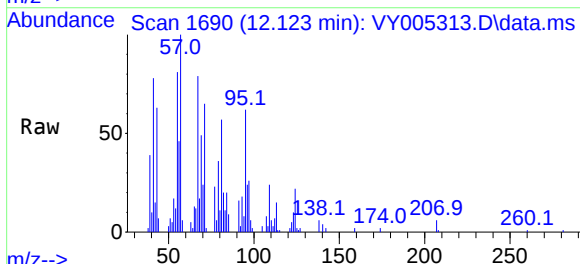




#75
1,1,2,2-Tetrachloroethane
Concen: 1.230 ug/l
RT: 12.568 min Scan# 1763
Delta R.T. -0.018 min
Lab File: VY005313.D
Acq: 01 Jul 2021 14:52




Instrument :
MSVOA_Y
ClientSampled :
FS-03


Tgt Ion: 83 Resp: 2711
Ion Ratio Lower Upper
83 100
131 0.0 5.9 17.6#
85 0.0 32.5 97.5#

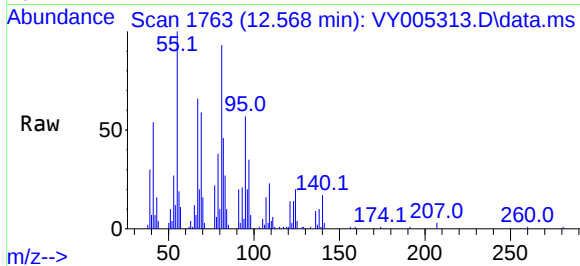

#76
1,2,3-Trichloropropane
Concen: 51.322 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. -0.152 min
Lab File: VY005313.D
Acq: 01 Jul 2021 14:52

Tgt Ion: 75 Resp: 78515
Ion Ratio Lower Upper
75 100
77 5.6 0.0 0.0#


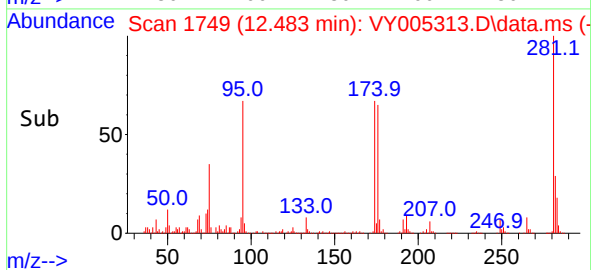

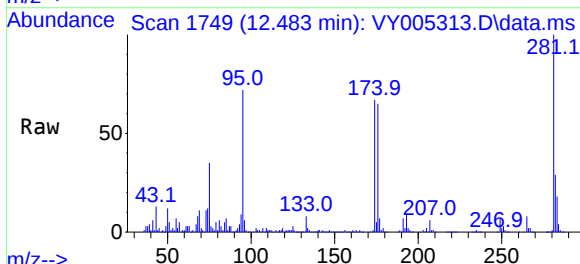




#78
n-propylbenzene
Concen: 8.758 ug/l
RT: 12.672 min Scan# 1780
Delta R.T. -0.000 min
Lab File: VY005313.D
Acq: 01 Jul 2021 14:52




Instrument :
MSVOA_Y
ClientSampleId :
FS-03


Tgt Ion: 91 Resp: 115547
Ion Ratio Lower Upper
91 100
120 24.3 12.4 37.0

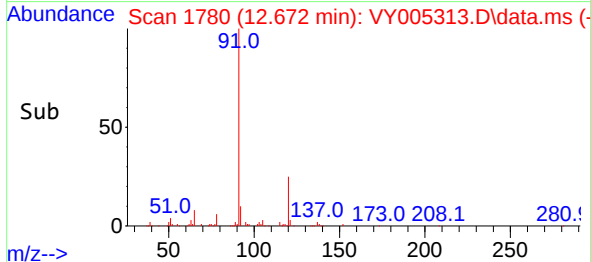

#79
2-Chlorotoluene
Concen: 1.203 ug/l
RT: 12.770 min Scan# 1796
Delta R.T. 0.012 min
Lab File: VY005313.D
Acq: 01 Jul 2021 14:52

Tgt Ion: 91 Resp: 8953
Ion Ratio Lower Upper
91 100
126 1.4 18.6 55.6#


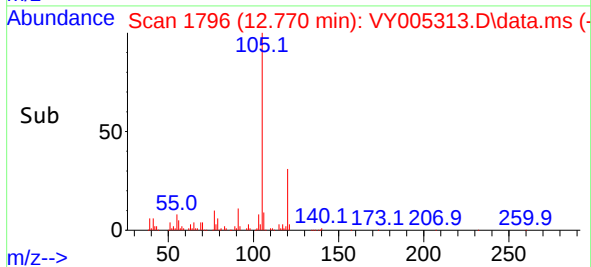

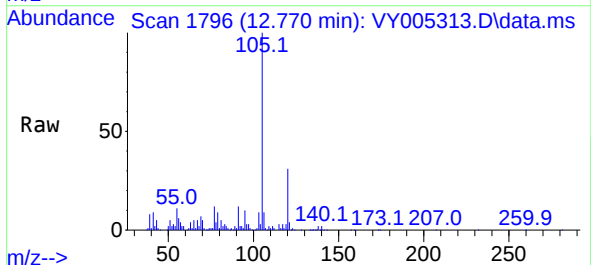




#80
1,3,5-Trimethylbenzene
Concen: 7.768 ug/l
RT: 12.812 min Scan# 1803
Delta R.T. -0.000 min
Lab File: VY005313.D
Acq: 01 Jul 2021 14:52




Instrument :
MSVOA_Y
ClientSampled :
FS-03


Tgt Ion:105 Resp: 71892
Ion Ratio Lower Upper
105 100
120 52.3 25.9 77.7

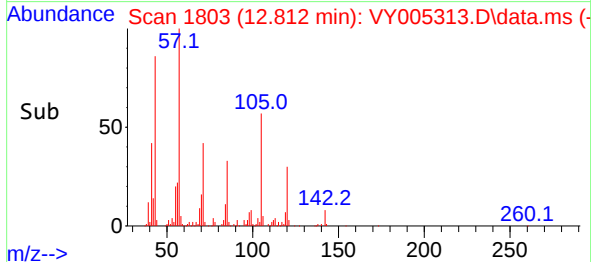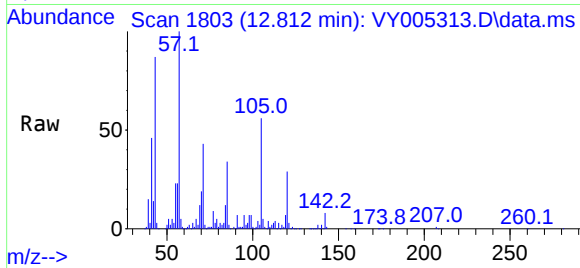

#81
trans-1,4-Dichloro-2-butene
Concen: 95.755 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.104 min
Lab File: VY005313.D
Acq: 01 Jul 2021 14:52

Tgt Ion: 75 Resp: 78515
Ion Ratio Lower Upper
75 100
53 8.3 63.0 94.4#
89 2.2 38.0 57.0#


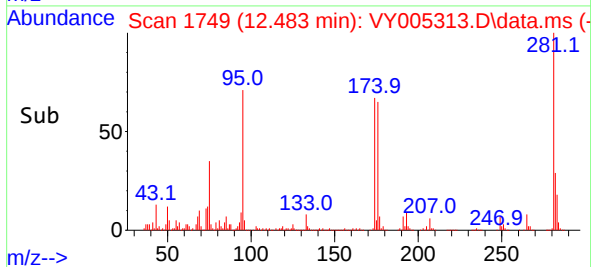

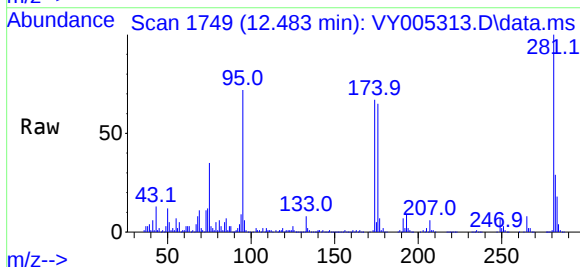




#83
tert-Butylbenzene
Concen: 3.263 ug/l
RT: 13.123 min Scan# 1854
Delta R.T. 0.043 min
Lab File: VY005313.D
Acq: 01 Jul 2021 14:52




Instrument :
MSVOA_Y
ClientSampleId :
FS-03


Tgt Ion:119 Resp: 26923
Ion Ratio Lower Upper
119 100
91 73.2 29.5 88.5
134 0.0 13.5 40.5#

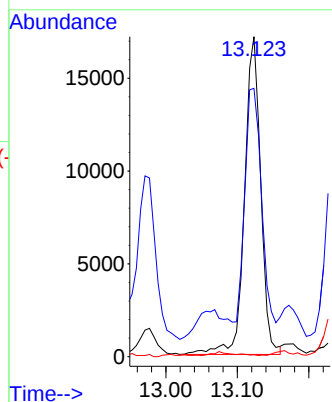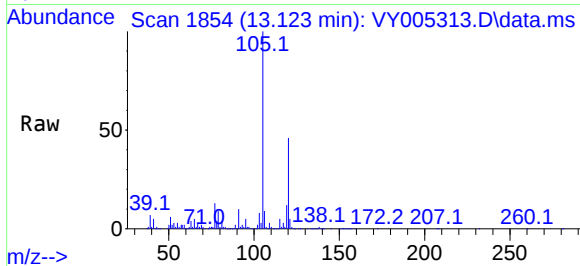

#84
1,2,4-Trimethylbenzene
Concen: 22.217 ug/l
RT: 13.123 min Scan# 1854
Delta R.T. -0.000 min
Lab File: VY005313.D
Acq: 01 Jul 2021 14:52

Tgt Ion:105 Resp: 203295
Ion Ratio Lower Upper
105 100
120 46.8 23.6 71.0


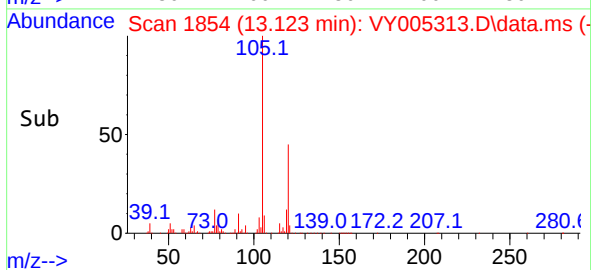

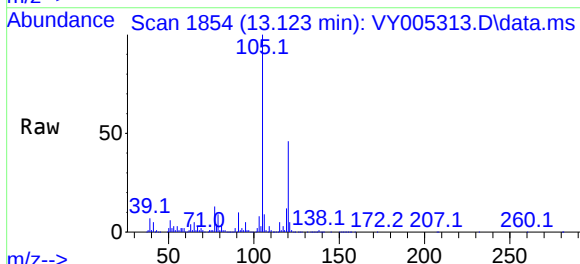




#85
 sec-Butylbenzene
 Concen: 1.853 ug/l
 RT: 13.251 min Scan# 1875
 Delta R.T. -0.006 min
 Lab File: VY005313.D
 Acq: 01 Jul 2021 14:52




Instrument :
 MSVOA_Y
 ClientSampleId :
 FS-03


Tgt Ion:105 Resp: 22245
 Ion Ratio Lower Upper
 105 100
 134 40.0 10.9 32.6#

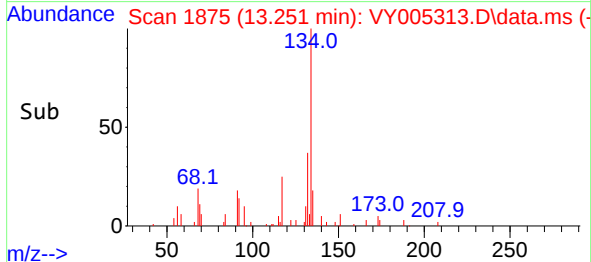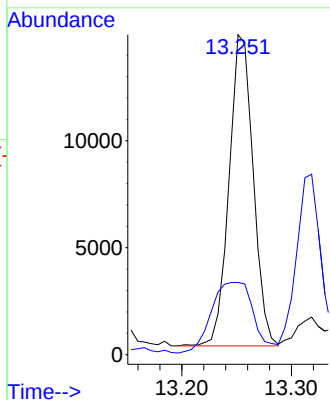

#86
 p-Isopropyltoluene
 Concen: 4.174 ug/l
 RT: 13.318 min Scan# 1886
 Delta R.T. -0.055 min
 Lab File: VY005313.D
 Acq: 01 Jul 2021 14:52

Tgt Ion:119 Resp: 43237
 Ion Ratio Lower Upper
 119 100
 134 29.3 13.9 41.6
 91 28.1 10.8 32.3


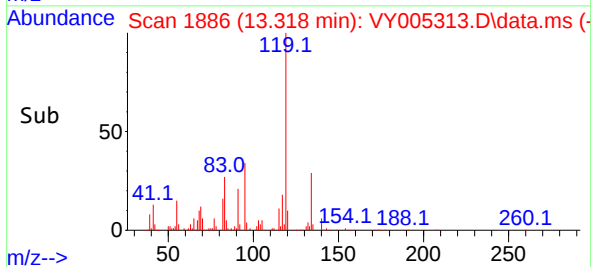
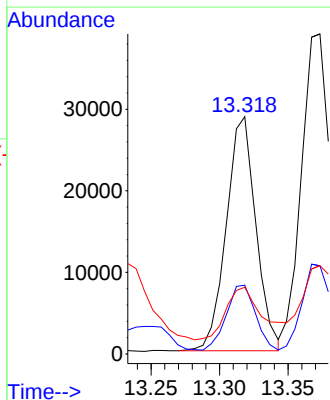
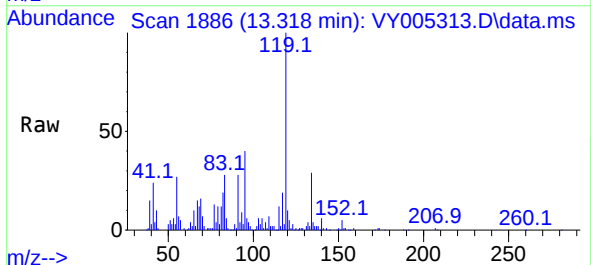




#89
n-Butylbenzene
Concen: 21.636 ug/l
RT: 13.696 min Scan# 1948
Delta R.T. -0.000 min
Lab File: VY005313.D
Acq: 01 Jul 2021 14:52




Instrument :
MSVOA_Y
ClientSampled :
FS-03


Tgt Ion: 91 Resp: 196855
Ion Ratio Lower Upper
91 100
92 48.6 27.0 81.0
134 0.0 14.6 44.0#

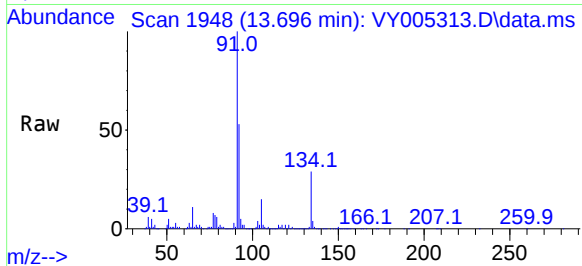

#90
Hexachloroethane
Concen: 10.981 ug/l
RT: 13.971 min Scan# 1993
Delta R.T. 0.006 min
Lab File: VY005313.D
Acq: 01 Jul 2021 14:52

Tgt Ion: 117 Resp: 20545
Ion Ratio Lower Upper
117 100
201 0.0 49.4 148.2#


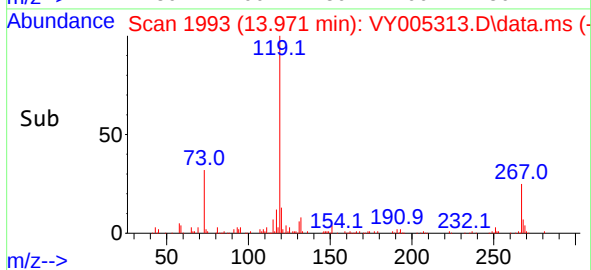

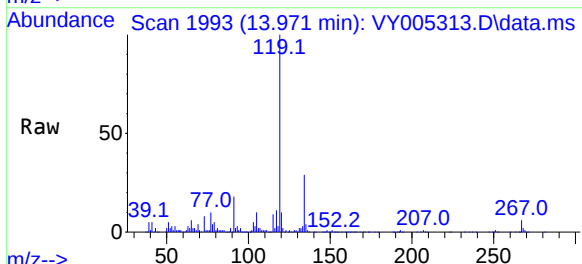




#92
1,2-Dibromo-3-Chloropropane
Concen: 17.954 ug/l
RT: 14.385 min Scan# 2061
Delta R.T. 0.024 min
Lab File: VY005313.D
Acq: 01 Jul 2021 14:52

Instrument :
MSVOA_Y
ClientSampleId :
FS-03

Tgt Ion: 75 Resp: 6593
Ion Ratio Lower Upper
75 100
155 0.0 52.4 157.3#
157 0.3 67.3 201.8#

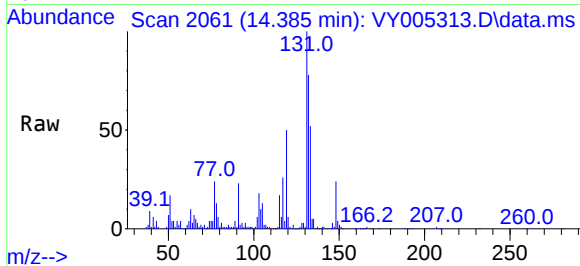

#95
Naphthalene
Concen: 22.275 ug/l
RT: 15.239 min Scan# 2201
Delta R.T. -0.000 min
Lab File: VY005313.D
Acq: 01 Jul 2021 14:52

Tgt Ion:128 Resp: 145595
Ion Ratio Lower Upper
128 100
127 13.3 10.2 15.4
129 12.4 8.7 13.1

