


Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY070220\
Data File : VY003074.D
Acq On : 02 Jul 2020 09:59
Operator : SY/MD
Sample : BFB
Misc : 5.00G/5ML/MSVOA Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y062920S.M
Title : SW846 8260
Last Update : Tue Jun 30 04:11:35 2020

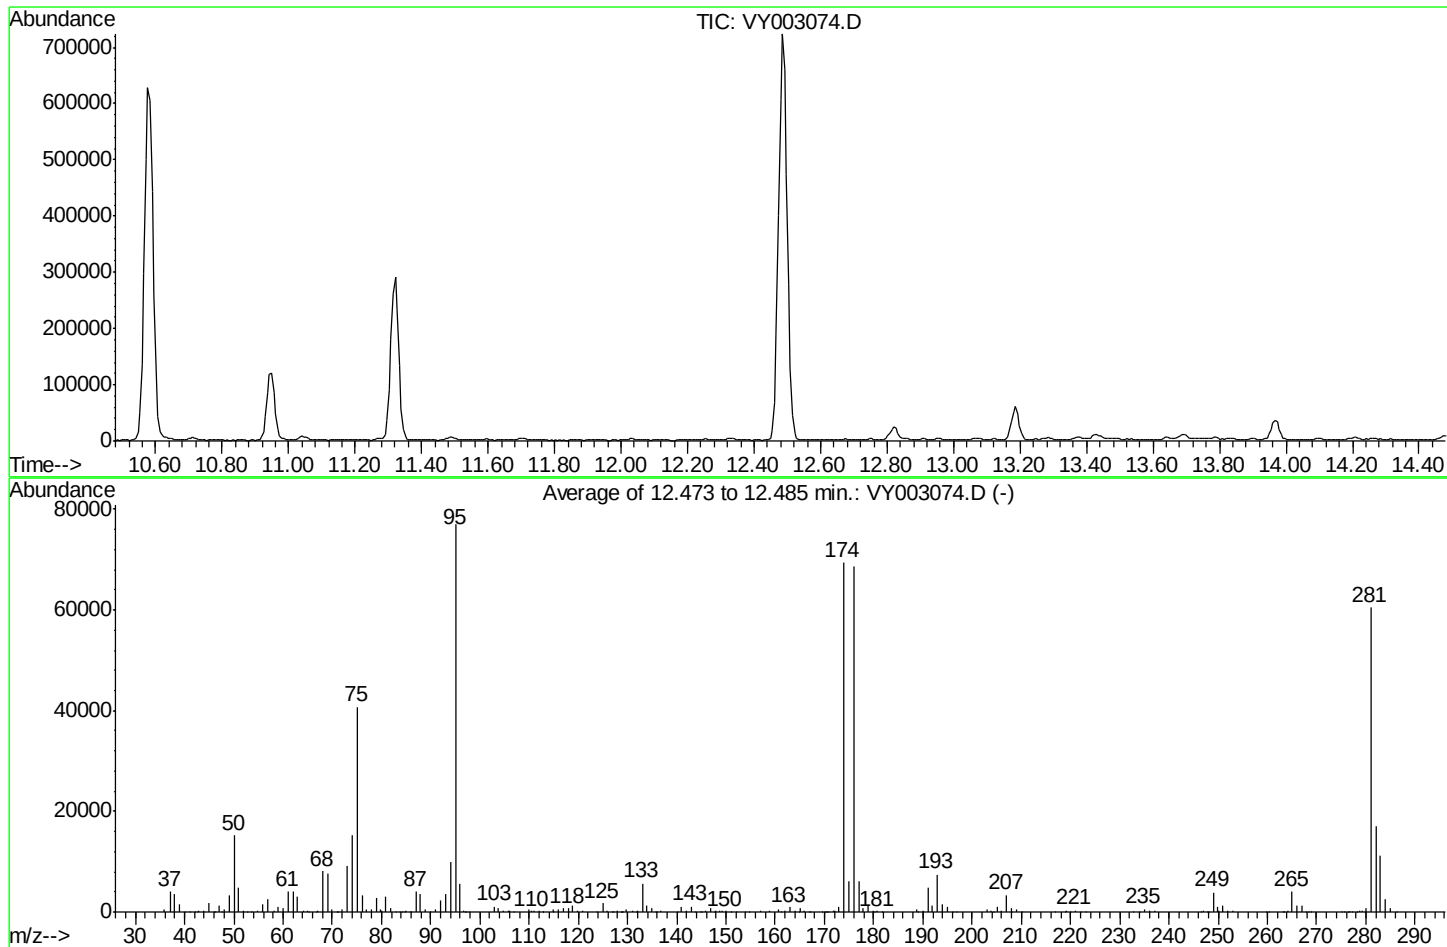

AutoFind: Scans 1761, 1762, 1763; Background Corrected with Scan 1754

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	15182	PASS
75	95	30	60	52.9	40704	PASS
95	95	100	100	100.0	77016	PASS
96	95	5	9	7.3	5598	PASS
173	174	0.00	2	1.3	925	PASS
174	95	50	100	90.1	69408	PASS
175	174	5	9	8.7	6066	PASS
176	174	95	101	99.1	68762	PASS
177	176	5	9	8.8	6035	PASS