
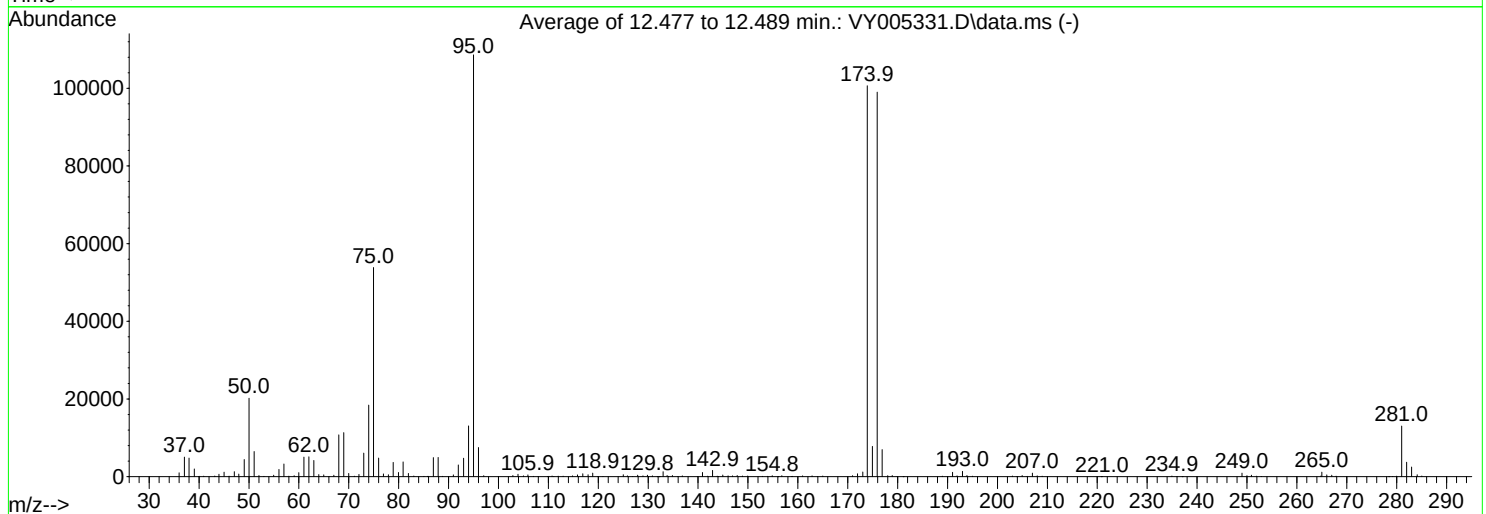


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY070221\
Data File : VY005331.D
Acq On : 02 Jul 2021 09:44
Operator : SY/MD
Sample : BFB
Misc : 5.00G/5ML/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y062221S.M
Title : SW846 8260
Last Update : Wed Jun 23 07:57:52 2021

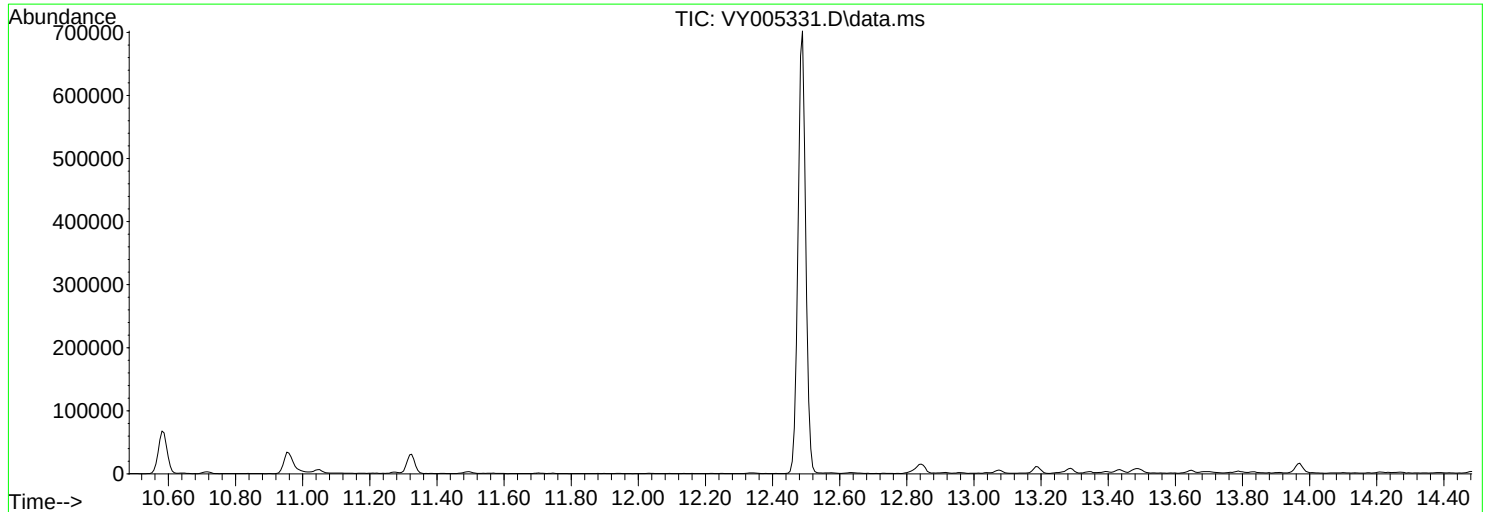

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.6	20192	PASS
75	95	30	60	49.6	53835	PASS
95	95	100	100	100.0	108613	PASS
96	95	5	9	6.9	7492	PASS
173	174	0.00	2	1.2	1208	PASS
174	95	50	100	92.7	100640	PASS
175	174	5	9	7.8	7801	PASS
176	174	95	101	98.4	99000	PASS
177	176	5	9	7.0	6946	PASS