
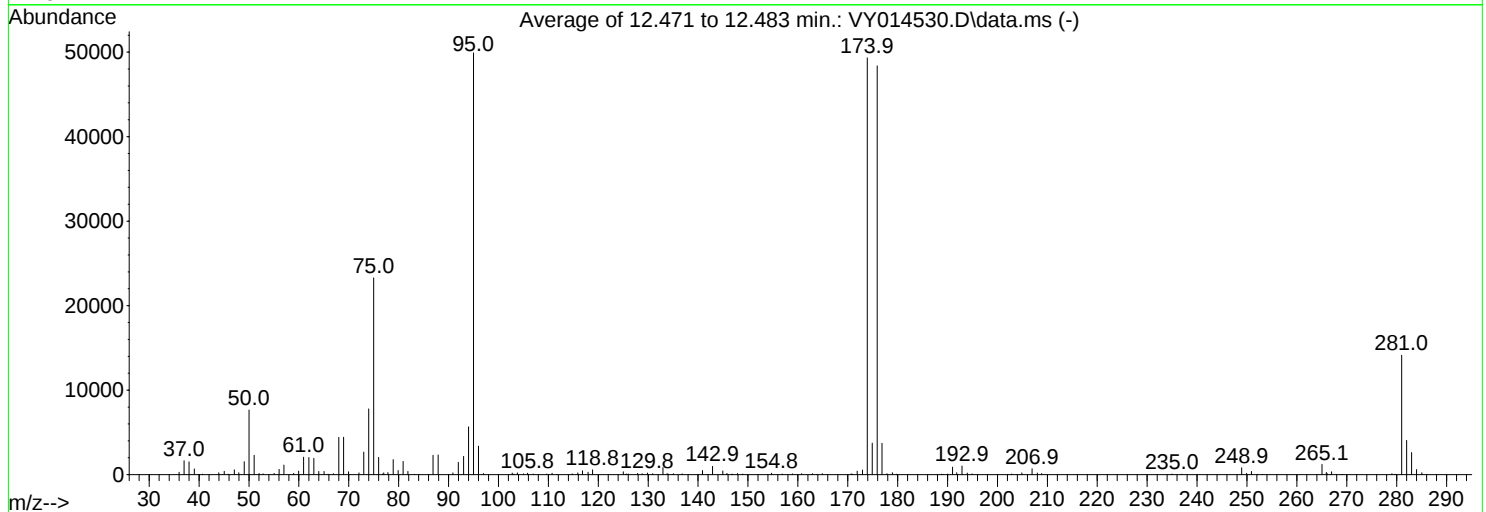


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY070323\
Data File : VY014530.D
Acq On : 03 Jul 2023 10:04
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y063023S.M
Title : SW846 8260
Last Update : Fri Jun 30 19:02:11 2023

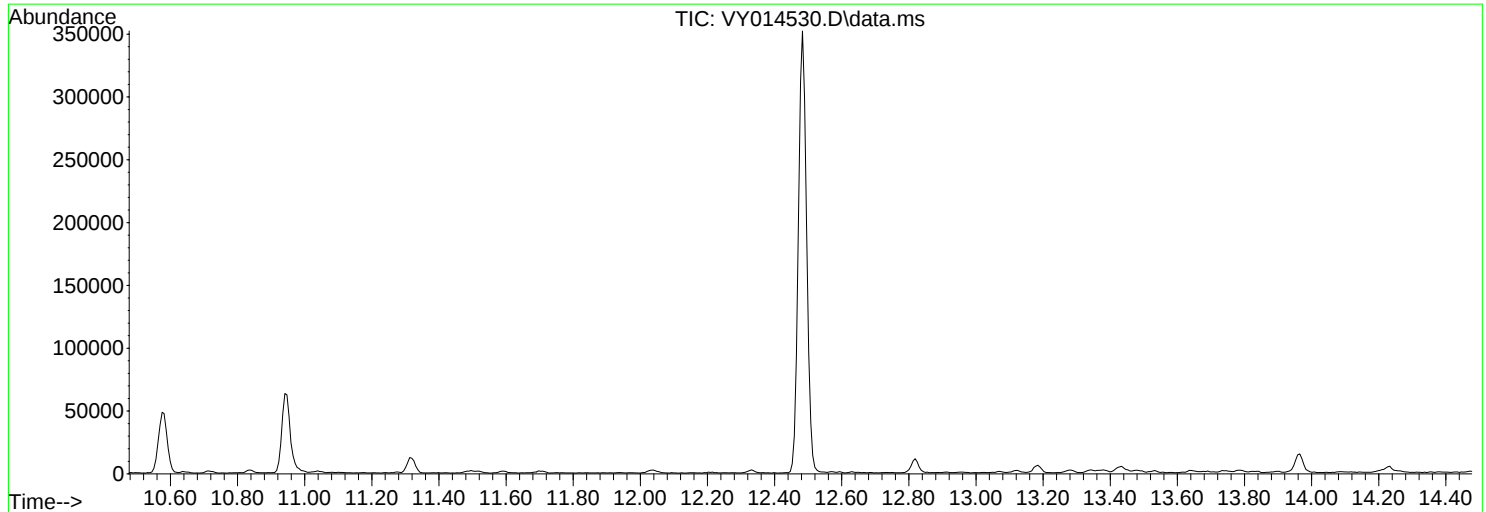

AutoFind: Scans 1747, 1748, 1749; Background Corrected with Scan 1739

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.3	7642	PASS
75	95	30	60	46.7	23293	PASS
95	95	100	100	100.0	49917	PASS
96	95	5	9	6.7	3363	PASS
173	174	0.00	2	1.1	556	PASS
174	95	50	100	98.8	49325	PASS
175	174	5	9	7.6	3739	PASS
176	174	95	101	98.1	48381	PASS
177	176	5	9	7.7	3710	PASS