

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY070523\
 Data File : VY014558.D
 Acq On : 05 Jul 2023 15:09
 Operator : KP/MD
 Sample : 03483-01
 Misc : 5.06g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 RO-CHRT-24801

Quant Time: Jul 05 15:19:07 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y063023S.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 30 19:02:11 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.783	168	241490	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	392588	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	377255	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	173956	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	151781	63.181	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	126.360%
35) Dibromofluoromethane	7.710	113	130305	53.899	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	107.800%
50) Toluene-d8	10.179	98	474197	49.618	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	99.240%
62) 4-Bromofluorobenzene	12.477	95	153612	46.288	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	92.580%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY070523\
Data File : VY014558.D
Acq On : 05 Jul 2023 15:09
Operator : KP/MD
Sample : 03483-01
Misc : 5.06g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
RO-CHRT-24801

Quant Time: Jul 05 15:19:07 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y063023S.M
Quant Title : SW846 8260
QLast Update : Fri Jun 30 19:02:11 2023
Response via : Initial Calibration




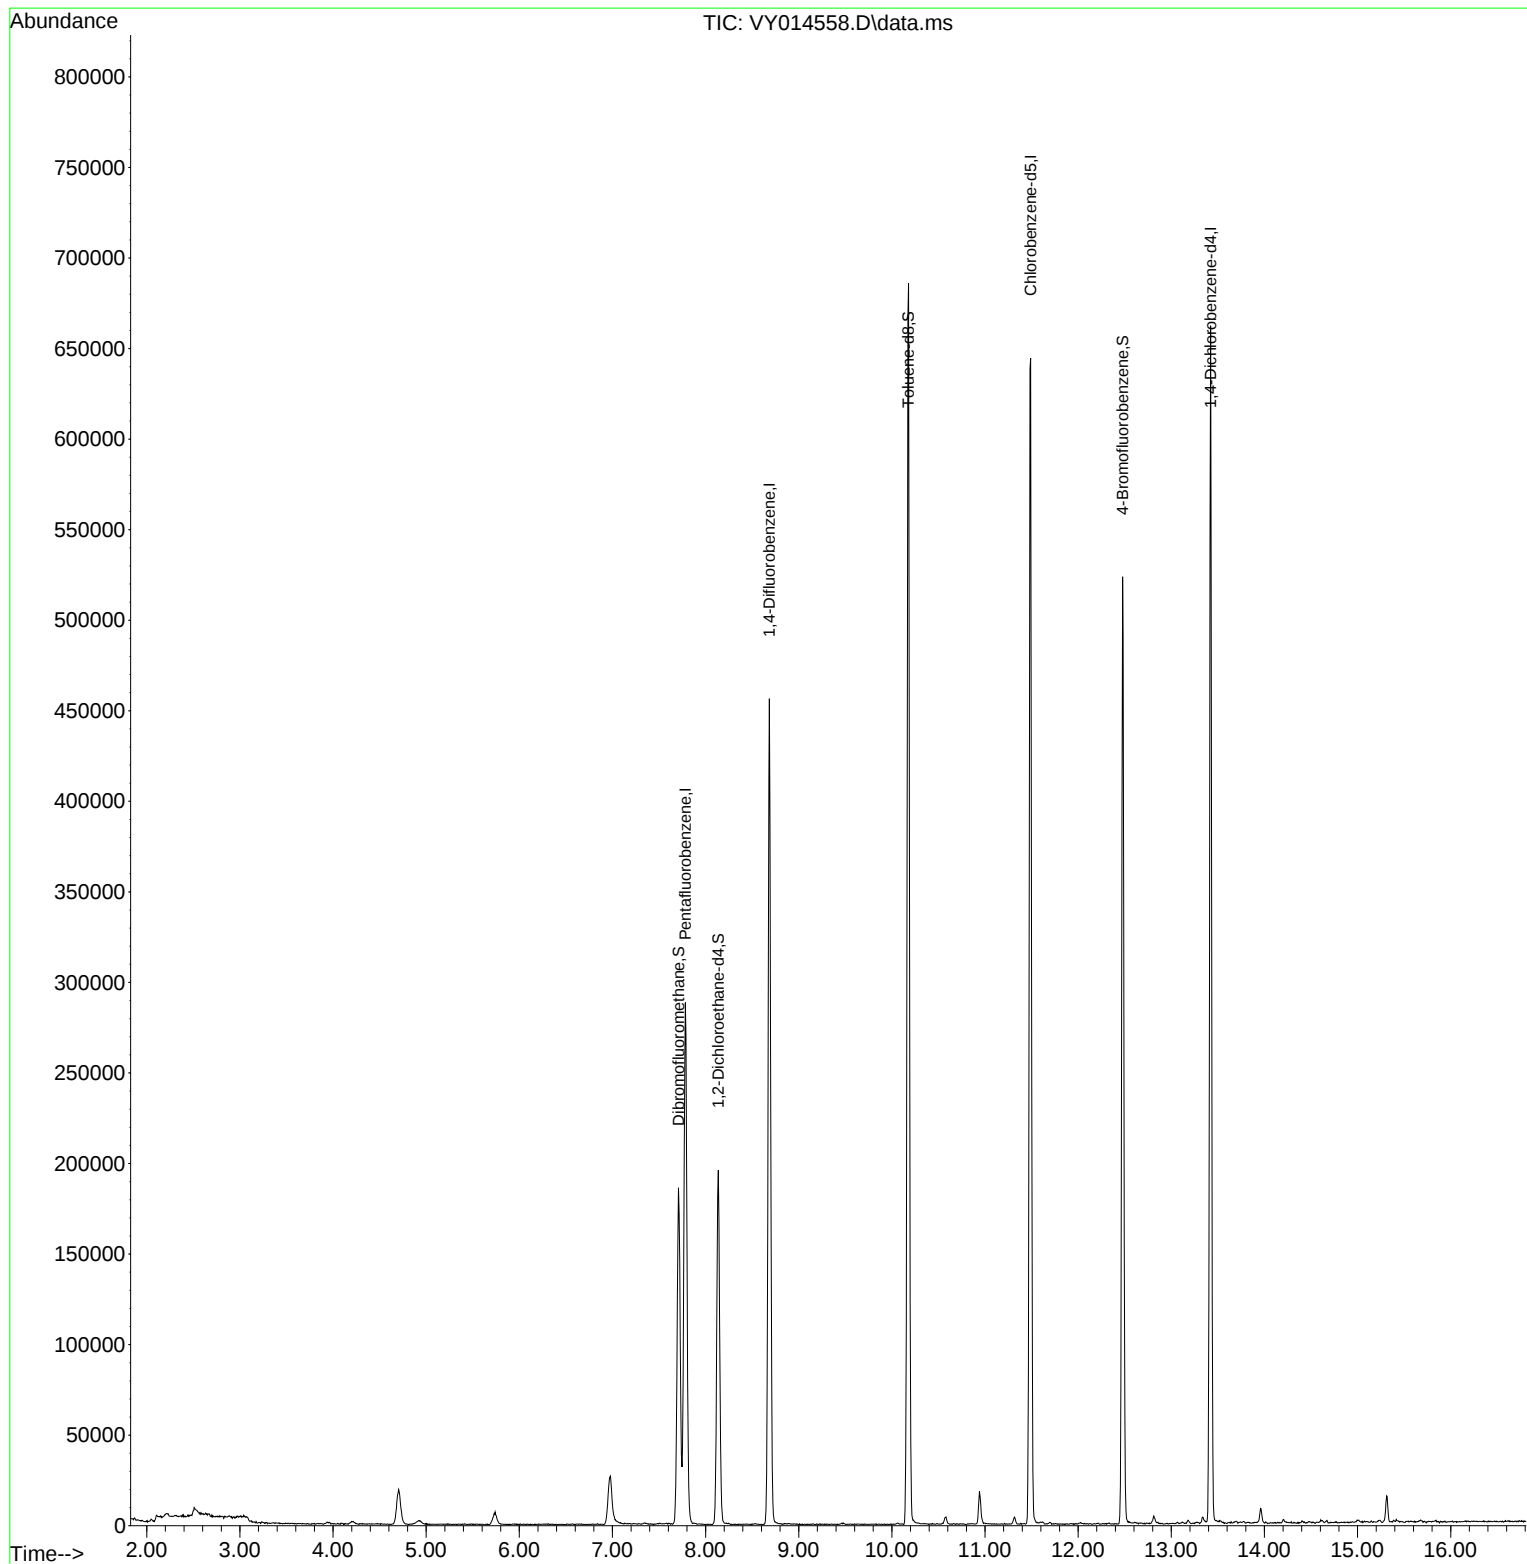


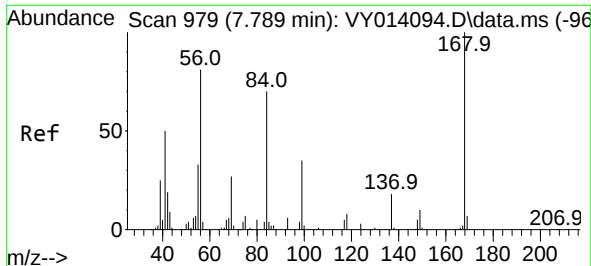

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.783 min Scan# 91
Delta R.T. -0.006 min
Lab File: VY014558.D
Acq: 05 Jul 2023 15:09




Instrument :
MSVOA_Y
ClientSampleId :
RO-CHRT-24801


Tgt Ion:168 Resp: 241490
Ion Ratio Lower Upper
168 100
99 48.2 43.4 65.0

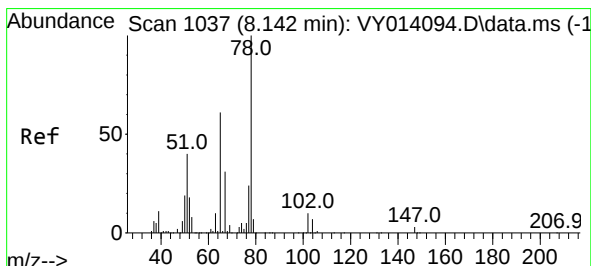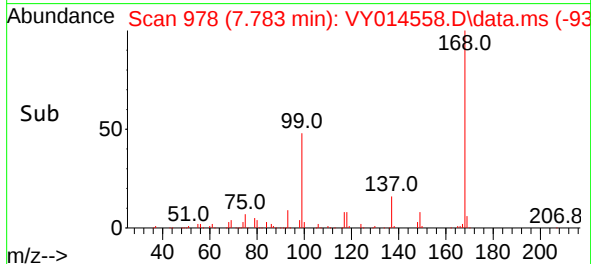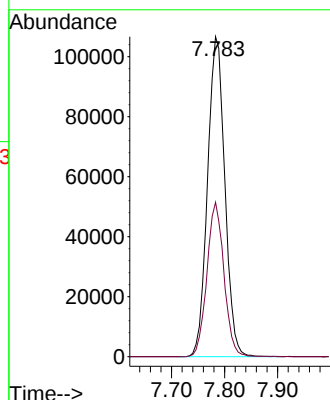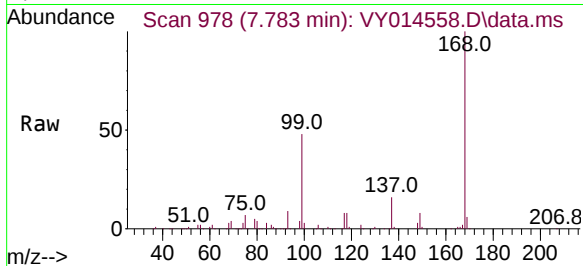

#33
1,2-Dichloroethane-d4
Concen: 63.181 ug/l
RT: 8.136 min Scan# 1036
Delta R.T. -0.006 min
Lab File: VY014558.D
Acq: 05 Jul 2023 15:09

Tgt Ion: 65 Resp: 151781
Ion Ratio Lower Upper
65 100
67 53.6 0.0 101.8

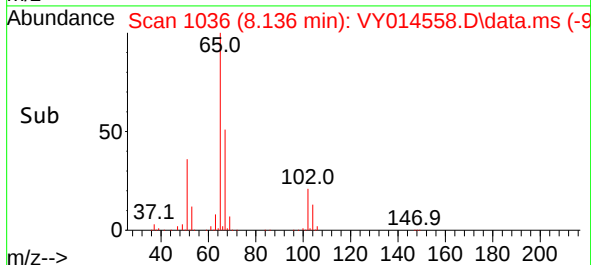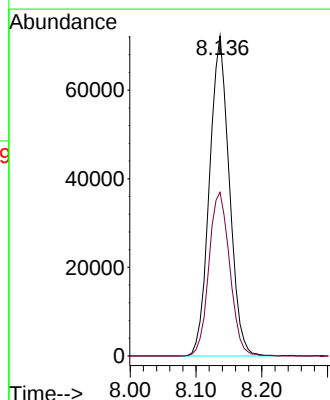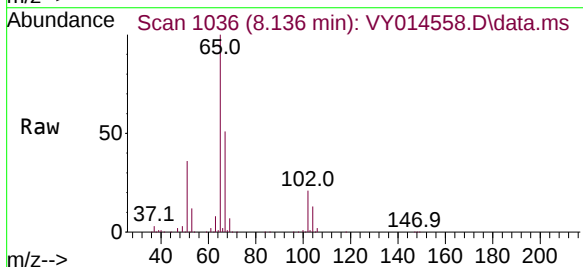

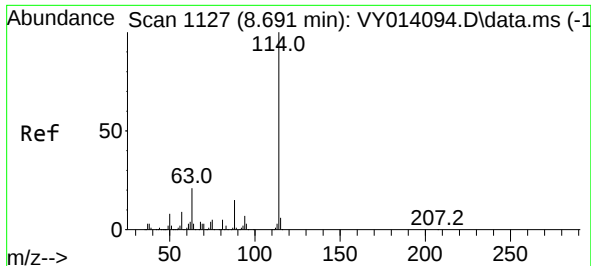

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.685 min Scan# 1126

Delta R.T. -0.006 min

Lab File: VY014558.D

Acq: 05 Jul 2023 15:09

Instrument :

MSVOA_Y

ClientSampleId :

RO-CHRT-24801





Tgt Ion:114 Resp: 392588

Ion Ratio Lower Upper

114 100

63 19.2 0.0 42.4

88 14.8 0.0 30.6

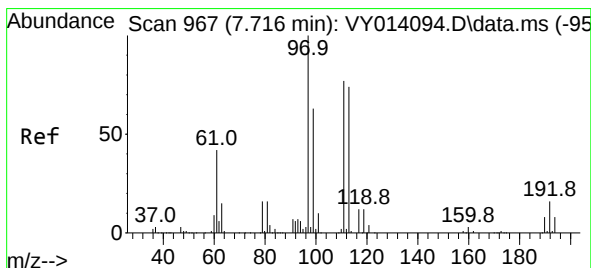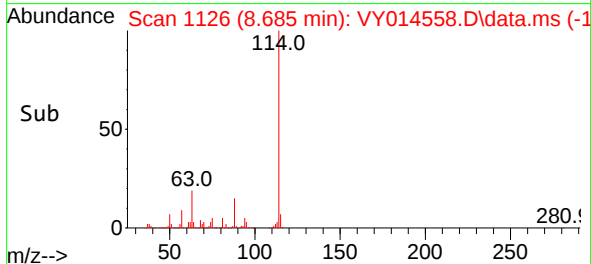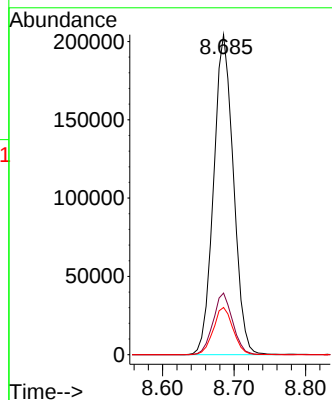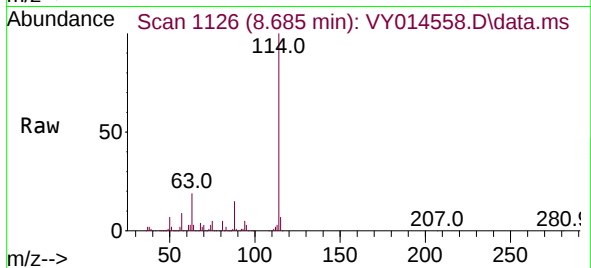

#35

Dibromofluoromethane

Concen: 53.899 ug/l

RT: 7.710 min Scan# 966

Delta R.T. -0.006 min

Lab File: VY014558.D

Acq: 05 Jul 2023 15:09




Tgt Ion:113 Resp: 130305


Ion Ratio Lower Upper

113 100

111 103.1 81.3 121.9

192 22.7 16.9 25.3


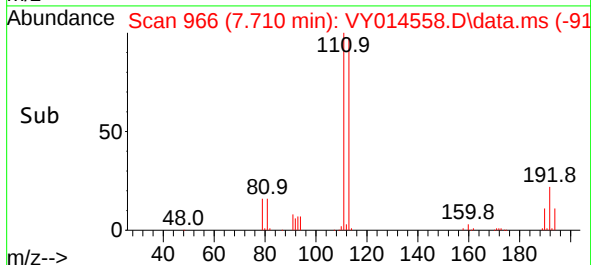
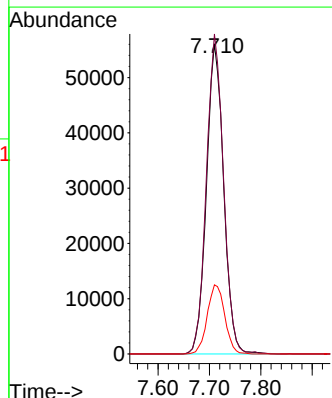
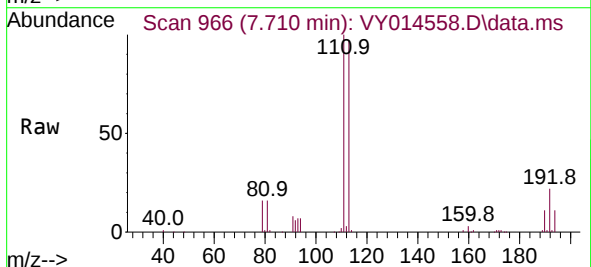


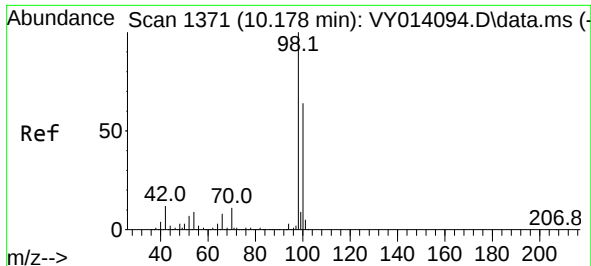

#50
Toluene-d8
Concen: 49.618 ug/l
RT: 10.179 min Scan# 11
Delta R.T. 0.001 min
Lab File: VY014558.D
Acq: 05 Jul 2023 15:09




Instrument :
MSVOA_Y
ClientSampleId :
RO-CHRT-24801


Tgt Ion: 98 Resp: 474197
Ion Ratio Lower Upper
98 100
100 62.6 50.1 75.1

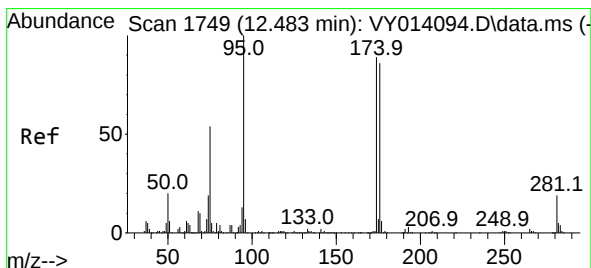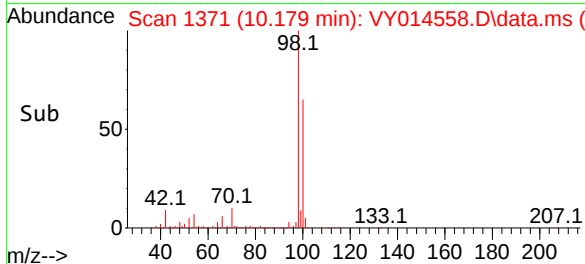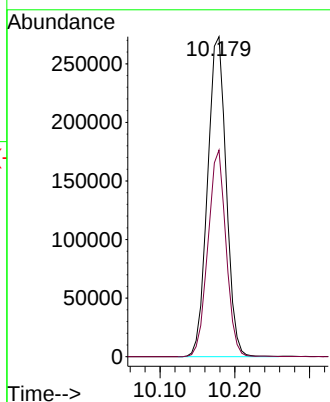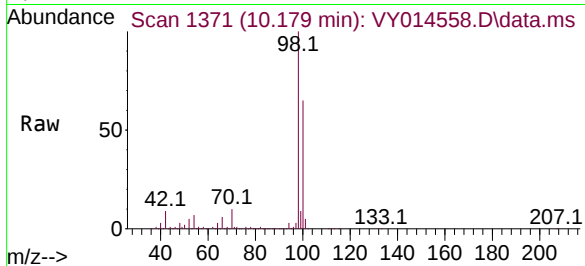

#62
4-Bromofluorobenzene
Concen: 46.288 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. -0.006 min
Lab File: VY014558.D
Acq: 05 Jul 2023 15:09

Tgt Ion: 95 Resp: 153612
Ion Ratio Lower Upper
95 100
174 96.5 0.0 178.2
176 91.9 0.0 173.8


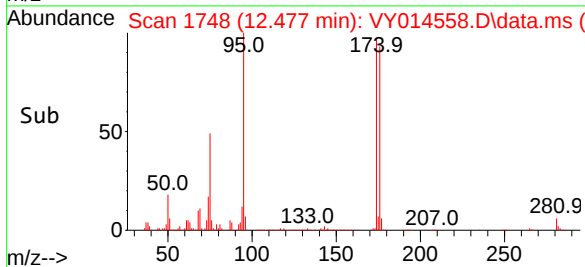
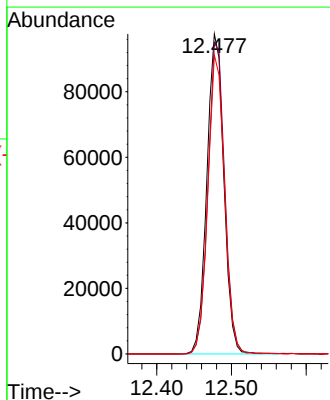
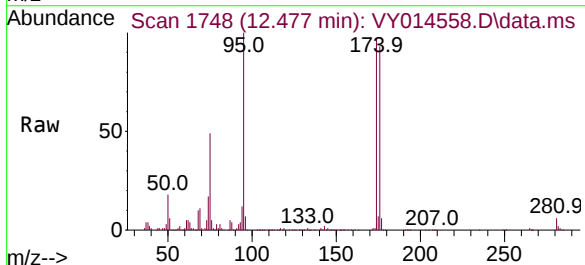


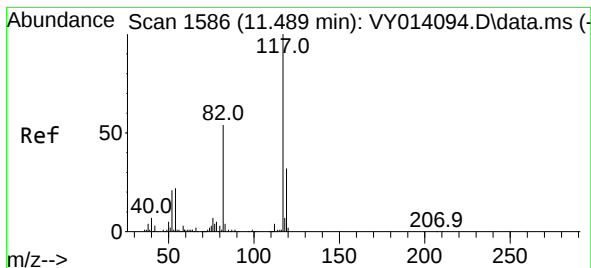

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY014558.D
Acq: 05 Jul 2023 15:09

Instrument :
MSVOA_Y
ClientSampleId :
RO-CHRT-24801

Tgt Ion:117 Resp: 377255
Ion Ratio Lower Upper
117 100
82 51.0 43.4 65.0
119 32.6 26.3 39.5

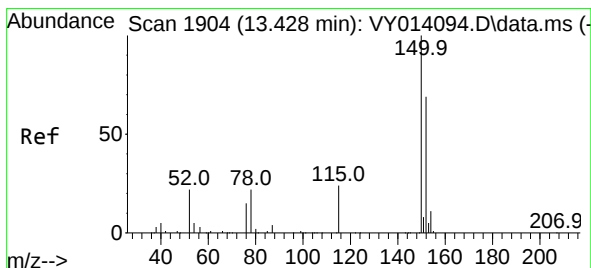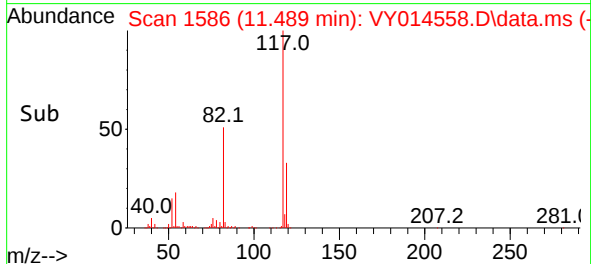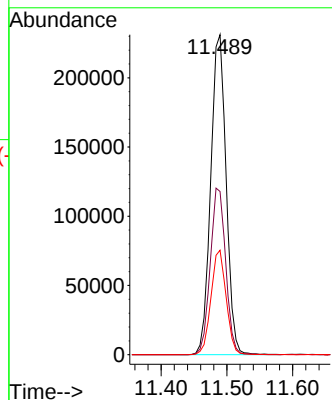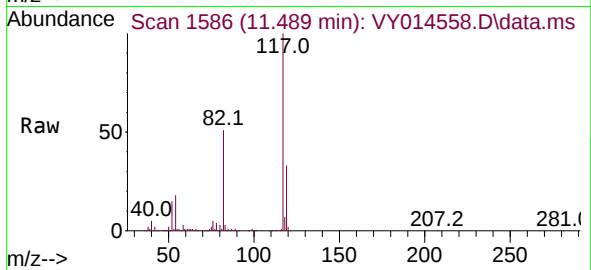

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.422 min Scan# 1903
Delta R.T. -0.006 min
Lab File: VY014558.D
Acq: 05 Jul 2023 15:09

Tgt Ion:152 Resp: 173956
Ion Ratio Lower Upper
152 100
115 54.6 28.8 86.5
150 157.2 0.0 348.8

