
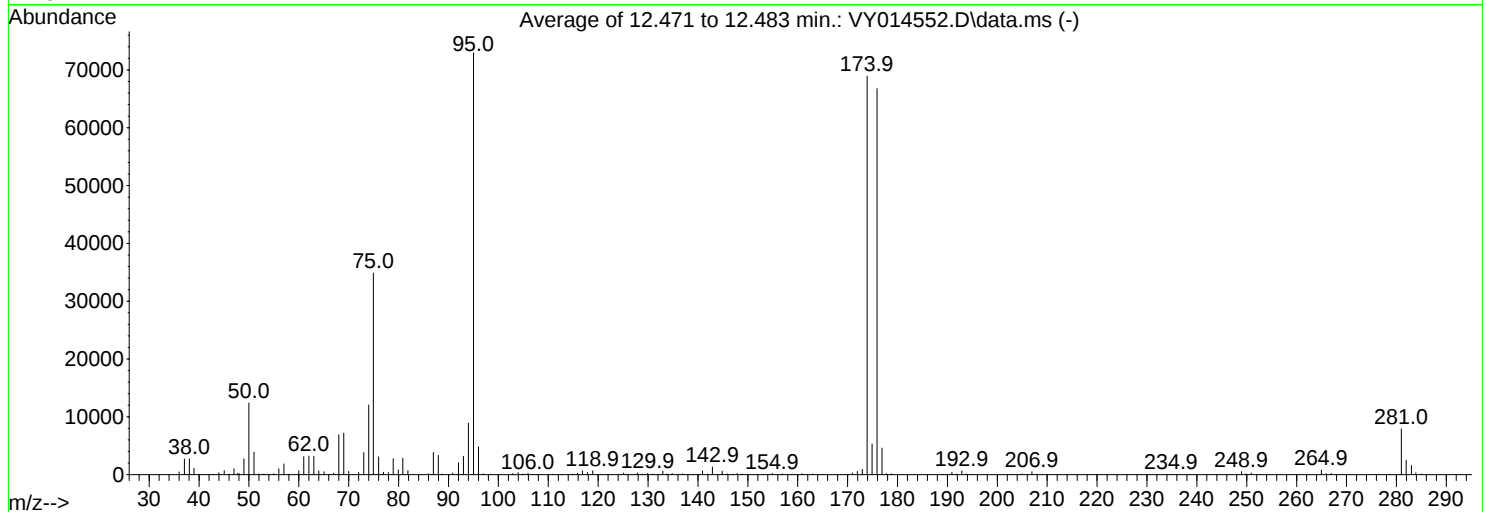


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY070523\
Data File : VY014552.D
Acq On : 05 Jul 2023 11:54
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y063023S.M
Title : SW846 8260
Last Update : Fri Jun 30 19:02:11 2023

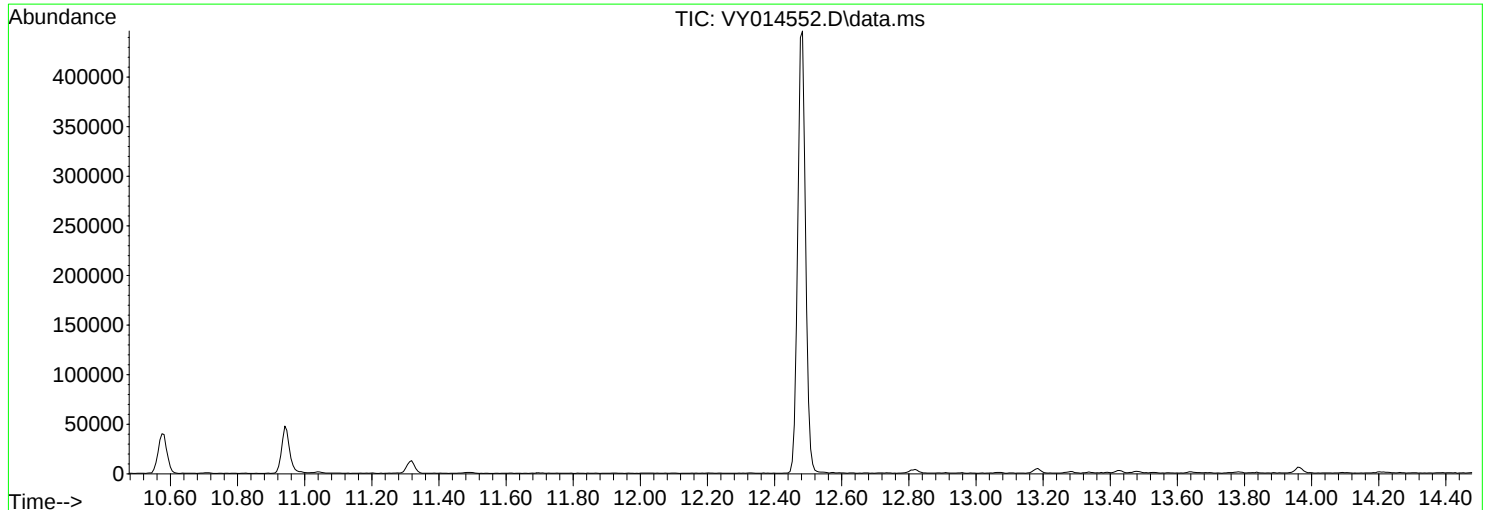

AutoFind: Scans 1747, 1748, 1749; Background Corrected with Scan 1739

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	12394	PASS
75	95	30	60	47.8	34872	PASS
95	95	100	100	100.0	72955	PASS
96	95	5	9	6.6	4822	PASS
173	174	0.00	2	1.3	900	PASS
174	95	50	100	94.5	68939	PASS
175	174	5	9	7.7	5309	PASS
176	174	95	101	96.9	66781	PASS
177	176	5	9	6.9	4585	PASS