

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY070622\
 Data File : VY009454.D
 Acq On : 06 Jul 2022 15:18
 Operator : KP/MD
 Sample : N3584-01
 Misc : 4.80g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 CHRT-26572

Quant Time: Jul 07 01:50:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y062822S.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 29 17:35:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.783	168	225948	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	389280	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.483	117	347687	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	159966	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	96800	53.488	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 106.980%	
35) Dibromofluoromethane	7.710	113	88960	41.522	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 83.040%	
50) Toluene-d8	10.173	98	336399	51.211	ug/l	0.00
Spiked Amount	50.000	Range	78 - 125	Recovery	= 102.420%	
62) 4-Bromofluorobenzene	12.477	95	115744	37.152	ug/l	0.00
Spiked Amount	50.000	Range	50 - 146	Recovery	= 74.300%	
Target Compounds						
16) Acetone	3.948	43	16096	27.081	ug/l	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY070622\
Data File : VY009454.D
Acq On : 06 Jul 2022 15:18
Operator : KP/MD
Sample : N3584-01
Misc : 4.80g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
CHRT-26572

Quant Time: Jul 07 01:50:14 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y062822S.M
Quant Title : SW846 8260
QLast Update : Wed Jun 29 17:35:34 2022
Response via : Initial Calibration




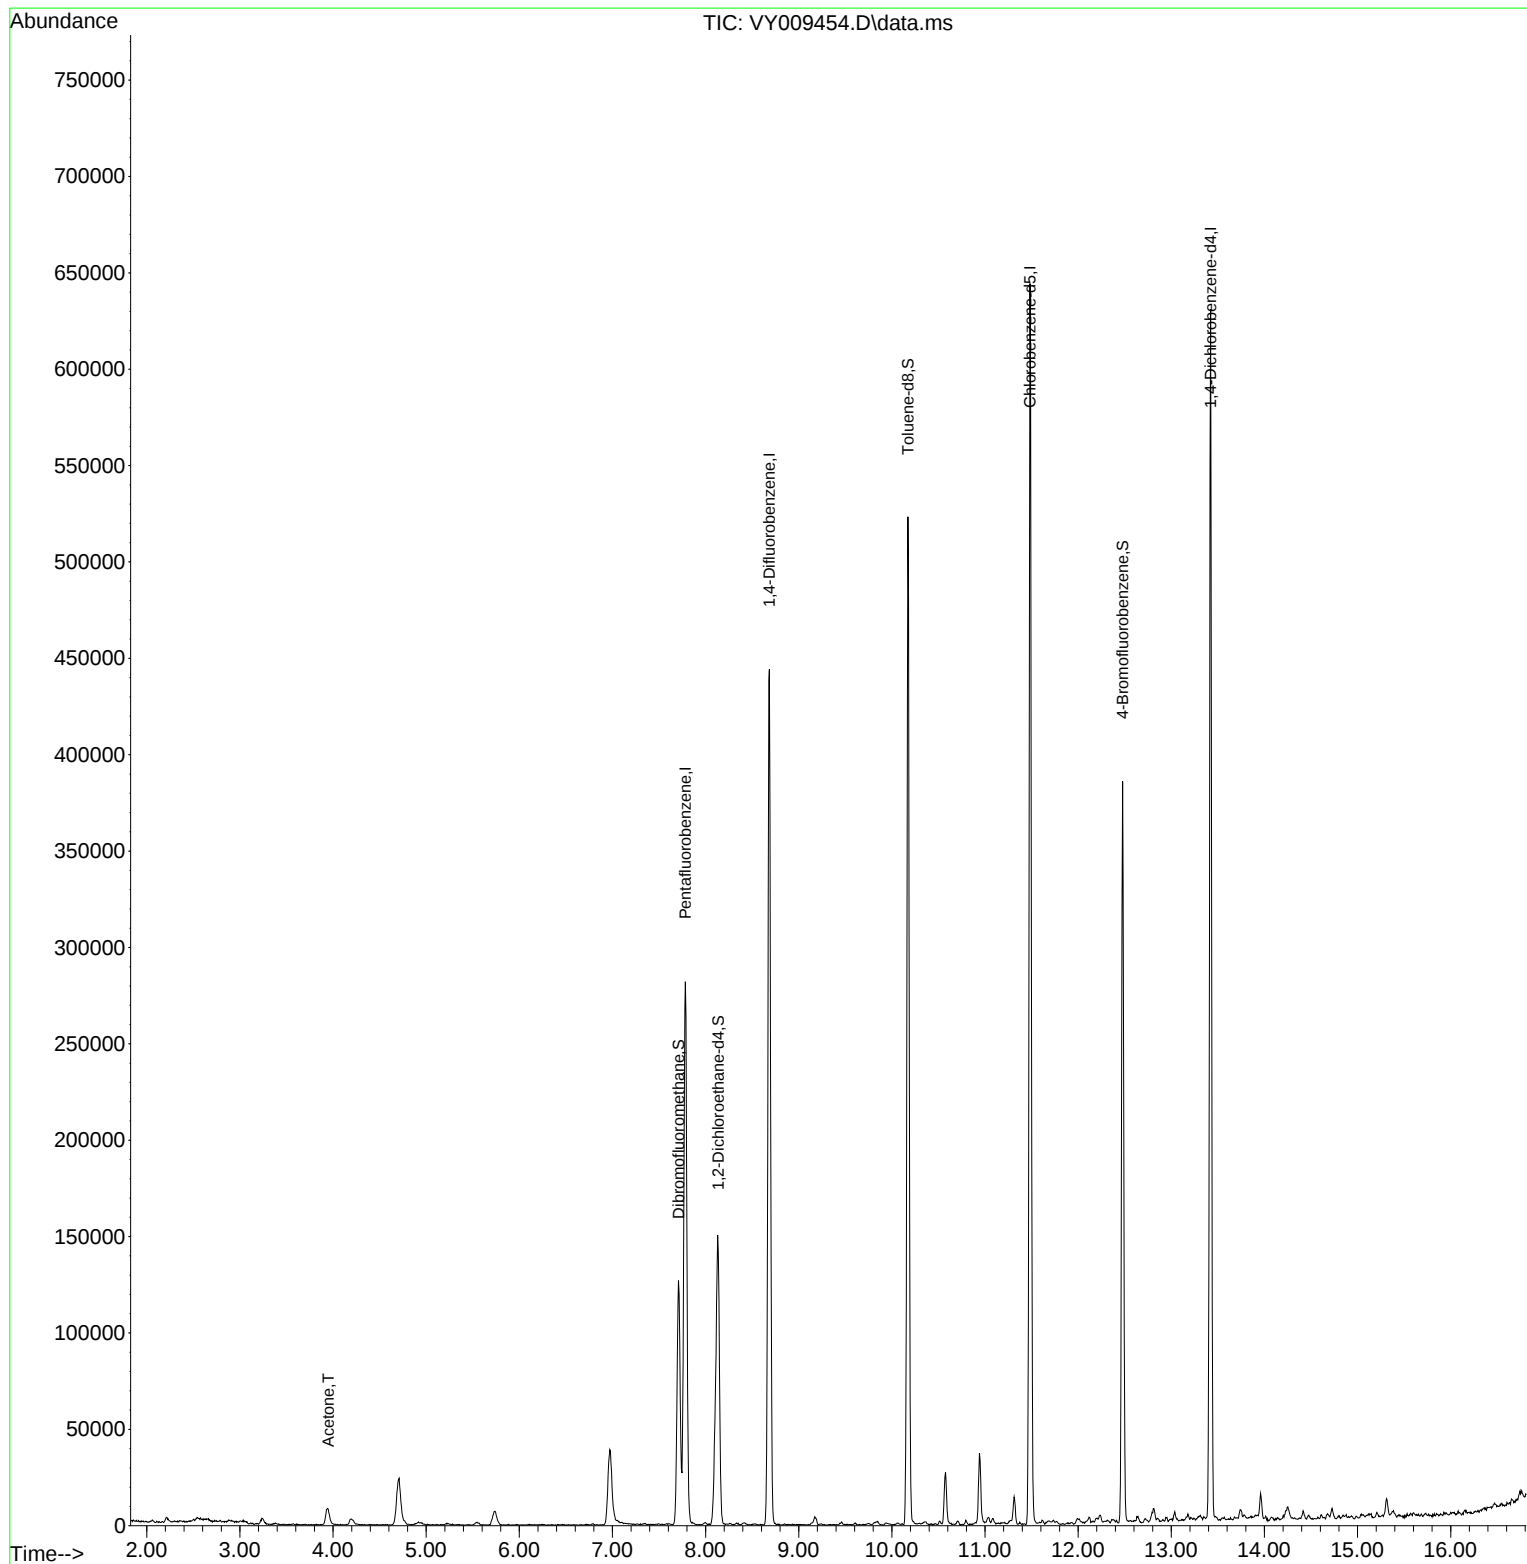


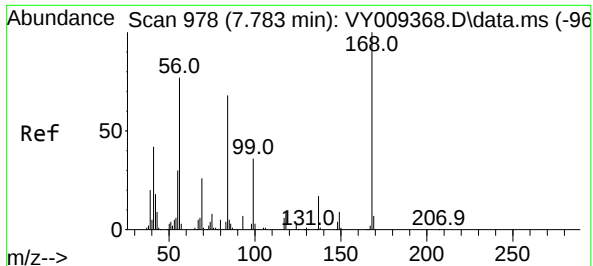

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.783 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY009454.D
Acq: 06 Jul 2022 15:18




Instrument :
MSVOA_Y
ClientSampleId :
CHRT-26572


Tgt Ion:168 Resp: 225948
Ion Ratio Lower Upper
168 100
99 54.3 46.9 70.3

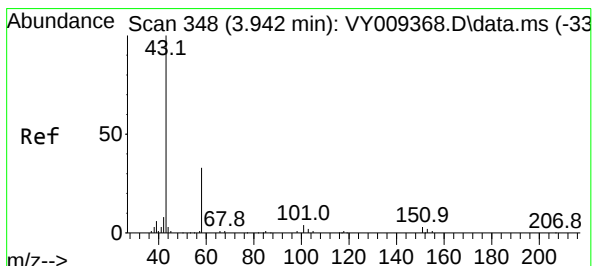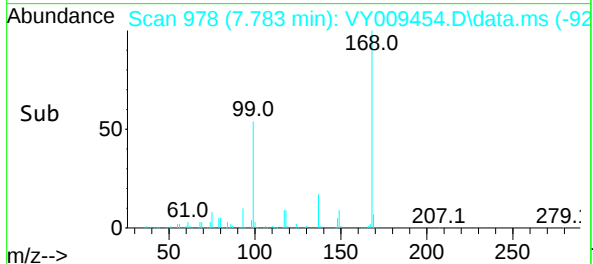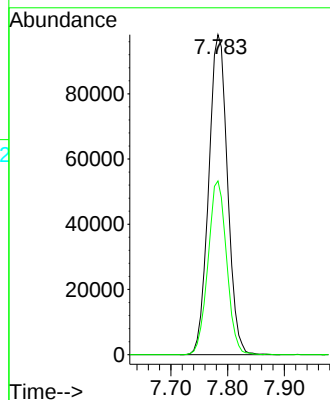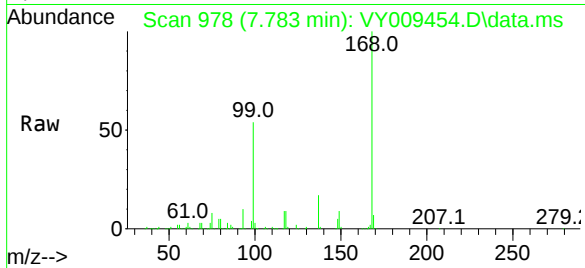

#16
Acetone
Concen: 27.081 ug/l
RT: 3.948 min Scan# 349
Delta R.T. 0.006 min
Lab File: VY009454.D
Acq: 06 Jul 2022 15:18

Tgt Ion: 43 Resp: 16096
Ion Ratio Lower Upper
43 100
58 29.1 22.0 33.0

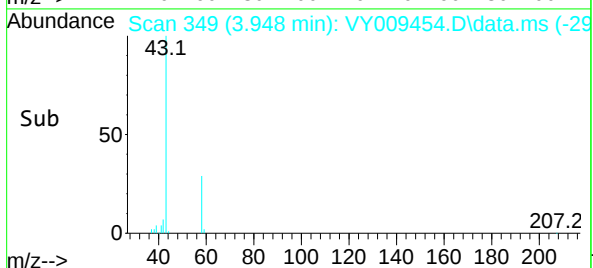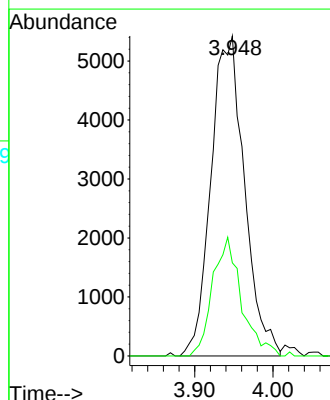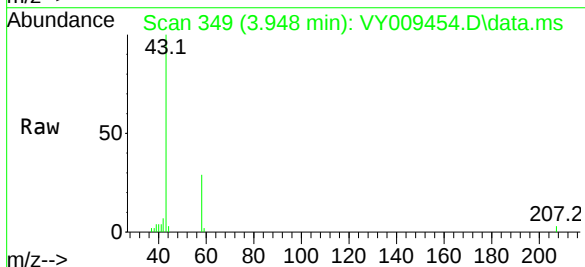

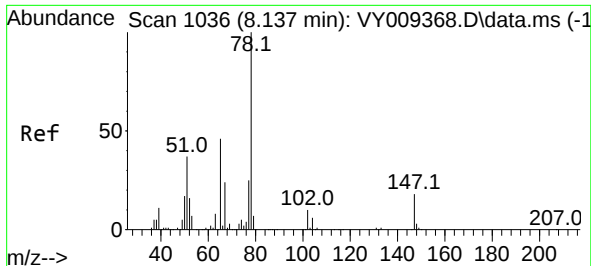

#33

1,2-Dichloroethane-d4

Concen: 53.488 ug/l

RT: 8.136 min Scan# 1036

Delta R.T. 0.000 min

Lab File: VY009454.D

Acq: 06 Jul 2022 15:18

Instrument :

MSVOA_Y

ClientSampleId :





CHRT-26572

Tgt Ion: 65 Resp: 96800

Ion Ratio Lower Upper

65 100

67 53.8 0.0 99.4

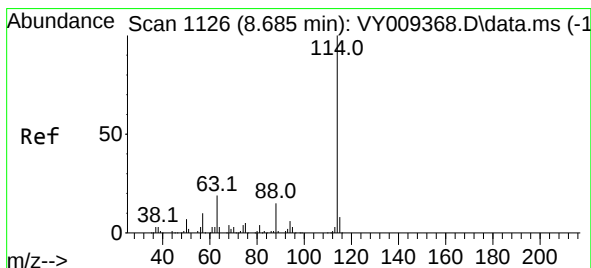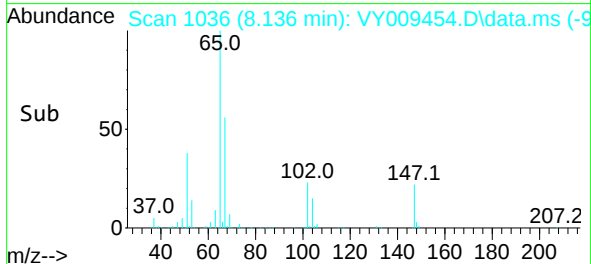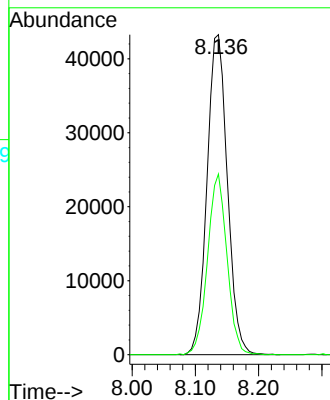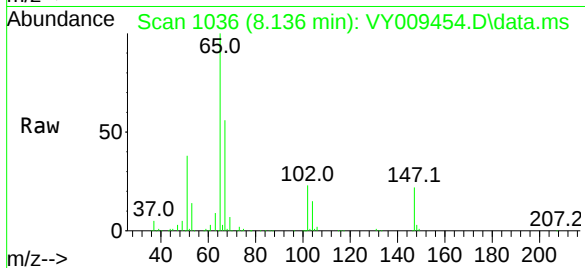

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.685 min Scan# 1126

Delta R.T. 0.000 min

Lab File: VY009454.D

Acq: 06 Jul 2022 15:18




Tgt Ion: 114 Resp: 389280


Ion Ratio Lower Upper

114 100

63 18.7 0.0 43.2

88 14.6 0.0 31.8


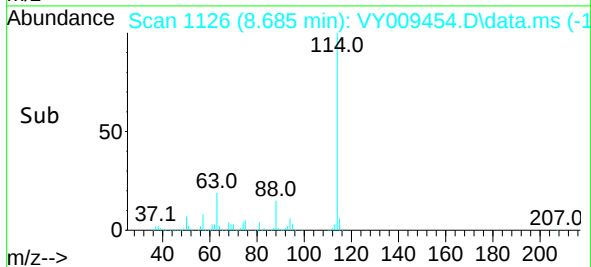
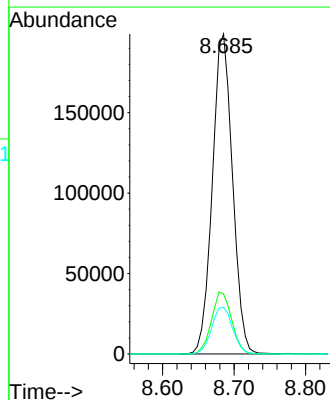
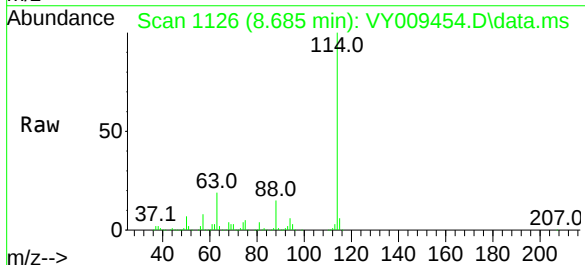


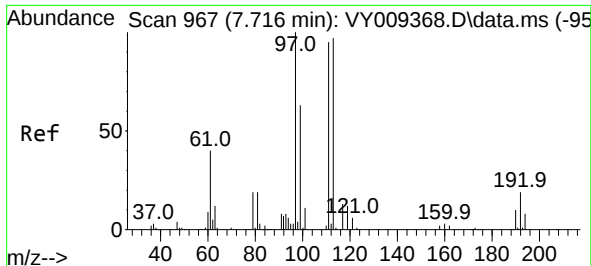

#35
Dibromofluoromethane
Concen: 41.522 ug/l
RT: 7.710 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY009454.D
Acq: 06 Jul 2022 15:18




Instrument :
MSVOA_Y
ClientSampleId :
CHRT-26572


Tgt Ion:113 Resp: 88960
Ion Ratio Lower Upper
113 100
111 103.2 82.6 124.0
192 20.5 17.6 26.4

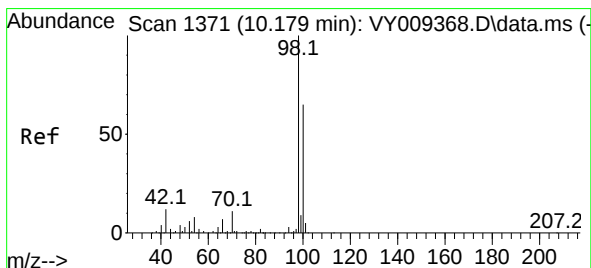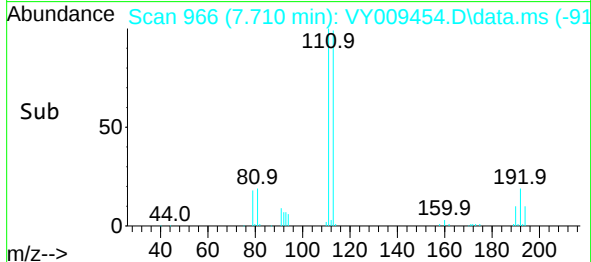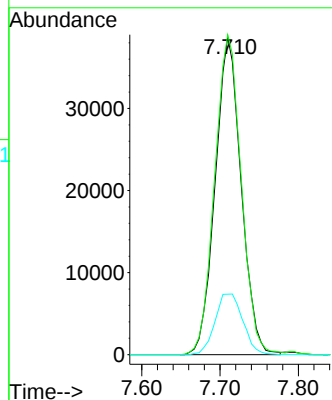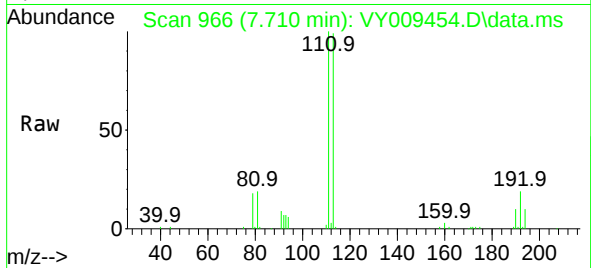

#50
Toluene-d8
Concen: 51.211 ug/l
RT: 10.173 min Scan# 1370
Delta R.T. -0.006 min
Lab File: VY009454.D
Acq: 06 Jul 2022 15:18

Tgt Ion: 98 Resp: 336399
Ion Ratio Lower Upper
98 100
100 65.5 50.2 75.2


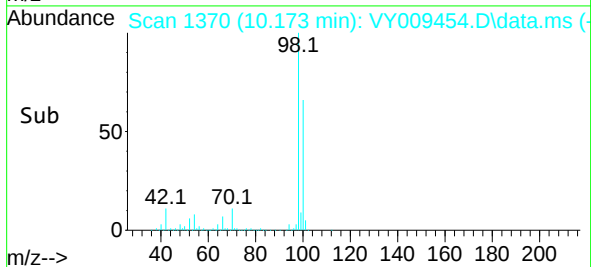
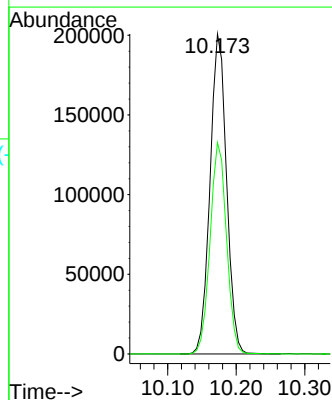
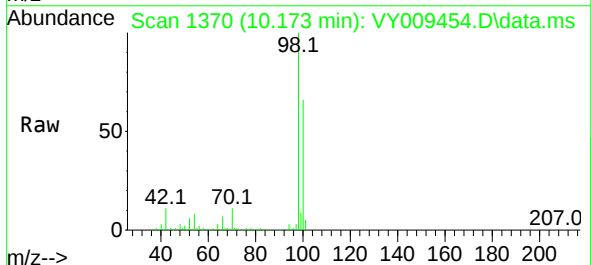


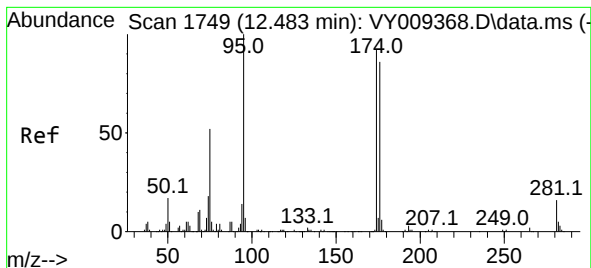

#62
4-Bromofluorobenzene
Concen: 37.152 ug/l
RT: 12.477 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY009454.D
Acq: 06 Jul 2022 15:18




Instrument :
MSVOA_Y
ClientSampleId :
CHRT-26572


Tgt Ion: 95 Resp: 115744
Ion Ratio Lower Upper
95 100
174 84.6 0.0 177.0
176 79.8 0.0 175.8

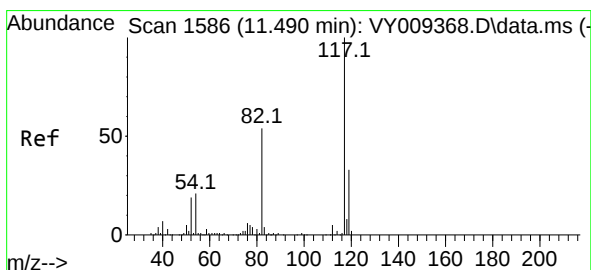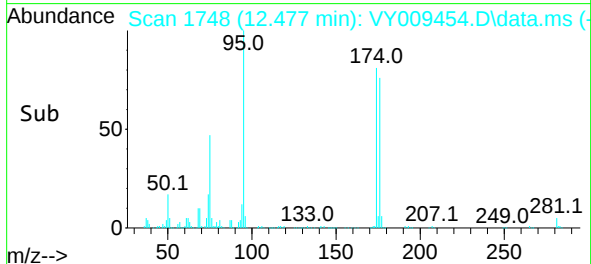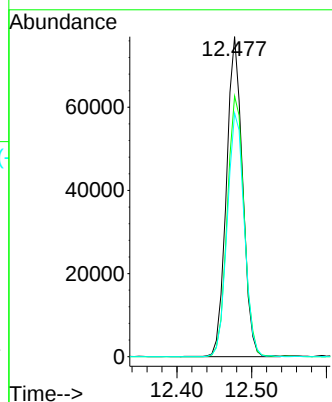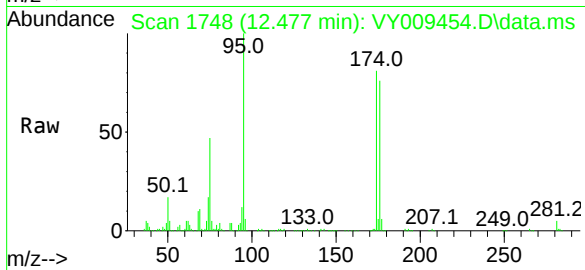

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.483 min Scan# 1585
Delta R.T. -0.007 min
Lab File: VY009454.D
Acq: 06 Jul 2022 15:18

Tgt Ion: 117 Resp: 347687
Ion Ratio Lower Upper
117 100
82 54.5 43.0 64.4
119 32.3 25.4 38.0

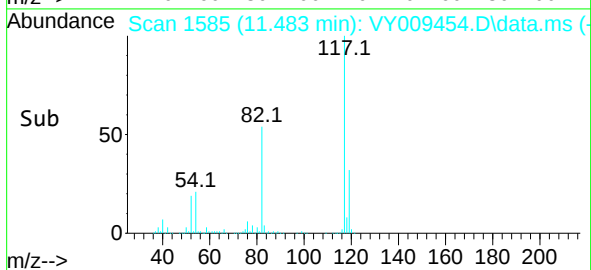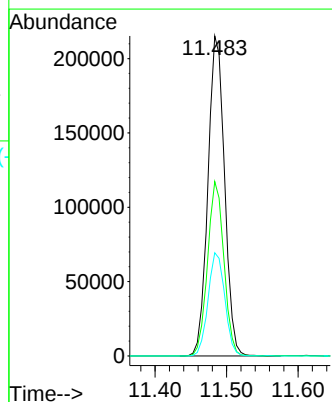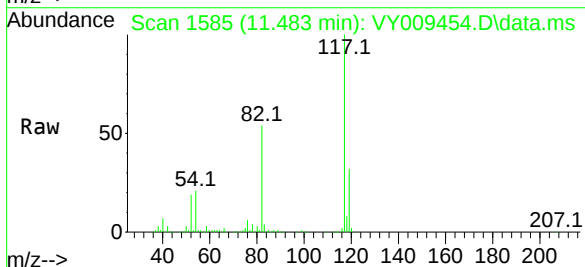

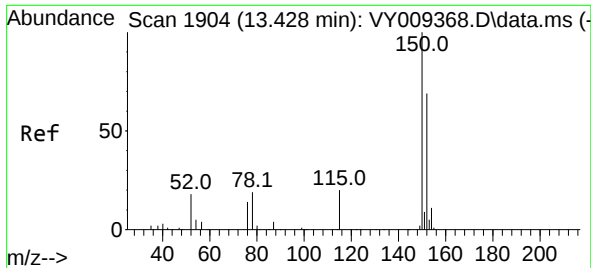

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.422 min Scan# 1903

Delta R.T. 0.000 min

Lab File: VY009454.D


Acq: 06 Jul 2022 15:18

Instrument :

MSVOA_Y

ClientSampleId :

CHRT-26572

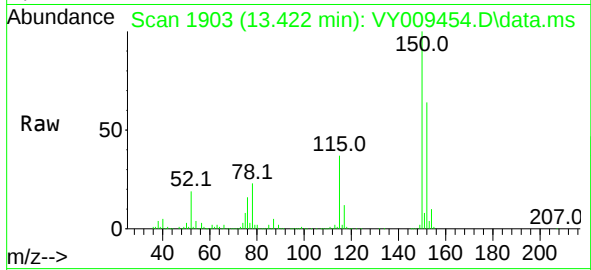

Tgt Ion:152 Resp: 159966

Ion Ratio Lower Upper

152 100

115 56.2 28.2 84.7

150 155.9 0.0 347.6

