

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY070623\
 Data File : VY014585.D
 Acq On : 06 Jul 2023 13:54
 Operator : KP/MD
 Sample : 03523-01
 Misc : 5.07g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 WALDWICK-COMP

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y063023S.M
 Title : SW846 8260

Signal : TIC: VY014585.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.796	159	160	162	rVB	480	229	2.38%	0.323%
2	2.954	185	186	190	rVB	386	351	3.65%	0.494%
3	2.997	190	193	196	rBV	234	359	3.73%	0.506%
4	3.028	196	198	199	rBV	440	226	2.35%	0.318%
5	3.247	233	234	238	rBV2	402	349	3.63%	0.492%
6	3.467	269	270	276	rVB3	305	273	2.84%	0.385%
7	3.643	298	299	303	rBV2	385	472	4.91%	0.665%
8	3.686	305	306	309	rVB2	367	252	2.62%	0.355%
9	3.759	316	318	321	rBV2	388	340	3.54%	0.479%
10	3.924	342	345	346	rBV2	298	333	3.46%	0.469%
11	4.168	383	385	388	rBV3	344	478	4.97%	0.673%
12	4.192	388	389	391	rVB2	470	257	2.67%	0.362%
13	4.418	424	426	430	rVB2	354	427	4.44%	0.602%
14	4.674	466	468	469	rVB	376	228	2.37%	0.321%
15	4.704	471	473	475	rVV3	417	351	3.65%	0.494%
16	4.771	482	484	487	rVB2	283	262	2.72%	0.369%
17	4.960	512	515	517	rBV2	292	395	4.11%	0.556%
18	5.247	559	562	565	rBV2	302	423	4.40%	0.596%
19	5.363	579	581	583	rBV2	390	390	4.05%	0.549%
20	5.454	594	596	597	rBV2	302	234	2.43%	0.330%
21	5.552	609	612	615	rBV2	301	440	4.57%	0.620%
22	5.588	616	618	621	rVB	393	333	3.46%	0.469%
23	5.722	639	640	643	rBV2	276	281	2.92%	0.396%
24	5.771	646	648	652	rBV2	225	295	3.07%	0.416%
25	5.838	657	659	660	rBV	346	300	3.12%	0.423%
26	6.027	687	690	691	rBV	276	331	3.44%	0.466%
27	6.240	723	725	726	rVB2	466	286	2.97%	0.403%
28	6.295	733	734	739	rVB3	440	459	4.77%	0.647%
29	6.533	768	773	775	rBV2	480	705	7.33%	0.993%
30	6.582	779	781	784	rBV2	260	296	3.08%	0.417%
31	6.917	831	836	837	rBV2	436	414	4.30%	0.583%
32	7.015	850	852	853	rBV	428	238	2.47%	0.335%
33	7.149	873	874	878	rVB	434	361	3.75%	0.509%
34	7.283	891	896	898	rBV2	321	461	4.79%	0.649%
35	7.320	900	902	905	rBV2	296	277	2.88%	0.390%
36	7.466	920	926	929	rBV4	323	773	8.04%	1.089%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY070623\
 Data File : VY014585.D
 Acq On : 06 Jul 2023 13:54
 Operator : KP/MD
 Sample : 03523-01
 Misc : 5.07g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 WALDWICK-COMP

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y063023S.M
 Title : SW846 8260

37	7.496	929	931	937	rVB3	520	768	7.99%	1.082%
38	7.576	942	944	947	rVB2	430	414	4.30%	0.583%
39	7.624	950	952	956	rBV2	326	388	4.03%	0.547%
40	7.698	962	964	965	rBV2	461	325	3.38%	0.458%
41	7.777	974	977	985	rVB4	1581	3394	35.29%	4.781%
42	7.917	995	1000	1001	rBV2	239	367	3.82%	0.517%
43	8.045	1020	1021	1022	rBV	424	235	2.44%	0.331%
44	8.063	1022	1024	1026	rVV3	280	324	3.37%	0.456%
45	8.130	1031	1035	1036	rBV	1733	2238	23.27%	3.153%
46	8.240	1051	1053	1055	rBV3	255	268	2.79%	0.378%
47	8.319	1064	1066	1068	rBV	440	281	2.92%	0.396%
48	8.447	1086	1087	1088	rBV	570	274	2.85%	0.386%
49	8.502	1094	1096	1100	rVB	193	233	2.42%	0.328%
50	8.685	1119	1126	1132	rBV2	2915	6468	67.25%	9.112%
51	8.929	1164	1166	1168	rVB	312	228	2.37%	0.321%
52	8.947	1168	1169	1172	rBV2	395	263	2.73%	0.371%
53	9.045	1181	1185	1188	rVB3	241	415	4.31%	0.585%
54	9.088	1188	1192	1193	rBV	287	299	3.11%	0.421%
55	9.148	1199	1202	1203	rVB2	292	273	2.84%	0.385%
56	9.173	1203	1206	1208	rBV2	295	353	3.67%	0.497%
57	9.319	1229	1230	1233	rBV	289	255	2.65%	0.359%
58	9.392	1239	1242	1243	rBV	427	350	3.64%	0.493%
59	9.581	1267	1273	1274	rBV2	269	423	4.40%	0.596%
60	10.051	1348	1350	1352	rBV	352	289	3.00%	0.407%
61	10.136	1363	1364	1366	rBV	354	376	3.91%	0.530%
62	10.179	1366	1371	1378	rVB	5713	9618	100.00%	13.549%
63	10.337	1395	1397	1399	rBV2	348	268	2.79%	0.378%
64	10.569	1432	1435	1436	rBV	576	561	5.83%	0.790%
65	10.721	1458	1460	1463	rBV2	214	240	2.50%	0.338%
66	10.843	1479	1480	1483	rVB2	337	234	2.43%	0.330%
67	10.941	1494	1496	1500	rVB3	575	674	7.01%	0.949%
68	10.977	1500	1502	1505	rBV2	378	411	4.27%	0.579%
69	11.075	1517	1518	1522	rVB2	450	494	5.14%	0.696%
70	11.227	1540	1543	1545	rVB2	383	366	3.81%	0.516%
71	11.276	1550	1551	1554	rVB	265	256	2.66%	0.361%
72	11.331	1558	1560	1563	rBV	222	274	2.85%	0.386%
73	11.490	1580	1586	1596	rBV2	5346	8760	91.08%	12.341%
74	11.569	1596	1599	1600	rBV	454	334	3.47%	0.471%
75	11.715	1619	1623	1624	rBV2	473	665	6.91%	0.937%
76	11.733	1624	1626	1627	rBV	289	237	2.46%	0.334%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY070623\
 Data File : VY014585.D
 Acq On : 06 Jul 2023 13:54
 Operator : KP/MD
 Sample : 03523-01
 Misc : 5.07g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 WALDWICK-COMP

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y063023S.M
 Title : SW846 8260

77	11.788	1633	1635	1636	rVB2	386	249	2.59%	0.351%
78	12.008	1668	1671	1672	rBV2	357	328	3.41%	0.462%
79	12.093	1683	1685	1687	rBV2	272	230	2.39%	0.324%
80	12.215	1704	1705	1708	rBV2	413	276	2.87%	0.389%
81	12.264	1712	1713	1717	rBV2	297	315	3.28%	0.444%
82	12.428	1739	1740	1741	rBV	540	274	2.85%	0.386%
83	12.483	1744	1749	1756	rVB6	4288	6646	69.10%	9.363%
84	13.014	1834	1836	1838	rVB2	514	369	3.84%	0.520%
85	13.093	1848	1849	1852	rBV3	328	307	3.19%	0.432%
86	13.416	1900	1902	1909	rVB4	2277	3971	41.29%	5.594%
87	13.514	1916	1918	1921	rBV2	398	573	5.96%	0.807%
88	13.568	1926	1927	1930	rBV	367	321	3.34%	0.452%
89	13.800	1963	1965	1966	rBV2	435	348	3.62%	0.490%
90	13.946	1987	1989	1991	rBV2	630	400	4.16%	0.563%
91	14.221	2032	2034	2039	rVB3	448	606	6.30%	0.854%


Sum of corrected areas: 70985

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY070623\
Data File : VY014585.D
Acq On : 06 Jul 2023 13:54
Operator : KP/MD
Sample : 03523-01
Misc : 5.07g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
WALDWICK-COMP

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y063023S.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

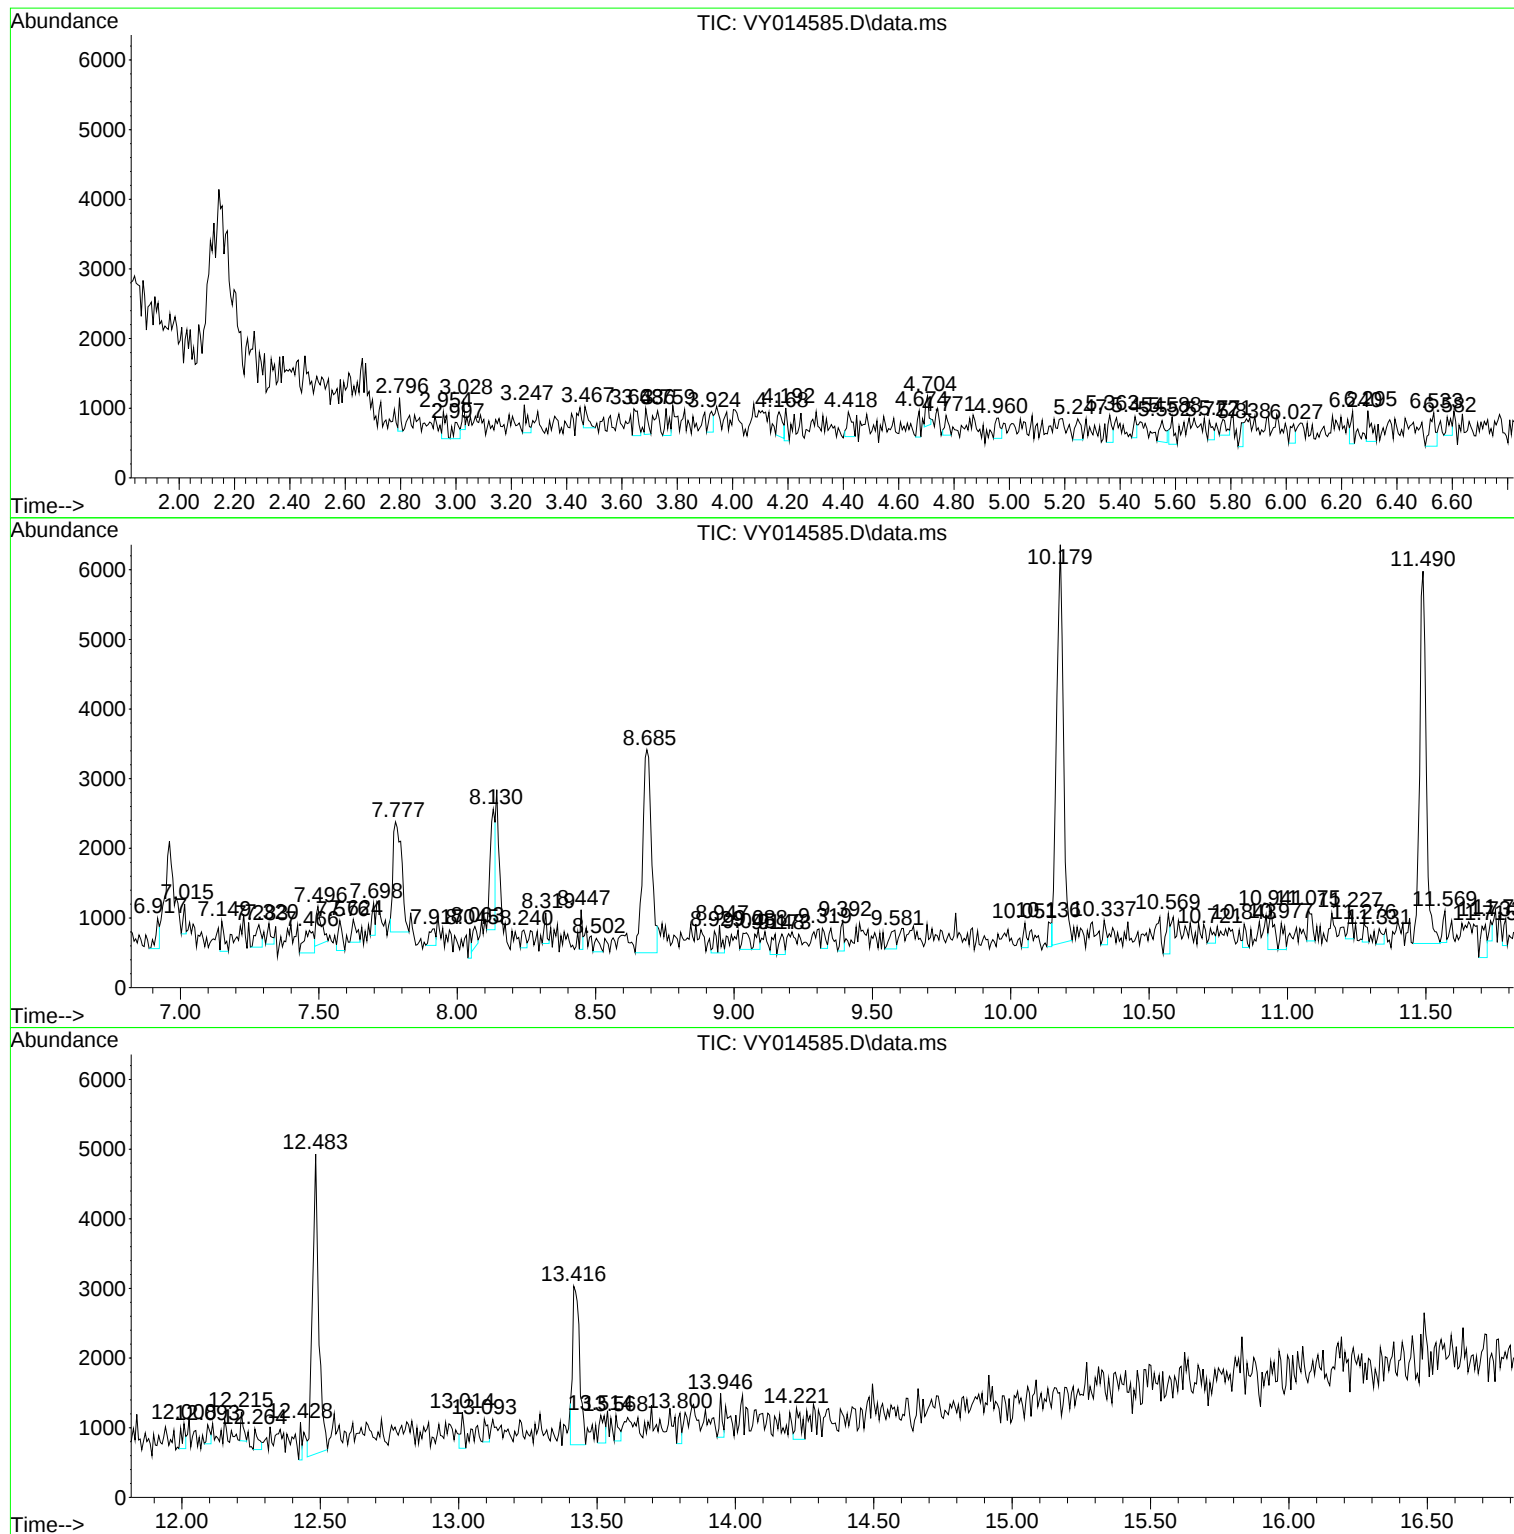

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY070623\
Data File : VY014585.D
Acq On : 06 Jul 2023 13:54
Operator : KP/MD
Sample : 03523-01
Misc : 5.07g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
WALDWICK-COMP

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y063023S.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY070623\
Data File : VY014585.D
Acq On : 06 Jul 2023 13:54
Operator : KP/MD
Sample : 03523-01
Misc : 5.07g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
WALDWICK-COMP

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y063023S.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------