
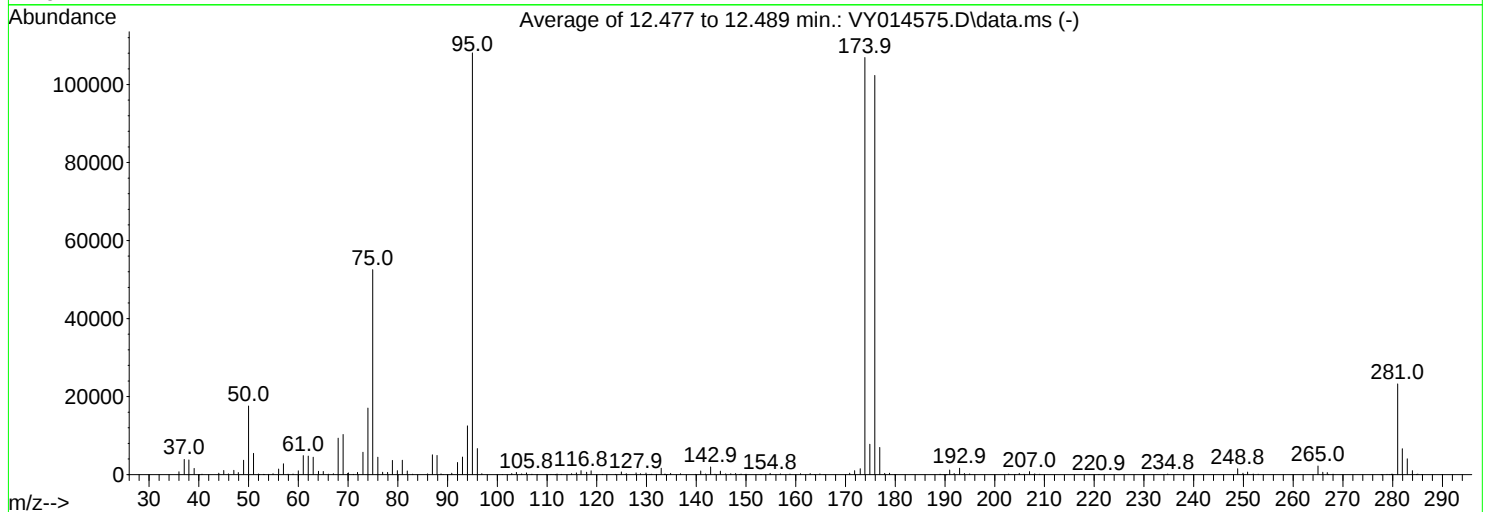


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY070623\
Data File : VY014575.D
Acq On : 06 Jul 2023 09:18
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y063023S.M
Title : SW846 8260
Last Update : Fri Jun 30 19:02:11 2023

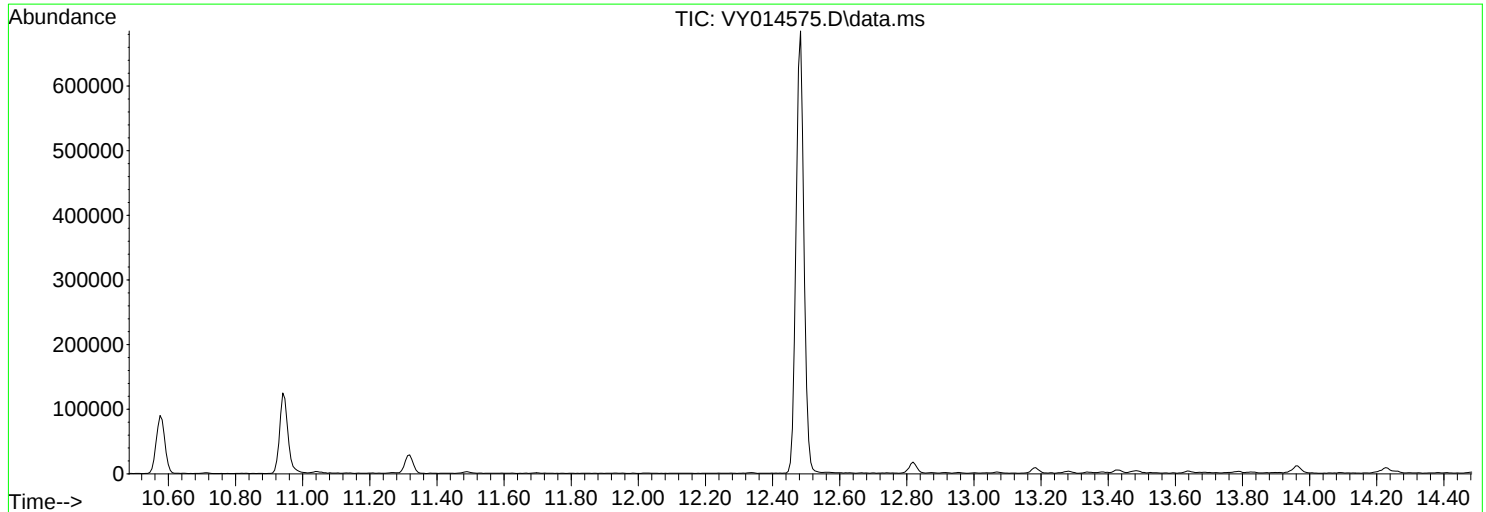

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1739

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.3	17612	PASS
75	95	30	60	48.6	52519	PASS
95	95	100	100	100.0	108107	PASS
96	95	5	9	6.2	6684	PASS
173	174	0.00	2	1.4	1530	PASS
174	95	50	100	98.9	106901	PASS
175	174	5	9	7.3	7808	PASS
176	174	95	101	95.7	102325	PASS
177	176	5	9	6.8	6990	PASS