
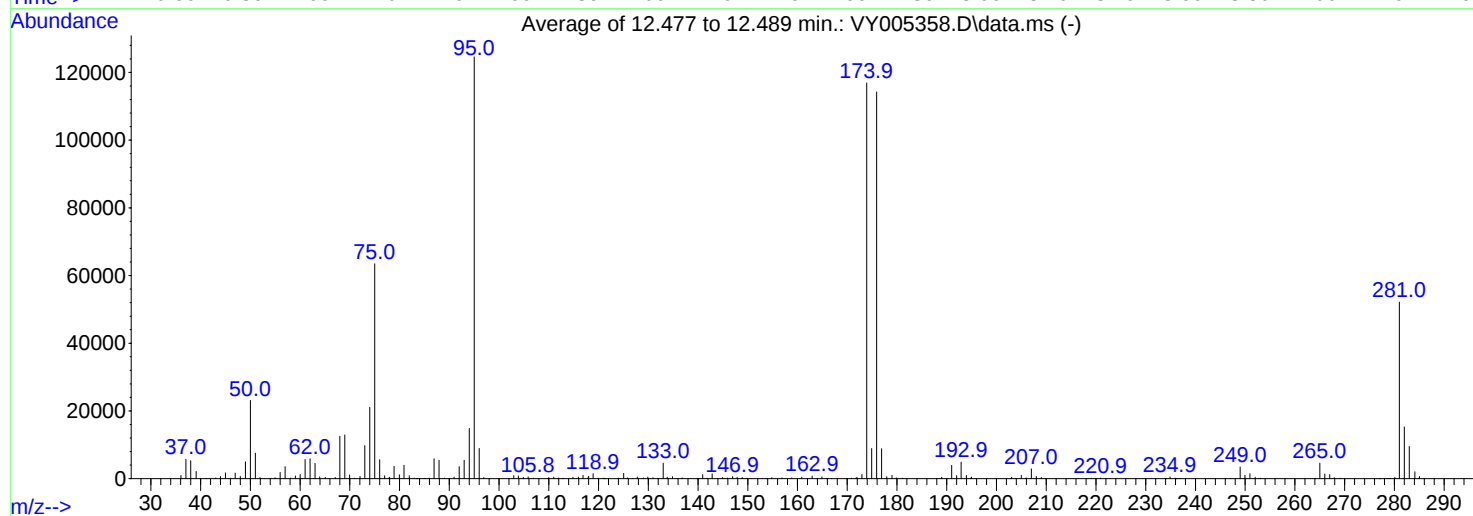


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY070721\
 Data File : VY005358.D
 Acq On : 07 Jul 2021 09:53
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y062221S.M
 Title : SW846 8260
 Last Update : Wed Jun 23 07:57:52 2021

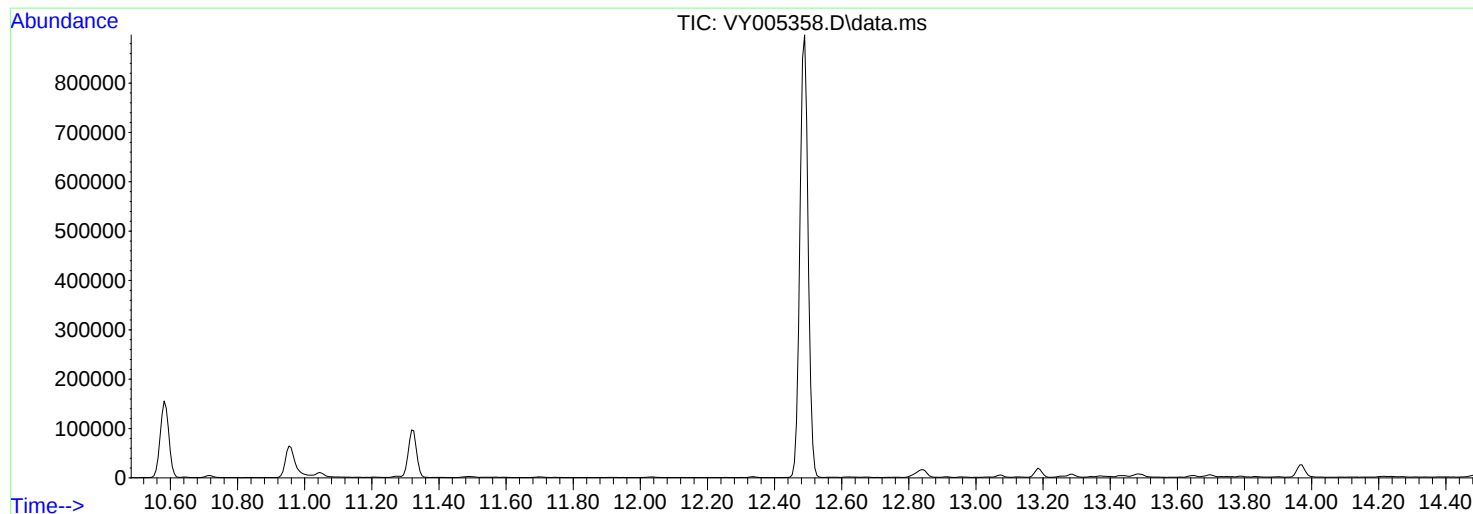

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	23112	PASS
75	95	30	60	51.0	63499	PASS
95	95	100	100	100.0	124608	PASS
96	95	5	9	7.2	8922	PASS
173	174	0.00	2	1.1	1236	PASS
174	95	50	100	93.8	116891	PASS
175	174	5	9	7.6	8899	PASS
176	174	95	101	97.7	114248	PASS
177	176	5	9	7.7	8832	PASS