


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\vv070820\
 Data File : VY003133.D
 Acq On : 08 Jul 2020 11:23
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y062920S.M
 Title : SW846 8260
 Last Update : Tue Jun 30 04:11:35 2020

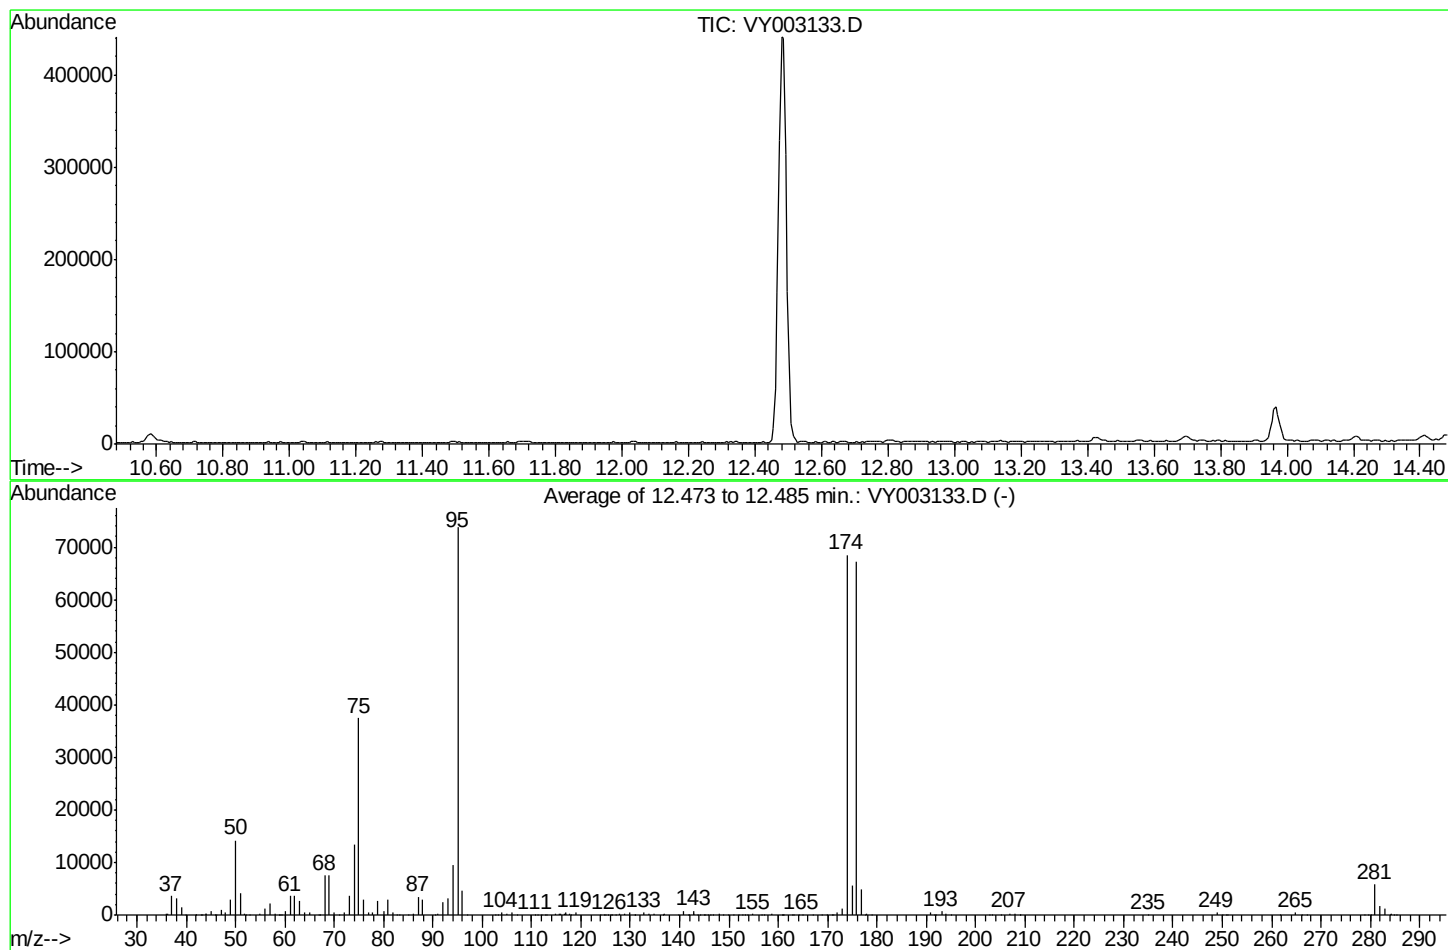

AutoFind: Scans 1761, 1762, 1763; Background Corrected with Scan 1753

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	14140	PASS
75	95	30	60	50.7	37410	PASS
95	95	100	100	100.0	73760	PASS
96	95	5	9	6.3	4658	PASS
173	174	0.00	2	1.8	1205	PASS
174	95	50	100	92.9	68552	PASS
175	174	5	9	8.1	5532	PASS
176	174	95	101	98.0	67208	PASS
177	176	5	9	7.1	4792	PASS