


Dichlorodifluoromethane

Response Ratio

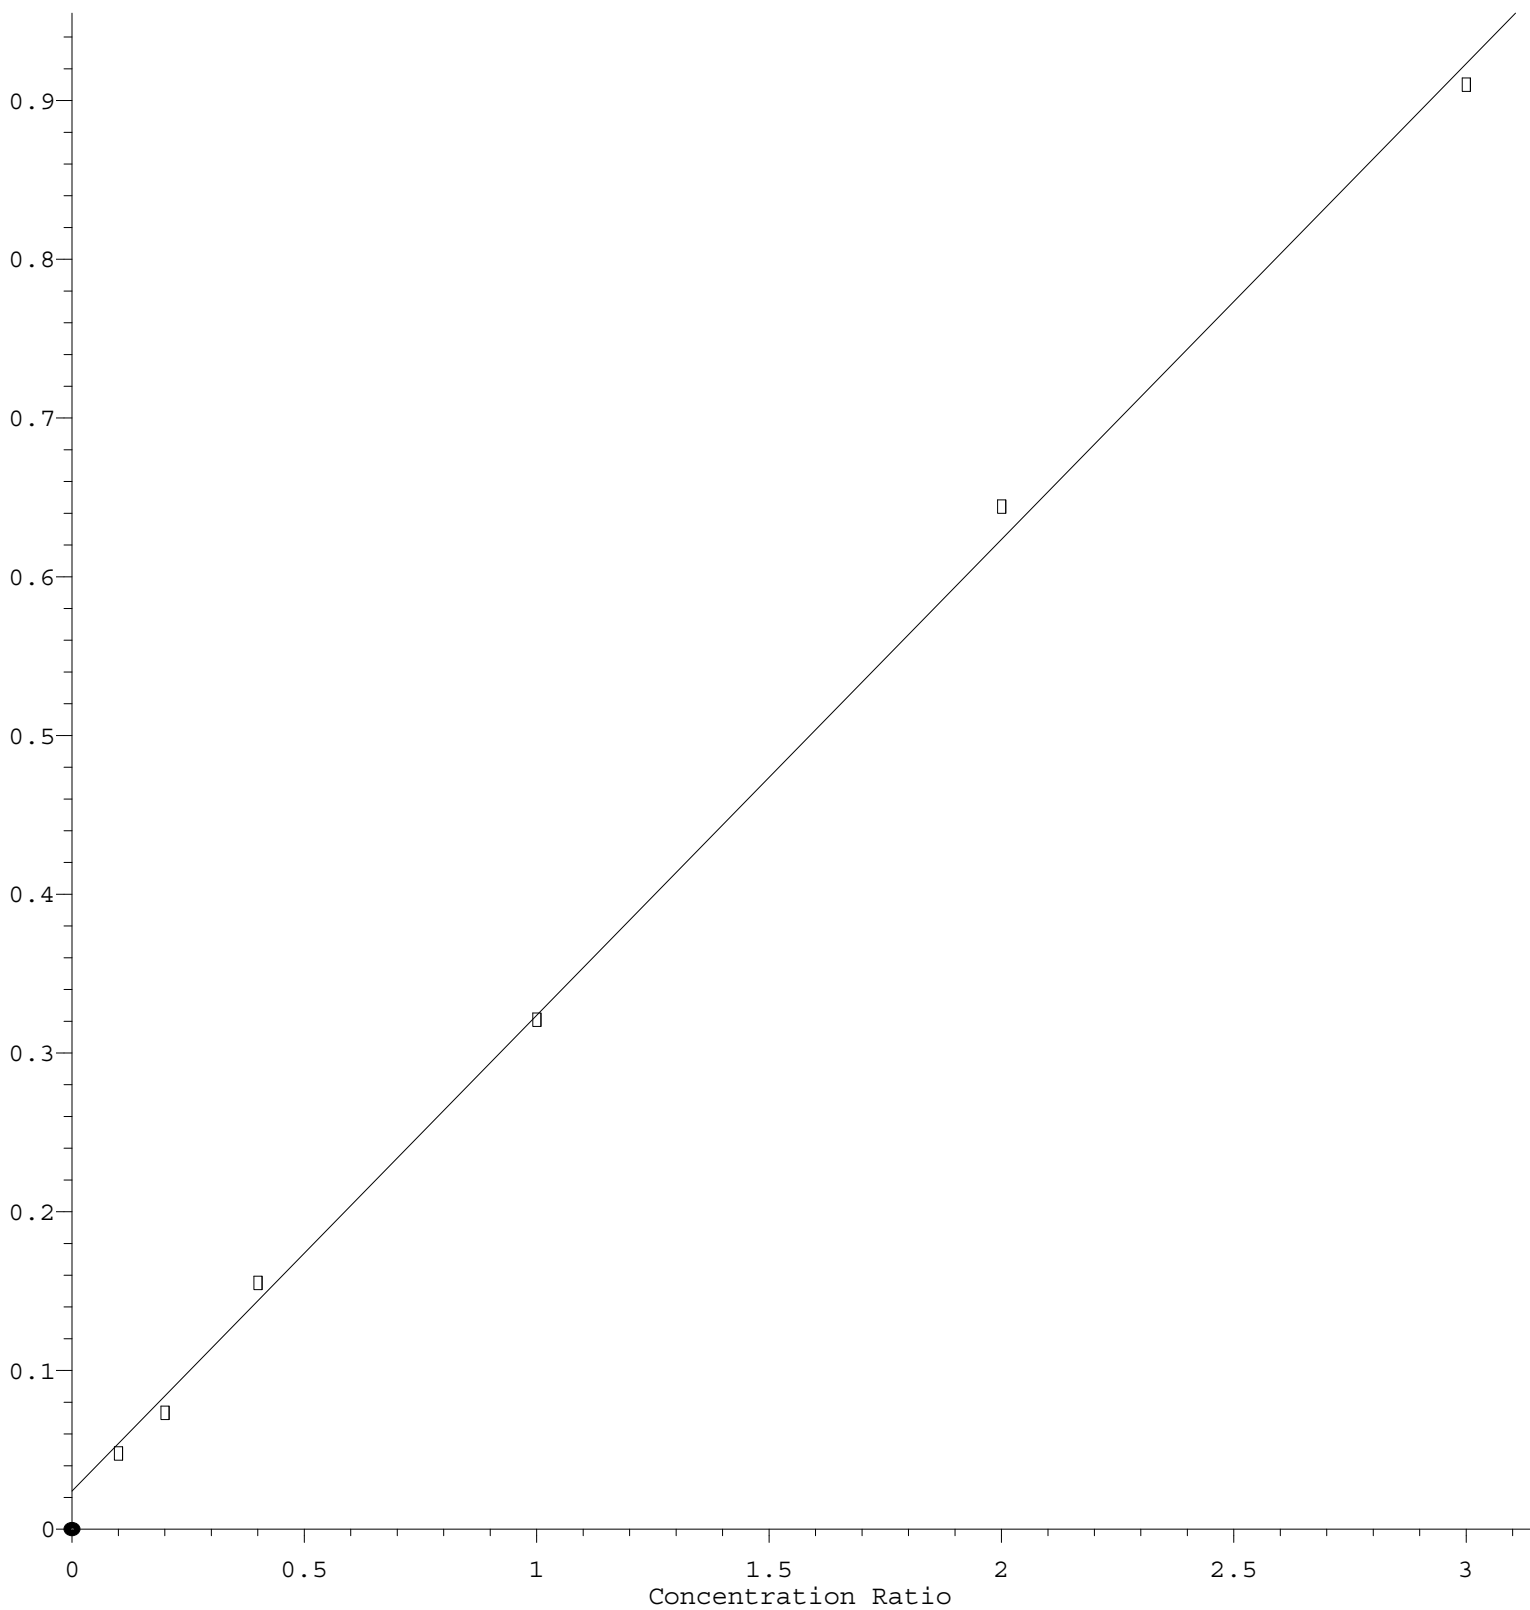

$$\text{Response} = 3.000\text{e-}001 * \text{Amt} + 2.352\text{e-}002$$


Coef of Det (r^2) = 0.998532 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y070821S.M

Calibration Table Last Updated: Fri Jul 09 07:16:38 2021

Bromomethane

Response Ratio

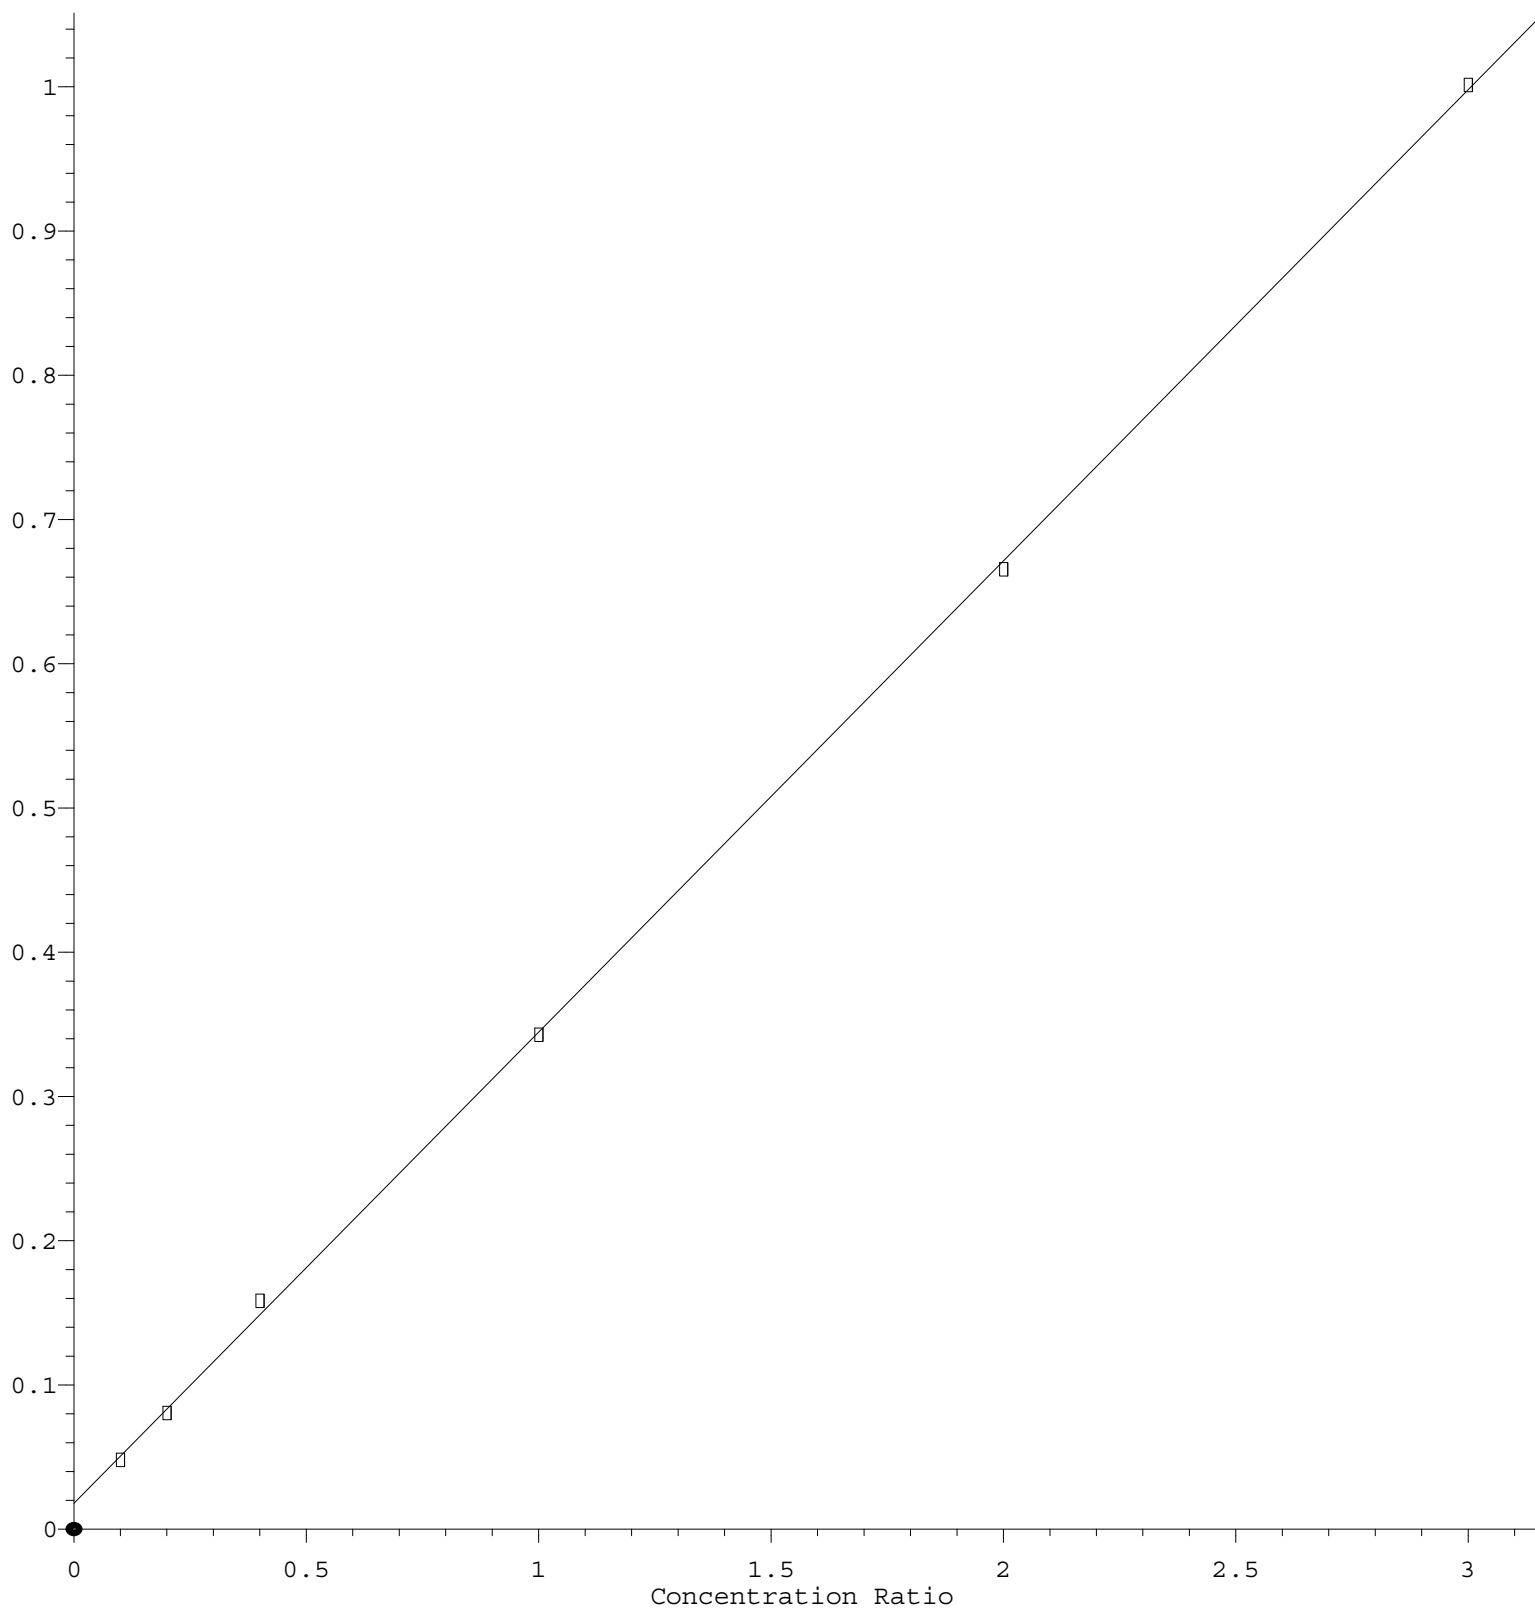


$$\text{Response} = 3.266\text{e-}001 * \text{Amt} + 1.802\text{e-}002$$

Coef of Det (r^2) = 0.999783 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y070821S.M

Calibration Table Last Updated: Fri Jul 09 07:16:38 2021

Methyl Acetate

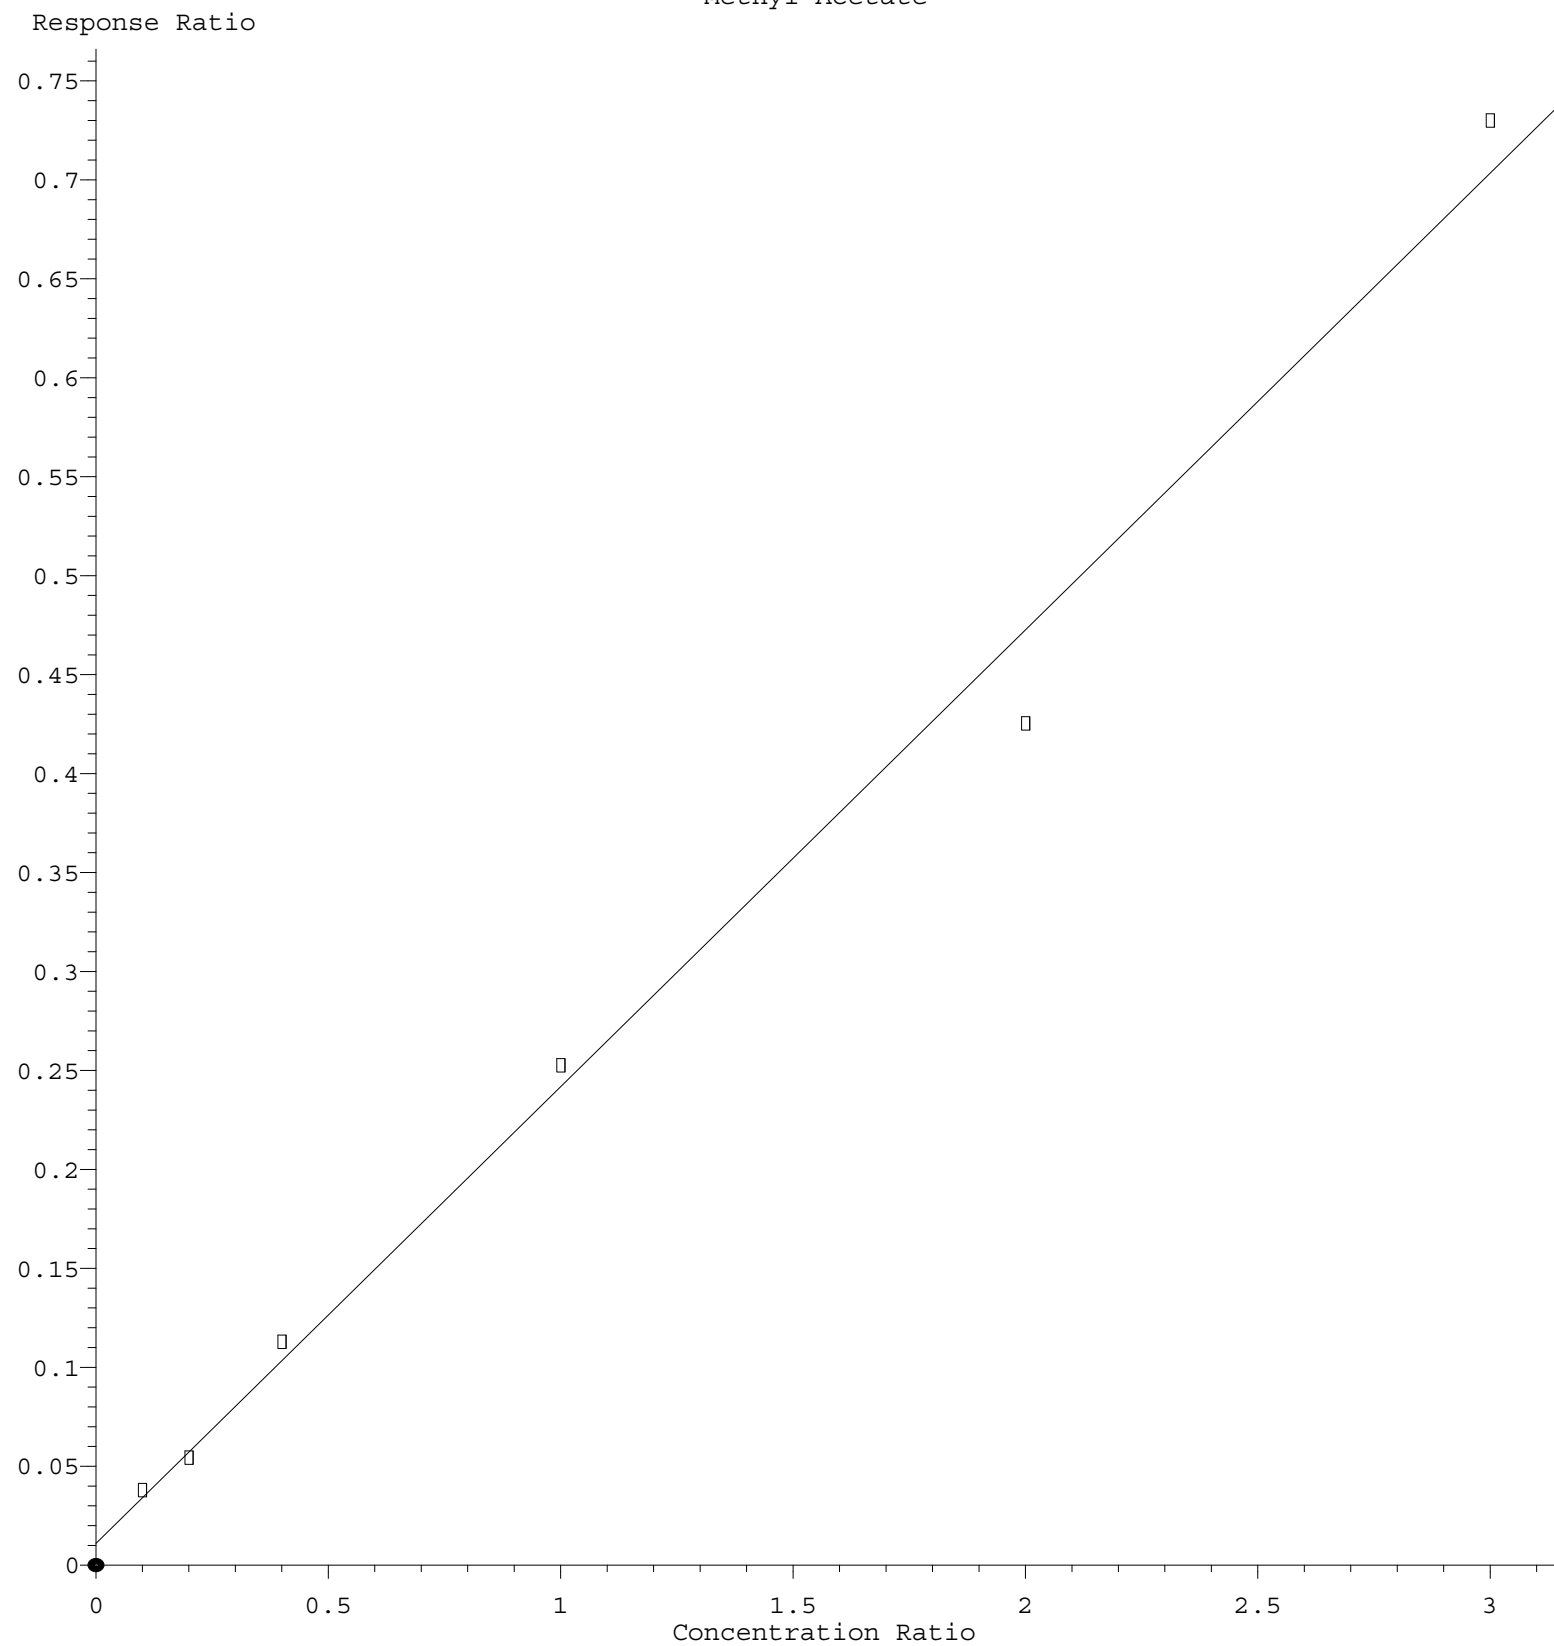

Response = 2.307e-001 * Amt + 1.126e-002
Coef of Det (r^2) = 0.991227 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y070821S.M
Calibration Table Last Updated: Fri Jul 09 07:16:38 2021