


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\vv070920\
 Data File : VY003140.D
 Acq On : 09 Jul 2020 09:57
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y062920S.M
 Title : SW846 8260
 Last Update : Tue Jun 30 04:11:35 2020

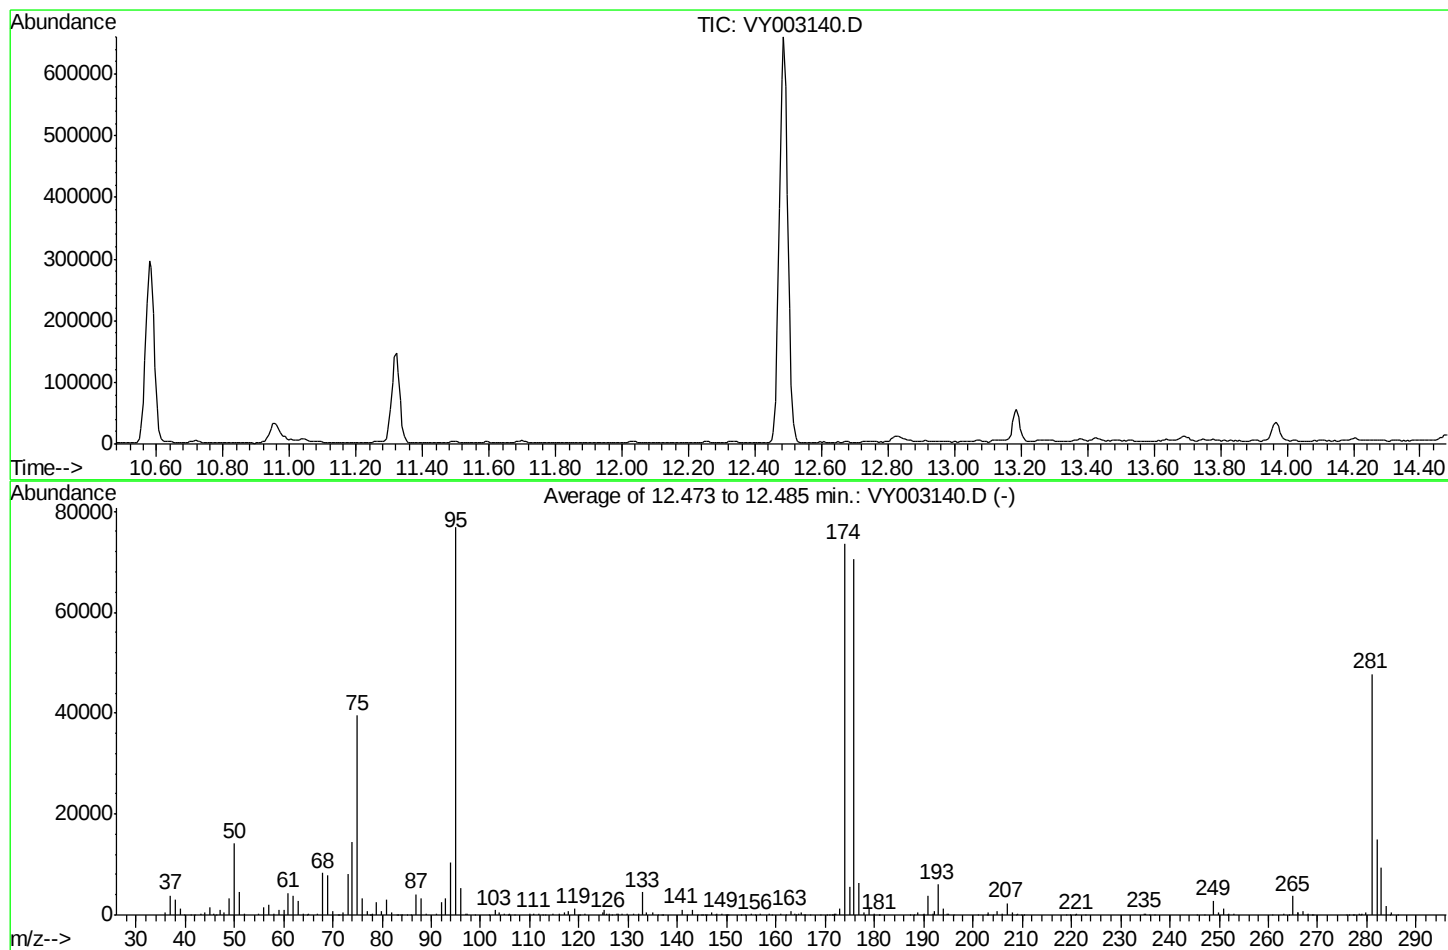

AutoFind: Scans 1761, 1762, 1763; Background Corrected with Scan 1751

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	14146	PASS
75	95	30	60	51.4	39464	PASS
95	95	100	100	100.0	76829	PASS
96	95	5	9	6.8	5216	PASS
173	174	0.00	2	1.6	1198	PASS
174	95	50	100	95.7	73517	PASS
175	174	5	9	7.7	5664	PASS
176	174	95	101	95.9	70522	PASS
177	176	5	9	9.0	6343	PASS