

Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY071020\
 Data File : VY003163.D
 Acq On : 10 Jul 2020 15:11
 Operator : SY/MD
 Sample : VY0710SBL01
 Misc : 5.00G/5ML/MSVOA Y/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0710SBL01

Quant Time: Jul 11 06:18:25 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y071020S.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 10 13:18:03 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.80	168	485989	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.69	114	712939	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.49	117	652979	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.42	152	334901	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.14	65	197173	48.07	ug/l	0.00
Spiked Amount	50.000		Recovery	=	96.14%	
35) Dibromofluoromethane	7.72	113	193925	47.27	ug/l	0.00
Spiked Amount	50.000		Recovery	=	94.54%	
50) Toluene-d8	10.18	98	715461	46.90	ug/l	0.00
Spiked Amount	50.000		Recovery	=	93.80%	
62) 4-Bromofluorobenzene	12.48	95	252001	45.73	ug/l	0.00
Spiked Amount	50.000		Recovery	=	91.46%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA Y\DATA\VY071020\
Data File : VY003163.D
Acq On : 10 Jul 2020 15:11
Operator : SY/MD
Sample : VY0710SBL01
Misc : 5.00G/5ML/MSVOA Y/SOIL
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY0710SBL01

Quant Time: Jul 11 06:18:25 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_Y\METHODS\82Y071020S.M
Quant Title : SW846 8260
QLast Update : Fri Jul 10 13:18:03 2020
Response via : Initial Calibration

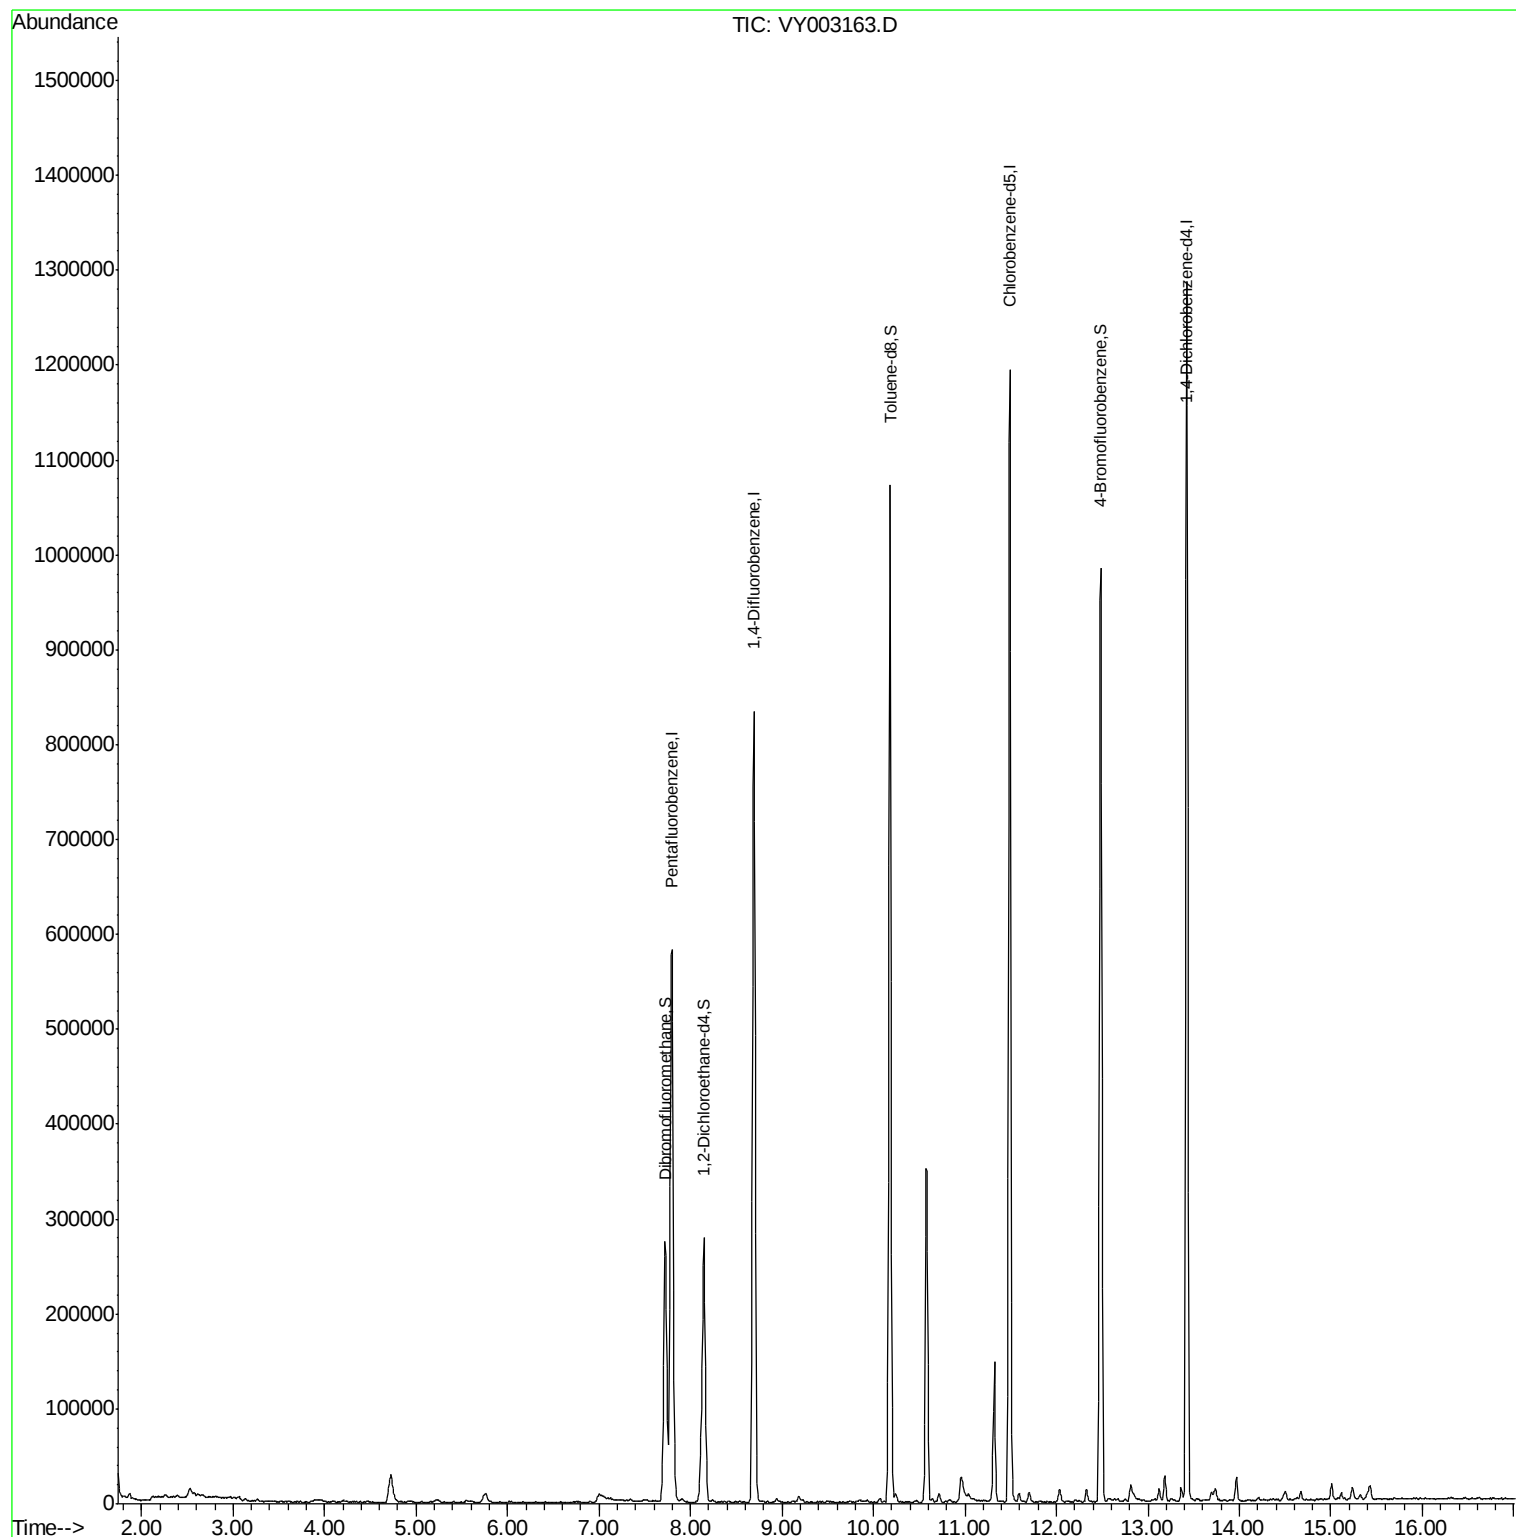

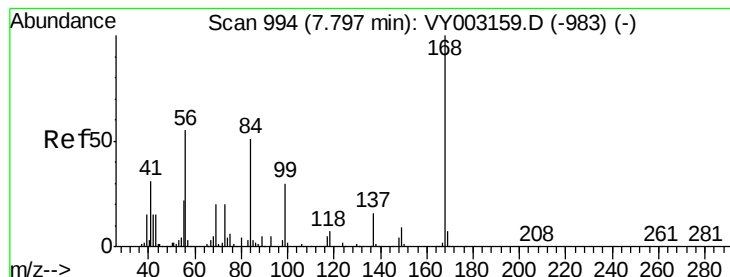

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.80 min Scan# 994

Delta R.T. 0.00 min

Lab File: VY003163.D

Acq: 10 Jul 2020 15:11

Instrument :

MSVOA_Y

ClientSampleId :


VY0710SBL01

Tot Ion:168 Resp: 485989

Ion Ratio Lower Upper

168 100

99 49.2 37.3 55.9

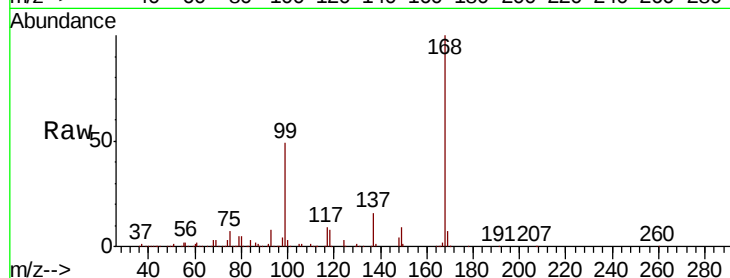

Abundance Ion 167.90 (167.60 to 168.60): VY003159.D (-983) (-)

Ion 98.90 (98.60 to 99.60): VY003159.D (-983) (-)

7.80

200000



150000

100000

50000

0

Time-->

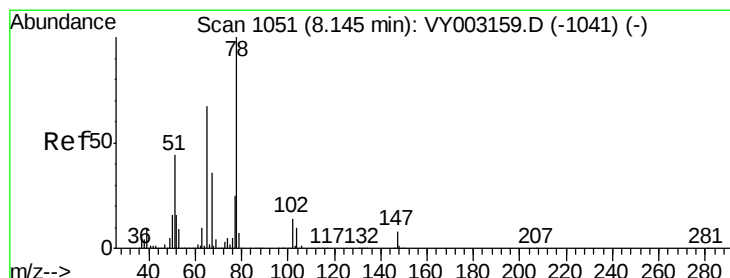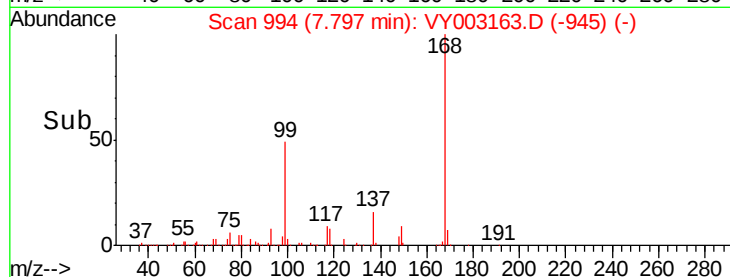

#33

1,2-Dichloroethane-d4

Concen: 48.069 ug/l

RT: 8.14 min Scan# 1051

Delta R.T. 0.00 min

Lab File: VY003163.D


Acq: 10 Jul 2020 15:11

Tgt Ion: 65 Resp: 197173

Ion Ratio Lower Upper

65 100

67 52.9 0.0 105.2

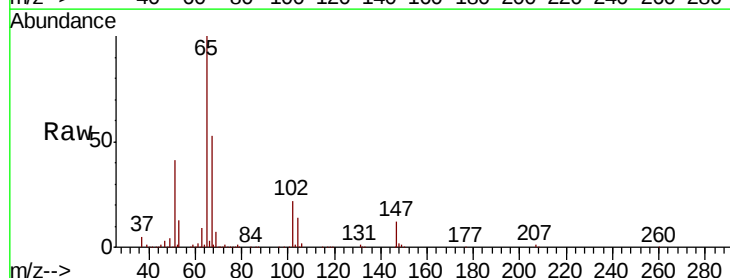

Abundance Ion 64.90 (64.60 to 65.60): VY003159.D (-1041) (-)

Ion 66.90 (66.60 to 67.60): VY003159.D (-1041) (-)

8.14

100000

80000


60000


40000

20000

0

Time-->




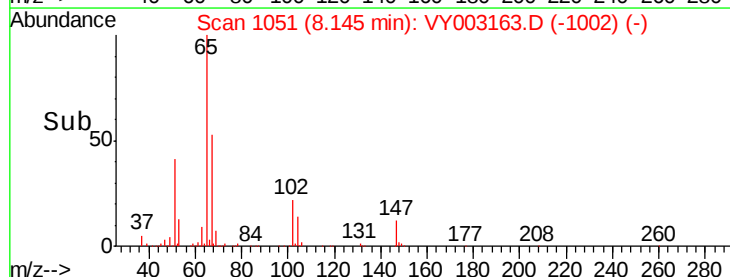


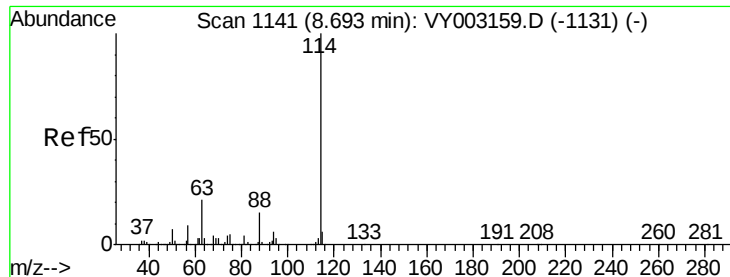

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.69 min Scan# 1141
 Delta R.T. 0.00 min
 Lab File: VY003163.D
 Acq: 10 Jul 2020 15:11




Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0710SBL01


Tot Ion	Ratio	Lower	Upper
114	100		
63	19.2	0.0	41.2
88	14.7	0.0	30.2

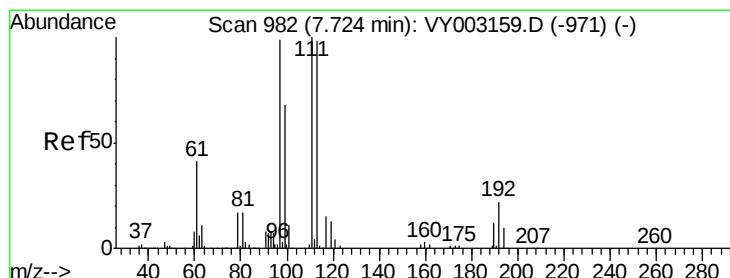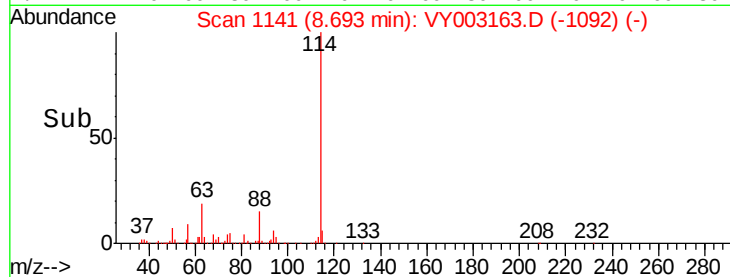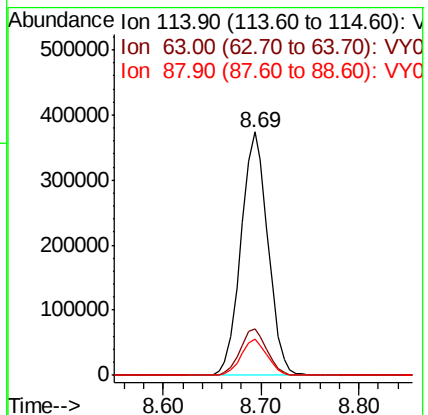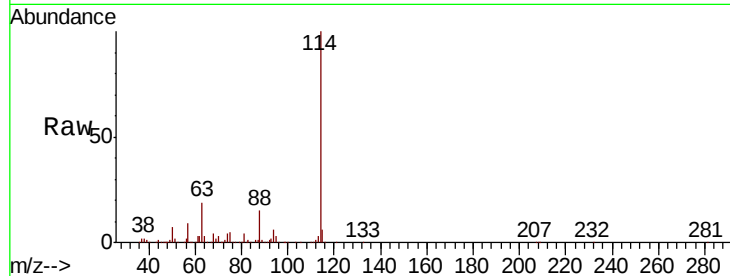

#35
 Dibromofluoromethane
 Concen: 47.267 ug/l
 RT: 7.72 min Scan# 982
 Delta R.T. 0.00 min
 Lab File: VY003163.D
 Acq: 10 Jul 2020 15:11

Tgt Ion	Ratio	Lower	Upper
113	100		
111	102.6	82.1	123.1
192	23.7	18.8	28.2

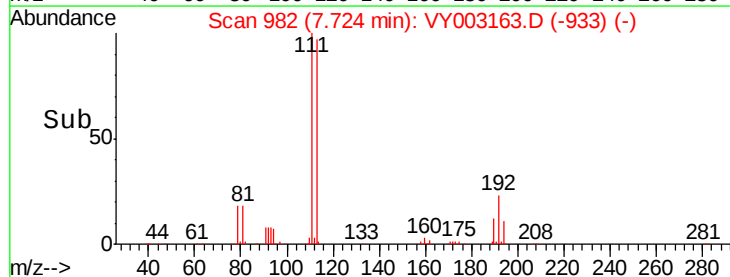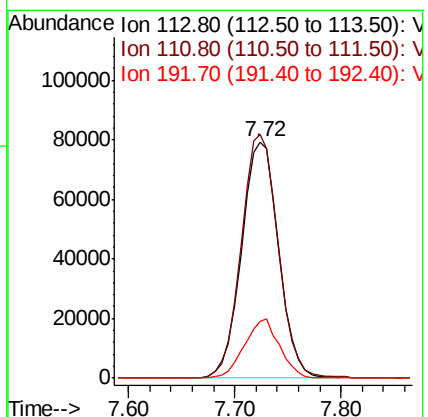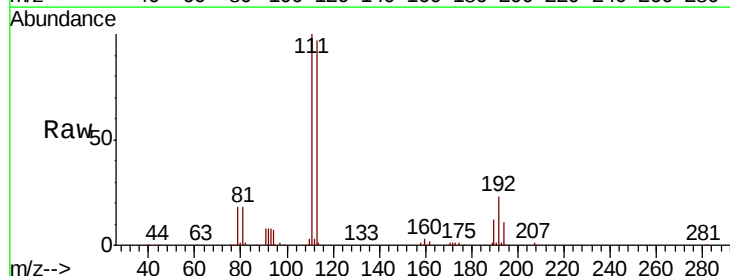

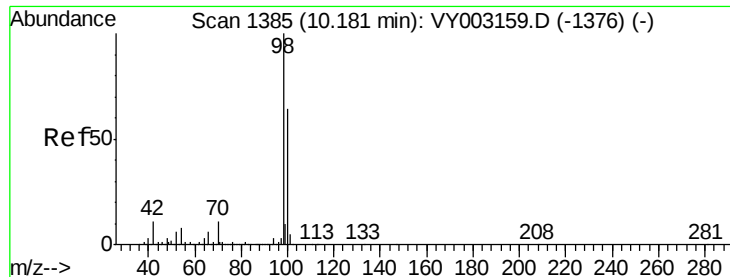

#50

Toluene-d8

Concen: 46.905 ug/l

RT: 10.18 min Scan# 1385

Delta R.T. 0.00 min

Lab File: VY003163.D

Acq: 10 Jul 2020 15:11

Instrument :

MSVOA_Y

ClientSampleId :





VY0710SBL01

Tot Ion: 98 Resp: 715461

Ion Ratio Lower Upper

98 100

100 63.8 50.7 76.1

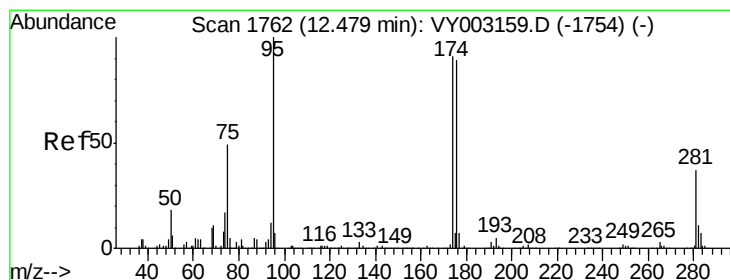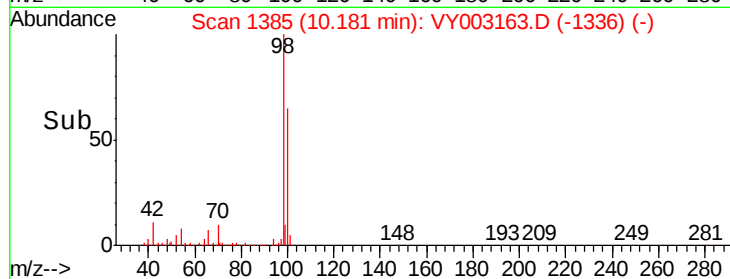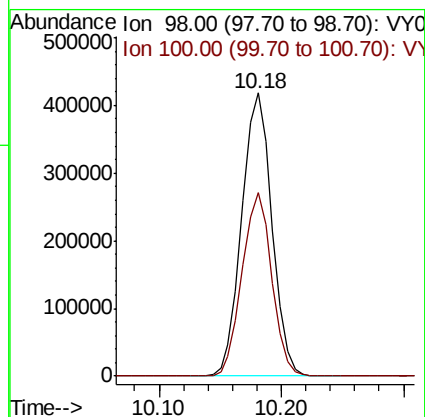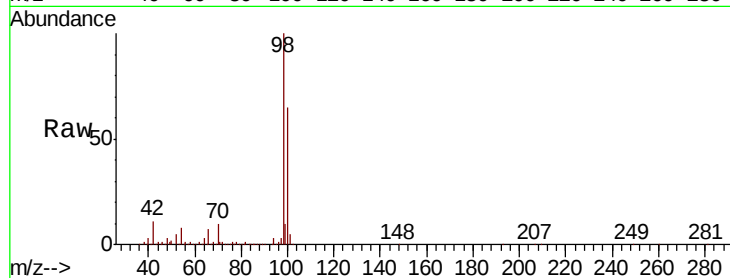

#62

4-Bromofluorobenzene

Concen: 45.731 ug/l

RT: 12.48 min Scan# 1762

Delta R.T. 0.00 min

Lab File: VY003163.D

Acq: 10 Jul 2020 15:11




Tgt Ion: 95 Resp: 252001


Ion Ratio Lower Upper

95 100

174 96.1 0.0 190.6

176 93.2 0.0 186.4

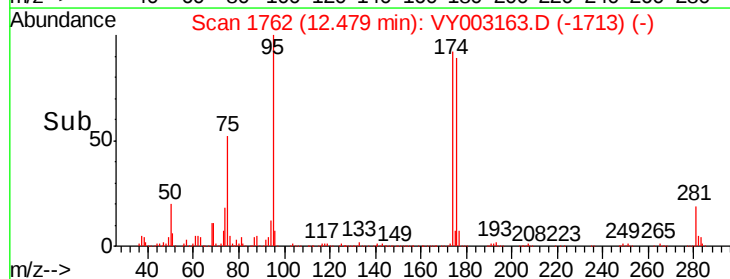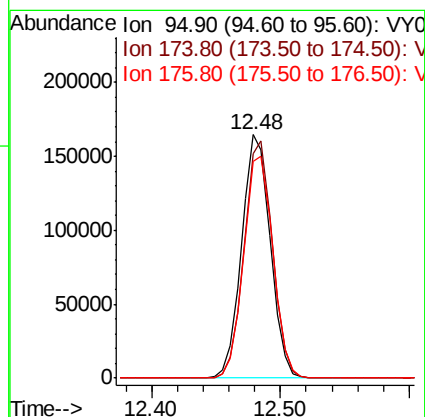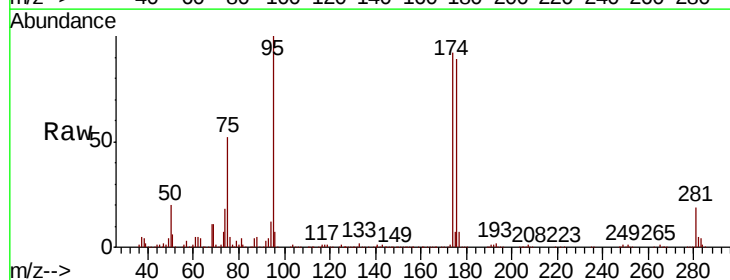


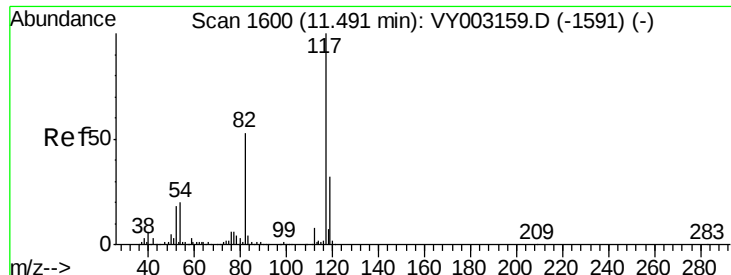




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.49 min Scan# 1600
Delta R.T. 0.00 min
Lab File: VY003163.D
Acq: 10 Jul 2020 15:11

Instrument :
MSVOA_Y
ClientSampleId :
VY0710SBL01

Tot Ion	Ratio	Lower	Upper
117	100		
82	51.7	42.0	63.0
119	32.0	25.5	38.3

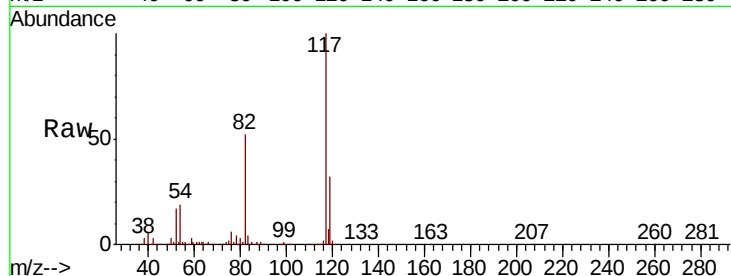


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VY0
Ion 118.90 (118.60 to 119.60): V

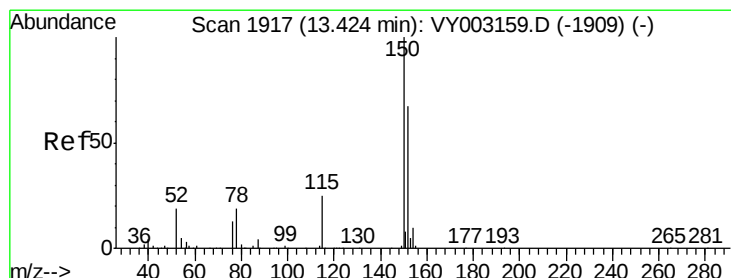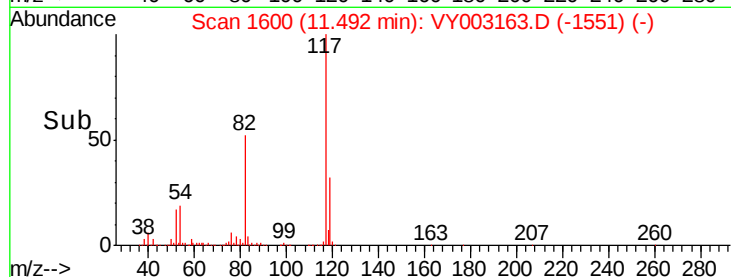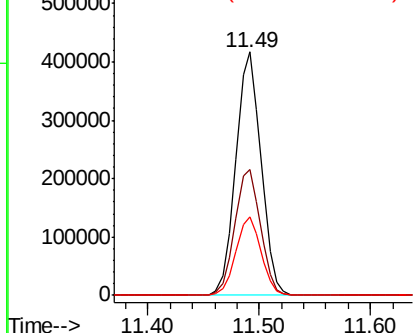

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.42 min Scan# 1917
Delta R.T. 0.00 min
Lab File: VY003163.D
Acq: 10 Jul 2020 15:11

Tgt Ion	Ratio	Lower	Upper
152	100		
115	55.1	26.9	80.7
150	156.6	0.0	338.0

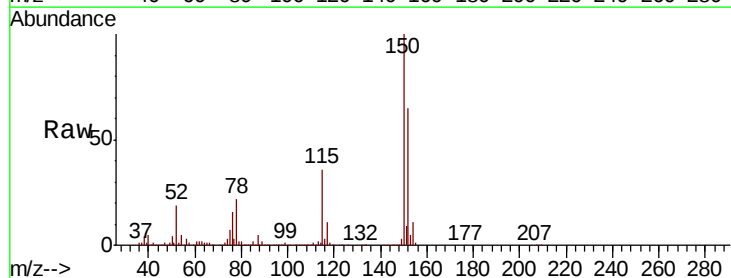

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

