


Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY071020\
Data File : VY003155.D
Acq On : 10 Jul 2020 10:09
Operator : SY/MD
Sample : BFB
Misc : 5.00G/5ML/MSVOA Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y071020S.M
Title : SW846 8260
Last Update : Fri Jul 10 13:18:03 2020

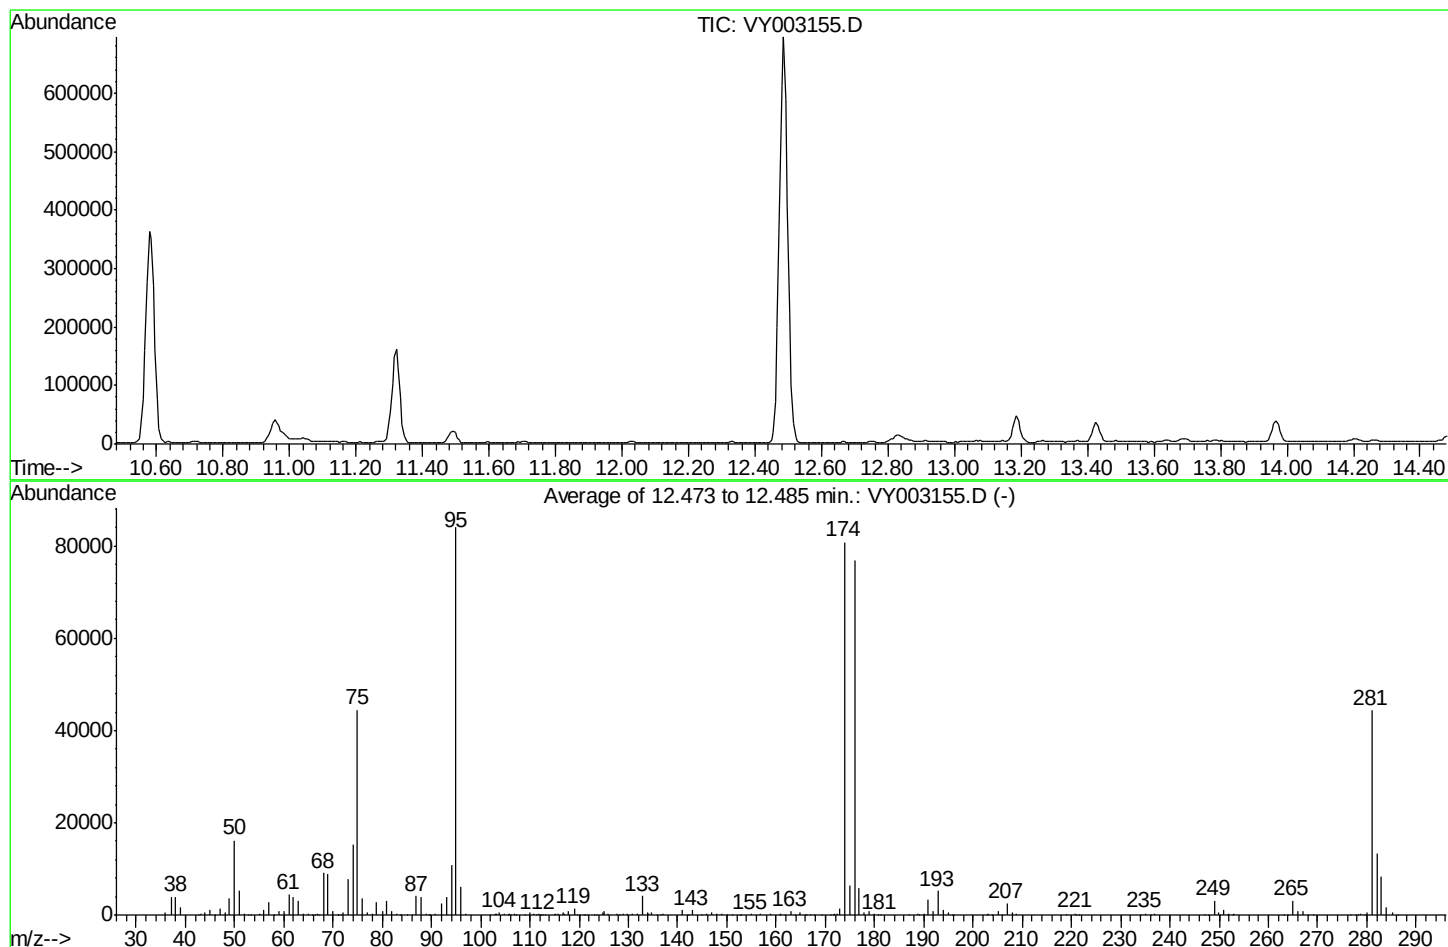

AutoFind: Scans 1761, 1762, 1763; Background Corrected with Scan 1753

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	16170	PASS
75	95	30	60	52.8	44413	PASS
95	95	100	100	100.0	84061	PASS
96	95	5	9	7.2	6053	PASS
173	174	0.00	2	1.8	1451	PASS
174	95	50	100	96.2	80877	PASS
175	174	5	9	8.1	6519	PASS
176	174	95	101	95.1	76888	PASS
177	176	5	9	7.8	5961	PASS