

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY071023\  
 Data File : VY014615.D  
 Acq On : 10 Jul 2023 14:06  
 Operator : SY/MD  
 Sample : 03555-01RE  
 Misc : 5.05g/5.0mL/MSVOA\_Y/SOIL  
 ALS Vial : 10 Sample Multiplier: 1

Instrument :  
 MSVOA\_Y  
 ClientSampleId :  
 ETGI-330RE

Quant Time: Jul 11 03:18:42 2023  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y063023S.M  
 Quant Title : SW846 8260  
 QLast Update : Fri Jun 30 19:02:11 2023  
 Response via : Initial Calibration

| Compound                   | R.T.   | QIon | Response | Conc   | Units | Dev(Min) |
|----------------------------|--------|------|----------|--------|-------|----------|
| -----                      |        |      |          |        |       |          |
| Internal Standards         |        |      |          |        |       |          |
| 1) Pentafluorobenzene      | 7.789  | 168  | 83935    | 50.000 | ug/l  | 0.00     |
| 34) 1,4-Difluorobenzene    | 8.685  | 114  | 123567   | 50.000 | ug/l  | 0.00     |
| 63) Chlorobenzene-d5       | 11.490 | 117  | 110025   | 50.000 | ug/l  | 0.00     |
| 72) 1,4-Dichlorobenzene-d4 | 13.422 | 152  | 38008    | 50.000 | ug/l  | 0.00     |

|                             |        |       |          |          |      |          |
|-----------------------------|--------|-------|----------|----------|------|----------|
| System Monitoring Compounds |        |       |          |          |      |          |
| 33) 1,2-Dichloroethane-d4   | 8.136  | 65    | 44614    | 53.432   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 50 - 163 | Recovery | =    | 106.860% |
| 35) Dibromofluoromethane    | 7.716  | 113   | 44063    | 57.906   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 54 - 147 | Recovery | =    | 115.820% |
| 50) Toluene-d8              | 10.179 | 98    | 142757   | 47.458   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 58 - 134 | Recovery | =    | 94.920%  |
| 62) 4-Bromofluorobenzene    | 12.477 | 95    | 37439    | 35.843   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 30 - 143 | Recovery | =    | 71.680%  |


| Target Compounds | Qvalue |
|------------------|--------|
| -----            |        |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY071023\  
Data File : VY014615.D  
Acq On : 10 Jul 2023 14:06  
Operator : SY/MD  
Sample : 03555-01RE  
Misc : 5.05g/5.0mL/MSVOA\_Y/SOIL  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
MSVOA\_Y  
ClientSampleId :  
ETGI-330RE

Quant Time: Jul 11 03:18:42 2023  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y063023S.M  
Quant Title : SW846 8260  
QLast Update : Fri Jun 30 19:02:11 2023  
Response via : Initial Calibration




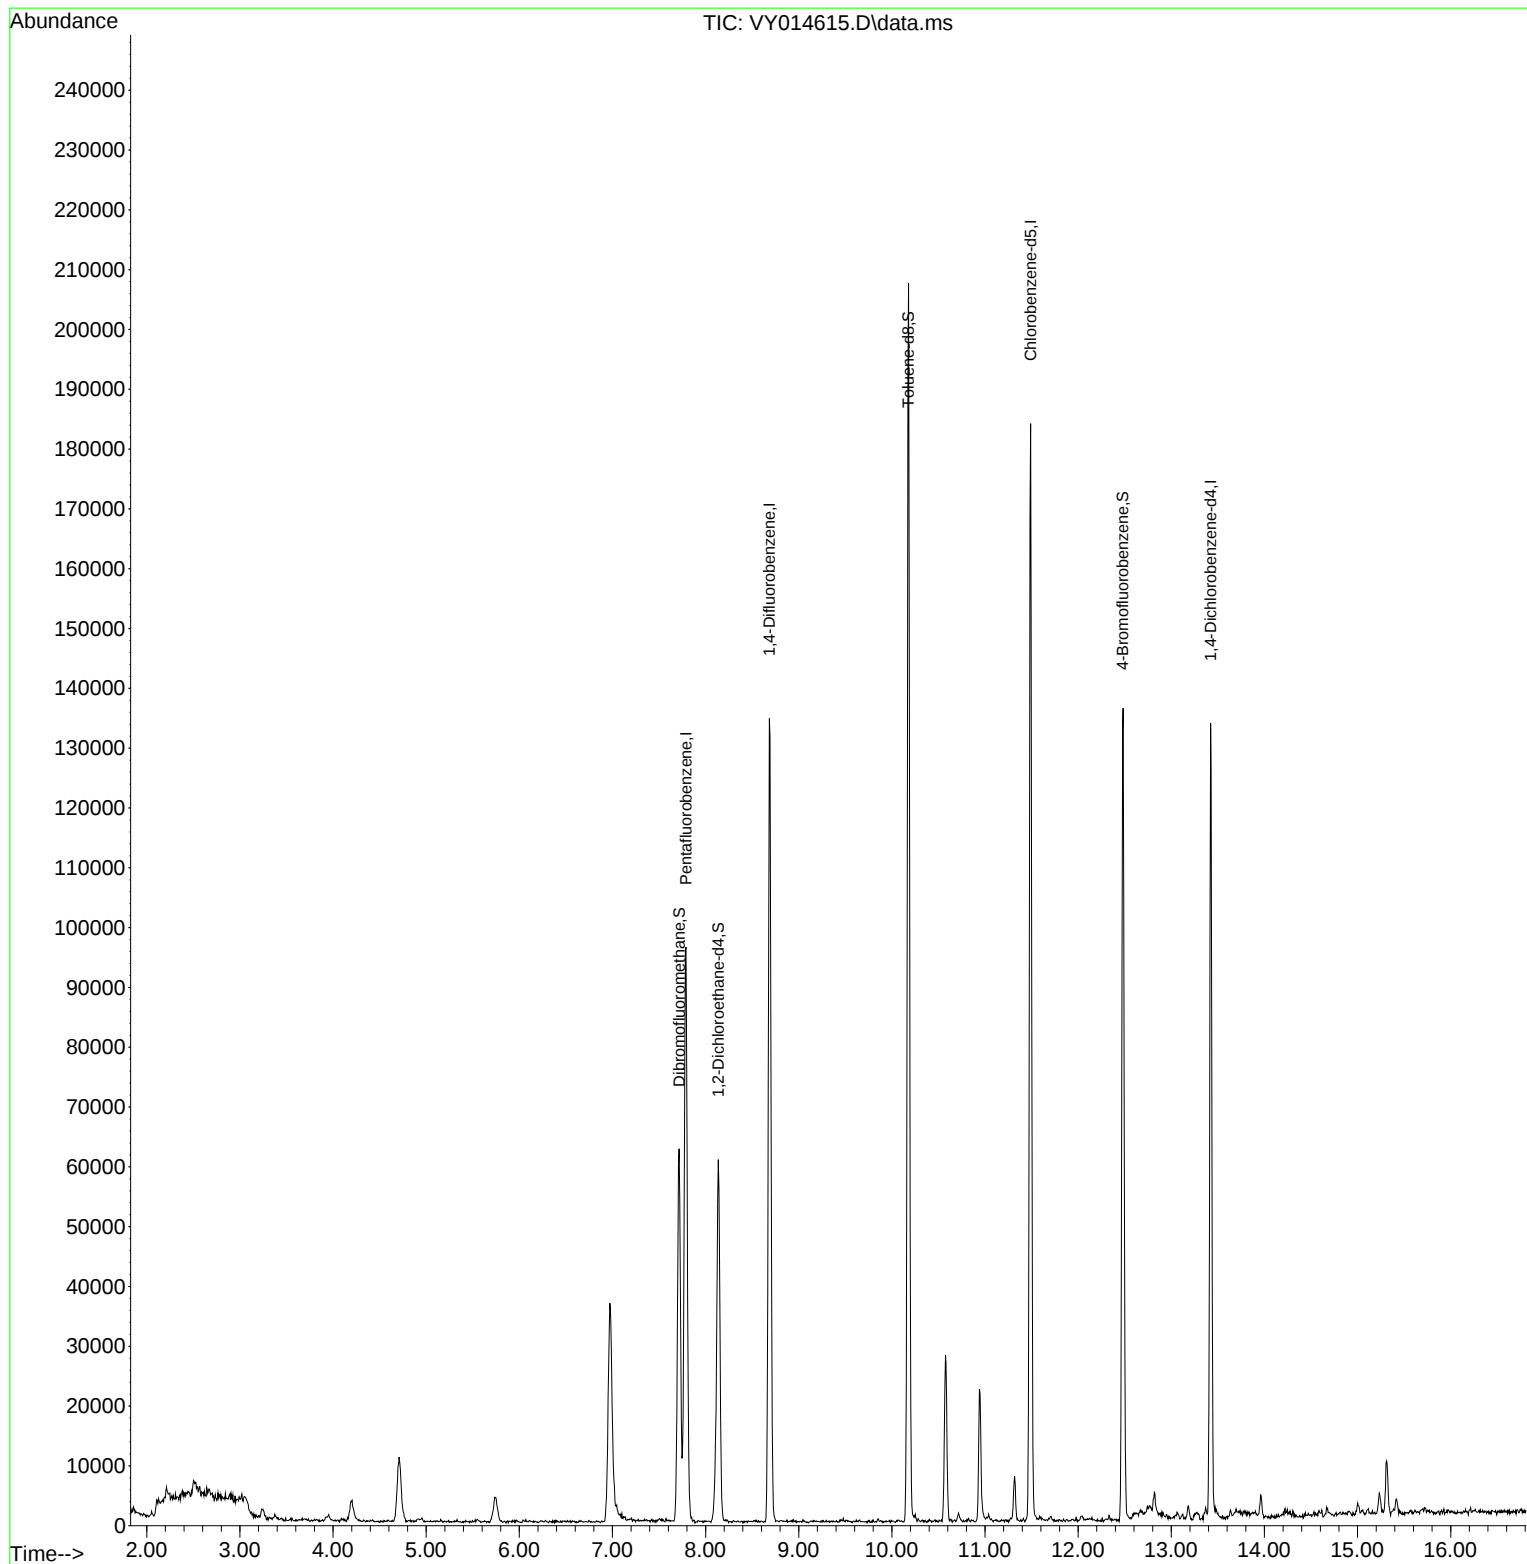




#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 7.789 min Scan# 91  
Delta R.T. -0.000 min  
Lab File: VY014615.D  
Acq: 10 Jul 2023 14:06




Instrument :  
MSVOA\_Y  
ClientSampleId :  
ETGI-330RE

Tgt Ion:168 Resp: 83935  
Ion Ratio Lower Upper  
168 100  
99 44.2 43.4 65.0

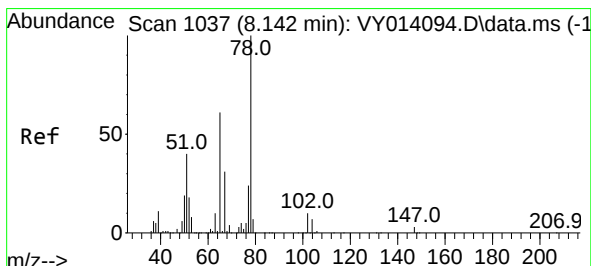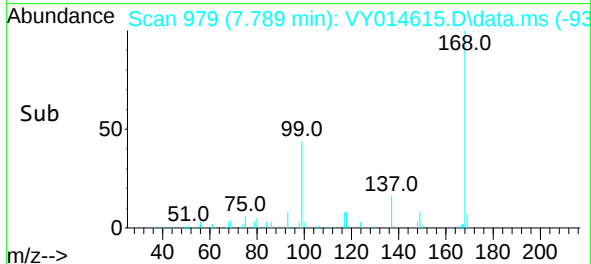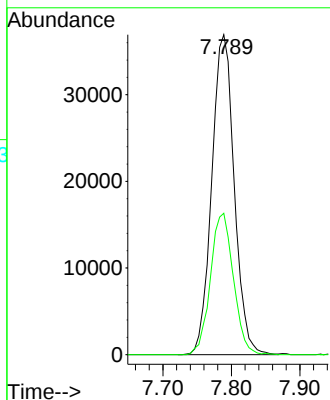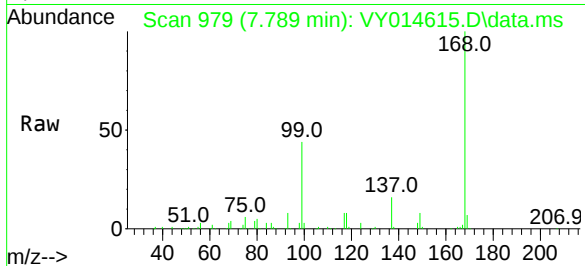

#33  
1,2-Dichloroethane-d4  
Concen: 53.432 ug/l  
RT: 8.136 min Scan# 1036  
Delta R.T. -0.006 min  
Lab File: VY014615.D  
Acq: 10 Jul 2023 14:06

Tgt Ion: 65 Resp: 44614  
Ion Ratio Lower Upper  
65 100  
67 55.3 0.0 101.8

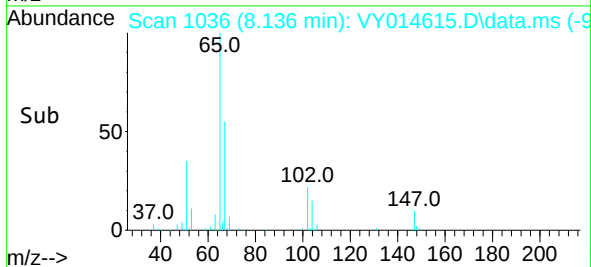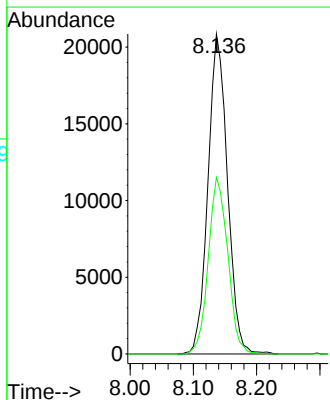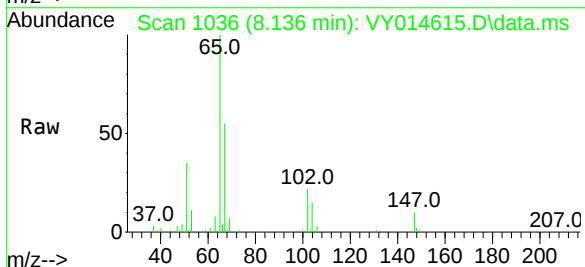



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.685 min Scan# 1126

Delta R.T. -0.006 min

Lab File: VY014615.D

Acq: 10 Jul 2023 14:06

Instrument :

MSVOA\_Y

ClientSampleId :

ETGI-330RE





Tgt Ion:114 Resp: 123567

Ion Ratio Lower Upper

114 100

63 18.1 0.0 42.4

88 14.2 0.0 30.6

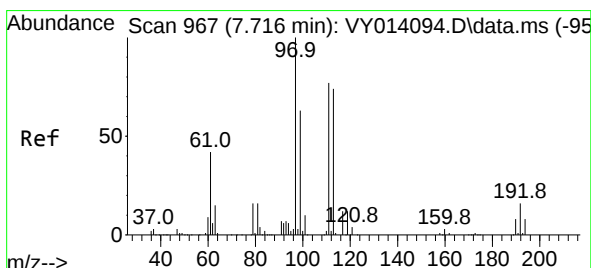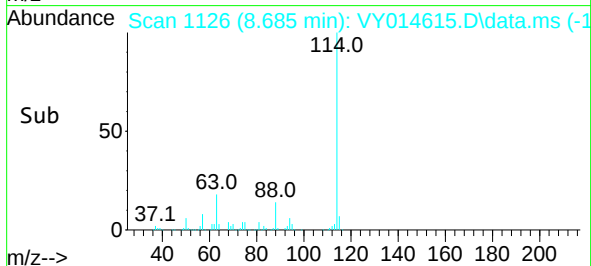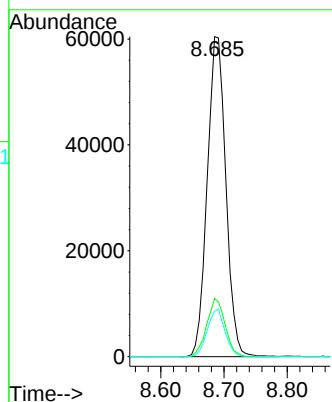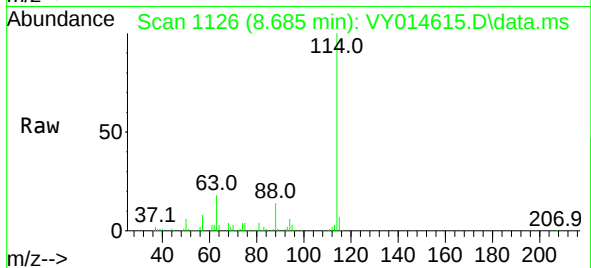

#35

Dibromofluoromethane

Concen: 57.906 ug/l

RT: 7.716 min Scan# 967

Delta R.T. -0.000 min

Lab File: VY014615.D

Acq: 10 Jul 2023 14:06




Tgt Ion:113 Resp: 44063


Ion Ratio Lower Upper

113 100

111 100.0 81.3 121.9

192 23.6 16.9 25.3


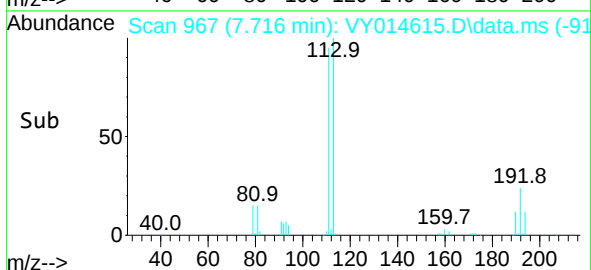
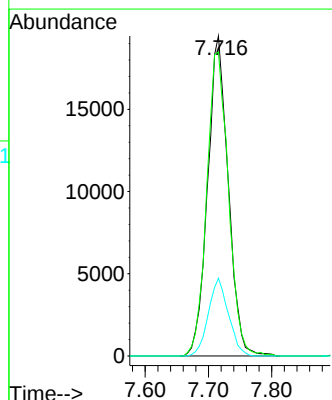
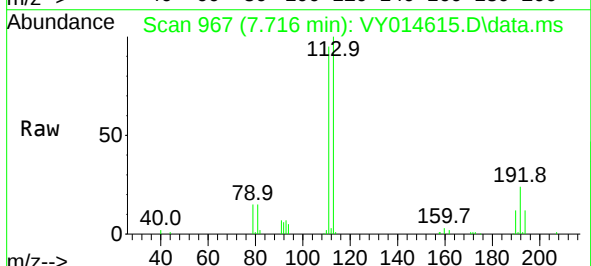


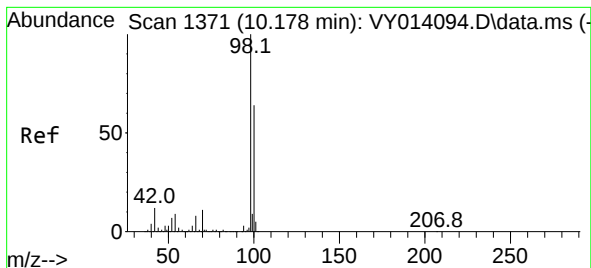

#50  
Toluene-d8  
Concen: 47.458 ug/l  
RT: 10.179 min Scan# 1371  
Delta R.T. 0.001 min  
Lab File: VY014615.D  
Acq: 10 Jul 2023 14:06




Instrument :  
MSVOA\_Y  
ClientSampleId :  
ETGI-330RE


Tgt Ion: 98 Resp: 142757  
Ion Ratio Lower Upper  
98 100  
100 62.4 50.1 75.1

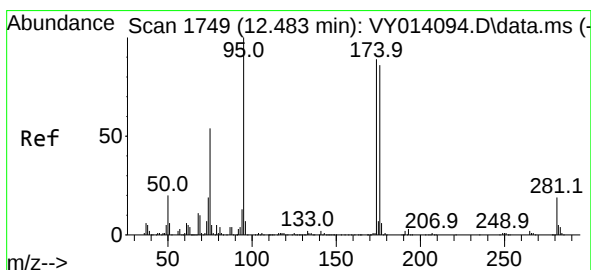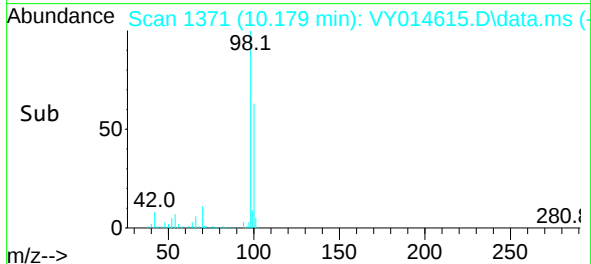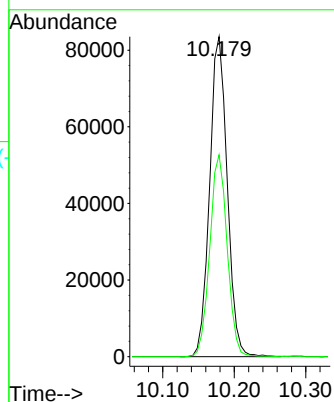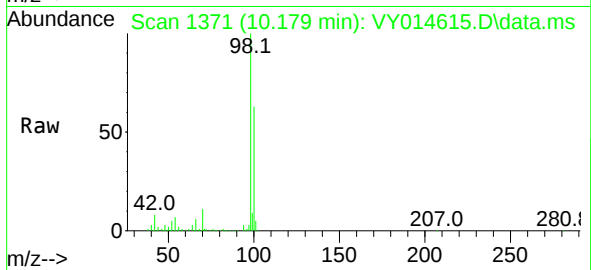

#62  
4-Bromofluorobenzene  
Concen: 35.843 ug/l  
RT: 12.477 min Scan# 1748  
Delta R.T. -0.006 min  
Lab File: VY014615.D  
Acq: 10 Jul 2023 14:06

Tgt Ion: 95 Resp: 37439  
Ion Ratio Lower Upper  
95 100  
174 101.7 0.0 178.2  
176 98.0 0.0 173.8

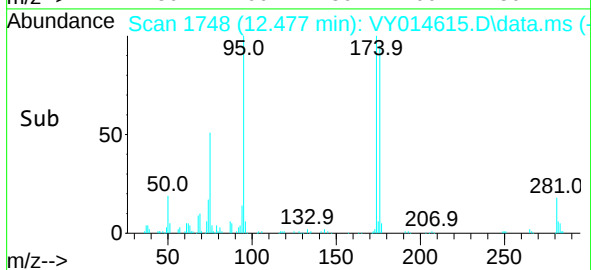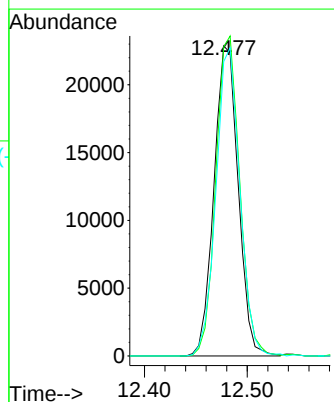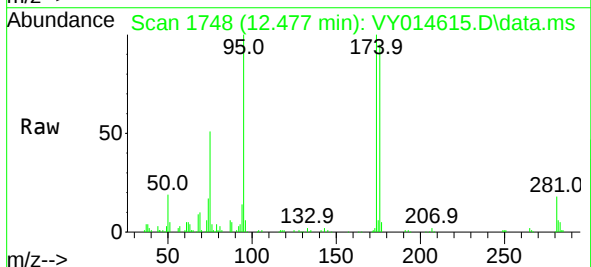

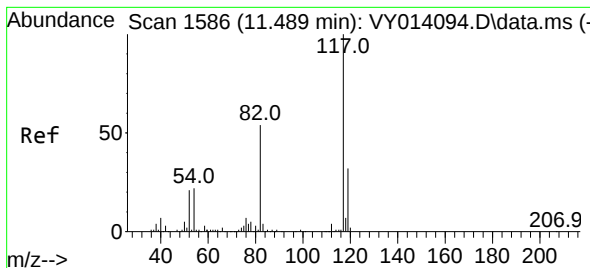

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.490 min Scan# 11

Delta R.T. 0.001 min

Lab File: VY014615.D

Acq: 10 Jul 2023 14:06

Instrument :

MSVOA\_Y

ClientSampleId :

ETGI-330RE





Tgt Ion:117 Resp: 110025

Ion Ratio Lower Upper

117 100

82 48.5 43.4 65.0

119 32.3 26.3 39.5

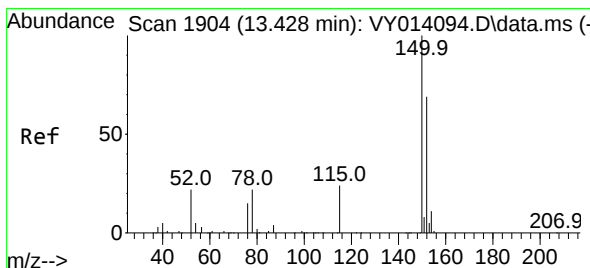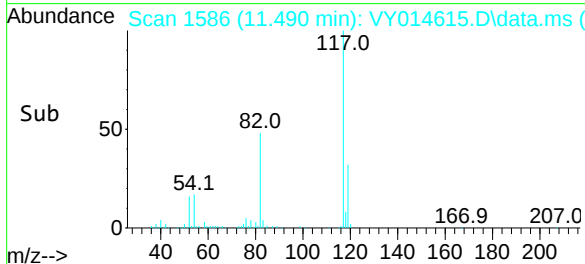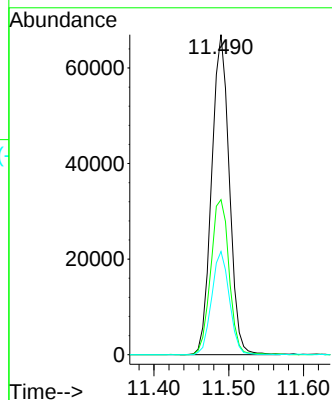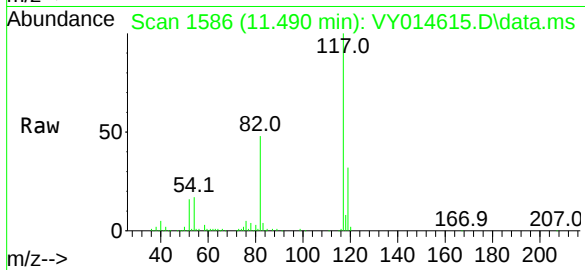

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.422 min Scan# 1903

Delta R.T. -0.006 min

Lab File: VY014615.D

Acq: 10 Jul 2023 14:06

Tgt Ion:152 Resp: 38008

Ion Ratio Lower Upper

152 100

115 52.5 28.8 86.5

150 155.0 0.0 348.8

