


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\vv071320\
Data File : VY003176.D
Acq On : 13 Jul 2020 09:32
Operator : SY/MD
Sample : BFB
Misc : 5.00G/5ML/MSVOA Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y071020S.M
Title : SW846 8260
Last Update : Fri Jul 10 13:18:03 2020

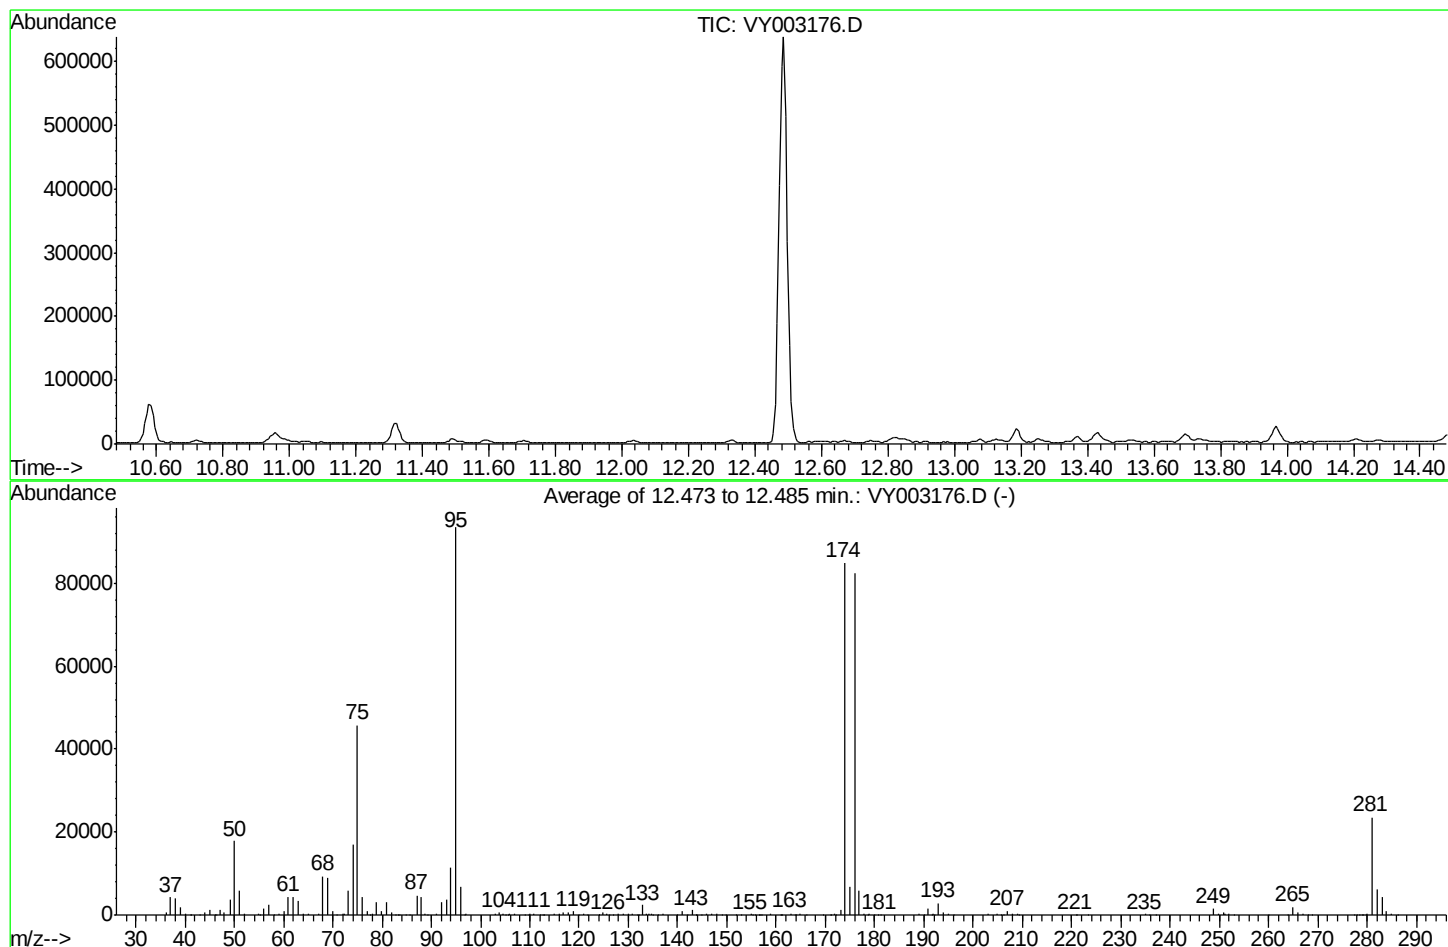

AutoFind: Scans 1761, 1762, 1763; Background Corrected with Scan 1754

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	17852	PASS
75	95	30	60	48.9	45730	PASS
95	95	100	100	100.0	93482	PASS
96	95	5	9	7.1	6679	PASS
173	174	0.00	2	1.5	1289	PASS
174	95	50	100	90.8	84922	PASS
175	174	5	9	8.0	6832	PASS
176	174	95	101	97.0	82384	PASS
177	176	5	9	7.3	6005	PASS