
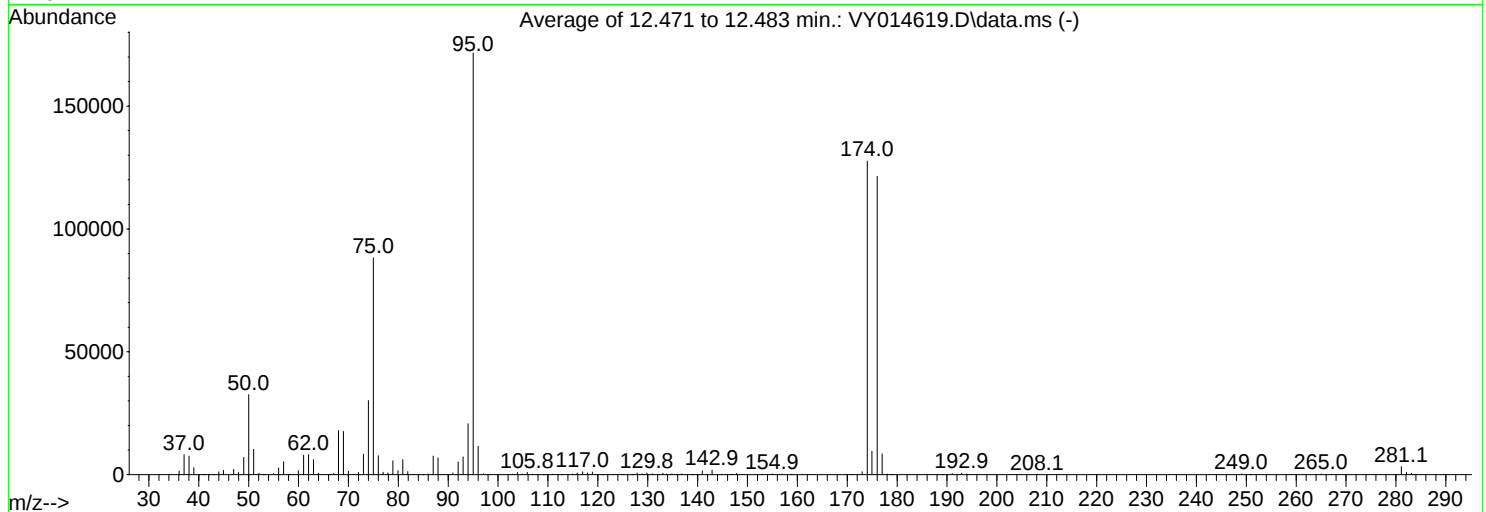


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY071323\
Data File : VY014619.D
Acq On : 13 Jul 2023 08:36
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y071323S.M
Title : SW846 8260
Last Update : Fri Jul 14 02:09:50 2023

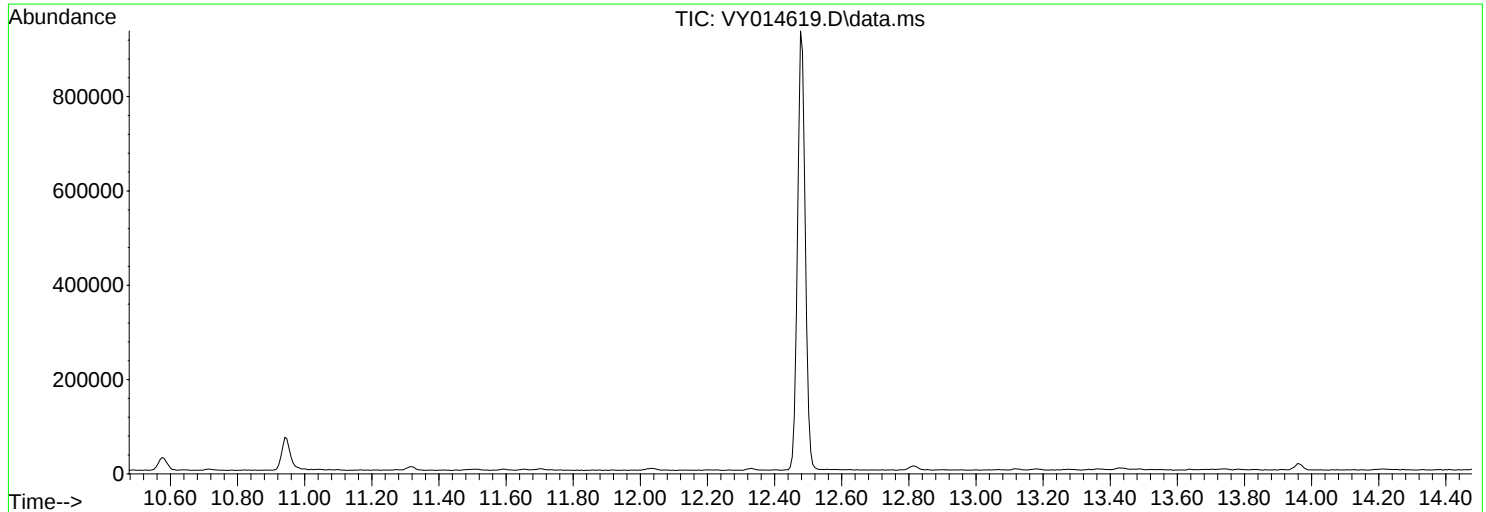

AutoFind: Scans 1747, 1748, 1749; Background Corrected with Scan 1738

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	32571	PASS
75	95	30	60	51.4	88243	PASS
95	95	100	100	100.0	171691	PASS
96	95	5	9	6.8	11611	PASS
173	174	0.00	2	0.9	1160	PASS
174	95	50	100	74.3	127627	PASS
175	174	5	9	7.4	9495	PASS
176	174	95	101	95.1	121429	PASS
177	176	5	9	7.0	8441	PASS