
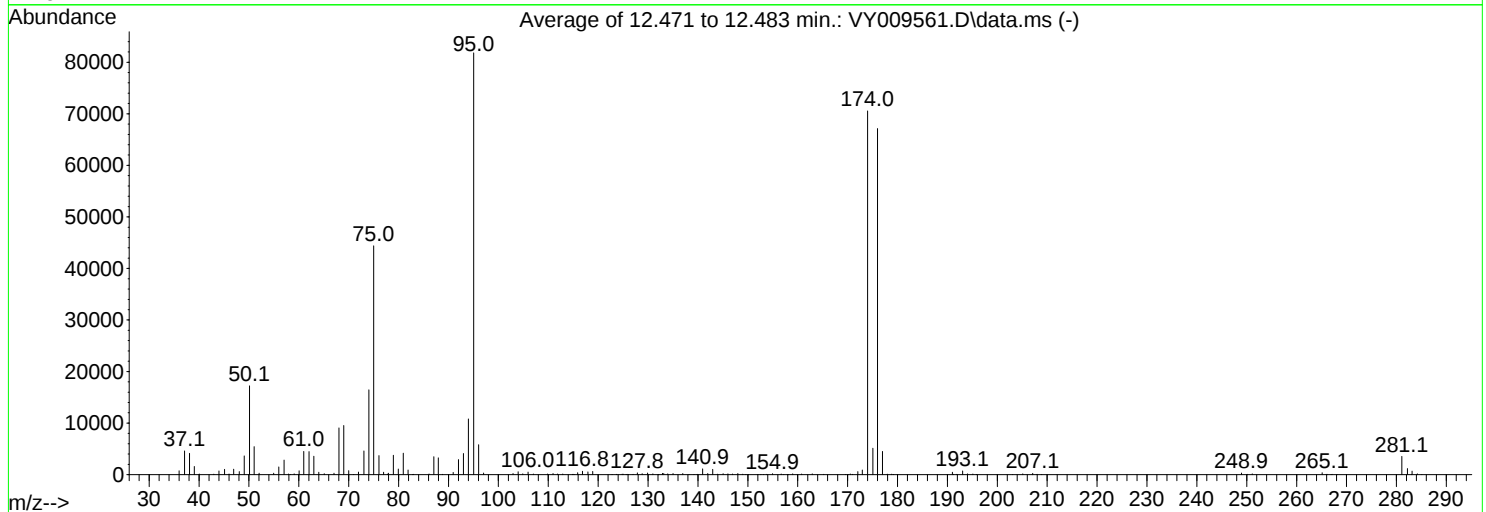


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY071422\
 Data File : VY009561.D
 Acq On : 14 Jul 2022 09:01
 Operator : KP/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y070722S.M
 Title : SW846 8260
 Last Update : Fri Jul 08 11:00:56 2022

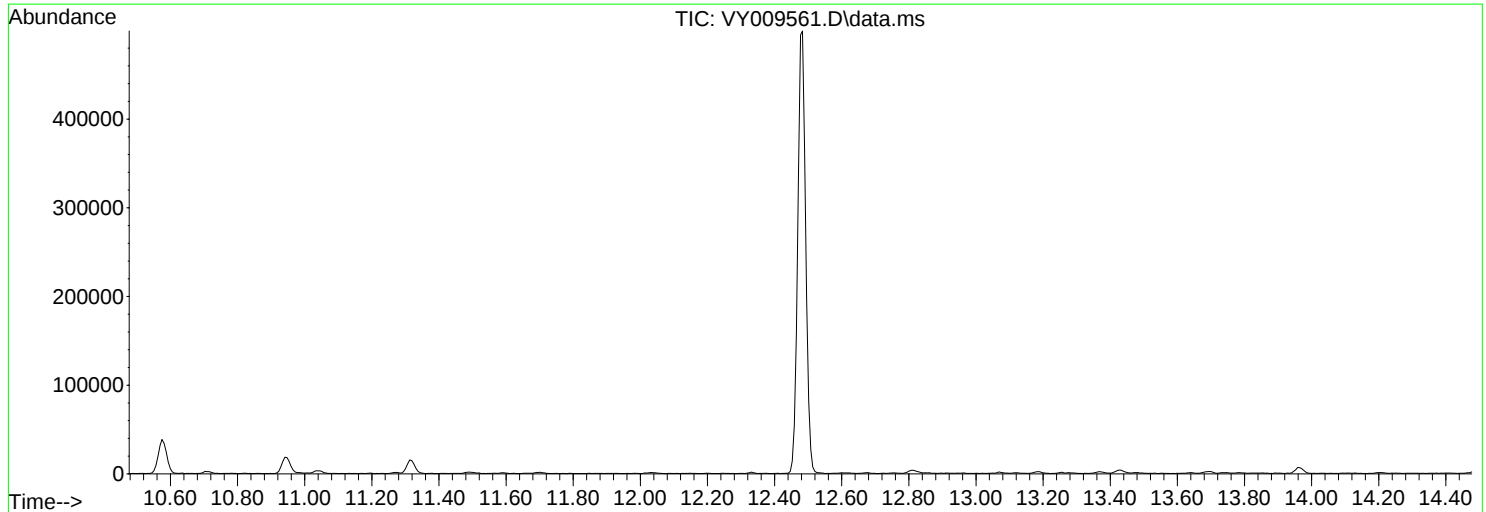

AutoFind: Scans 1747, 1748, 1749; Background Corrected with Scan 1739

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	17228	PASS
75	95	30	60	54.3	44400	PASS
95	95	100	100	100.0	81821	PASS
96	95	5	9	7.1	5797	PASS
173	174	0.00	2	1.3	901	PASS
174	95	50	100	86.2	70565	PASS
175	174	5	9	7.3	5129	PASS
176	174	95	101	95.2	67149	PASS
177	176	5	9	6.7	4512	PASS