

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY071423\
 Data File : VY014646.D
 Acq On : 14 Jul 2023 14:39
 Operator : SY/MD
 Sample : 03615-06
 Misc : 5.09g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VNJ-204

Quant Time: Jul 14 23:10:24 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y071323S.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 14 02:09:50 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.783	168	227354	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	394077	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.484	117	356912	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	155170	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.137	65	141504	54.618	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	109.240%
35) Dibromofluoromethane	7.710	113	124744	49.727	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	99.460%
50) Toluene-d8	10.173	98	461722	49.923	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	99.840%
62) 4-Bromofluorobenzene	12.477	95	166780	47.029	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	94.060%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY071423\
Data File : VY014646.D
Acq On : 14 Jul 2023 14:39
Operator : SY/MD
Sample : 03615-06
Misc : 5.09g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VNJ-204

Quant Time: Jul 14 23:10:24 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y071323S.M
Quant Title : SW846 8260
QLast Update : Fri Jul 14 02:09:50 2023
Response via : Initial Calibration




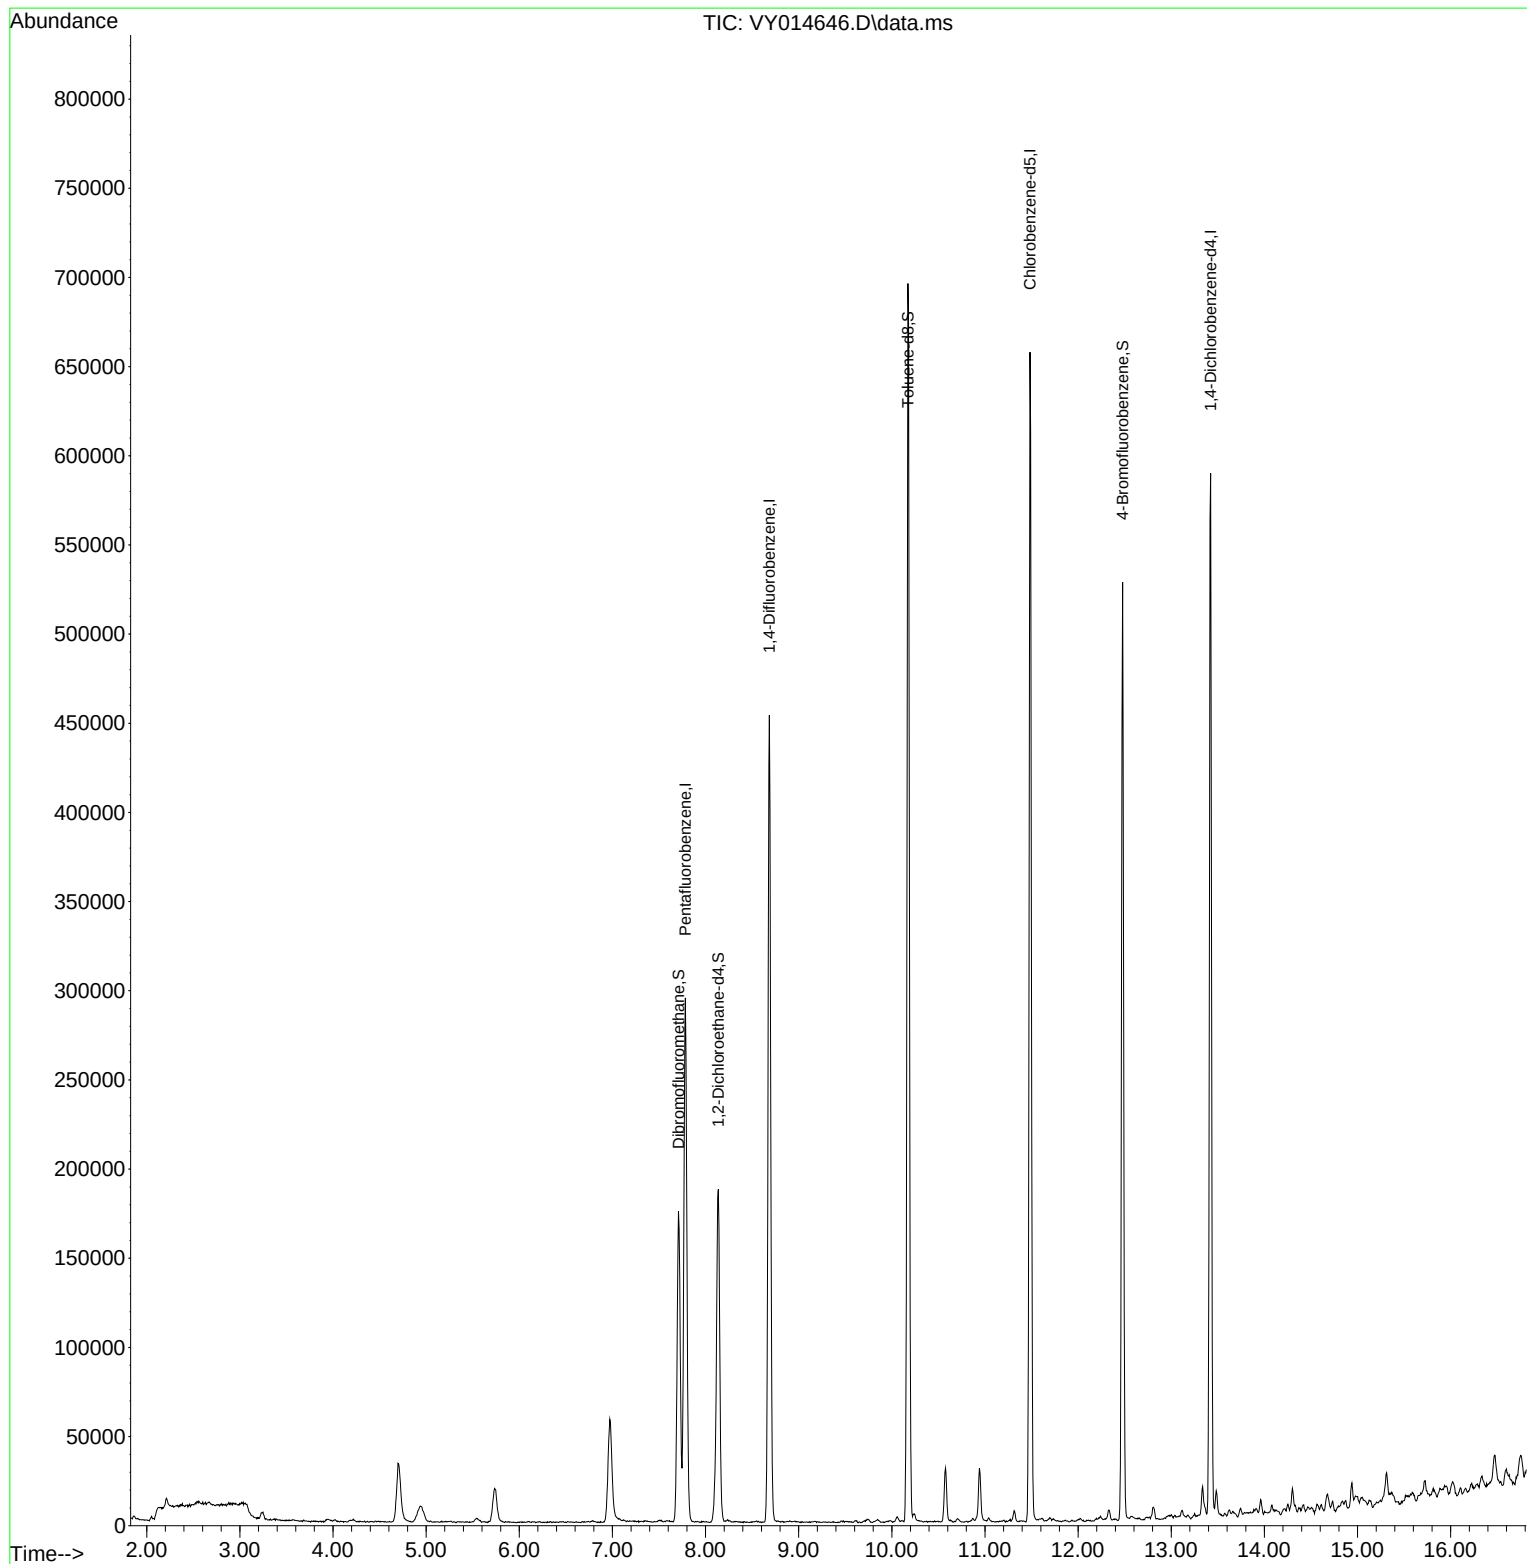


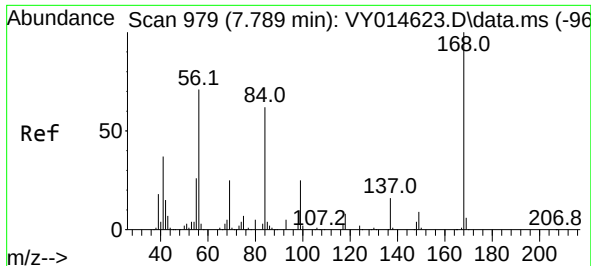

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.783 min Scan# 91
Delta R.T. -0.006 min
Lab File: VY014646.D
Acq: 14 Jul 2023 14:39




Instrument :
MSVOA_Y
ClientSampleId :
VNJ-204


Tgt Ion:168 Resp: 227354
Ion Ratio Lower Upper
168 100
99 56.1 43.4 65.0

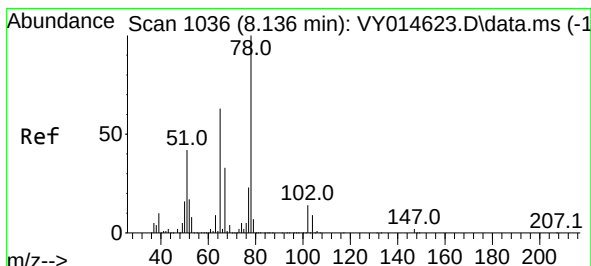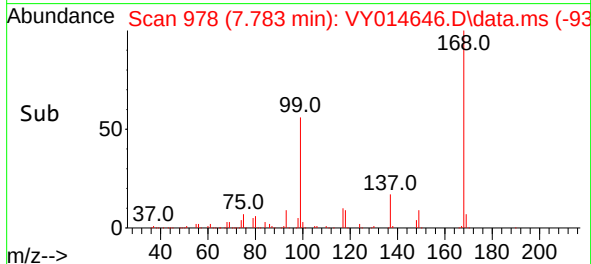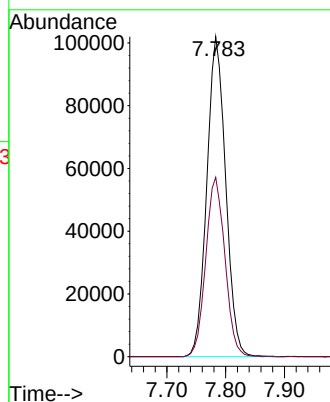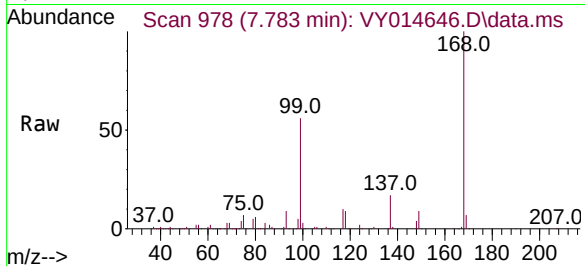

#33
1,2-Dichloroethane-d4
Concen: 54.618 ug/l
RT: 8.137 min Scan# 1036
Delta R.T. 0.001 min
Lab File: VY014646.D
Acq: 14 Jul 2023 14:39

Tgt Ion: 65 Resp: 141504
Ion Ratio Lower Upper
65 100
67 52.7 0.0 101.8


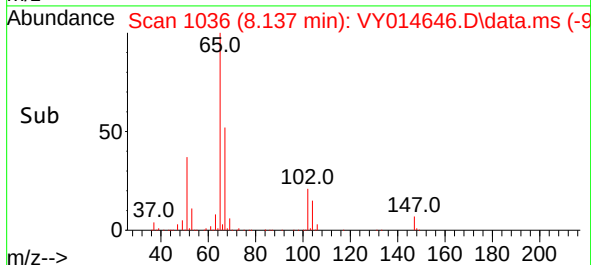
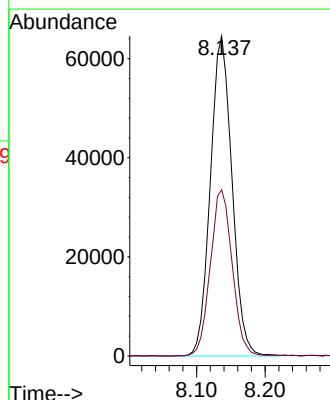
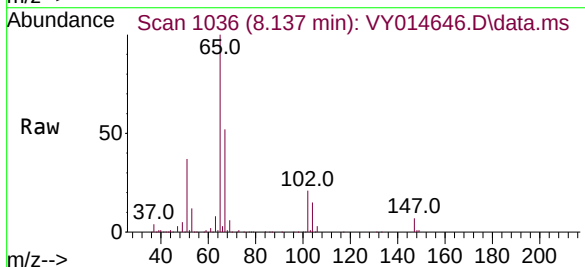


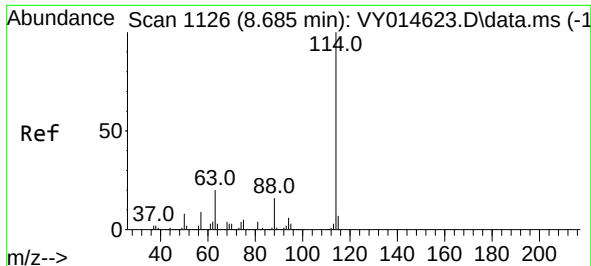

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.685 min Scan# 1126
Delta R.T. 0.000 min
Lab File: VY014646.D
Acq: 14 Jul 2023 14:39




Instrument :
MSVOA_Y
ClientSampleId :
VNJ-204


Tgt Ion:	114	Resp:	394077
Ion	Ratio	Lower	Upper
114	100		
63	19.2	0.0	42.4
88	16.4	0.0	30.6

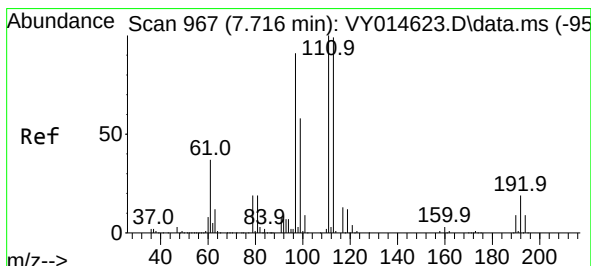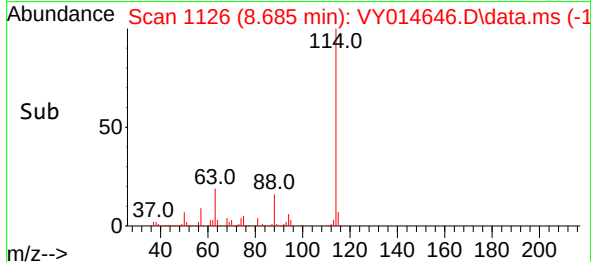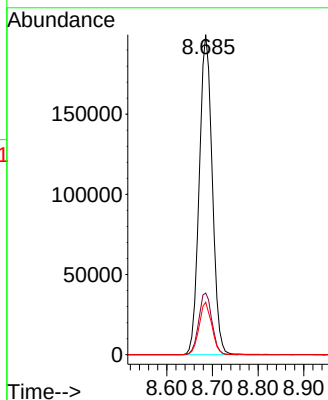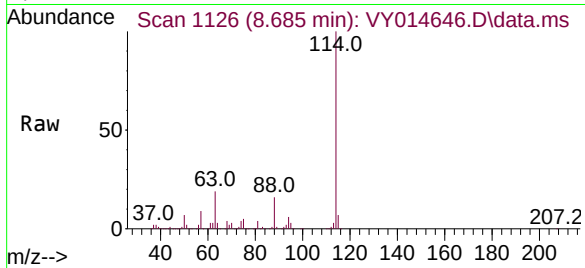

#35
Dibromofluoromethane
Concen: 49.727 ug/l
RT: 7.710 min Scan# 966
Delta R.T. -0.006 min
Lab File: VY014646.D
Acq: 14 Jul 2023 14:39

Tgt Ion:	113	Resp:	124744
Ion	Ratio	Lower	Upper
113	100		
111	102.1	81.3	121.9
192	19.6	16.9	25.3

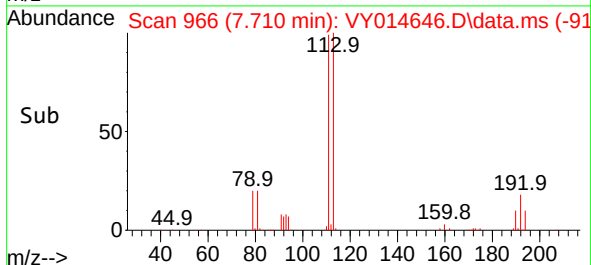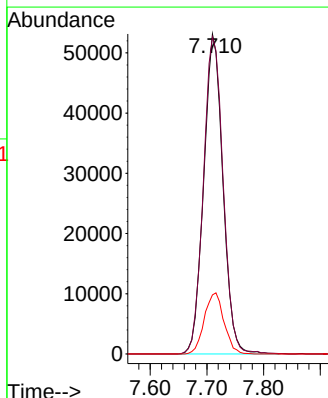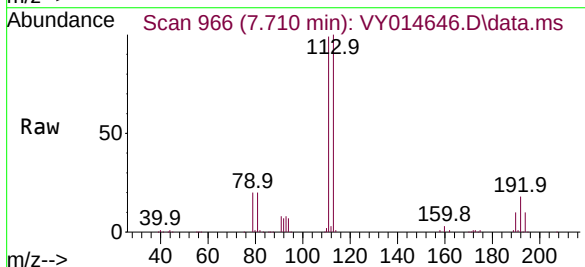

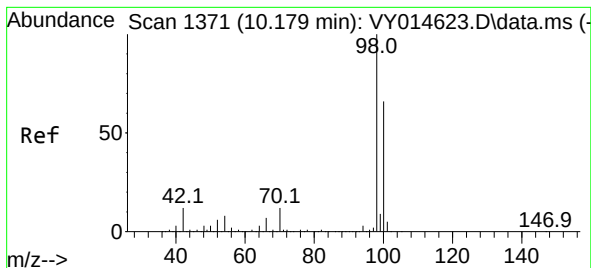

#50

Toluene-d8

Concen: 49.923 ug/l

RT: 10.173 min Scan# 1

Delta R.T. -0.006 min

Lab File: VY014646.D

Acq: 14 Jul 2023 14:39

Instrument :

MSVOA_Y

ClientSampleId :





VNJ-204

Tgt Ion: 98 Resp: 461722

Ion Ratio Lower Upper

98 100

100 65.8 50.1 75.1

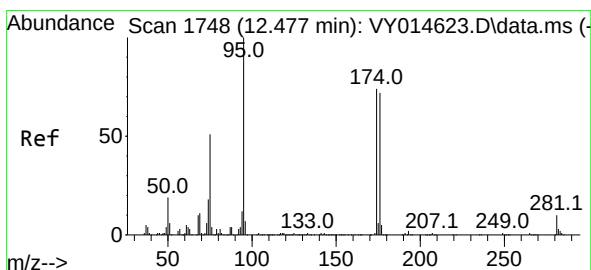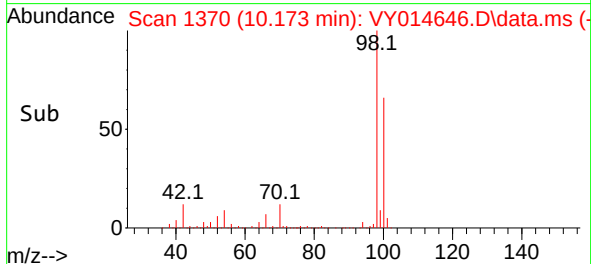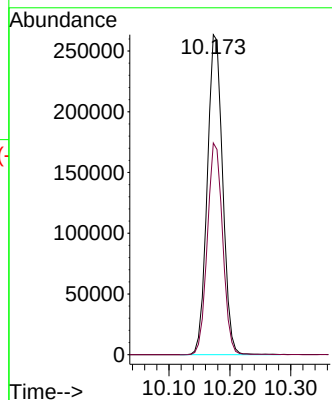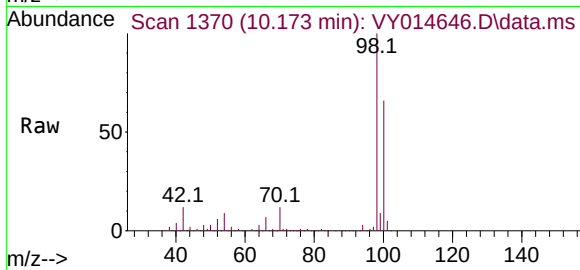

#62

4-Bromofluorobenzene

Concen: 47.029 ug/l

RT: 12.477 min Scan# 1748

Delta R.T. 0.000 min

Lab File: VY014646.D

Acq: 14 Jul 2023 14:39




Tgt Ion: 95 Resp: 166780


Ion Ratio Lower Upper

95 100

174 79.2 0.0 178.2

176 75.8 0.0 173.8

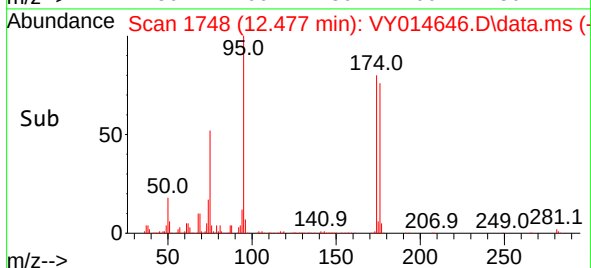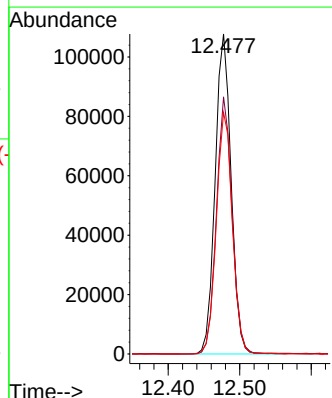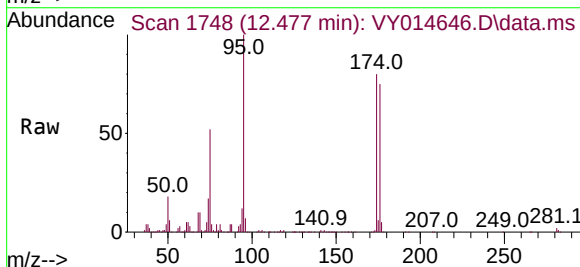

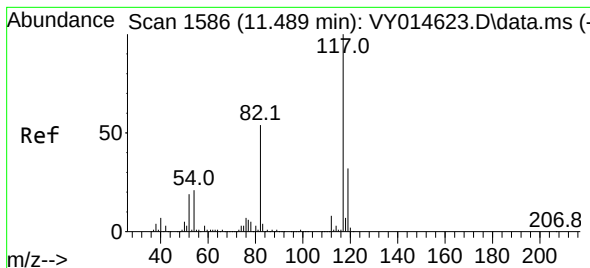

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.484 min Scan# 11

Delta R.T. -0.005 min

Lab File: VY014646.D

Acq: 14 Jul 2023 14:39

Instrument :

MSVOA_Y

ClientSampleId :

VNJ-204





Tgt Ion:117 Resp: 356912

Ion Ratio Lower Upper

117 100

82 56.3 43.4 65.0

119 32.1 26.3 39.5

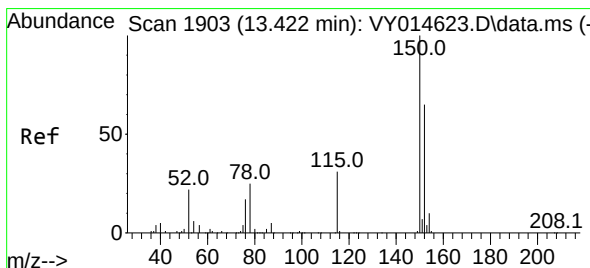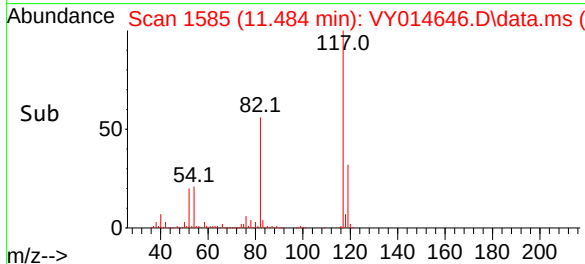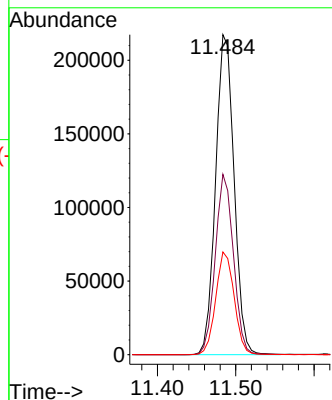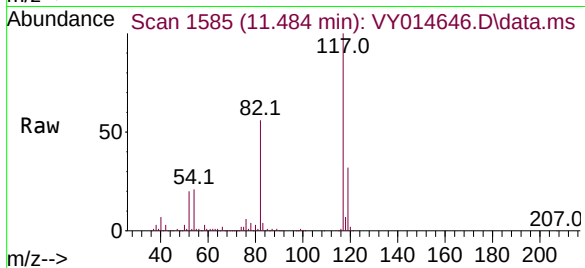

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.422 min Scan# 1903

Delta R.T. 0.000 min

Lab File: VY014646.D

Acq: 14 Jul 2023 14:39

Tgt Ion:152 Resp: 155170

Ion Ratio Lower Upper

152 100

115 59.3 28.8 86.5

150 156.3 0.0 348.8

