
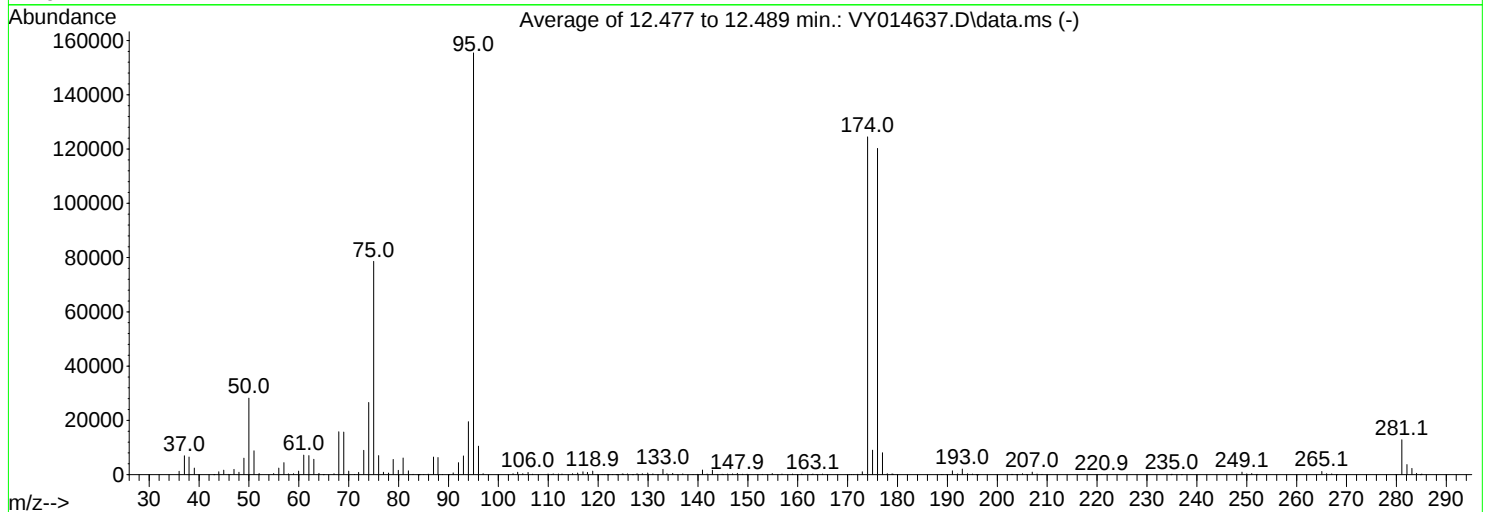


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY071423\
Data File : VY014637.D
Acq On : 14 Jul 2023 08:53
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y071323S.M
Title : SW846 8260
Last Update : Fri Jul 14 02:09:50 2023

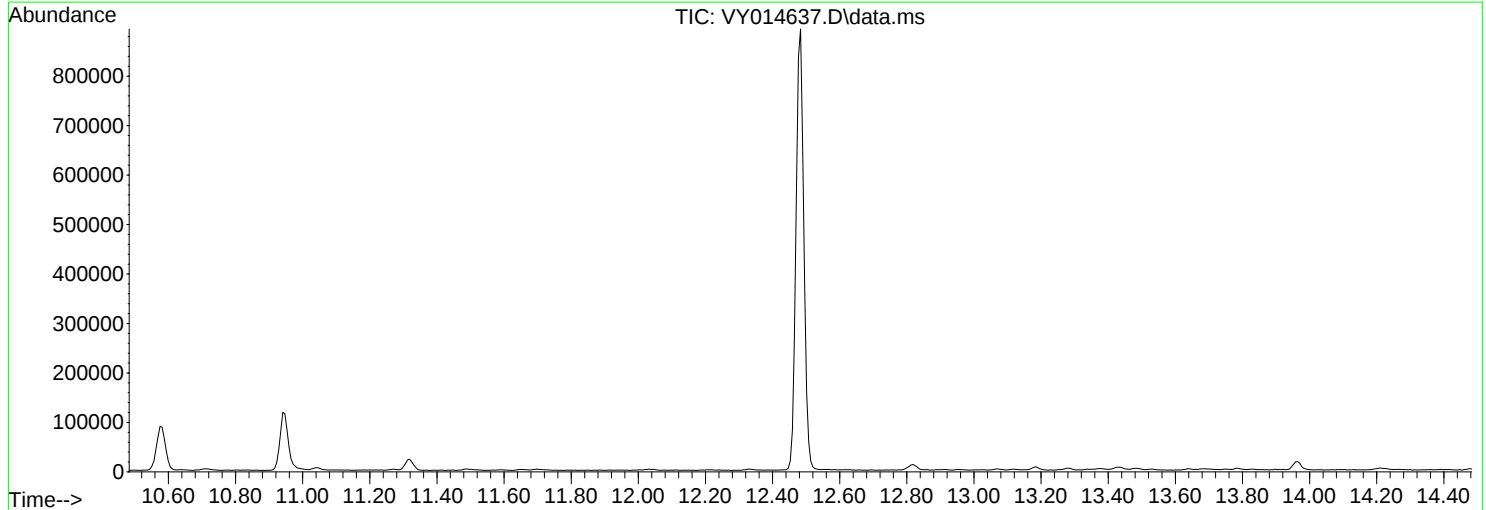

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1738

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	28197	PASS
75	95	30	60	50.6	78592	PASS
95	95	100	100	100.0	155453	PASS
96	95	5	9	6.8	10502	PASS
173	174	0.00	2	0.8	1042	PASS
174	95	50	100	80.1	124472	PASS
175	174	5	9	7.2	9022	PASS
176	174	95	101	96.6	120229	PASS
177	176	5	9	6.7	8082	PASS