
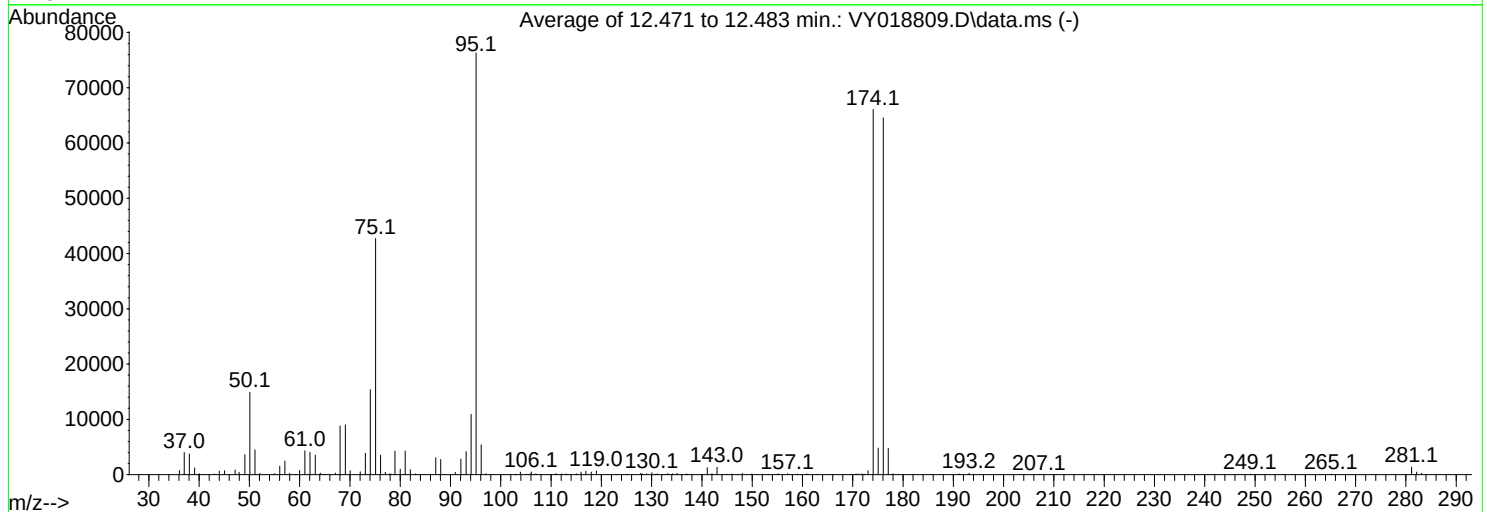


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY071524\
Data File : VY018809.D
Acq On : 15 Jul 2024 09:22
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y070924S.M
Title : SW846 8260
Last Update : Tue Jul 09 14:28:51 2024

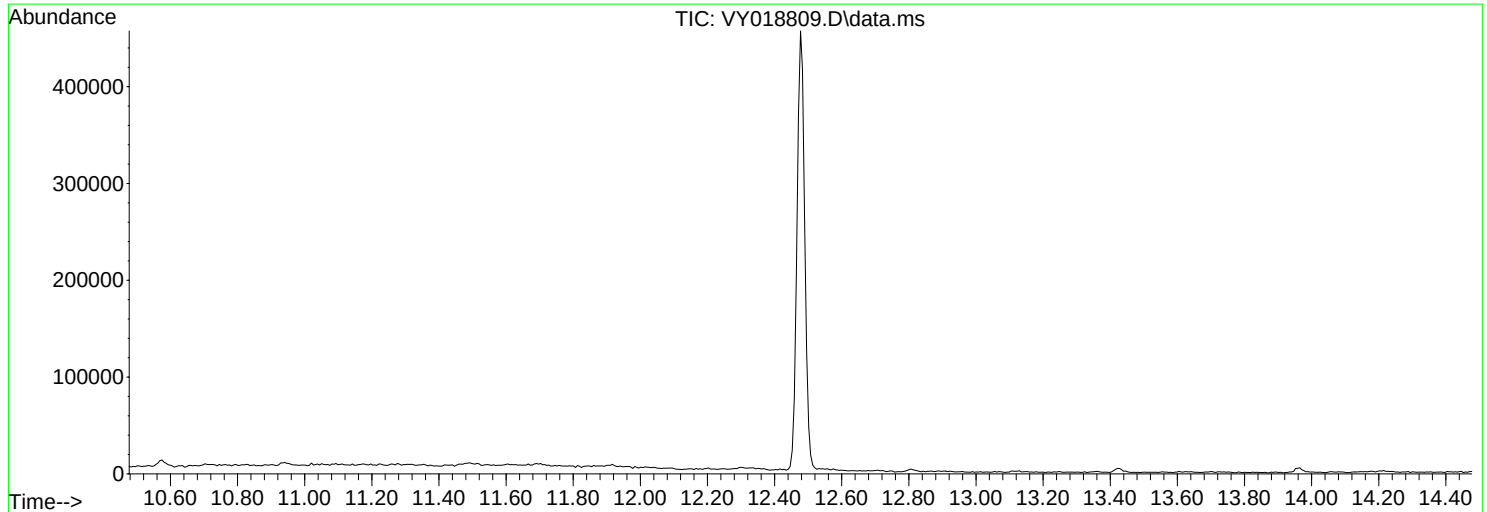

AutoFind: Scans 1747, 1748, 1749; Background Corrected with Scan 1740

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.5	14899	PASS
75	95	30	60	56.0	42733	PASS
95	95	100	100	100.0	76315	PASS
96	95	5	9	7.0	5377	PASS
173	174	0.00	2	1.1	727	PASS
174	95	50	100	86.6	66091	PASS
175	174	5	9	7.3	4805	PASS
176	174	95	101	97.7	64544	PASS
177	176	5	9	7.4	4759	PASS