

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY071624\
 Data File : VY018832.D
 Acq On : 16 Jul 2024 15:05
 Operator : SY/MD
 Sample : P3246-04
 Misc : 7.26g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 WC-CTW2-BL-01-G

Quant Time: Jul 17 01:56:43 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y070924S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jul 09 14:28:51 2024
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.771	168	200901	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.679	114	349905	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.484	117	330237	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	141377	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.124	65	120392	60.899	ug/l	0.00
Spiked Amount	50.000	Range 50 - 163	Recovery	=	121.800%	
35) Dibromofluoromethane	7.698	113	114993	52.472	ug/l	0.00
Spiked Amount	50.000	Range 54 - 147	Recovery	=	104.940%	
50) Toluene-d8	10.173	98	403368	48.582	ug/l	0.00
Spiked Amount	50.000	Range 58 - 134	Recovery	=	97.160%	
62) 4-Bromofluorobenzene	12.477	95	139760	49.290	ug/l	0.00
Spiked Amount	50.000	Range 30 - 143	Recovery	=	98.580%	
Target Compounds						
						Qvalue
16) Acetone	3.930	43	14483	39.738	ug/l #	86
25) 2-Butanone	6.972	43	1792	3.508	ug/l #	65
95) Naphthalene	15.233	128	4508	1.027	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY071624\
Data File : VY018832.D
Acq On : 16 Jul 2024 15:05
Operator : SY/MD
Sample : P3246-04
Misc : 7.26g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
WC-CTW2-BL-01-G

Quant Time: Jul 17 01:56:43 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y070924S.M
Quant Title : SW846 8260
QLast Update : Tue Jul 09 14:28:51 2024
Response via : Initial Calibration




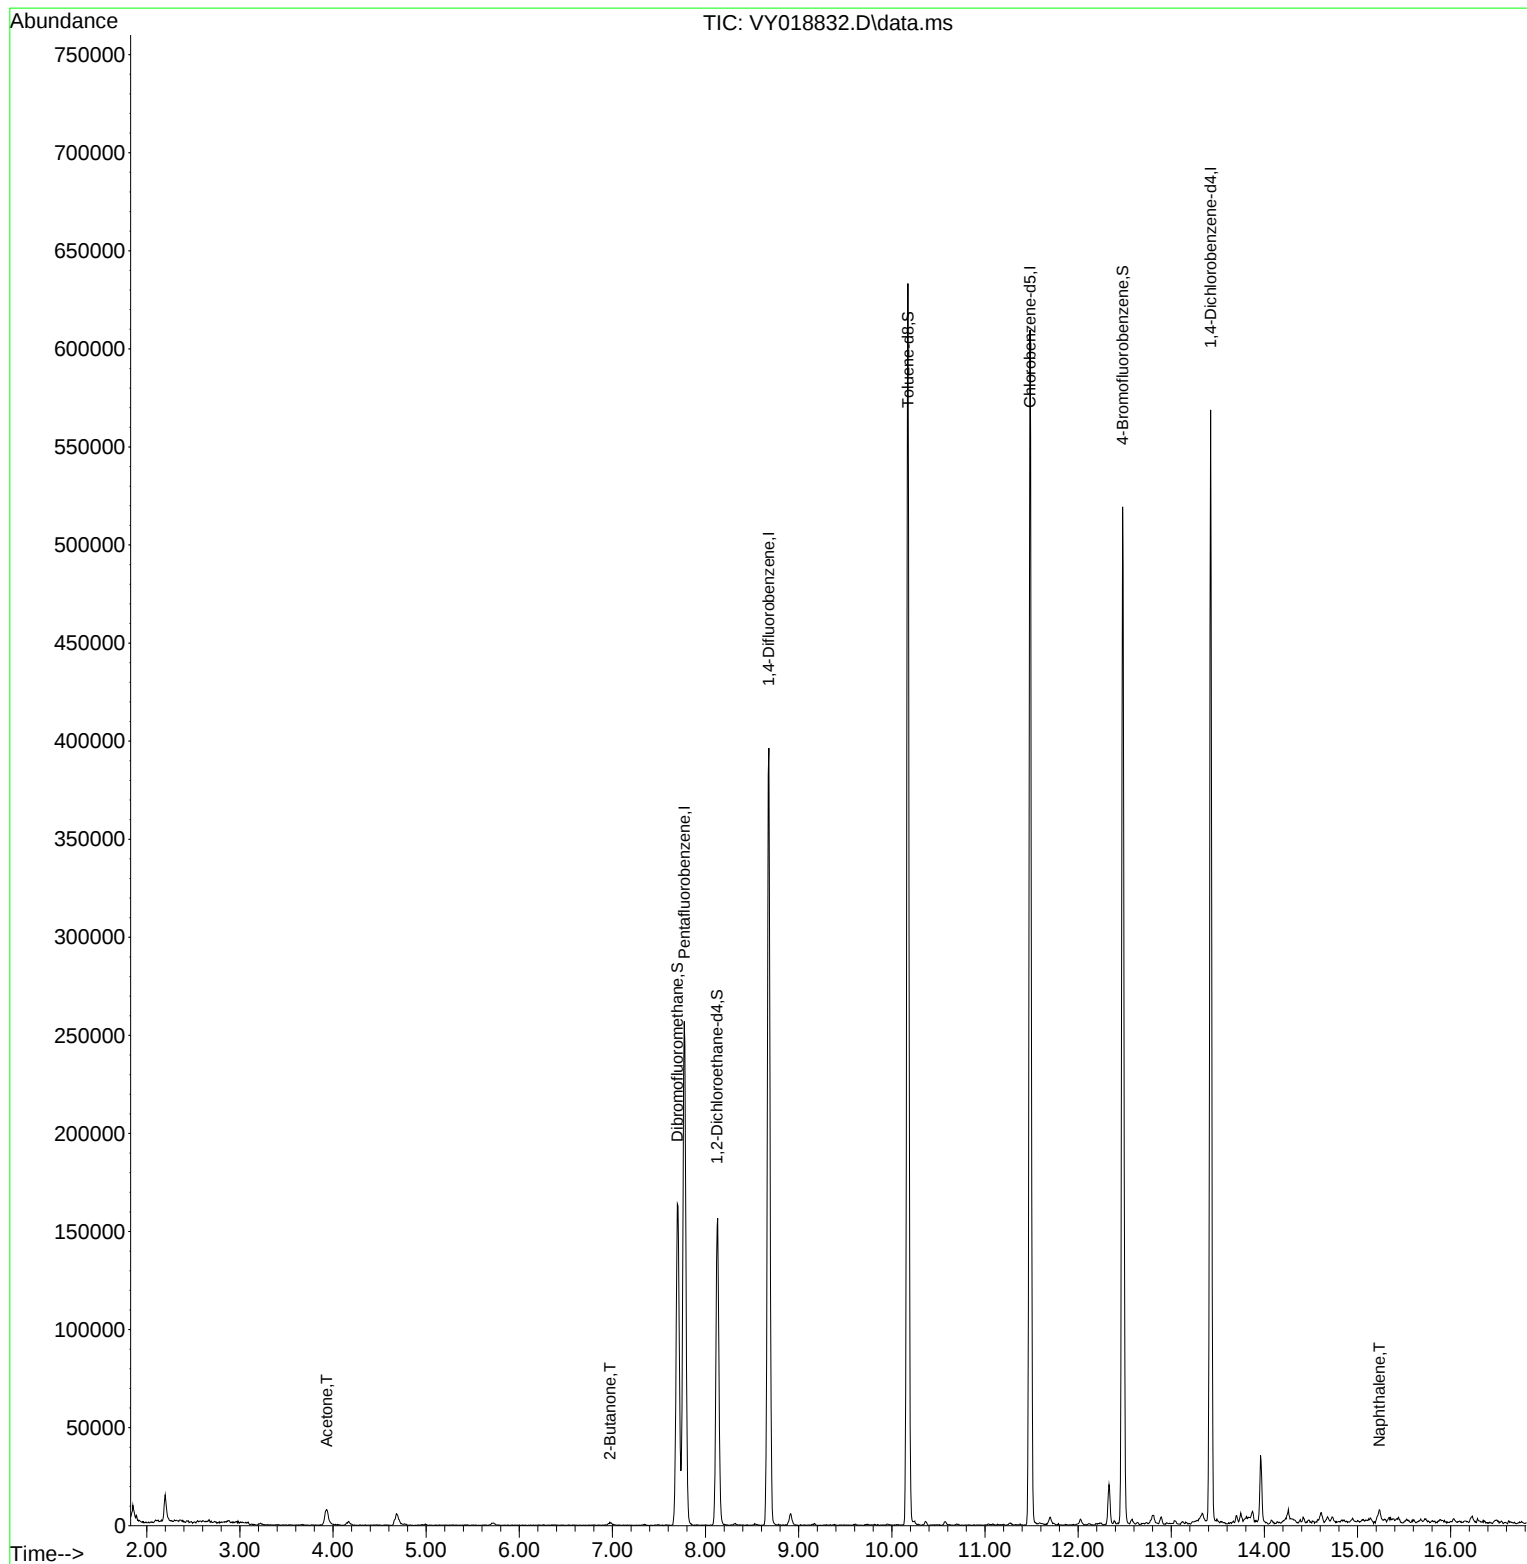


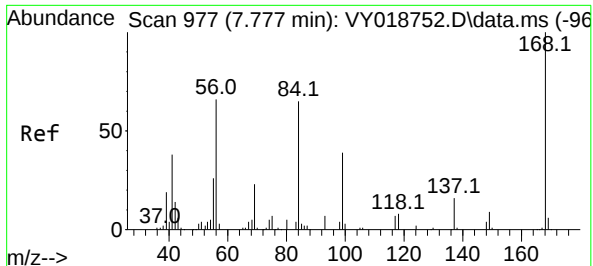

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.771 min Scan# 91
Delta R.T. -0.006 min
Lab File: VY018832.D
Acq: 16 Jul 2024 15:05




Instrument :
MSVOA_Y
ClientSampleId :
WC-CTW2-BL-01-G


Tgt Ion:168 Resp: 200901
Ion Ratio Lower Upper
168 100
99 54.5 39.1 58.7

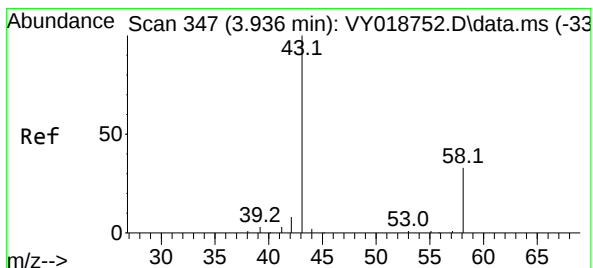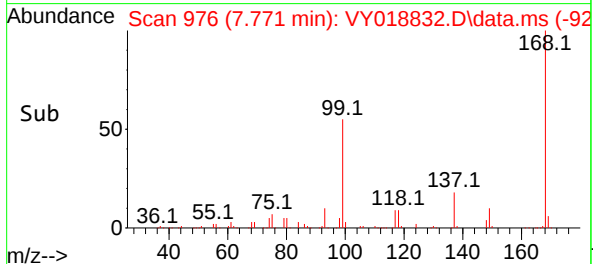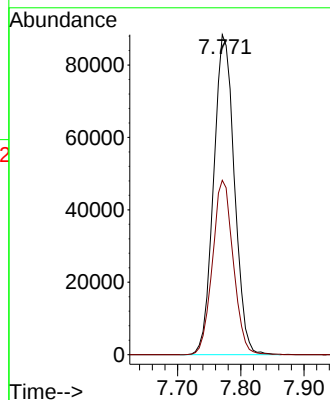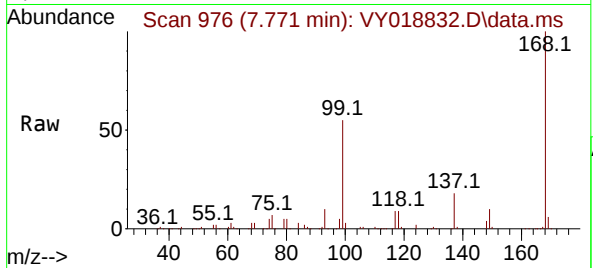

#16
Acetone
Concen: 39.738 ug/l
RT: 3.930 min Scan# 346
Delta R.T. -0.006 min
Lab File: VY018832.D
Acq: 16 Jul 2024 15:05

Tgt Ion: 43 Resp: 14483
Ion Ratio Lower Upper
43 100
58 31.1 31.7 47.5#

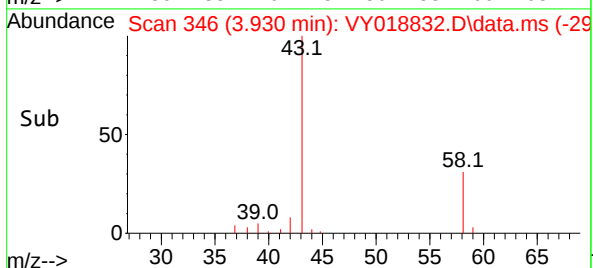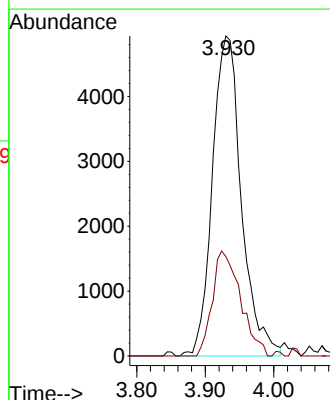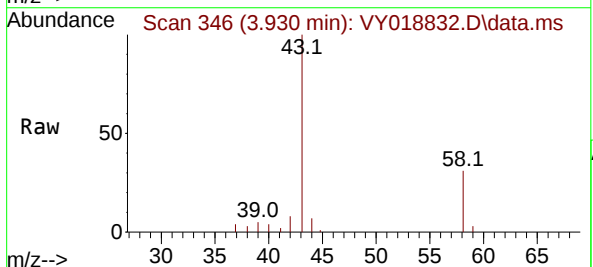

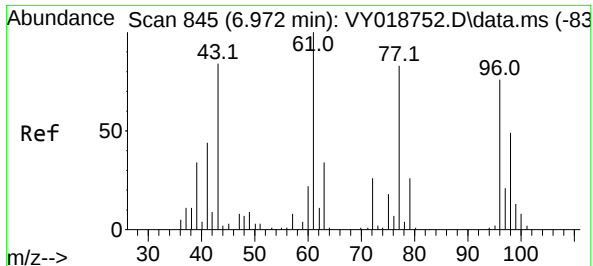

#25

2-Butanone

Concen: 3.508 ug/l

RT: 6.972 min Scan# 845

Delta R.T. 0.000 min

Lab File: VY018832.D

Acq: 16 Jul 2024 15:05

Instrument :

MSVOA_Y

ClientSampleId :





WC-CTW2-BL-01-G

Tgt Ion: 43 Resp: 1792

Ion Ratio Lower Upper

43 100

72 54.1 27.3 40.9#

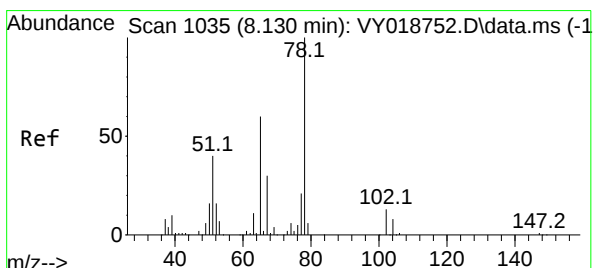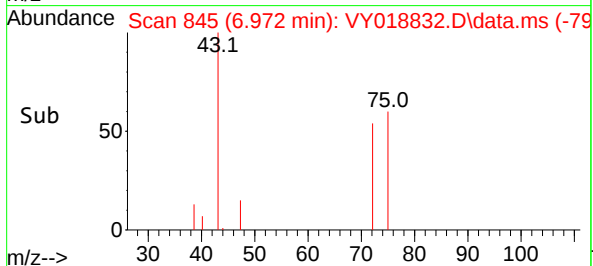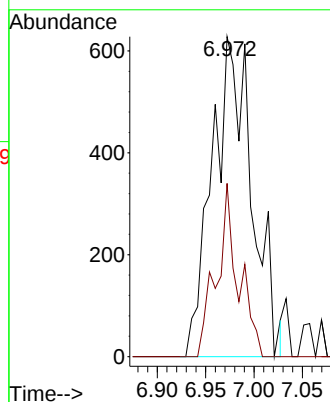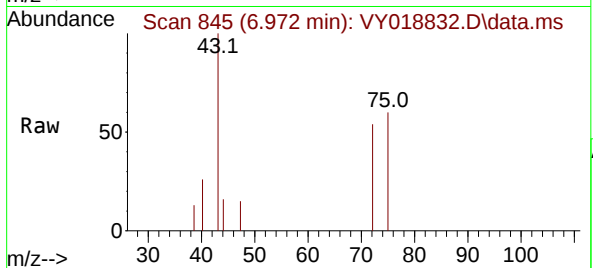

#33

1,2-Dichloroethane-d4

Concen: 60.899 ug/l

RT: 8.124 min Scan# 1034

Delta R.T. -0.006 min

Lab File: VY018832.D




Acq: 16 Jul 2024 15:05


Tgt Ion: 65 Resp: 120392

Ion Ratio Lower Upper

65 100

67 50.8 0.0 109.6

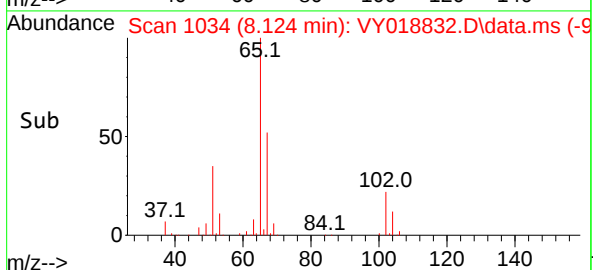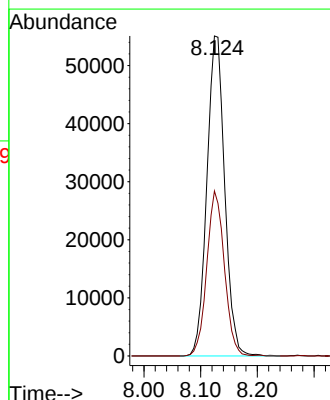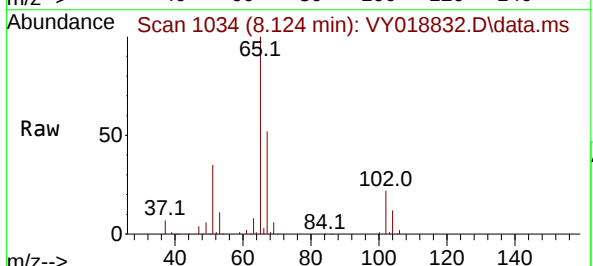

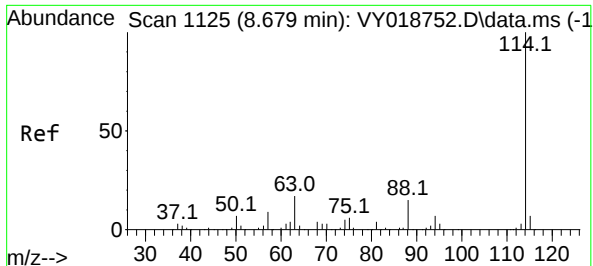

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.679 min Scan# 1125

Delta R.T. 0.000 min

Lab File: VY018832.D

Acq: 16 Jul 2024 15:05

Instrument :

MSVOA_Y

ClientSampleId :

WC-CTW2-BL-01-G





Tgt Ion:114 Resp: 349905

Ion Ratio Lower Upper

114 100

63 17.7 0.0 35.0

88 14.5 0.0 27.2

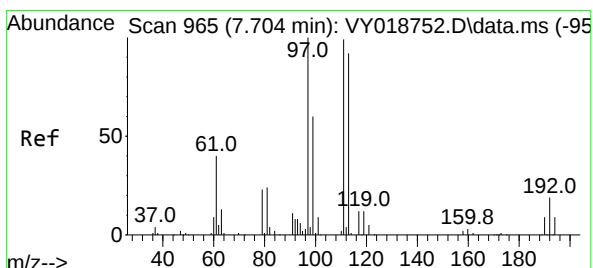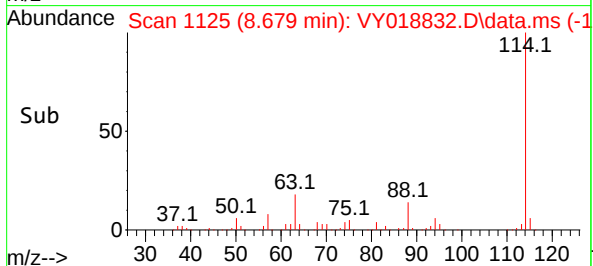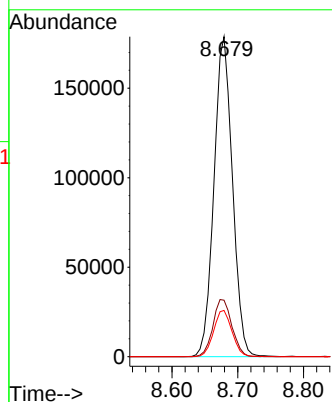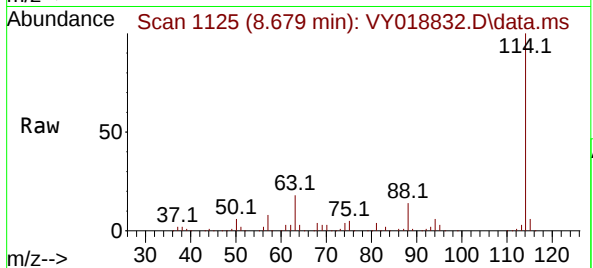

#35

Dibromofluoromethane

Concen: 52.472 ug/l

RT: 7.698 min Scan# 964

Delta R.T. -0.006 min

Lab File: VY018832.D

Acq: 16 Jul 2024 15:05




Tgt Ion:113 Resp: 114993


Ion Ratio Lower Upper

113 100

111 100.3 82.2 123.4

192 20.3 15.9 23.9

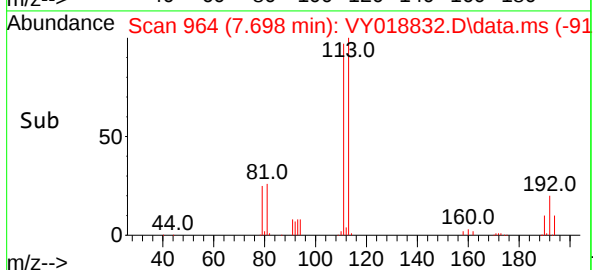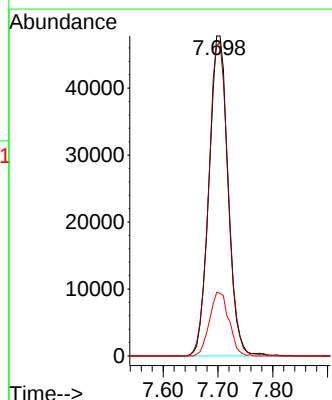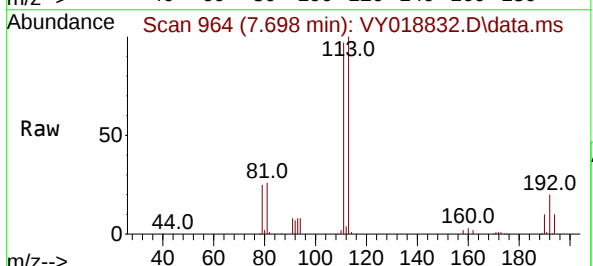

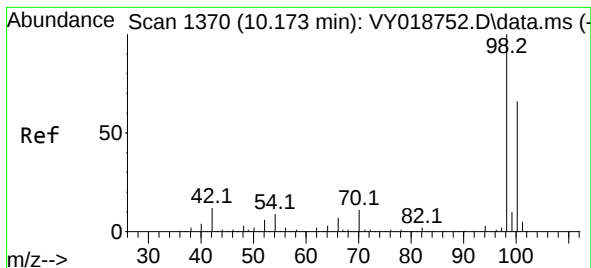

#50

Toluene-d8

Concen: 48.582 ug/l

RT: 10.173 min Scan# 1

Delta R.T. 0.000 min

Lab File: VY018832.D

Acq: 16 Jul 2024 15:05

Instrument :

MSVOA_Y

ClientSampleId :





WC-CTW2-BL-01-G

Tgt Ion: 98 Resp: 403368

Ion Ratio Lower Upper

98 100

100 65.9 52.0 78.0

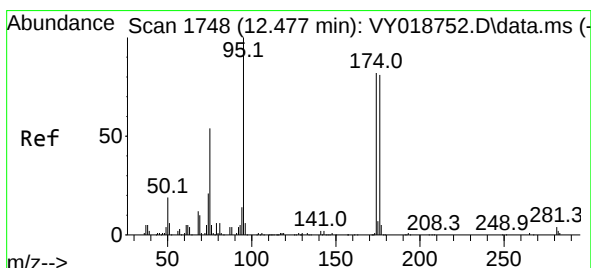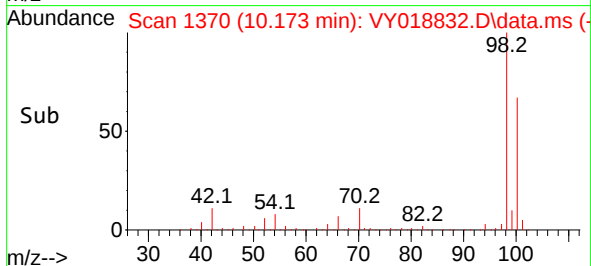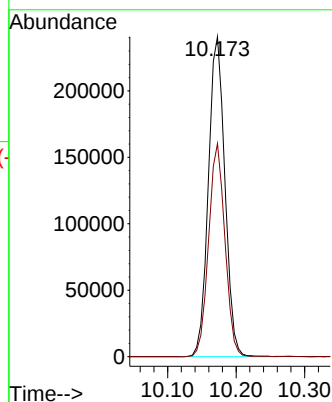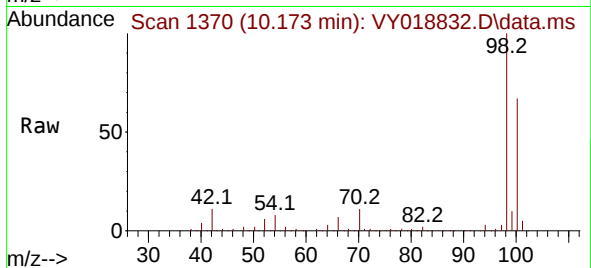

#62

4-Bromofluorobenzene

Concen: 49.290 ug/l

RT: 12.477 min Scan# 1748

Delta R.T. 0.000 min

Lab File: VY018832.D

Acq: 16 Jul 2024 15:05




Tgt Ion: 95 Resp: 139760


Ion Ratio Lower Upper

95 100

174 87.2 0.0 175.6

176 85.1 0.0 171.4

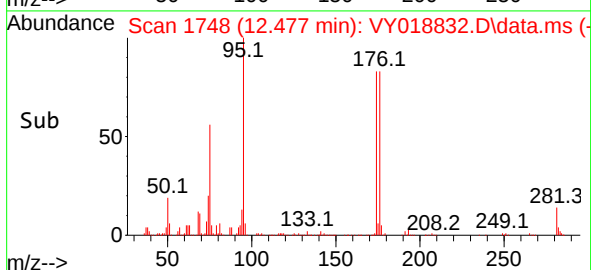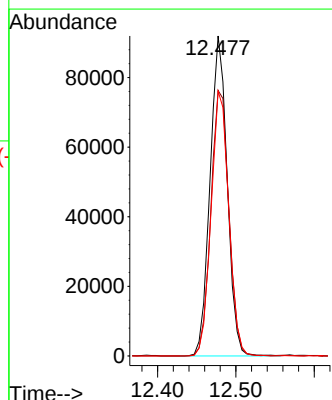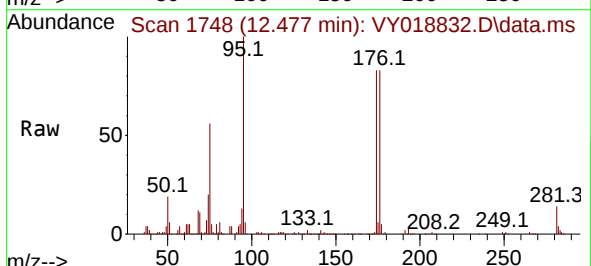

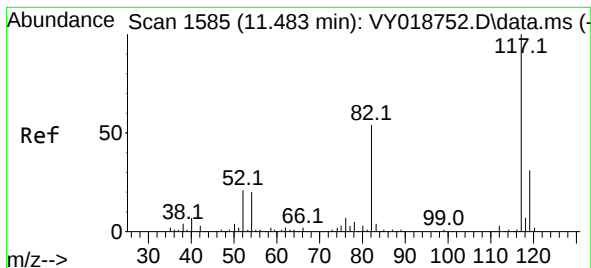

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.484 min Scan# 11

Delta R.T. 0.000 min

Lab File: VY018832.D

Acq: 16 Jul 2024 15:05

Instrument :

MSVOA_Y

ClientSampleId :

WC-CTW2-BL-01-G





Tgt Ion:117 Resp: 330237

Ion Ratio Lower Upper

117 100

82 52.3 42.4 63.6

119 32.8 25.9 38.9

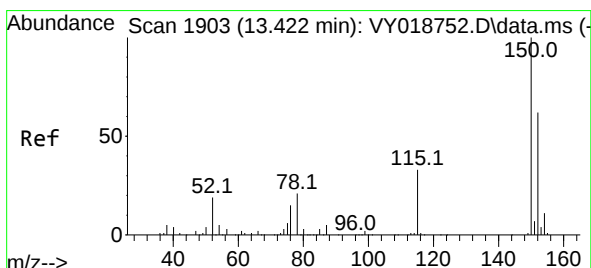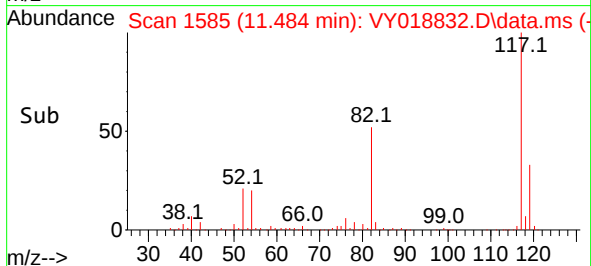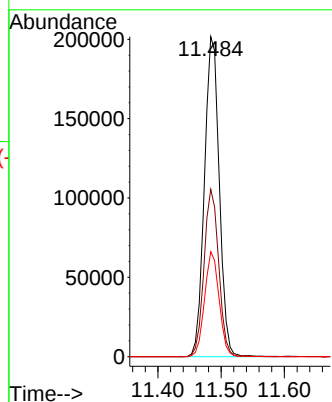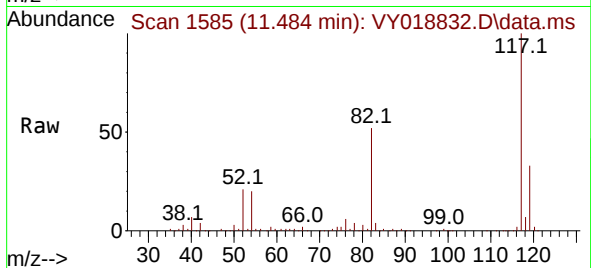

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.422 min Scan# 1903

Delta R.T. 0.000 min

Lab File: VY018832.D

Acq: 16 Jul 2024 15:05




Tgt Ion:152 Resp: 141377


Ion Ratio Lower Upper

152 100

115 57.4 28.2 84.7


150 157.1 0.0 345.6

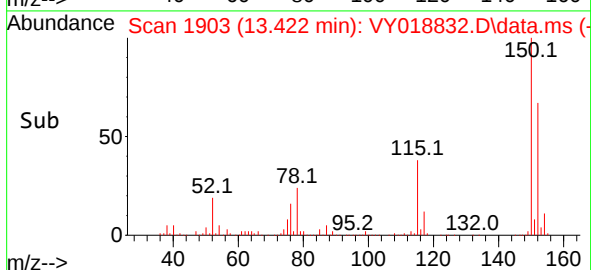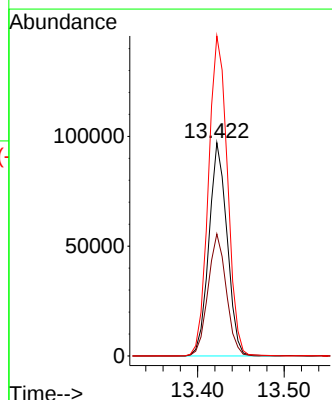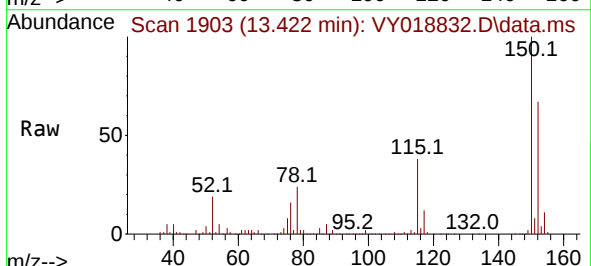

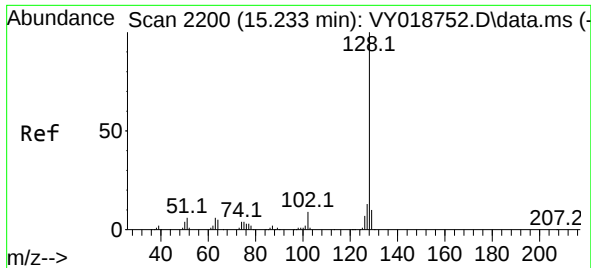

#95
Naphthalene
Concen: 1.027 ug/l
RT: 15.233 min Scan# 21
Delta R.T. 0.000 min
Lab File: VY018832.D
Acq: 16 Jul 2024 15:05

Instrument :
MSVOA_Y
ClientSampleId :
WC-CTW2-BL-01-G

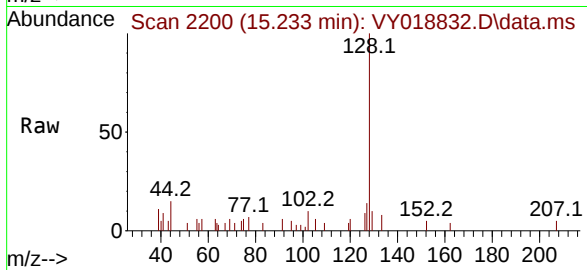

Tgt Ion:	128	Resp:	4508
Ion Ratio	Lower	Upper	
128	100		
127	13.8	10.6	16.0
129	11.9	8.6	13.0

