

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY071723\
 Data File : VY014677.D
 Acq On : 17 Jul 2023 17:07
 Operator : SY/MD
 Sample : 03631-01
 Misc : 3.95g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 SB-02(2-4)

Quant Time: Jul 18 06:12:01 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y071323S.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 14 02:09:50 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.789	168	221348	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	376974	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	332775	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	150203	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.137	65	116417	46.154	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	92.300%
35) Dibromofluoromethane	7.710	113	114302	47.631	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	95.260%
50) Toluene-d8	10.179	98	441837	49.940	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	99.880%
62) 4-Bromofluorobenzene	12.477	95	154043	45.408	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	90.820%
Target Compounds						
					Qvalue	
3) Chloromethane	2.107	50	2224	1.097	ug/l #	87
20) Methylene Chloride	4.710	84	26153	6.389	ug/l	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY071723\
Data File : VY014677.D
Acq On : 17 Jul 2023 17:07
Operator : SY/MD
Sample : 03631-01
Misc : 3.95g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
SB-02(2-4)

Quant Time: Jul 18 06:12:01 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y071323S.M
Quant Title : SW846 8260
QLast Update : Fri Jul 14 02:09:50 2023
Response via : Initial Calibration




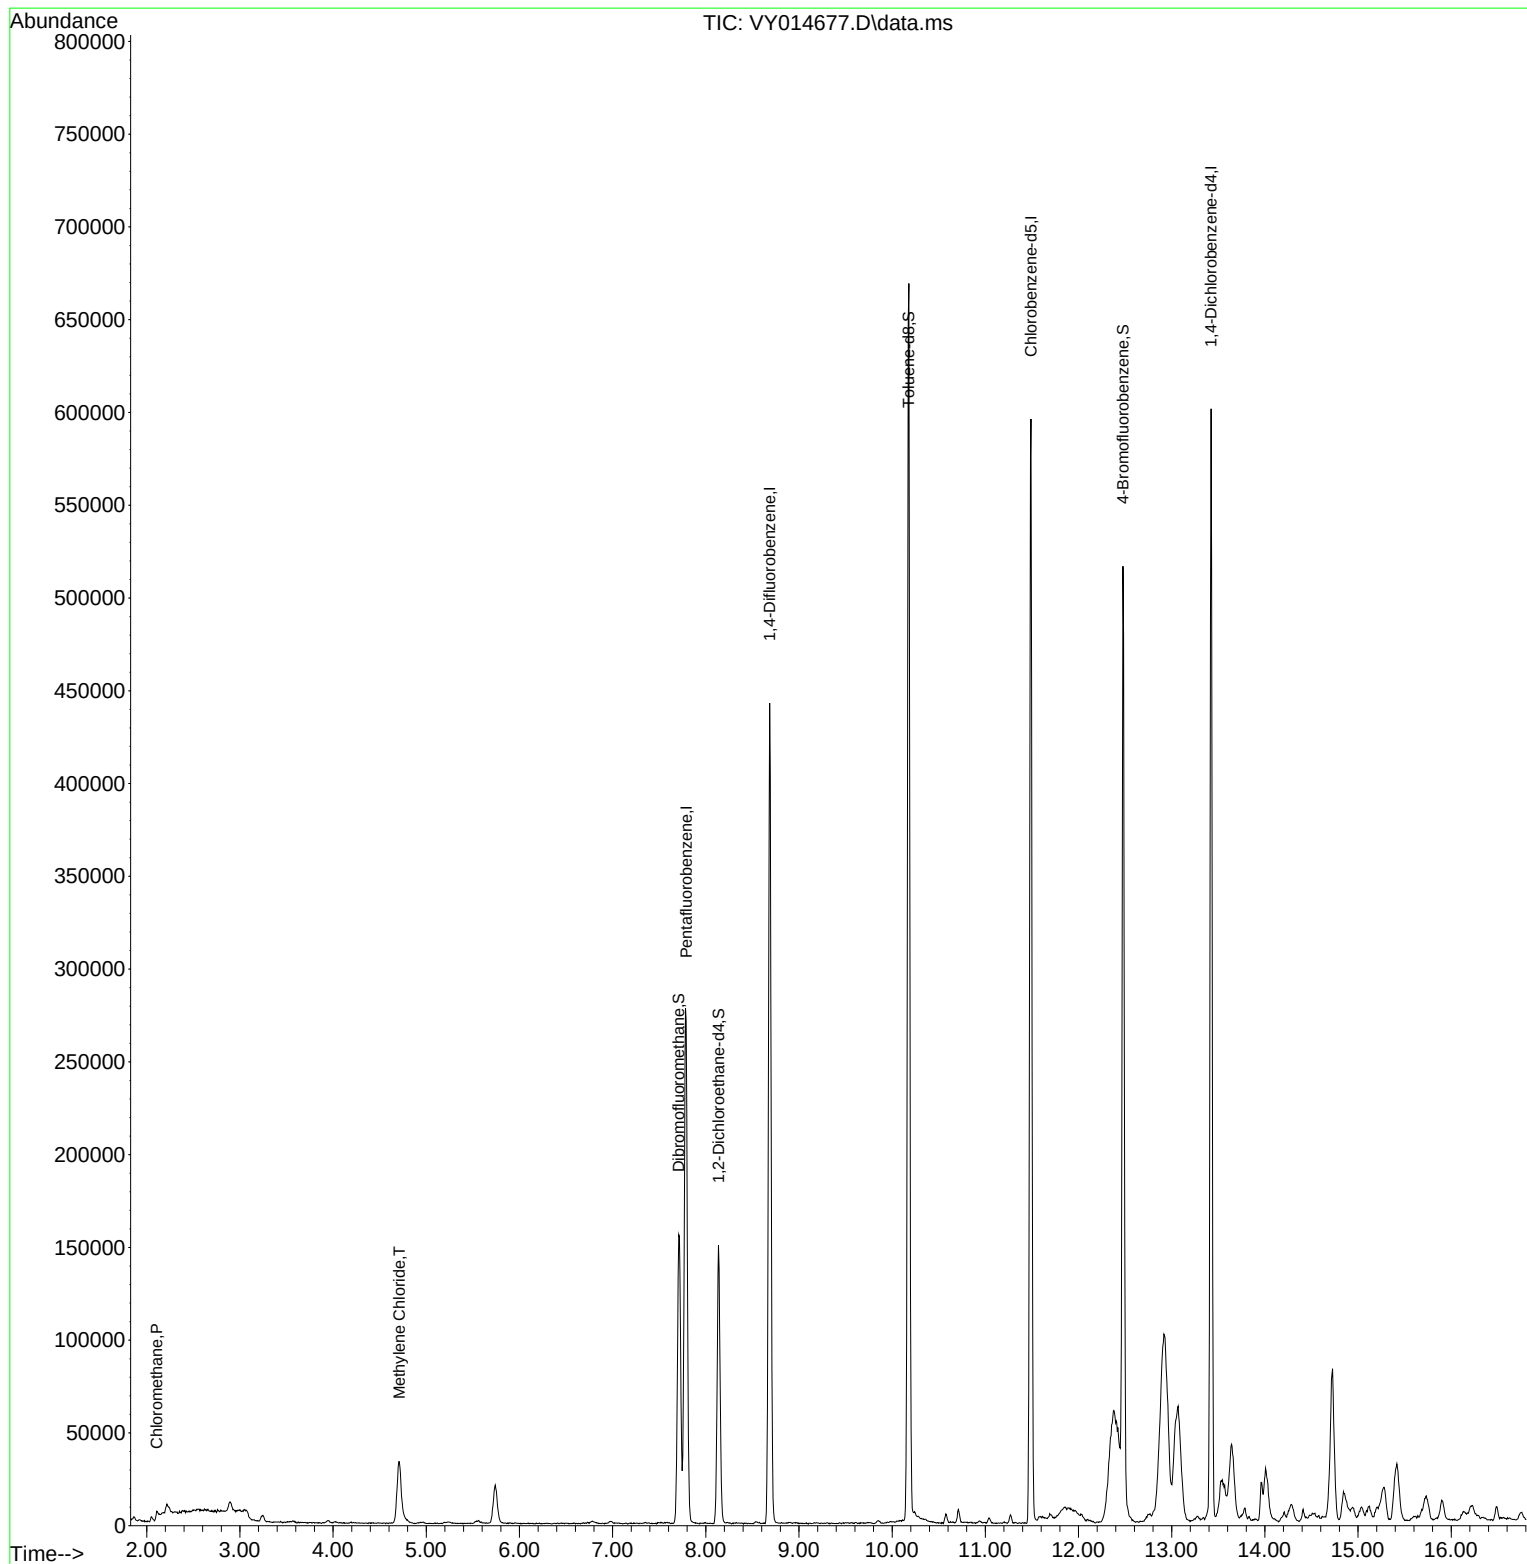


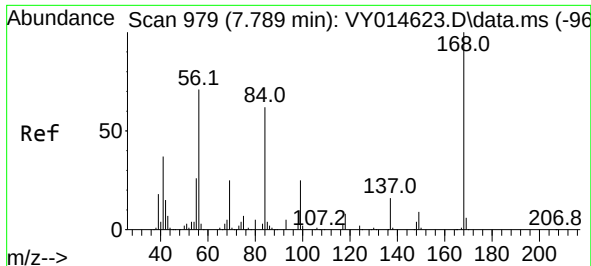

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. 0.000 min
Lab File: VY014677.D
Acq: 17 Jul 2023 17:07




Instrument :
MSVOA_Y
ClientSampleId :
SB-02(2-4)


Tgt Ion:168 Resp: 221348
Ion Ratio Lower Upper
168 100
99 55.1 43.4 65.0

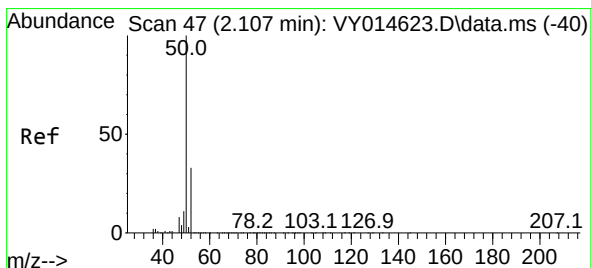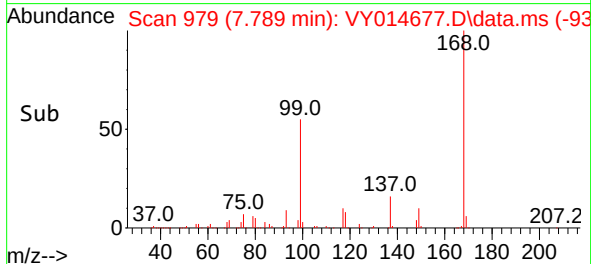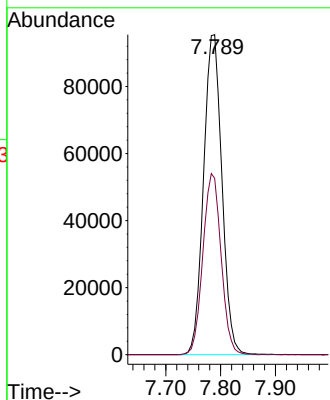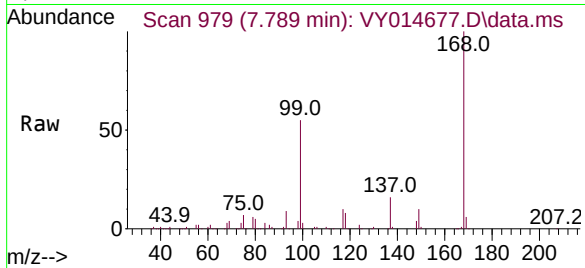

#3
Chloromethane
Concen: 1.097 ug/l
RT: 2.107 min Scan# 47
Delta R.T. 0.000 min
Lab File: VY014677.D
Acq: 17 Jul 2023 17:07

Tgt Ion: 50 Resp: 2224
Ion Ratio Lower Upper
50 100
52 38.8 25.4 38.2#

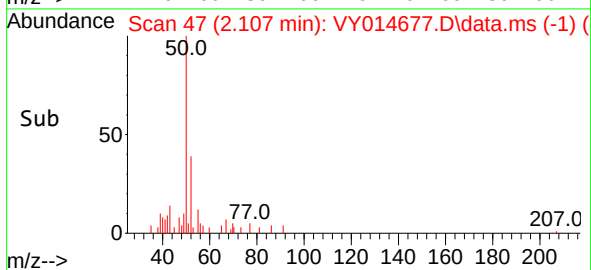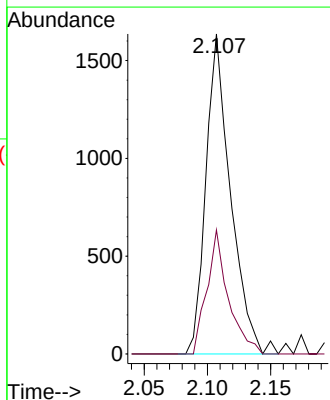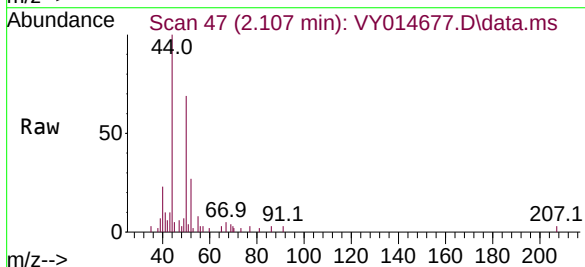




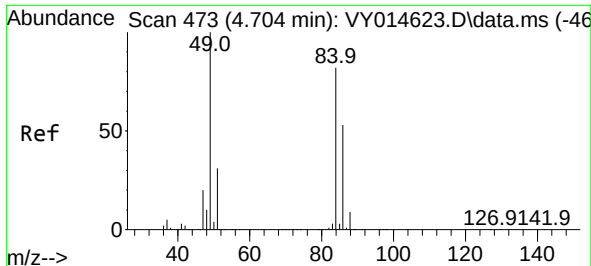


#20
Methylene Chloride
Concen: 6.389 ug/l
RT: 4.710 min Scan# 41
Delta R.T. 0.006 min
Lab File: VY014677.D
Acq: 17 Jul 2023 17:07

Instrument :
MSVOA_Y
ClientSampleId :
SB-02(2-4)

Tgt Ion: 84 Resp: 26153




Ion	Ratio	Lower	Upper
84	100		
49	117.1	106.9	160.3
51	35.9	33.2	49.8
86	59.4	51.0	76.6

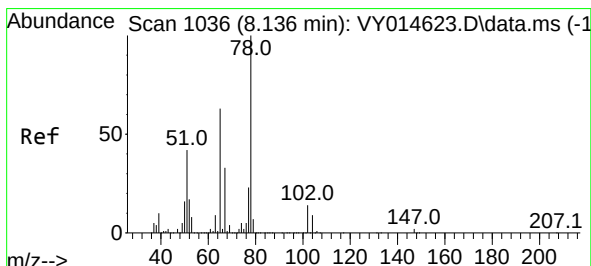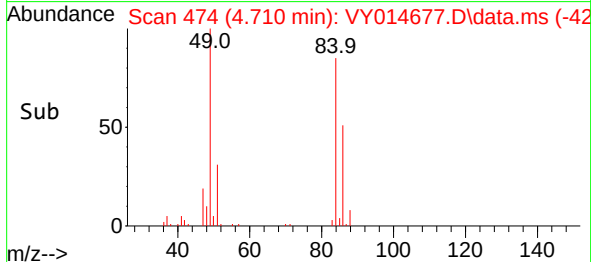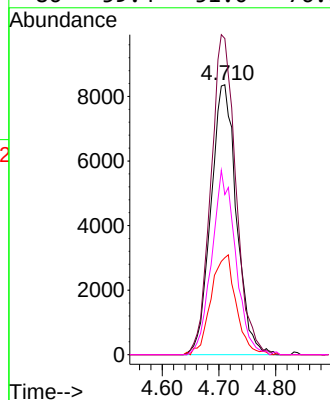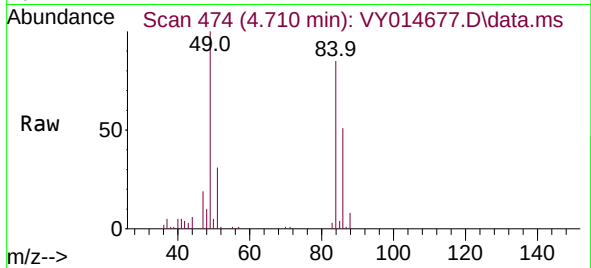


#33
1,2-Dichloroethane-d4
Concen: 46.154 ug/l
RT: 8.137 min Scan# 1036
Delta R.T. 0.001 min
Lab File: VY014677.D
Acq: 17 Jul 2023 17:07

Tgt Ion: 65 Resp: 116417

Ion	Ratio	Lower	Upper
65	100		
67	51.8	0.0	101.8


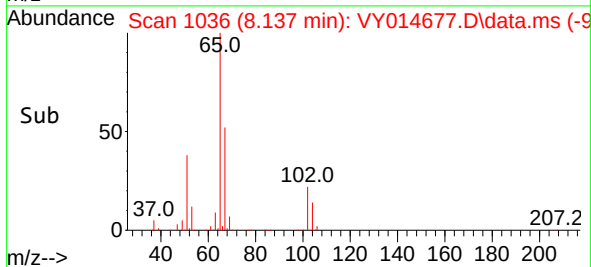
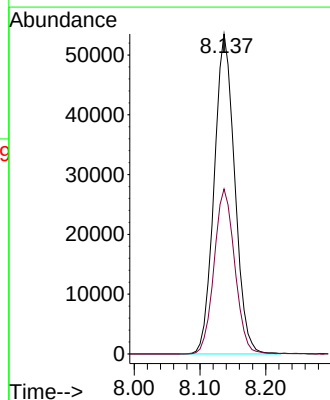
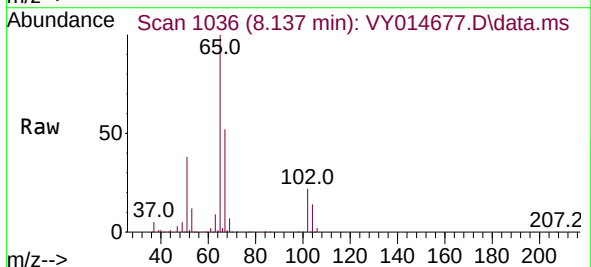


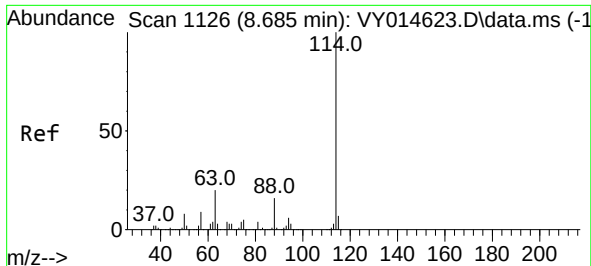

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.685 min Scan# 1126
Delta R.T. 0.000 min
Lab File: VY014677.D
Acq: 17 Jul 2023 17:07




Instrument :
MSVOA_Y
ClientSampleId :
SB-02(2-4)


Tgt Ion:114 Resp: 376974
Ion Ratio Lower Upper
114 100
63 19.3 0.0 42.4
88 15.8 0.0 30.6

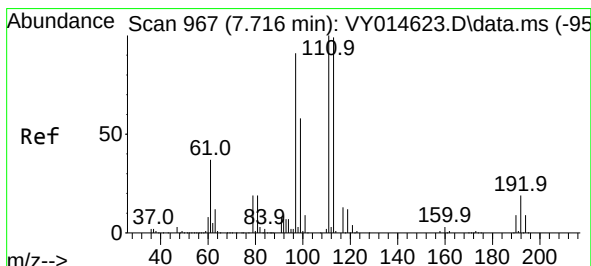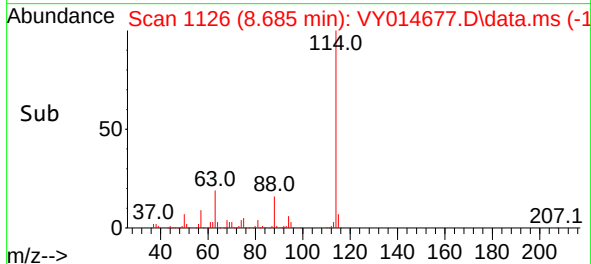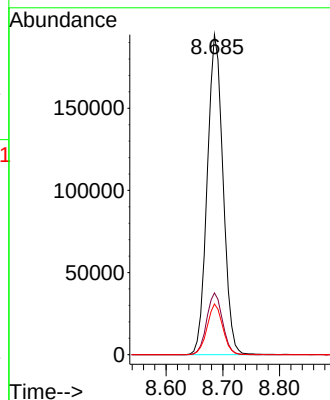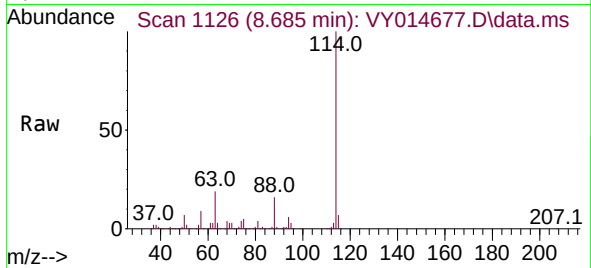

#35
Dibromofluoromethane
Concen: 47.631 ug/l
RT: 7.710 min Scan# 966
Delta R.T. -0.006 min
Lab File: VY014677.D
Acq: 17 Jul 2023 17:07

Tgt Ion:113 Resp: 114302
Ion Ratio Lower Upper
113 100
111 102.2 81.3 121.9
192 19.5 16.9 25.3


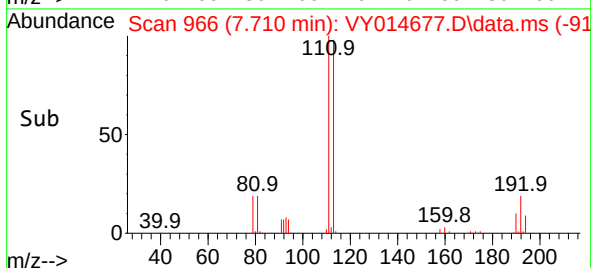
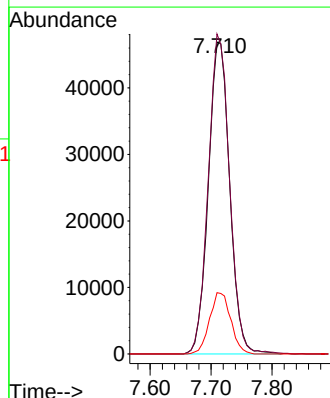
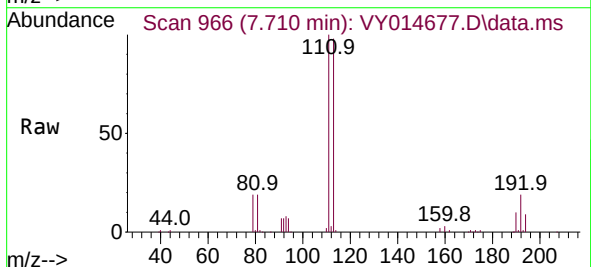


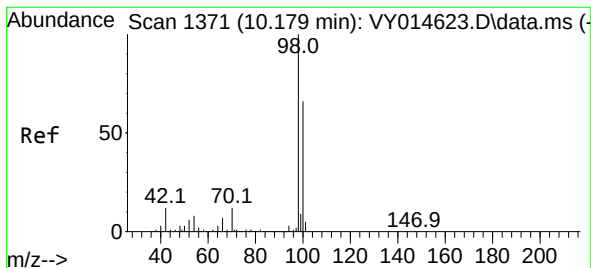

#50
Toluene-d8
Concen: 49.940 ug/l
RT: 10.179 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY014677.D
Acq: 17 Jul 2023 17:07




Instrument :
MSVOA_Y
ClientSampleId :
SB-02(2-4)


Tgt Ion: 98 Resp: 441837
Ion Ratio Lower Upper
98 100
100 65.1 50.1 75.1

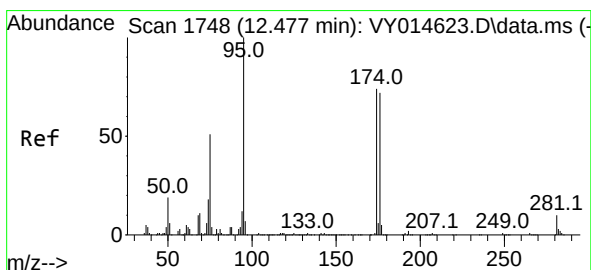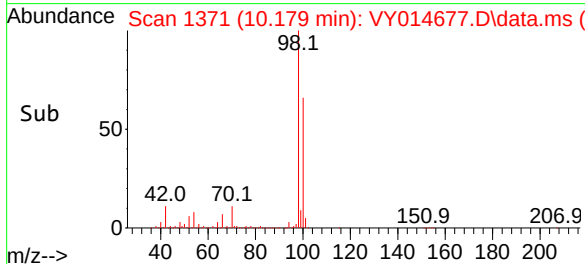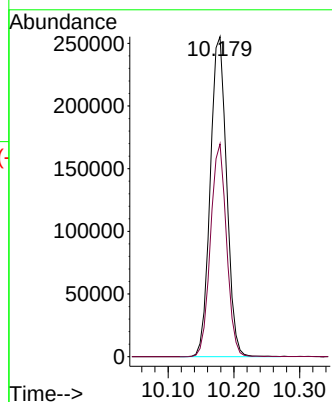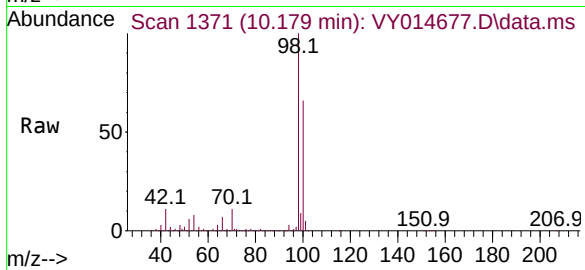

#62
4-Bromofluorobenzene
Concen: 45.408 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. 0.000 min
Lab File: VY014677.D
Acq: 17 Jul 2023 17:07

Tgt Ion: 95 Resp: 154043
Ion Ratio Lower Upper
95 100
174 80.4 0.0 178.2
176 77.1 0.0 173.8

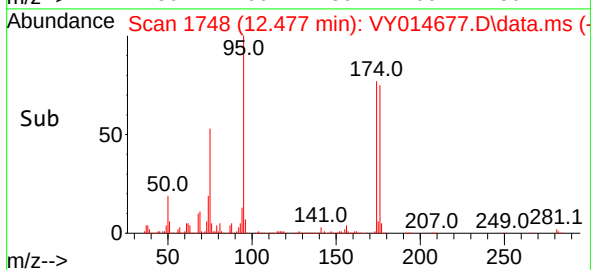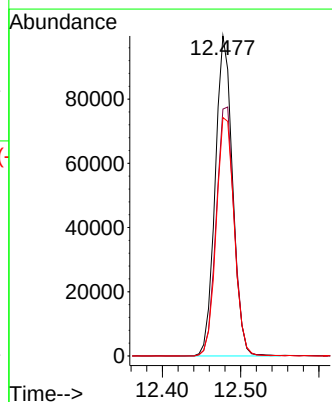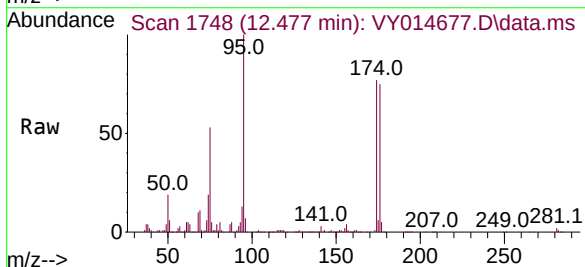

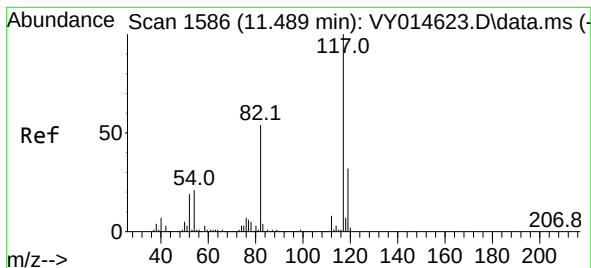

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.490 min Scan# 11

Delta R.T. 0.001 min

Lab File: VY014677.D

Acq: 17 Jul 2023 17:07

Instrument :

MSVOA_Y

ClientSampleId :

SB-02(2-4)





Tgt Ion:117 Resp: 332775

Ion Ratio Lower Upper

117 100

82 53.2 43.4 65.0

119 31.7 26.3 39.5

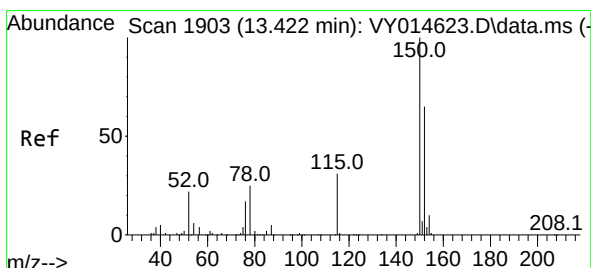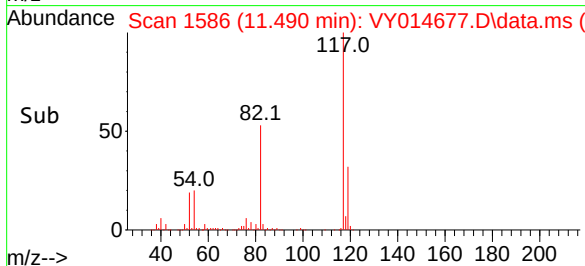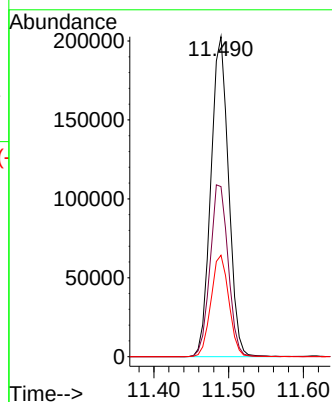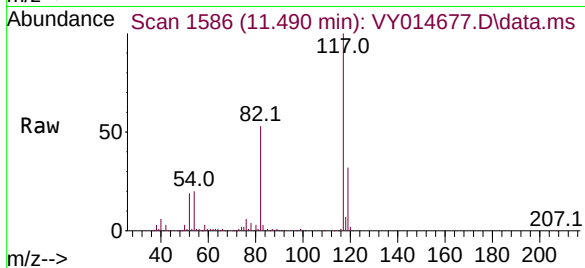

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.422 min Scan# 1903

Delta R.T. 0.000 min

Lab File: VY014677.D

Acq: 17 Jul 2023 17:07

Tgt Ion:152 Resp: 150203

Ion Ratio Lower Upper

152 100

115 60.1 28.8 86.5

150 156.5 0.0 348.8

