
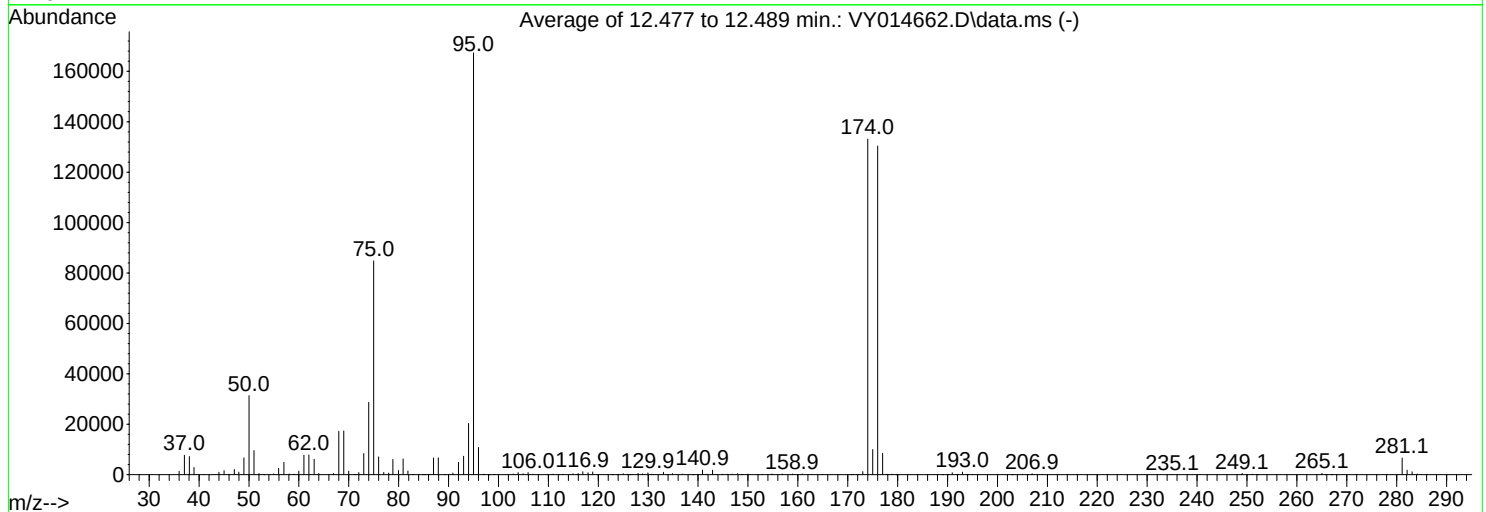


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY071723\
Data File : VY014662.D
Acq On : 17 Jul 2023 09:07
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y071323S.M
Title : SW846 8260
Last Update : Fri Jul 14 02:09:50 2023

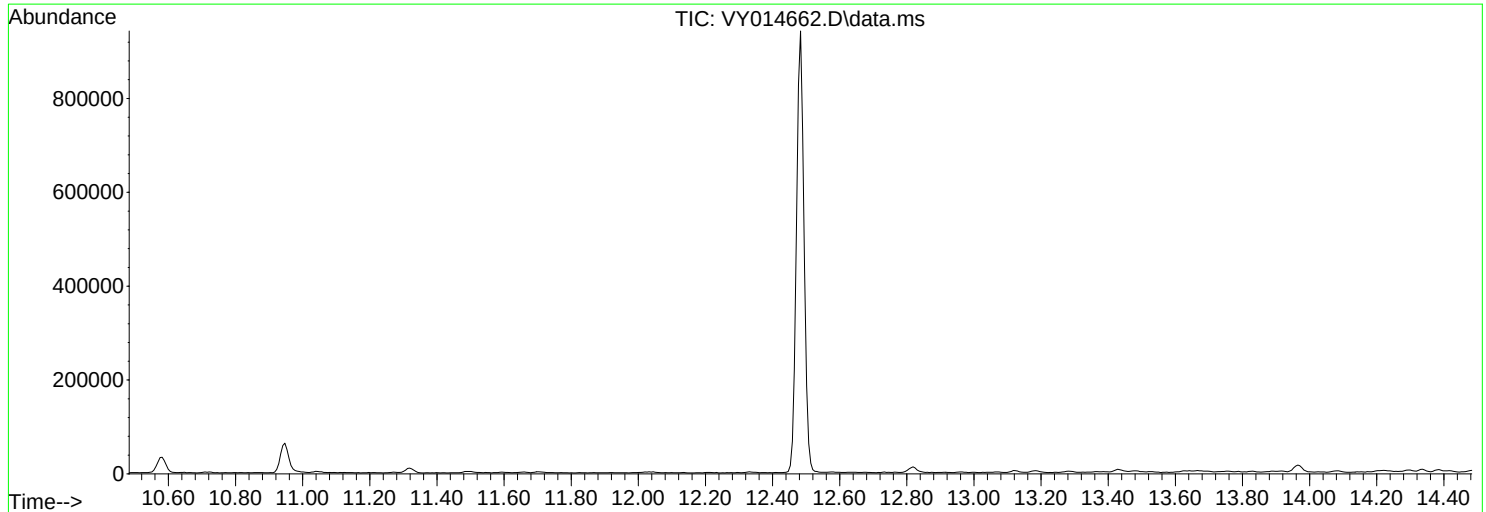

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1739

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.7	31360	PASS
75	95	30	60	50.7	84808	PASS
95	95	100	100	100.0	167339	PASS
96	95	5	9	6.5	10800	PASS
173	174	0.00	2	0.9	1201	PASS
174	95	50	100	79.6	133123	PASS
175	174	5	9	7.5	9946	PASS
176	174	95	101	98.0	130400	PASS
177	176	5	9	6.5	8417	PASS