

Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY072020\
 Data File : VY003244.D
 Acq On : 20 Jul 2020 20:02
 Operator : SY/MD
 Sample : L3308-18
 Misc : 5.00G/5ML/MSVOA Y/SOIL
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 18

Quant Time: Jul 21 05:20:53 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y071020S.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 10 13:18:03 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.80	168	323988	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.69	114	494025	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.49	117	432410	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.42	152	188001	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.14	65	181166	66.25	ug/l	0.00
Spiked Amount 50.000			Recovery	=	132.50%	
35) Dibromofluoromethane	7.72	113	161727	56.89	ug/l	0.00
Spiked Amount 50.000			Recovery	=	113.78%	
50) Toluene-d8	10.18	98	583074	55.16	ug/l	0.00
Spiked Amount 50.000			Recovery	=	110.32%	
62) 4-Bromofluorobenzene	12.48	95	177446	46.47	ug/l	0.00
Spiked Amount 50.000			Recovery	=	92.94%	
Target Compounds						
20) Methylene Chloride	4.73	84	35263	6.717	ug/l	Qvalue 95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA Y\DATA\VY072020\
Data File : VY003244.D
Acq On : 20 Jul 2020 20:02
Operator : SY/MD
Sample : L3308-18
Misc : 5.00G/5ML/MSVOA Y/SOIL
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
18

Quant Time: Jul 21 05:20:53 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_Y\METHODS\82Y071020S.M
Quant Title : SW846 8260
QLast Update : Fri Jul 10 13:18:03 2020
Response via : Initial Calibration

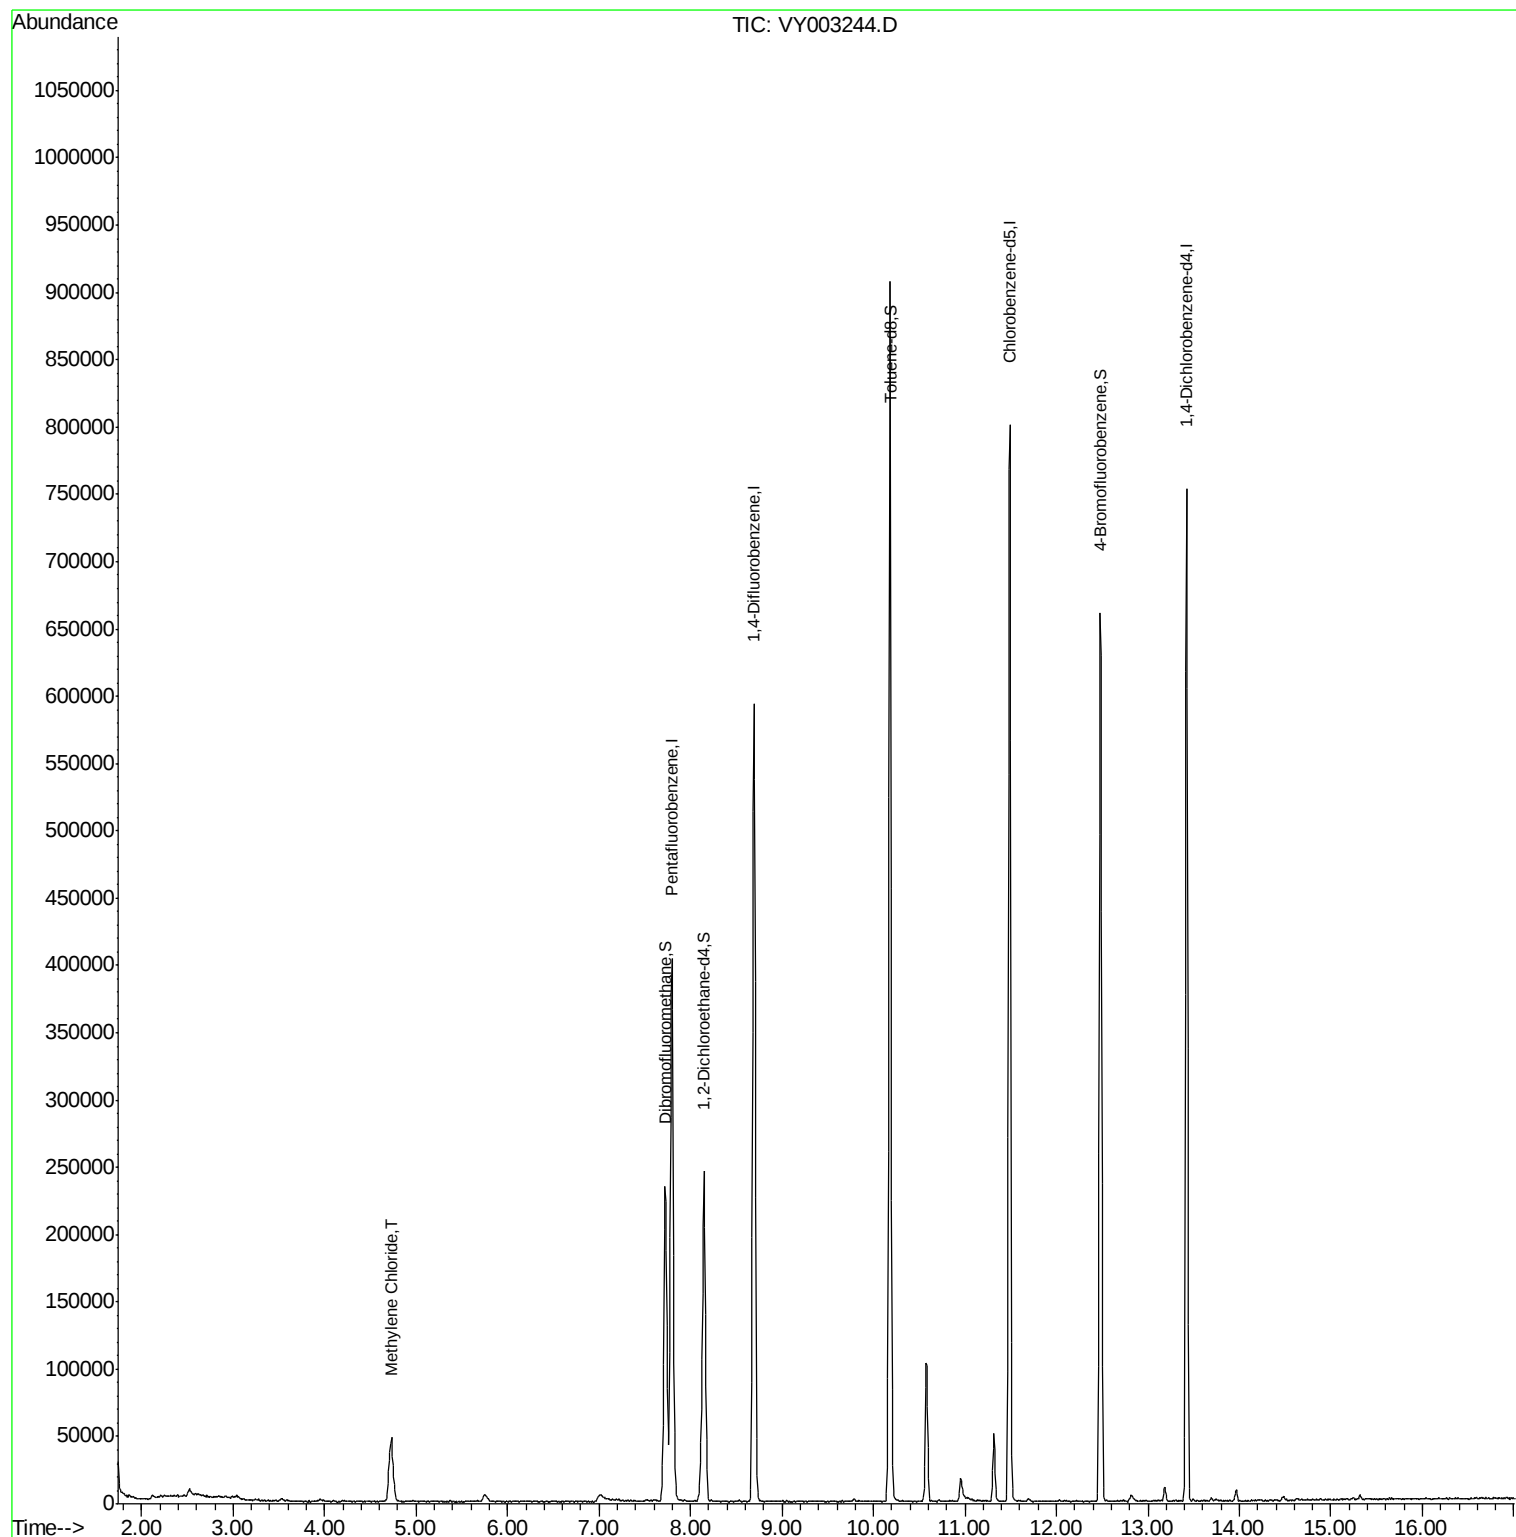



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.80 min Scan# 994

Delta R.T. -0.00 min

Lab File: VY003244.D

Acq: 20 Jul 2020 20:02

Instrument :

MSVOA_Y

ClientSampleId :


18

Tot Ion:168 Resp: 323988

Ion Ratio Lower Upper

168 100

99 51.0 37.3 55.9

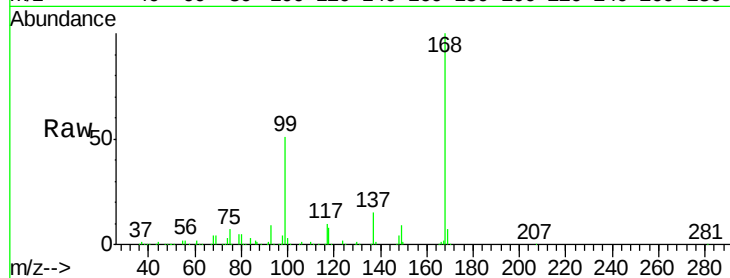

Abundance Ion 167.90 (167.60 to 168.60): VY003159.D (-983) (-)

Ion 98.90 (98.60 to 99.60): VY003159.D (-983) (-)

7.80



150000

100000

50000

0

Time-->

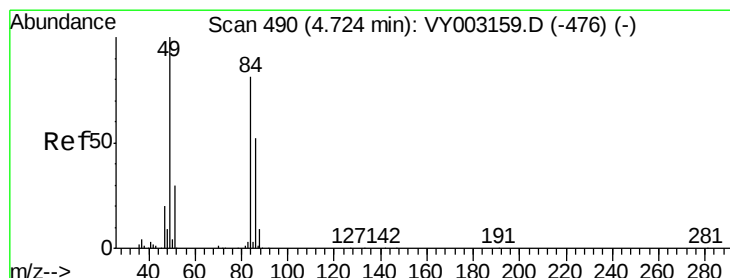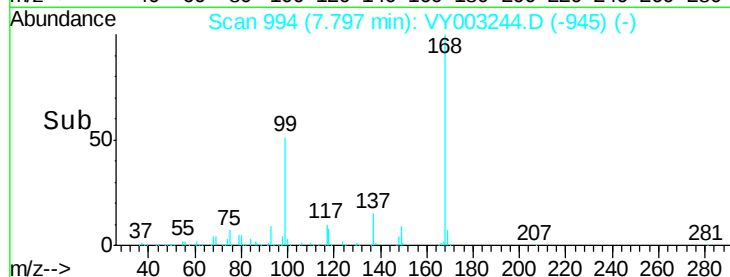

#20

Methylene Chloride

Concen: 6.717 ug/l

RT: 4.73 min Scan# 491

Delta R.T. 0.01 min

Lab File: VY003244.D

Acq: 20 Jul 2020 20:02

Tgt Ion: 84 Resp: 35263


Ion Ratio Lower Upper

84 100

49 130.2 98.2 147.4

51 37.2 29.8 44.6

86 59.7 51.2 76.8

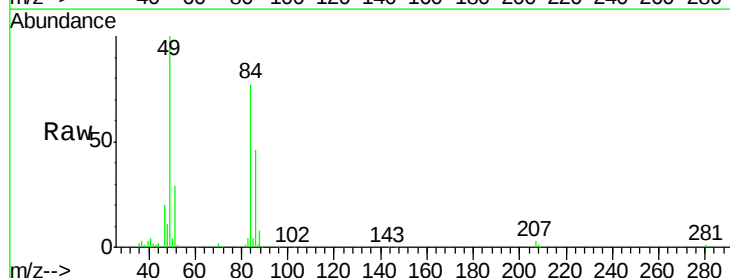

Abundance Ion 83.90 (83.60 to 84.60): VY003159.D (-476) (-)

Ion 48.90 (48.60 to 49.60): VY003159.D (-476) (-)

Ion 50.90 (50.60 to 51.60): VY003159.D (-476) (-)

Ion 85.90 (85.60 to 86.60): VY003159.D (-476) (-)

4.73

20000


15000


10000

5000

0

Time-->




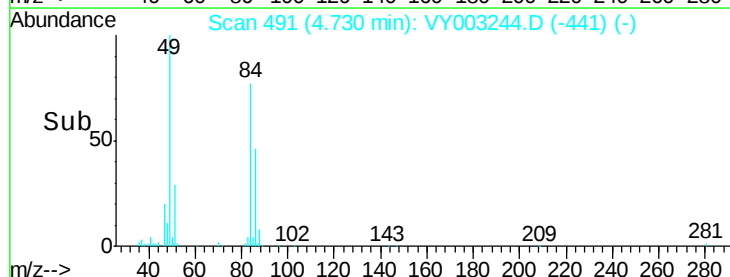


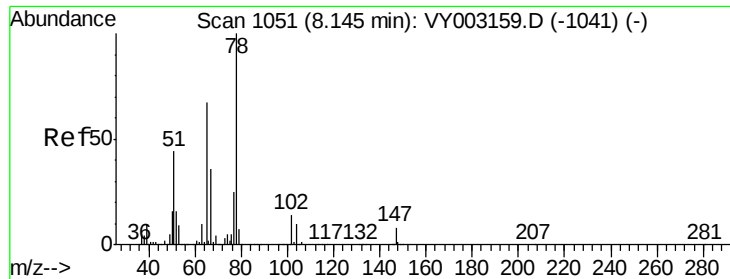

#33
 1,2-Dichloroethane-d4
 Concen: 66.250 ug/l
 RT: 8.14 min Scan# 1051
 Delta R.T. -0.00 min
 Lab File: VY003244.D
 Acq: 20 Jul 2020 20:02




Instrument :
 MSVOA_Y
 ClientSampleId :
 18


Tot Ion: 65 Resp: 181166
 Ion Ratio Lower Upper
 65 100
 67 52.1 0.0 105.2

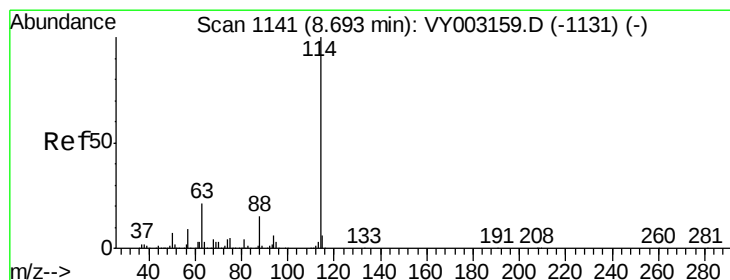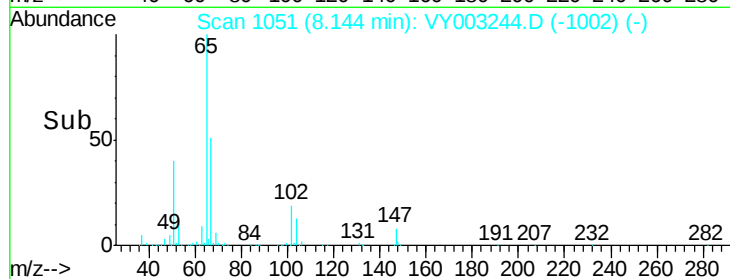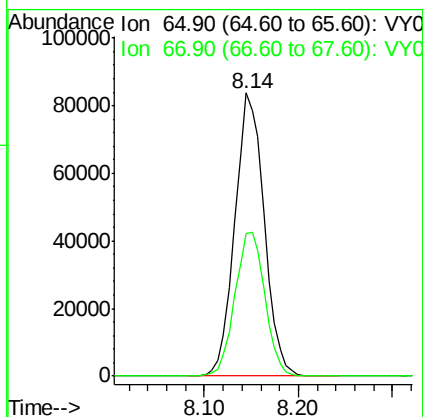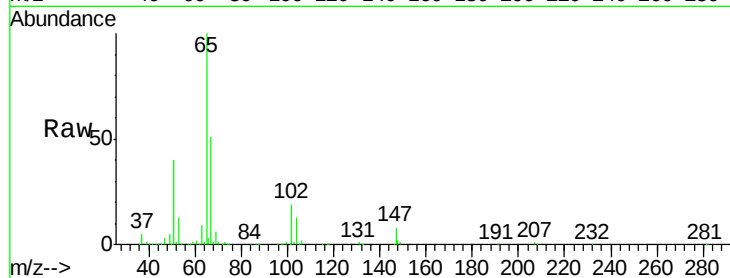

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.69 min Scan# 1141
 Delta R.T. -0.00 min
 Lab File: VY003244.D
 Acq: 20 Jul 2020 20:02

Tgt Ion: 114 Resp: 494025
 Ion Ratio Lower Upper
 114 100
 63 20.6 0.0 41.2
 88 15.0 0.0 30.2


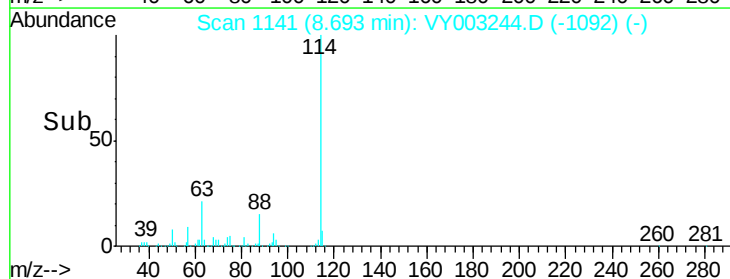
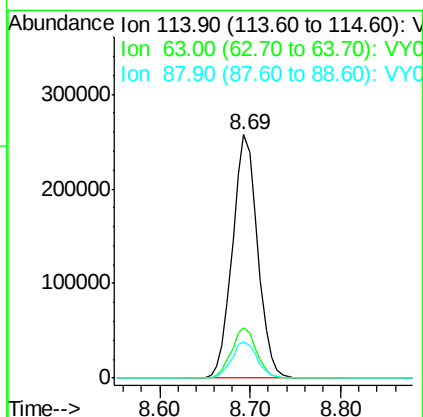
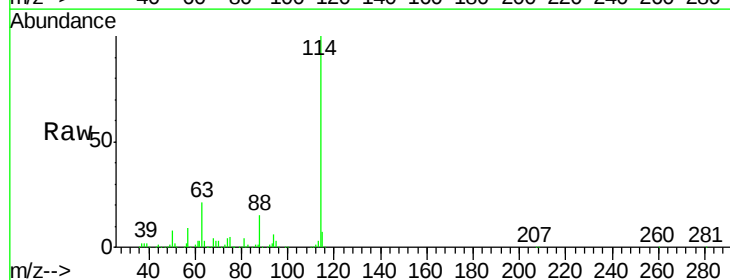


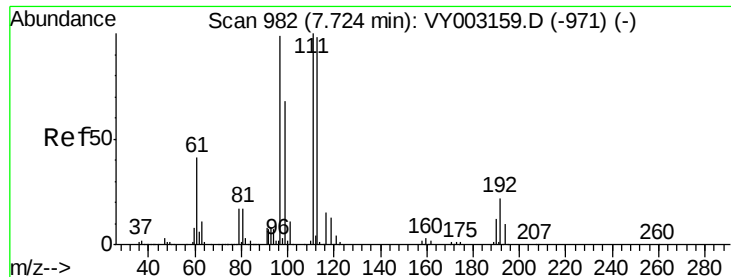

#35
Dibromofluoromethane
Concen: 56.886 ug/l
RT: 7.72 min Scan# 982
Delta R.T. -0.00 min
Lab File: VY003244.D
Acq: 20 Jul 2020 20:02




Instrument :
MSVOA_Y
ClientSampleId :
18


Tot Ion	Ratio	Lower	Upper
113	100		
111	102.4	82.1	123.1
192	22.3	18.8	28.2

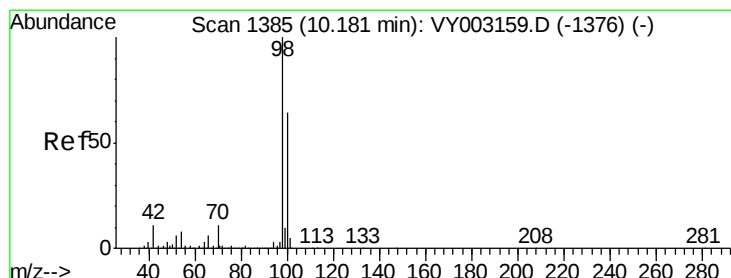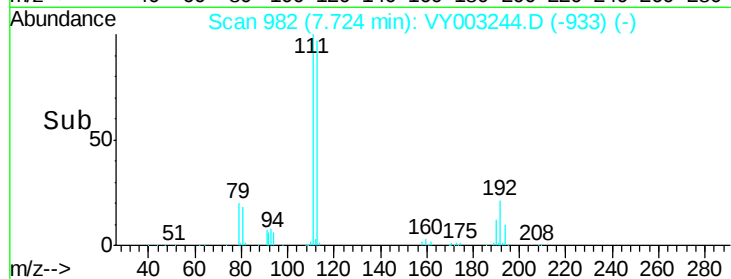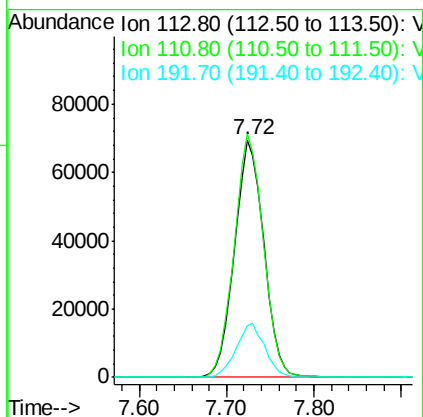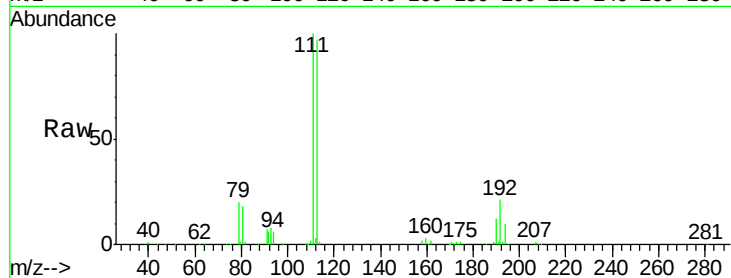

#50
Toluene-d8
Concen: 55.164 ug/l
RT: 10.18 min Scan# 1385
Delta R.T. -0.00 min
Lab File: VY003244.D
Acq: 20 Jul 2020 20:02

Tgt Ion	Ratio	Lower	Upper
98	100		
100	63.8	50.7	76.1

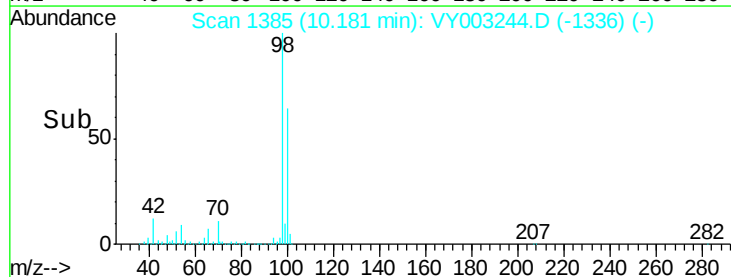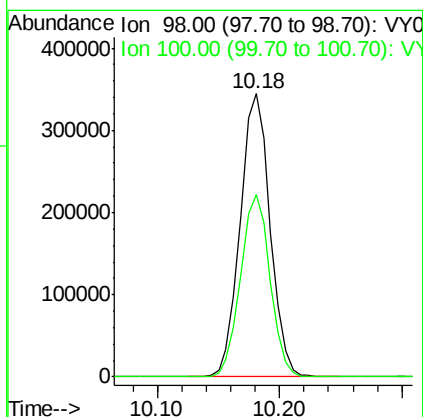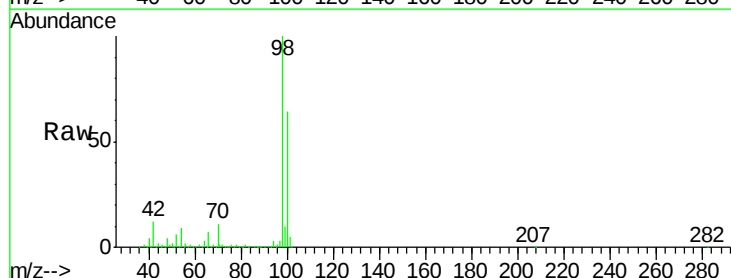

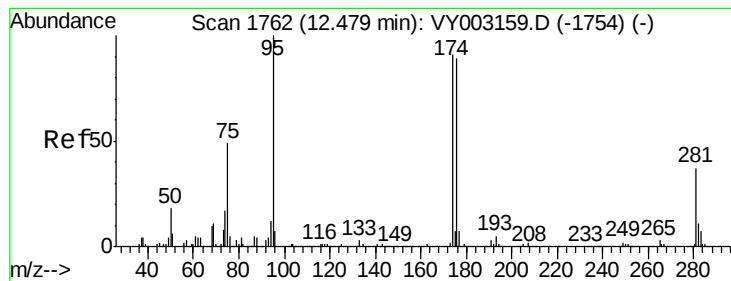

#62

4-Bromofluorobenzene

Concen: 46.471 ug/l

RT: 12.48 min Scan# 1762

Delta R.T. -0.00 min

Lab File: VY003244.D

Acq: 20 Jul 2020 20:02

Instrument :

MSVOA_Y

ClientSampleId :

18


Tot Ion: 95 Resp: 177446

Ion Ratio Lower Upper

95 100

174 94.8 0.0 190.6




176 91.4 0.0 186.4

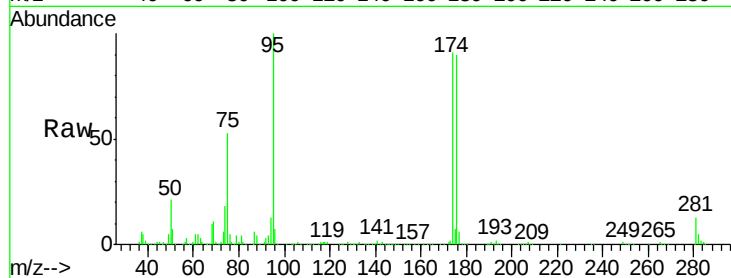

Abundance Ion 94.90 (94.60 to 95.60): VY003244.D (-1754) (-)

Ion 173.80 (173.50 to 174.50): VY003244.D (-1754) (-)

Ion 175.80 (175.50 to 176.50): VY003244.D (-1754) (-)

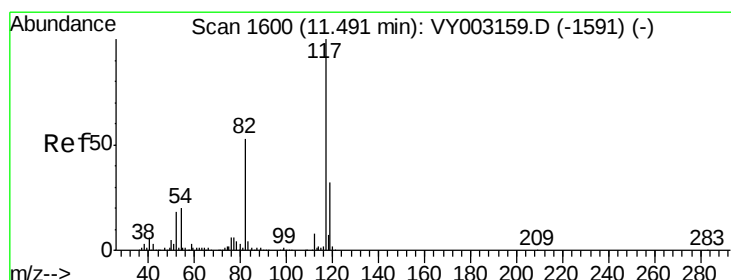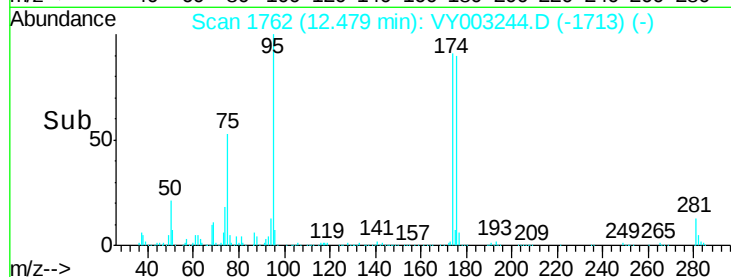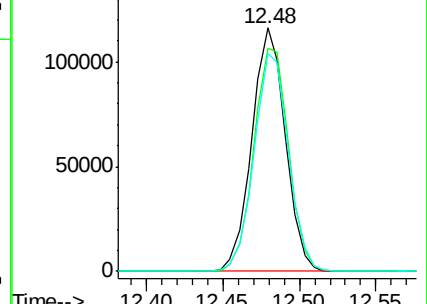

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.49 min Scan# 1600

Delta R.T. -0.00 min

Lab File: VY003244.D

Acq: 20 Jul 2020 20:02


Tgt Ion: 117 Resp: 432410

Ion Ratio Lower Upper

117 100

82 54.0 42.0 63.0



119 31.4 25.5 38.3

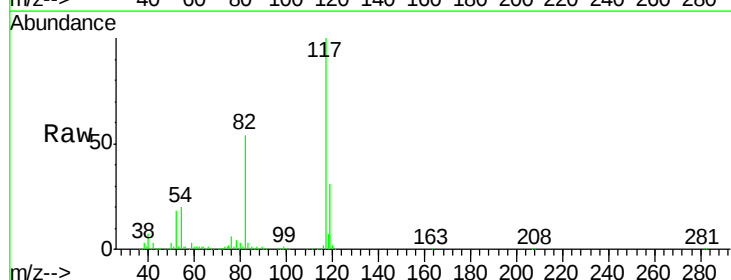


Abundance Ion 116.90 (116.60 to 117.60): VY003244.D (-1551) (-)

Ion 82.00 (81.70 to 82.70): VY003244.D (-1551) (-)

Ion 118.90 (118.60 to 119.60): VY003244.D (-1551) (-)

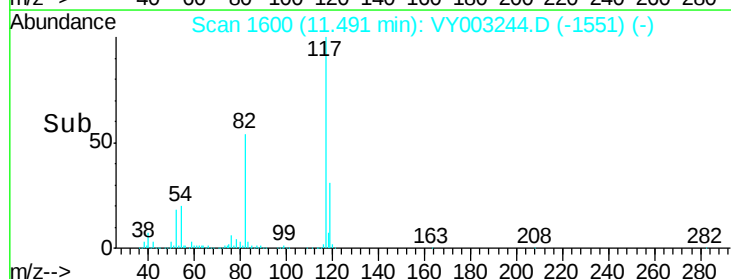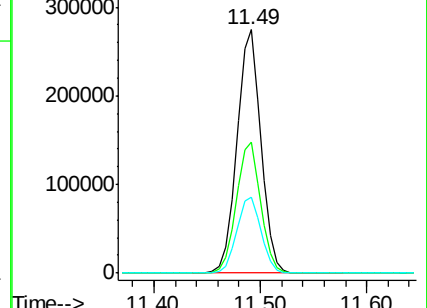

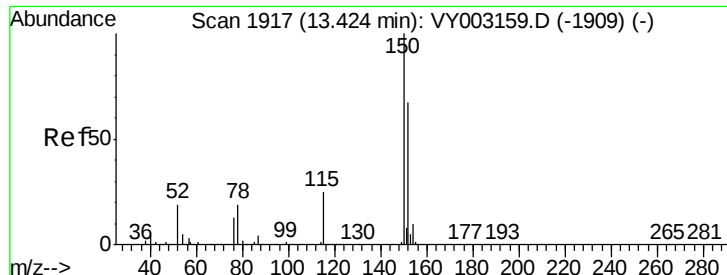

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.42 min Scan# 1917

Delta R.T. -0.00 min

Lab File: VY003244.D

Acq: 20 Jul 2020 20:02

Instrument :

MSVOA_Y

ClientSampleId :

18


Tot Ion:152 Resp: 188001

Ion Ratio Lower Upper

152 100

115 55.7 26.9 80.7

150 157.0 0.0 338.0

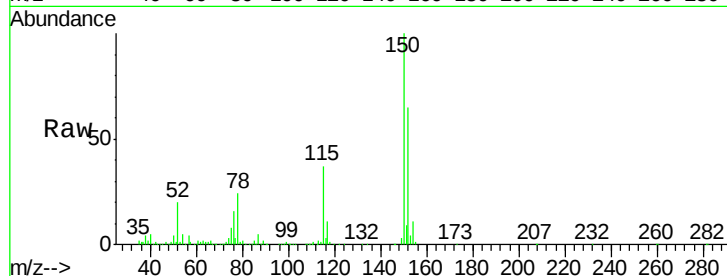

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

