

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY072023\
 Data File : VY014728.D
 Acq On : 20 Jul 2023 18:02
 Operator : SY/MD
 Sample : 03681-03
 Misc : 5.56g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 RPTP-1-GRAB-4

Quant Time: Jul 21 01:34:13 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y071323S.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 14 02:09:50 2023
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.789	168	238174	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	412381	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	384879	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	184624	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	139787	51.504	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	103.000%
35) Dibromofluoromethane	7.716	113	130005	49.523	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	99.040%
50) Toluene-d8	10.179	98	480287	49.625	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	99.260%
62) 4-Bromofluorobenzene	12.477	95	183034	49.322	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	98.640%
Target Compounds						
						Qvalue
95) Naphthalene	15.233	128	18647	2.143	ug/l	# 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY072023\
Data File : VY014728.D
Acq On : 20 Jul 2023 18:02
Operator : SY/MD
Sample : 03681-03
Misc : 5.56g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
RPTP-1-GRAB-4

Quant Time: Jul 21 01:34:13 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y071323S.M
Quant Title : SW846 8260
QLast Update : Fri Jul 14 02:09:50 2023
Response via : Initial Calibration




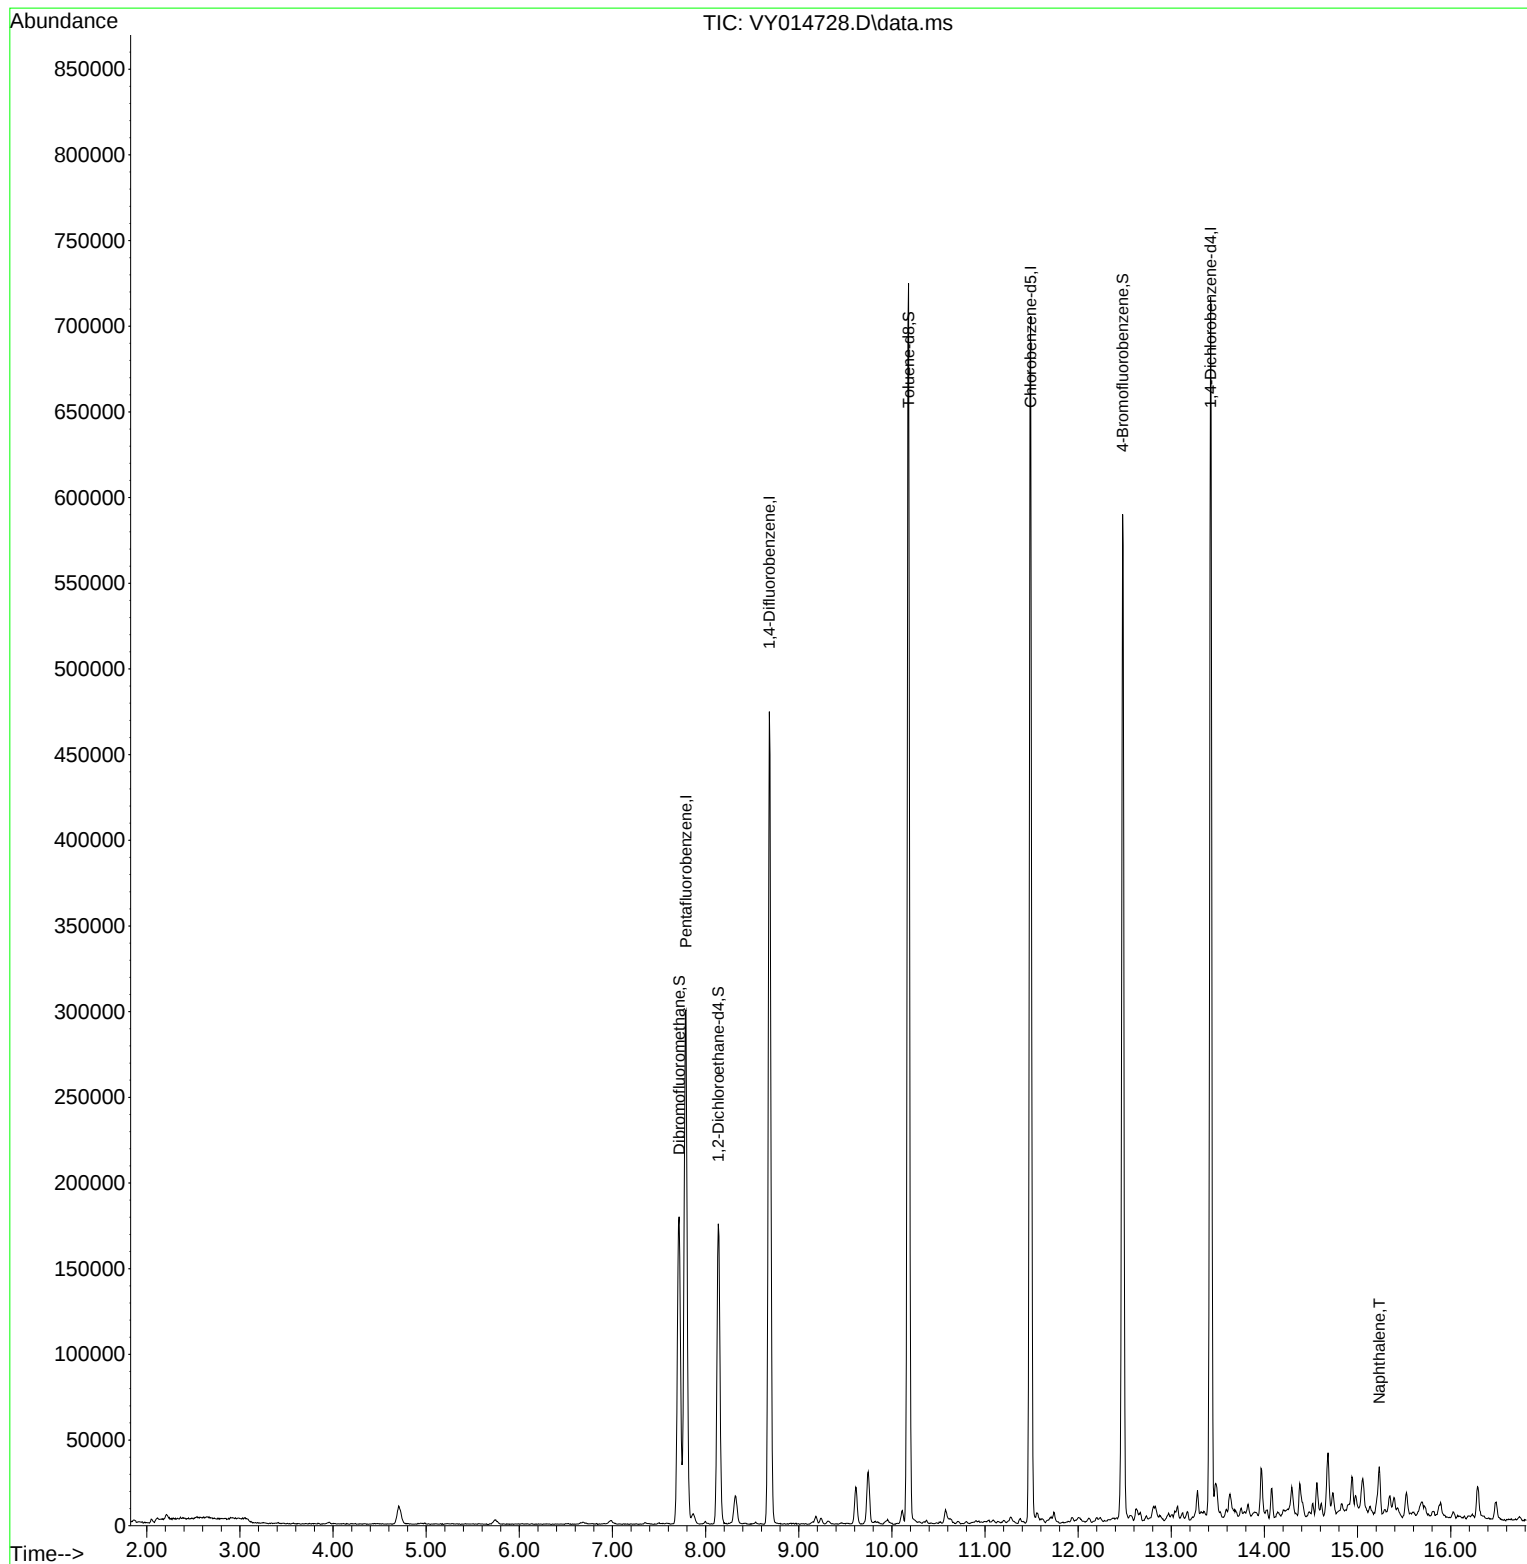


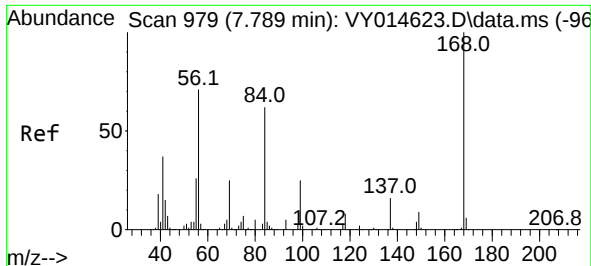

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. 0.000 min
Lab File: VY014728.D
Acq: 20 Jul 2023 18:02




Instrument :
MSVOA_Y
ClientSampleId :
RPTP-1-GRAB-4


Tgt Ion:168 Resp: 238174
Ion Ratio Lower Upper
168 100
99 54.2 43.4 65.0

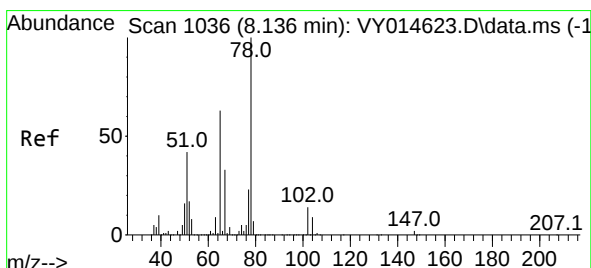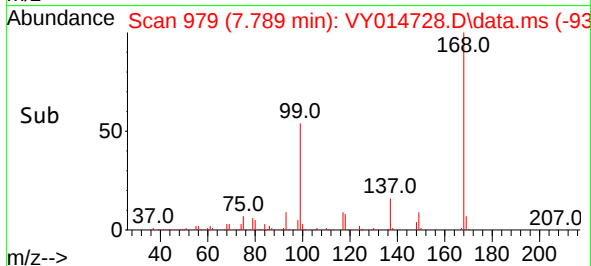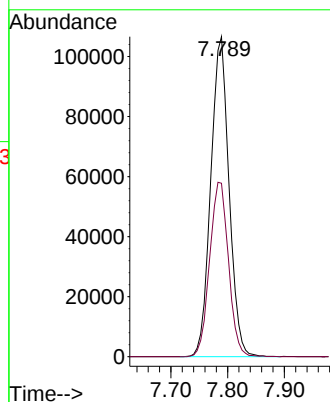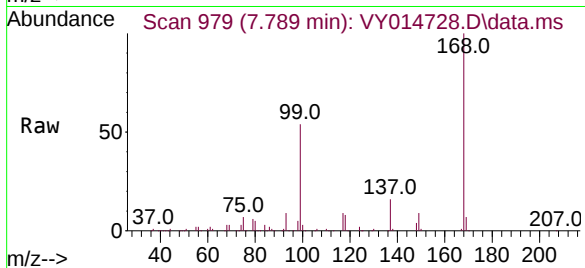

#33
1,2-Dichloroethane-d4
Concen: 51.504 ug/l
RT: 8.136 min Scan# 1036
Delta R.T. 0.001 min
Lab File: VY014728.D
Acq: 20 Jul 2023 18:02

Tgt Ion: 65 Resp: 139787
Ion Ratio Lower Upper
65 100
67 52.5 0.0 101.8

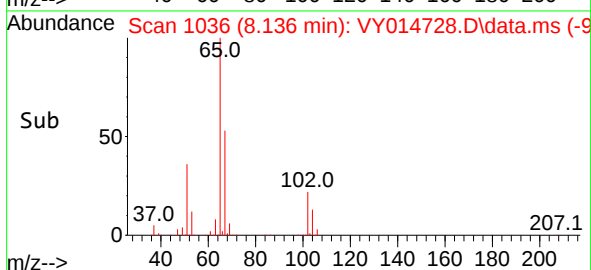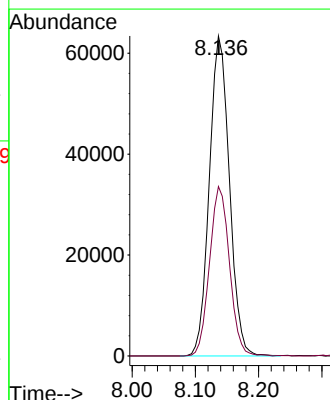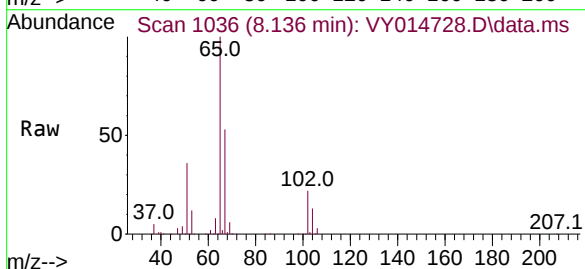

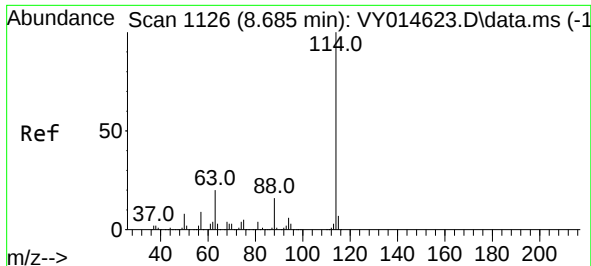

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.685 min Scan# 1126

Delta R.T. 0.000 min

Lab File: VY014728.D

Acq: 20 Jul 2023 18:02

Instrument :

MSVOA_Y

ClientSampleId :

RPTP-1-GRAB-4





Tgt Ion:114 Resp: 412381

Ion Ratio Lower Upper

114 100

63 18.9 0.0 42.4

88 15.6 0.0 30.6

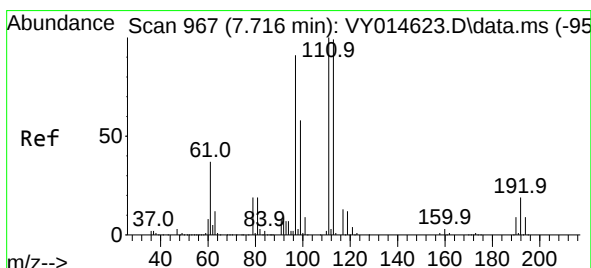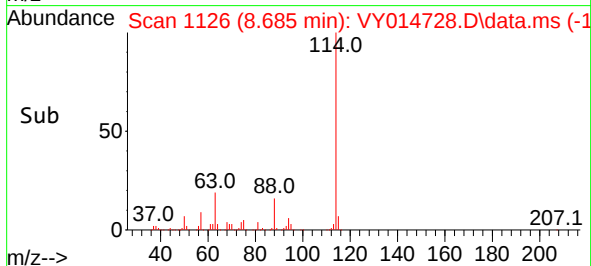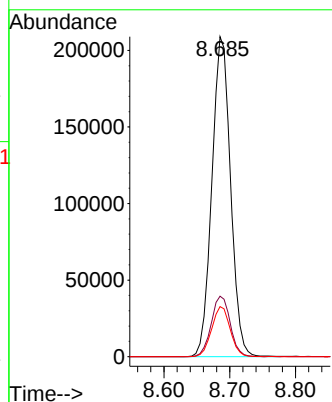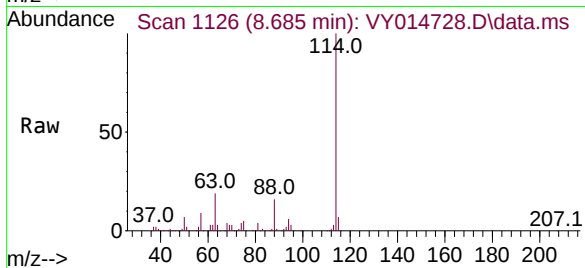

#35

Dibromofluoromethane

Concen: 49.523 ug/l

RT: 7.716 min Scan# 967

Delta R.T. -0.000 min

Lab File: VY014728.D

Acq: 20 Jul 2023 18:02




Tgt Ion:113 Resp: 130005


Ion Ratio Lower Upper

113 100

111 101.5 81.3 121.9

192 20.1 16.9 25.3

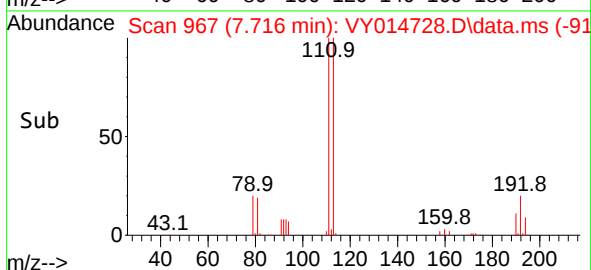
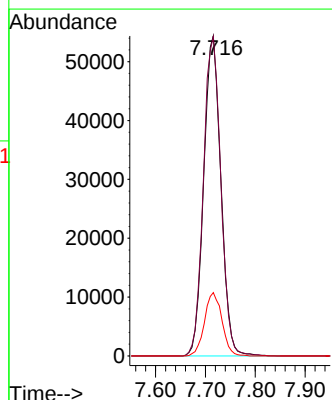
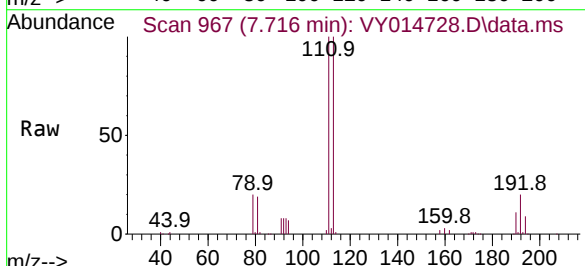


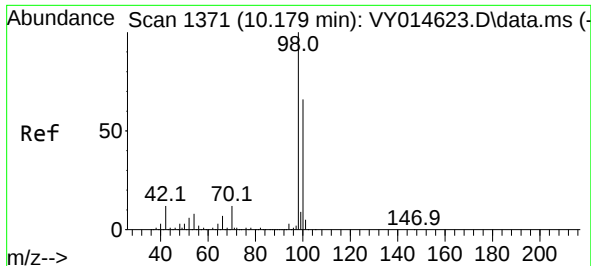

#50
Toluene-d8
Concen: 49.625 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. -0.000 min
Lab File: VY014728.D
Acq: 20 Jul 2023 18:02




Instrument :
MSVOA_Y
ClientSampleId :
RPTP-1-GRAB-4


Tgt Ion: 98 Resp: 480287
Ion Ratio Lower Upper
98 100
100 65.5 50.1 75.1

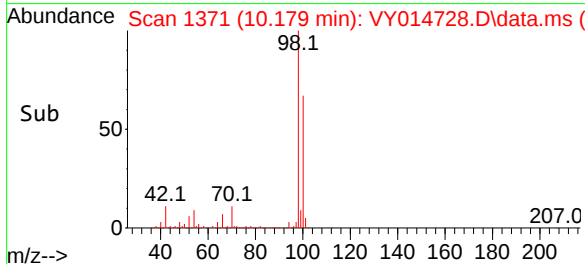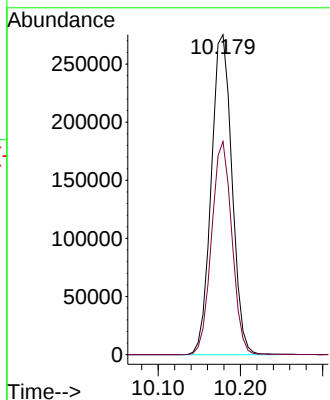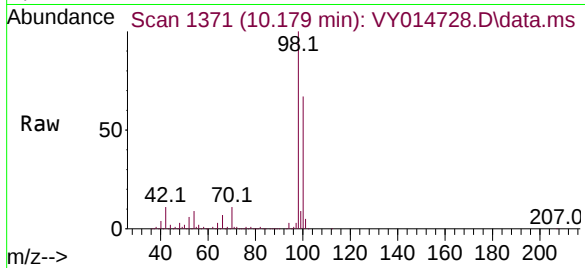

#62
4-Bromofluorobenzene
Concen: 49.322 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. 0.000 min
Lab File: VY014728.D
Acq: 20 Jul 2023 18:02

Tgt Ion: 95 Resp: 183034
Ion Ratio Lower Upper
95 100
174 81.8 0.0 178.2
176 78.8 0.0 173.8


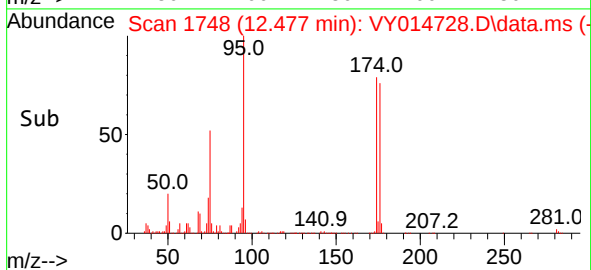
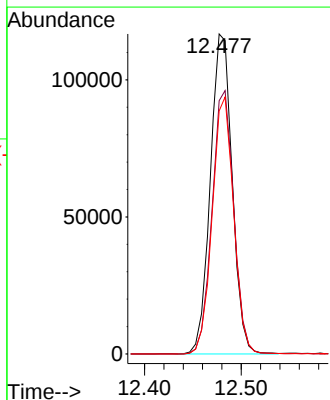
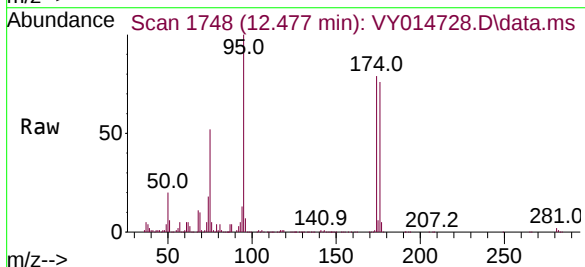


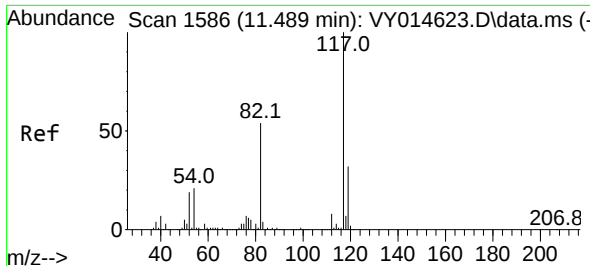

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.490 min Scan# 117
Delta R.T. 0.001 min
Lab File: VY014728.D
Acq: 20 Jul 2023 18:02




Instrument :
MSVOA_Y
ClientSampleId :
RPTP-1-GRAB-4


Tgt Ion:117 Resp: 384879
Ion Ratio Lower Upper
117 100
82 53.9 43.4 65.0
119 32.0 26.3 39.5

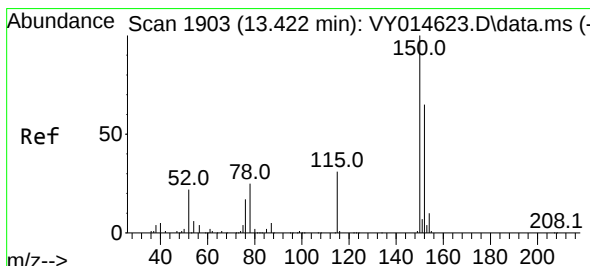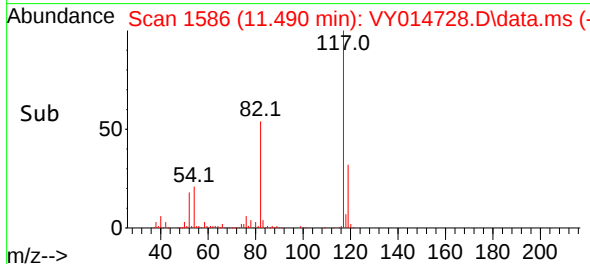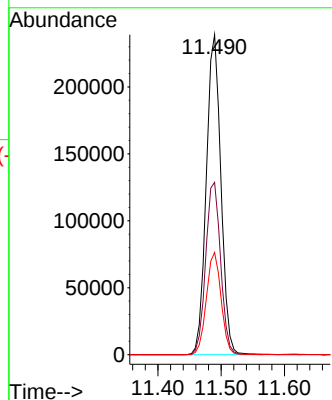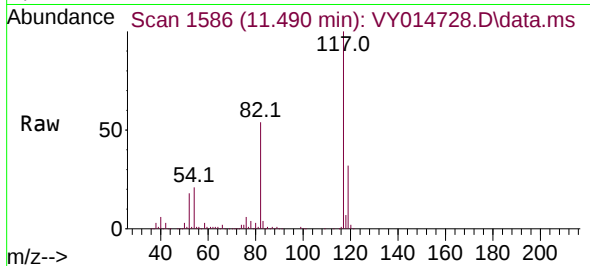

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.422 min Scan# 1903
Delta R.T. 0.000 min
Lab File: VY014728.D
Acq: 20 Jul 2023 18:02

Tgt Ion:152 Resp: 184624
Ion Ratio Lower Upper
152 100
115 58.6 28.8 86.5
150 156.6 0.0 348.8

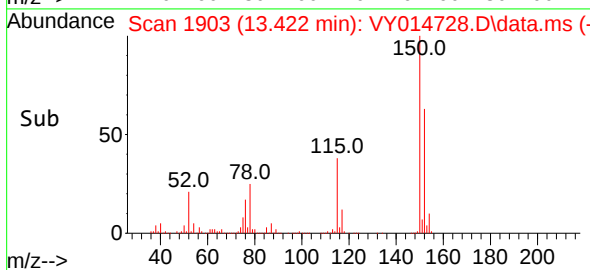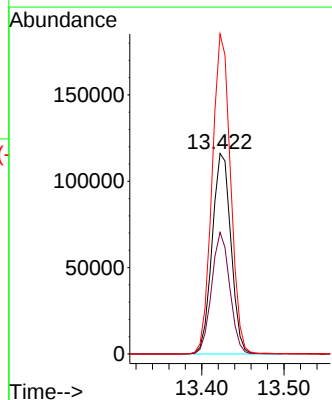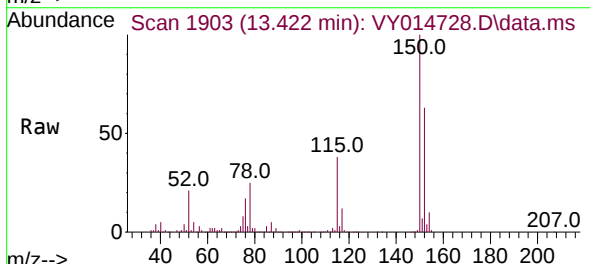

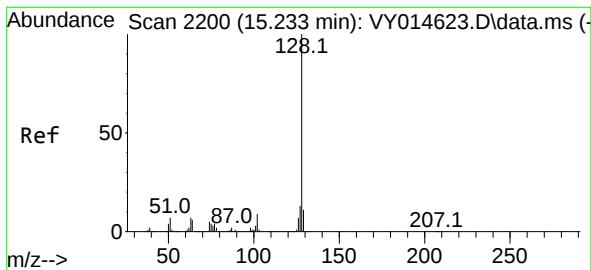

#95

Naphthalene

Concen: 2.143 ug/l

RT: 15.233 min Scan# 21

Delta R.T. -0.000 min

Lab File: VY014728.D


Acq: 20 Jul 2023 18:02

Instrument :

MSVOA_Y

ClientSampleId :

RPTP-1-GRAB-4

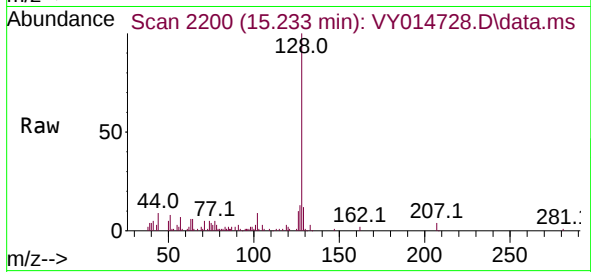

Tgt Ion:128 Resp: 18647

Ion Ratio Lower Upper

128 100

127 15.9 10.8 16.2

129 13.0 8.6 13.0#

