

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY072122\  
 Data File : VY009626.D  
 Acq On : 21 Jul 2022 12:14  
 Operator : KP/MD  
 Sample : N3726-01  
 Misc : 6.06g/5.0mL/MSVOA\_Y/SOIL  
 ALS Vial : 7 Sample Multiplier: 1

Instrument :  
 MSVOA\_Y  
 ClientSampleId :  
 HL-12-12.5

Quant Time: Jul 22 02:29:09 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y071822S.M  
 Quant Title : SW846 8260  
 QLast Update : Tue Jul 19 04:22:09 2022  
 Response via : Initial Calibration

| Compound                   | R.T.   | QIon | Response | Conc   | Units | Dev(Min) |
|----------------------------|--------|------|----------|--------|-------|----------|
| -----                      |        |      |          |        |       |          |
| Internal Standards         |        |      |          |        |       |          |
| 1) Pentafluorobenzene      | 7.783  | 168  | 192494   | 50.000 | ug/l  | # 0.00   |
| 34) 1,4-Difluorobenzene    | 8.685  | 114  | 310369   | 50.000 | ug/l  | 0.00     |
| 63) Chlorobenzene-d5       | 11.489 | 117  | 285765   | 50.000 | ug/l  | 0.00     |
| 72) 1,4-Dichlorobenzene-d4 | 13.422 | 152  | 136340   | 50.000 | ug/l  | 0.00     |

|                             |        |       |          |          |      |         |
|-----------------------------|--------|-------|----------|----------|------|---------|
| System Monitoring Compounds |        |       |          |          |      |         |
| 33) 1,2-Dichloroethane-d4   | 8.136  | 65    | 84707    | 46.529   | ug/l | 0.00    |
| Spiked Amount               | 50.000 | Range | 50 - 163 | Recovery | =    | 93.060% |
| 35) Dibromofluoromethane    | 7.710  | 113   | 81863    | 41.867   | ug/l | 0.00    |
| Spiked Amount               | 50.000 | Range | 54 - 147 | Recovery | =    | 83.740% |
| 50) Toluene-d8              | 10.173 | 98    | 301496   | 40.110   | ug/l | 0.00    |
| Spiked Amount               | 50.000 | Range | 78 - 125 | Recovery | =    | 80.220% |
| 62) 4-Bromofluorobenzene    | 12.477 | 95    | 95535    | 39.223   | ug/l | 0.00    |
| Spiked Amount               | 50.000 | Range | 50 - 146 | Recovery | =    | 78.440% |


| Target Compounds | Qvalue |
|------------------|--------|
| -----            |        |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY072122\  
Data File : VY009626.D  
Acq On : 21 Jul 2022 12:14  
Operator : KP/MD  
Sample : N3726-01  
Misc : 6.06g/5.0mL/MSVOA\_Y/SOIL  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
MSVOA\_Y  
ClientSampleId :  
HL-12-12.5

Quant Time: Jul 22 02:29:09 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y071822S.M  
Quant Title : SW846 8260  
QLast Update : Tue Jul 19 04:22:09 2022  
Response via : Initial Calibration




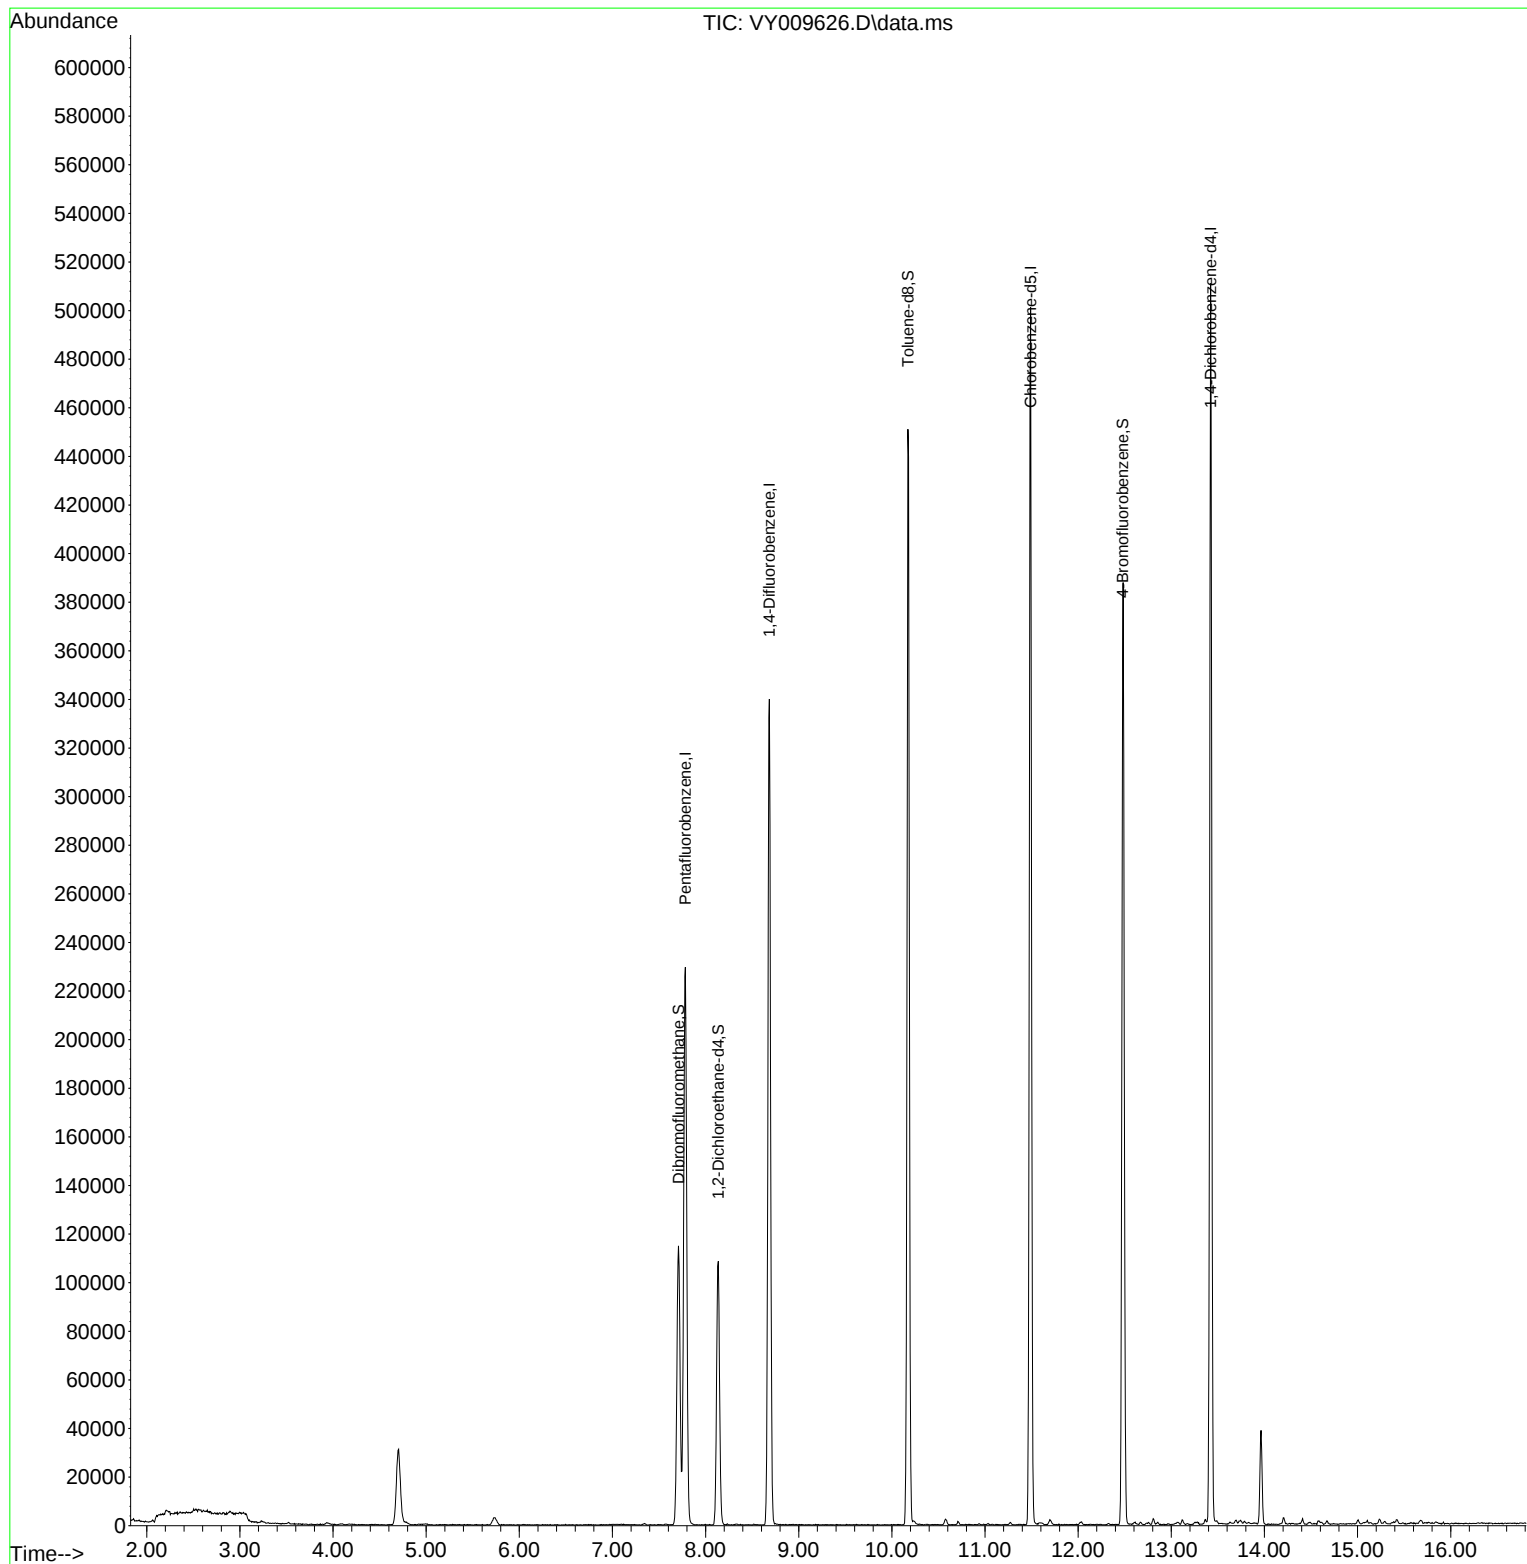


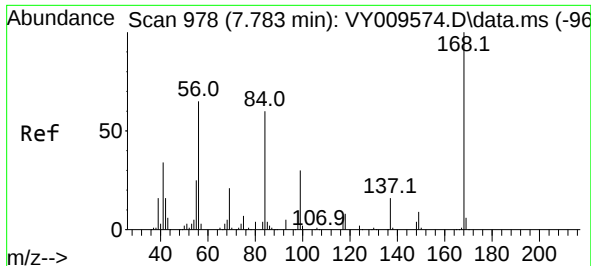

#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 7.783 min Scan# 91  
Delta R.T. -0.000 min  
Lab File: VY009626.D  
Acq: 21 Jul 2022 12:14




Instrument :  
MSVOA\_Y  
ClientSampleId :  
HL-12-12.5


Tgt Ion:168 Resp: 192494  
Ion Ratio Lower Upper  
168 100  
99 46.8 46.9 70.3#

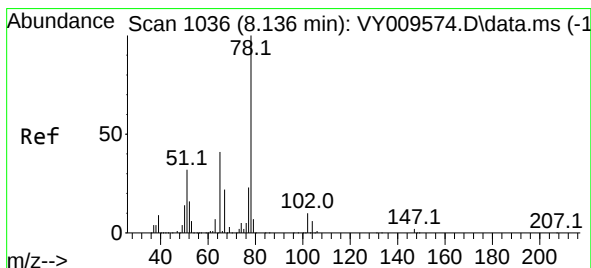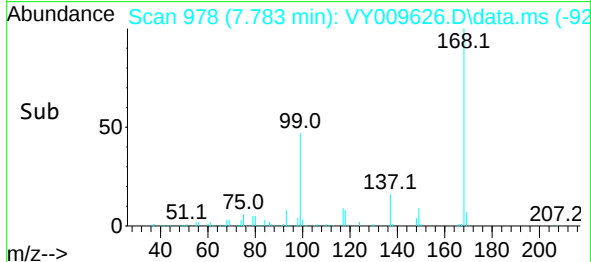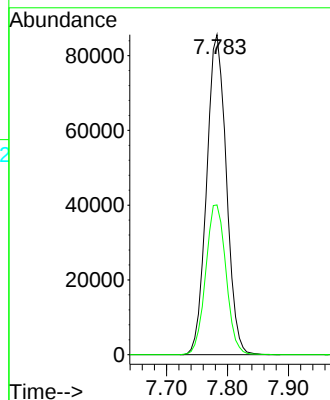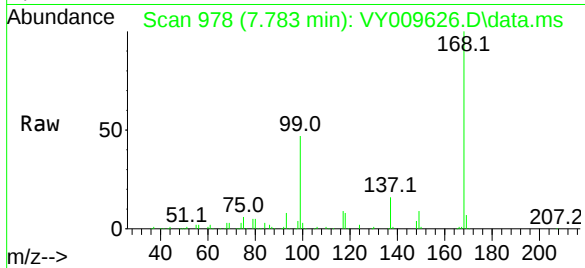

#33  
1,2-Dichloroethane-d4  
Concen: 46.529 ug/l  
RT: 8.136 min Scan# 1036  
Delta R.T. -0.000 min  
Lab File: VY009626.D  
Acq: 21 Jul 2022 12:14

Tgt Ion: 65 Resp: 84707  
Ion Ratio Lower Upper  
65 100  
67 52.8 0.0 99.4


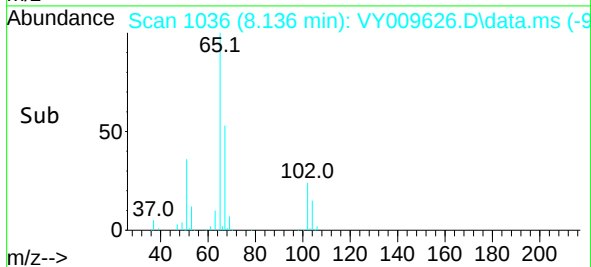
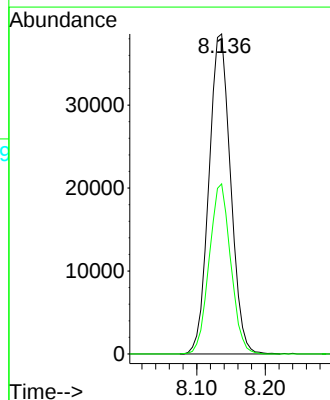
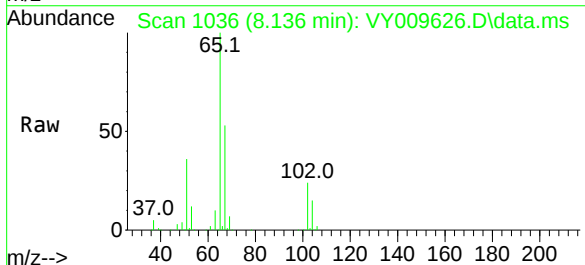


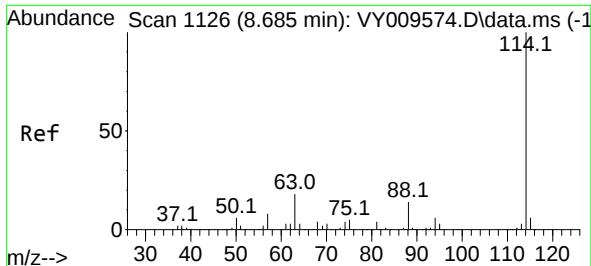

#34  
1,4-Difluorobenzene  
Concen: 50.000 ug/l  
RT: 8.685 min Scan# 1126  
Delta R.T. -0.000 min  
Lab File: VY009626.D  
Acq: 21 Jul 2022 12:14




Instrument :  
MSVOA\_Y  
ClientSampleId :  
HL-12-12.5


Tgt Ion:114 Resp: 310369  
Ion Ratio Lower Upper  
114 100  
63 16.5 0.0 43.2  
88 13.9 0.0 31.8

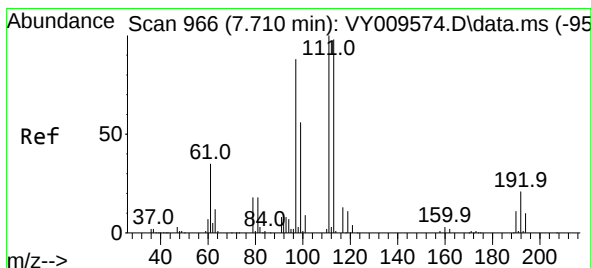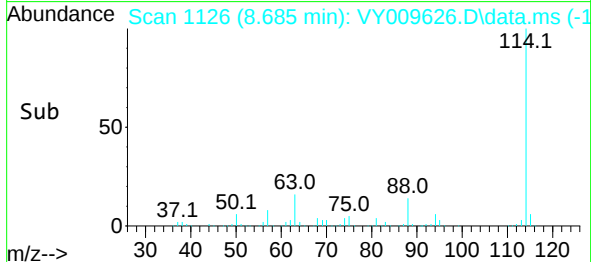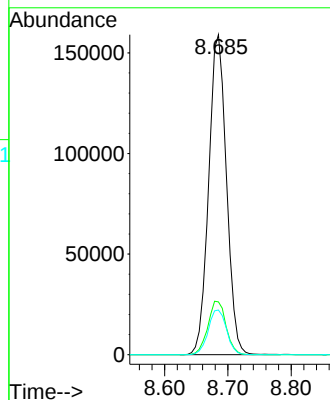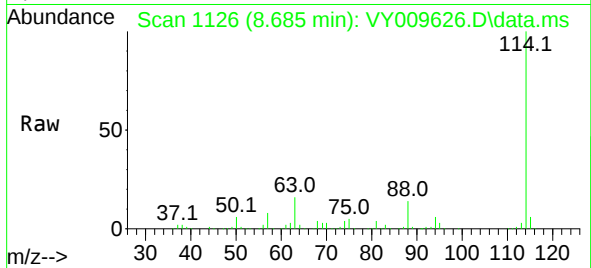

#35  
Dibromofluoromethane  
Concen: 41.867 ug/l  
RT: 7.710 min Scan# 966  
Delta R.T. -0.000 min  
Lab File: VY009626.D  
Acq: 21 Jul 2022 12:14

Tgt Ion:113 Resp: 81863  
Ion Ratio Lower Upper  
113 100  
111 102.9 82.6 124.0  
192 22.4 17.6 26.4


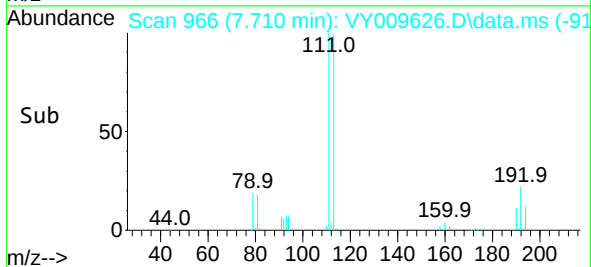
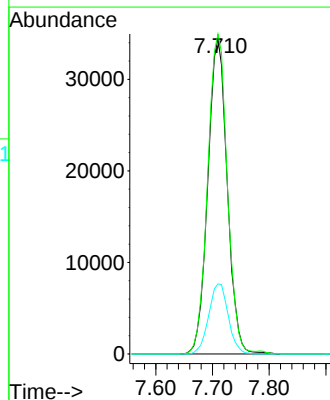
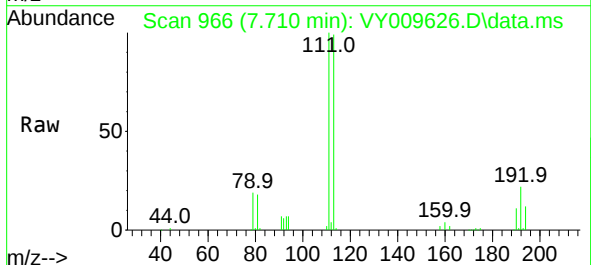


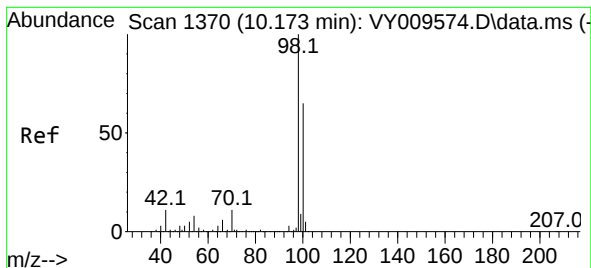

#50  
Toluene-d8  
Concen: 40.110 ug/l  
RT: 10.173 min Scan# 11  
Delta R.T. -0.000 min  
Lab File: VY009626.D  
Acq: 21 Jul 2022 12:14




Instrument :  
MSVOA\_Y  
ClientSampleId :  
HL-12-12.5


Tgt Ion: 98 Resp: 301496  
Ion Ratio Lower Upper  
98 100  
100 65.2 50.2 75.2

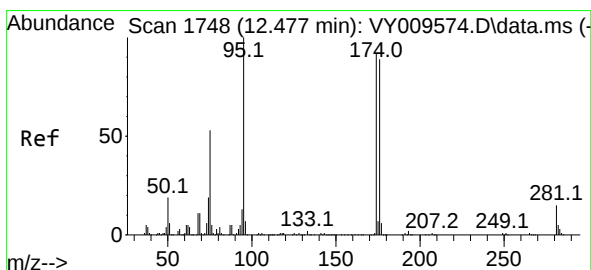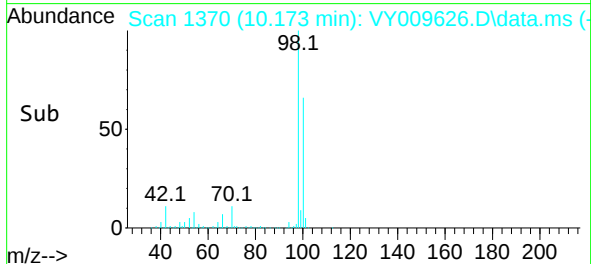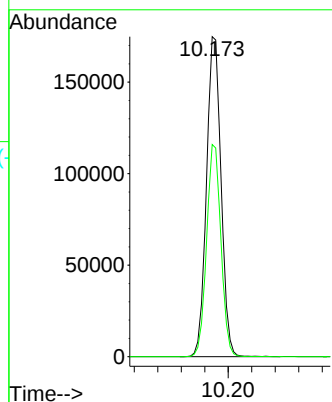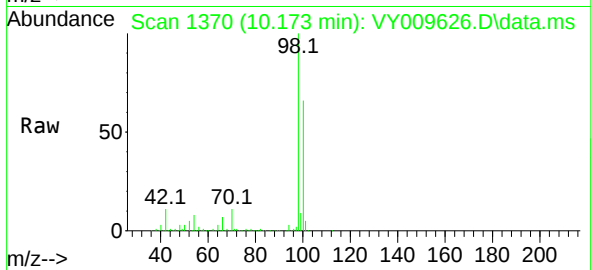

#62  
4-Bromofluorobenzene  
Concen: 39.223 ug/l  
RT: 12.477 min Scan# 1748  
Delta R.T. -0.000 min  
Lab File: VY009626.D  
Acq: 21 Jul 2022 12:14

Tgt Ion: 95 Resp: 95535  
Ion Ratio Lower Upper  
95 100  
174 96.5 0.0 177.0  
176 94.0 0.0 175.8

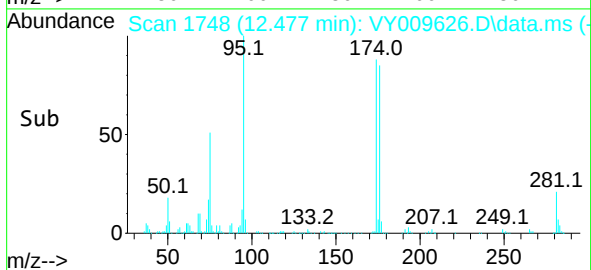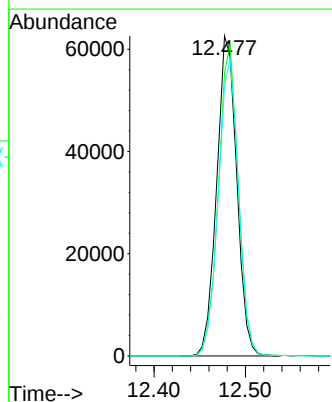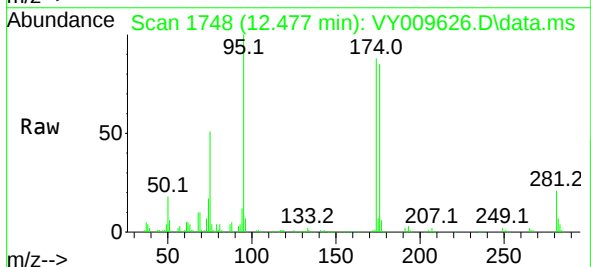

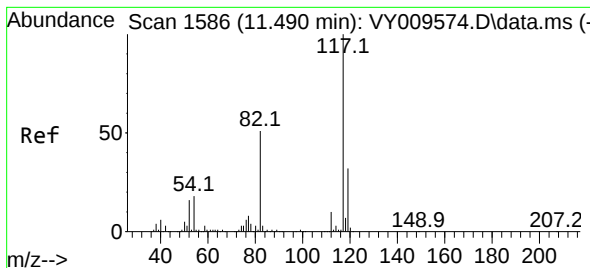

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.489 min Scan# 11

Delta R.T. -0.000 min

Lab File: VY009626.D

Acq: 21 Jul 2022 12:14

Instrument :

MSVOA\_Y

ClientSampleId :

HL-12-12.5





Tgt Ion:117 Resp: 285765

Ion Ratio Lower Upper

117 100

82 50.1 43.0 64.4

119 32.3 25.4 38.0

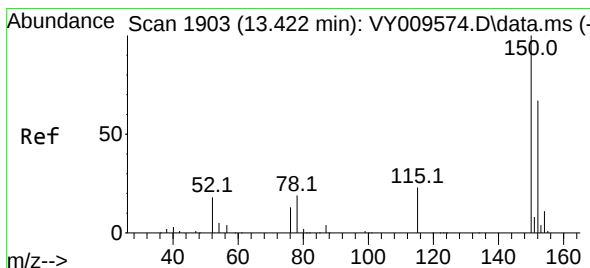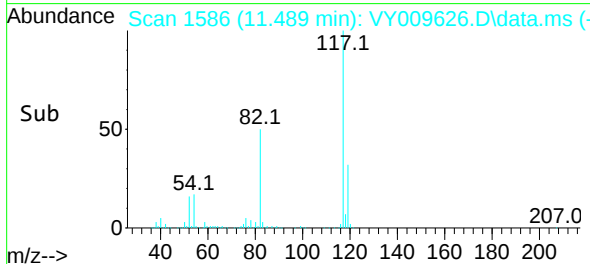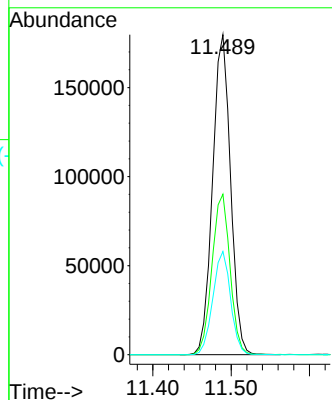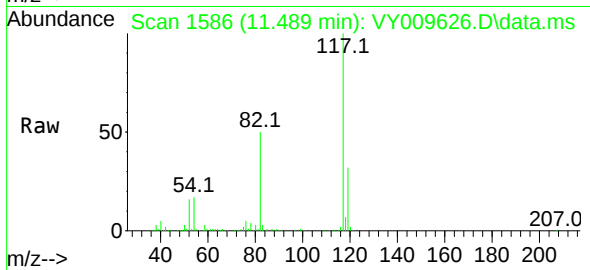

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.422 min Scan# 1903

Delta R.T. -0.000 min

Lab File: VY009626.D

Acq: 21 Jul 2022 12:14

Tgt Ion:152 Resp: 136340

Ion Ratio Lower Upper

152 100

115 54.3 28.2 84.7

150 156.2 0.0 347.6

