

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY072122\  
 Data File : VY009631.D  
 Acq On : 21 Jul 2022 14:19  
 Operator : KP/MD  
 Sample : N3786-03  
 Misc : 5.84g/5.0mL/MSVOA\_Y/SOIL  
 ALS Vial : 12 Sample Multiplier: 1

Instrument :  
 MSVOA\_Y  
 ClientSampleId :  
 0718-WC-TP-12EB

Quant Time: Jul 22 02:29:52 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y071822S.M  
 Quant Title : SW846 8260  
 QLast Update : Tue Jul 19 04:22:09 2022  
 Response via : Initial Calibration

| Compound                   | R.T.   | QIon | Response | Conc   | Units | Dev(Min) |
|----------------------------|--------|------|----------|--------|-------|----------|
| -----                      |        |      |          |        |       |          |
| Internal Standards         |        |      |          |        |       |          |
| 1) Pentafluorobenzene      | 7.783  | 168  | 134530   | 50.000 | ug/l  | 0.00     |
| 34) 1,4-Difluorobenzene    | 8.685  | 114  | 236004   | 50.000 | ug/l  | 0.00     |
| 63) Chlorobenzene-d5       | 11.490 | 117  | 227987   | 50.000 | ug/l  | 0.00     |
| 72) 1,4-Dichlorobenzene-d4 | 13.422 | 152  | 107383   | 50.000 | ug/l  | 0.00     |

|                             |        |       |          |          |      |          |
|-----------------------------|--------|-------|----------|----------|------|----------|
| System Monitoring Compounds |        |       |          |          |      |          |
| 33) 1,2-Dichloroethane-d4   | 8.130  | 65    | 80095    | 62.952   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 50 - 163 | Recovery | =    | 125.900% |
| 35) Dibromofluoromethane    | 7.704  | 113   | 76487    | 51.443   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 54 - 147 | Recovery | =    | 102.880% |
| 50) Toluene-d8              | 10.173 | 98    | 274566   | 48.037   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 78 - 125 | Recovery | =    | 96.080%  |
| 62) 4-Bromofluorobenzene    | 12.477 | 95    | 87514    | 47.252   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 50 - 146 | Recovery | =    | 94.500%  |


| Target Compounds | Qvalue |
|------------------|--------|
| -----            |        |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY072122\  
Data File : VY009631.D  
Acq On : 21 Jul 2022 14:19  
Operator : KP/MD  
Sample : N3786-03  
Misc : 5.84g/5.0mL/MSVOA\_Y/SOIL  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
MSVOA\_Y  
ClientSampleId :  
0718-WC-TP-12EB

Quant Time: Jul 22 02:29:52 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y071822S.M  
Quant Title : SW846 8260  
QLast Update : Tue Jul 19 04:22:09 2022  
Response via : Initial Calibration




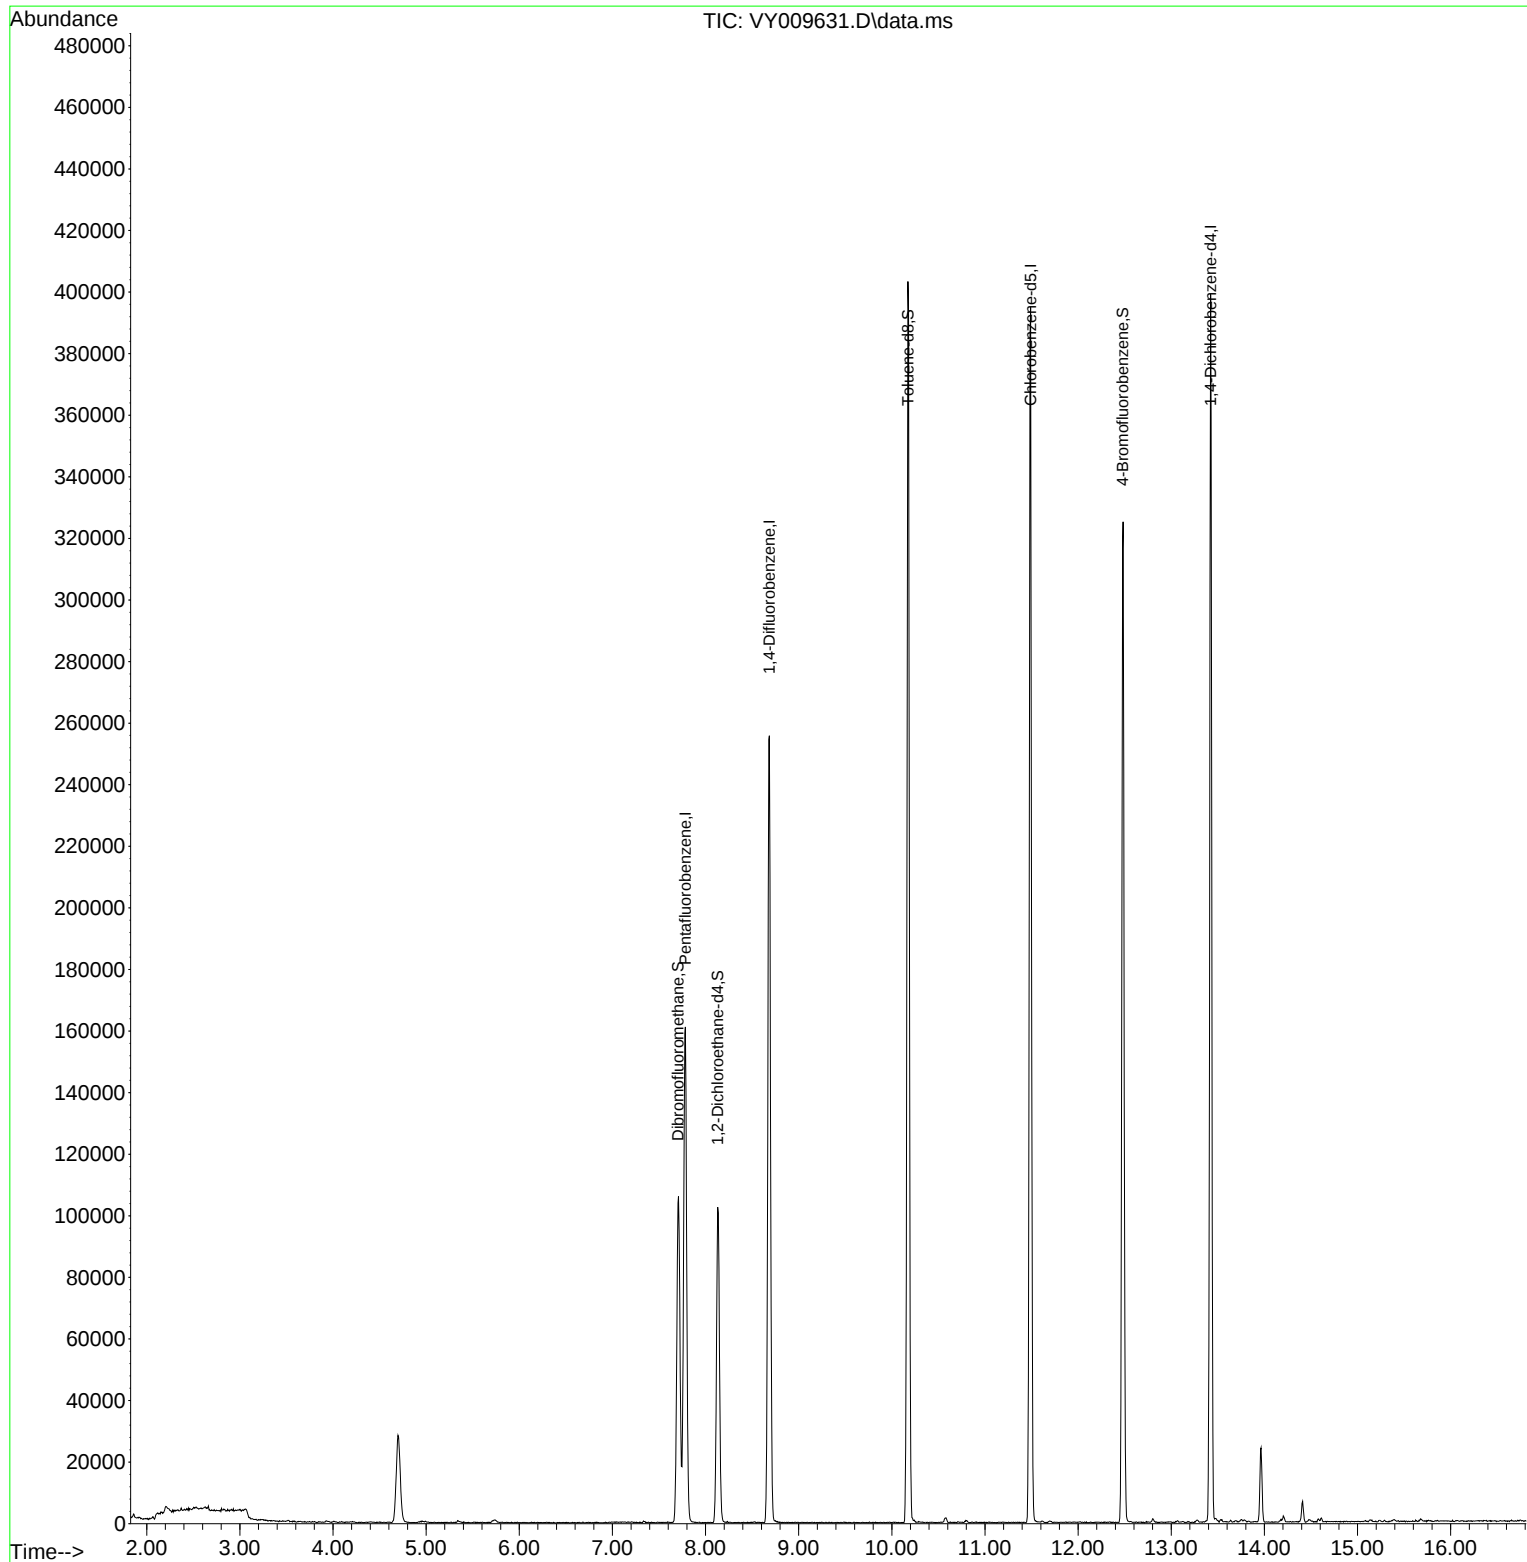


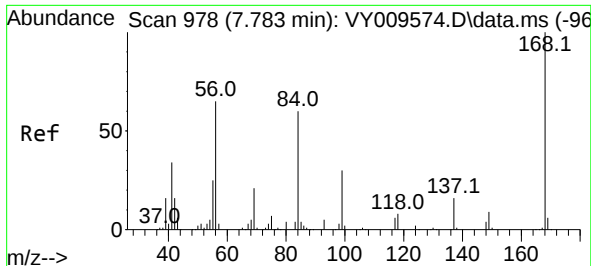

#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 7.783 min Scan# 91  
Delta R.T. -0.000 min  
Lab File: VY009631.D  
Acq: 21 Jul 2022 14:19




Instrument :  
MSVOA\_Y  
ClientSampleId :  
0718-WC-TP-12EB


Tgt Ion:168 Resp: 134530  
Ion Ratio Lower Upper  
168 100  
99 47.0 46.9 70.3

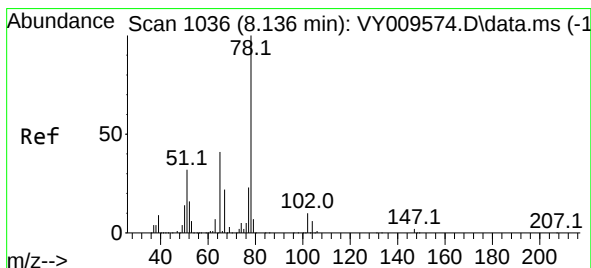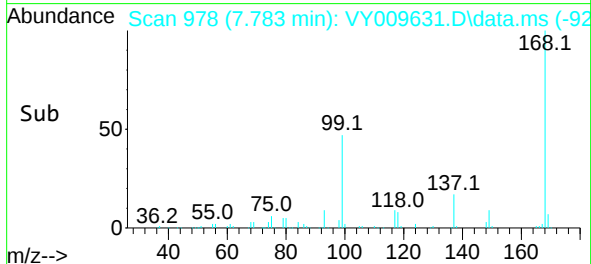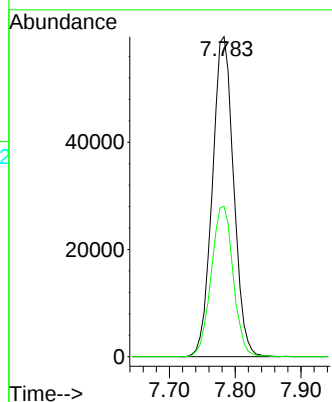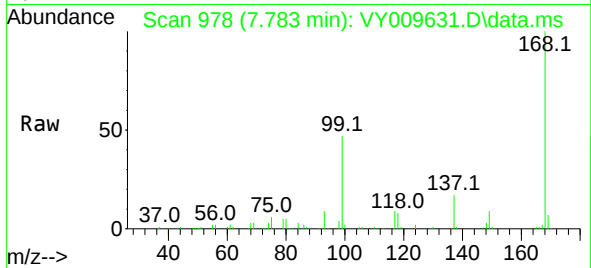

#33  
1,2-Dichloroethane-d4  
Concen: 62.952 ug/l  
RT: 8.130 min Scan# 1035  
Delta R.T. -0.006 min  
Lab File: VY009631.D  
Acq: 21 Jul 2022 14:19

Tgt Ion: 65 Resp: 80095  
Ion Ratio Lower Upper  
65 100  
67 52.4 0.0 99.4

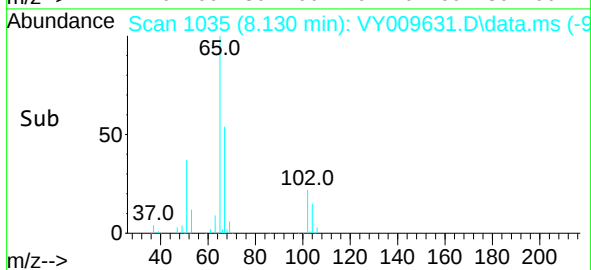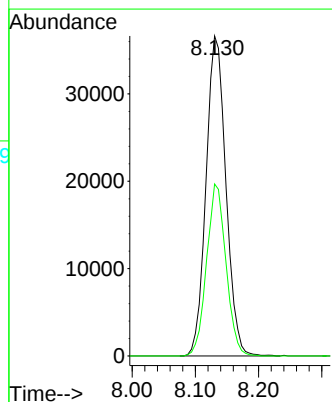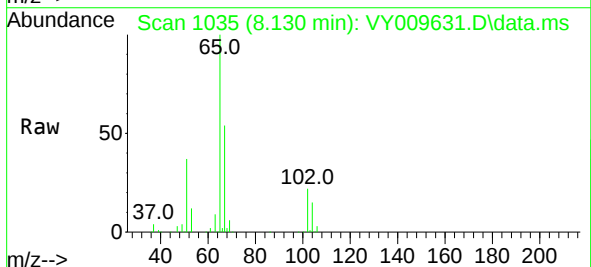

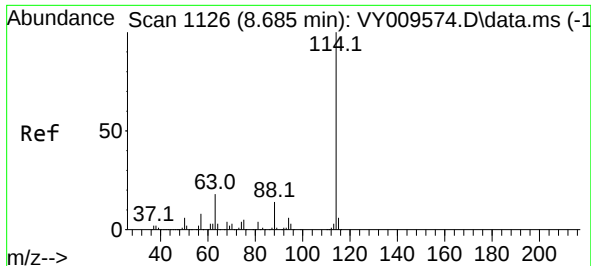

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.685 min Scan# 1126

Delta R.T. 0.000 min

Lab File: VY009631.D

Acq: 21 Jul 2022 14:19

Instrument :

MSVOA\_Y

ClientSampleId :

0718-WC-TP-12EB





Tgt Ion:114 Resp: 236004

Ion Ratio Lower Upper

114 100

63 16.6 0.0 43.2

88 14.1 0.0 31.8

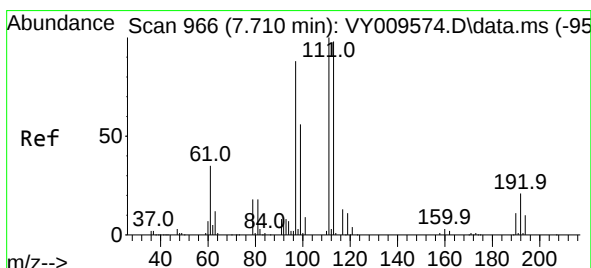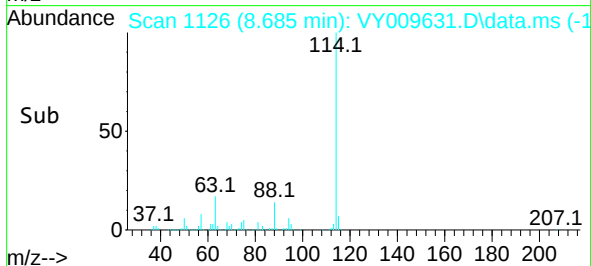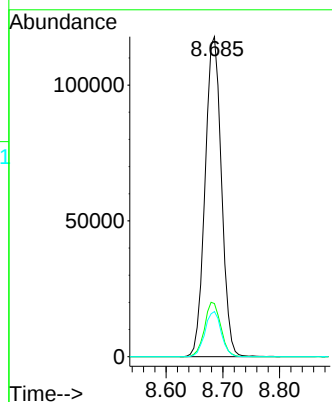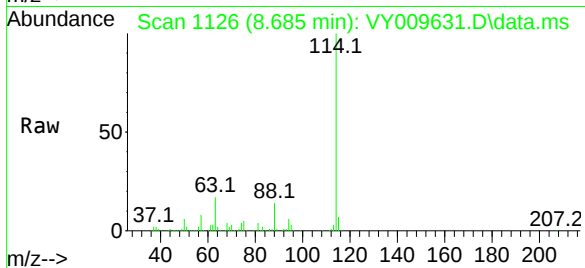

#35

Dibromofluoromethane

Concen: 51.443 ug/l

RT: 7.704 min Scan# 965

Delta R.T. -0.006 min

Lab File: VY009631.D

Acq: 21 Jul 2022 14:19




Tgt Ion:113 Resp: 76487


Ion Ratio Lower Upper

113 100

111 102.4 82.6 124.0

192 21.7 17.6 26.4

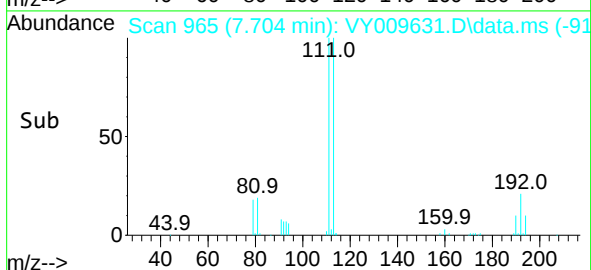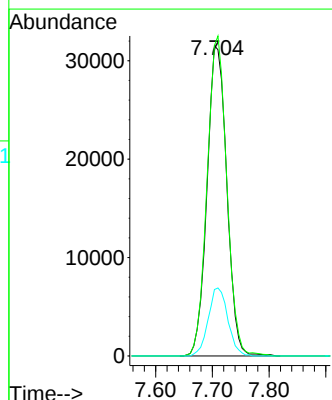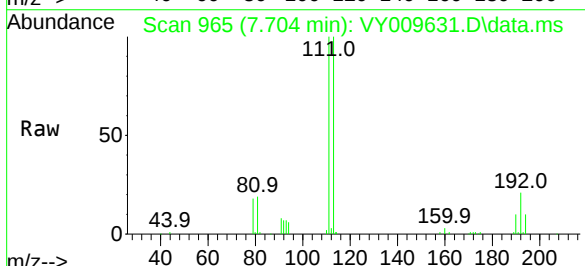

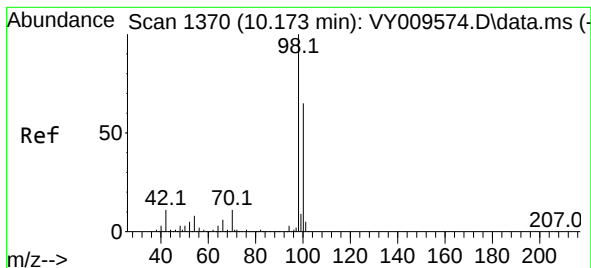

#50

Toluene-d8

Concen: 48.037 ug/l

RT: 10.173 min Scan# 1

Delta R.T. 0.000 min

Lab File: VY009631.D

Acq: 21 Jul 2022 14:19

Instrument :

MSVOA\_Y

ClientSampleId :





0718-WC-TP-12EB

Tgt Ion: 98 Resp: 274566

Ion Ratio Lower Upper

98 100

100 64.8 50.2 75.2

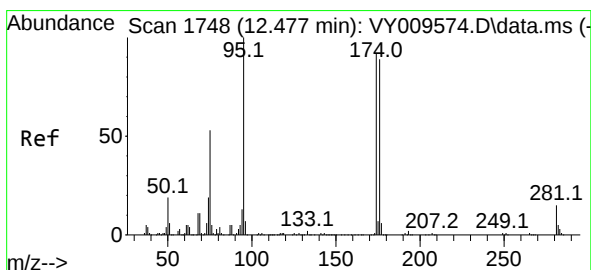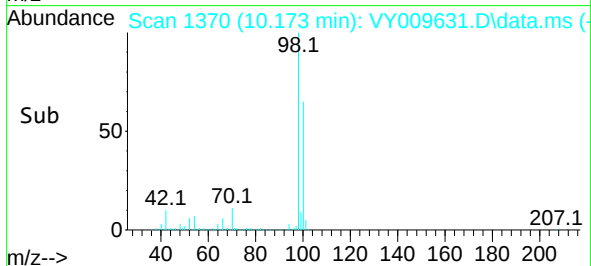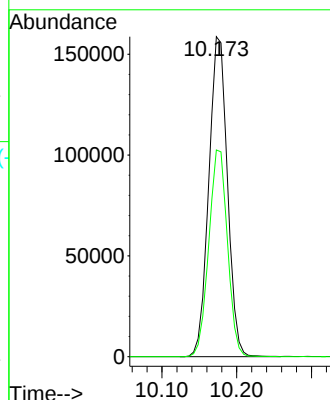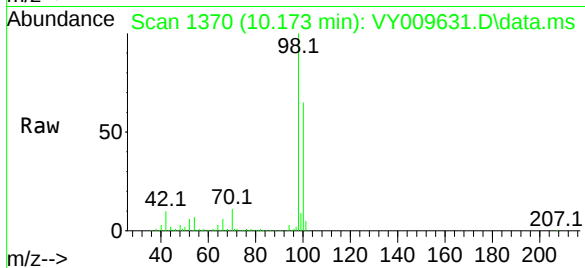

#62

4-Bromofluorobenzene

Concen: 47.252 ug/l

RT: 12.477 min Scan# 1748

Delta R.T. 0.000 min

Lab File: VY009631.D

Acq: 21 Jul 2022 14:19




Tgt Ion: 95 Resp: 87514


Ion Ratio Lower Upper

95 100

174 97.4 0.0 177.0

176 94.2 0.0 175.8


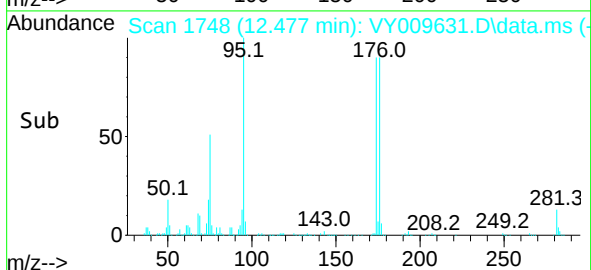
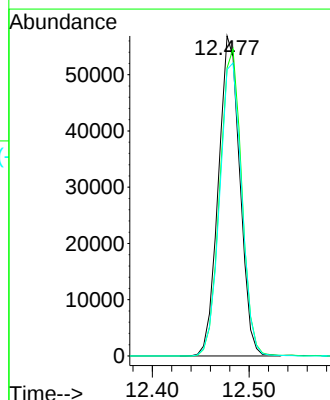
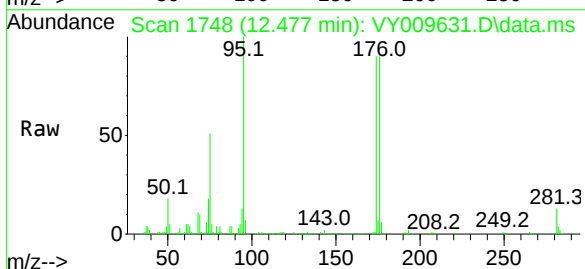


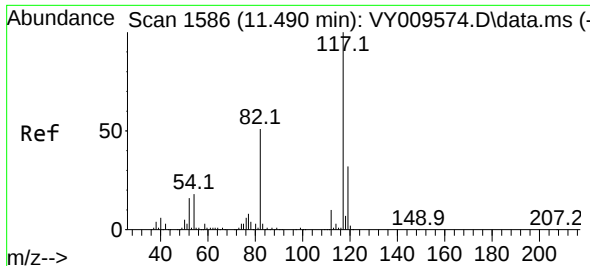

#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 11.490 min Scan# 117  
Delta R.T. 0.000 min  
Lab File: VY009631.D  
Acq: 21 Jul 2022 14:19

Instrument :  
MSVOA\_Y  
ClientSampleId :  
0718-WC-TP-12EB

Tgt Ion:117 Resp: 227987  
Ion Ratio Lower Upper  
117 100  
82 49.7 43.0 64.4  
119 31.9 25.4 38.0

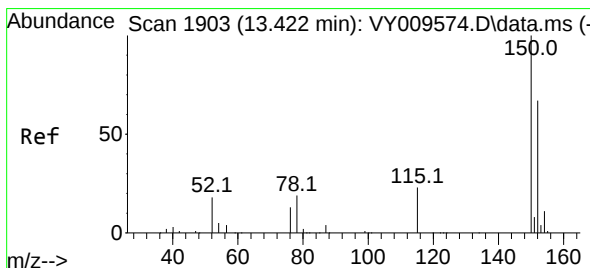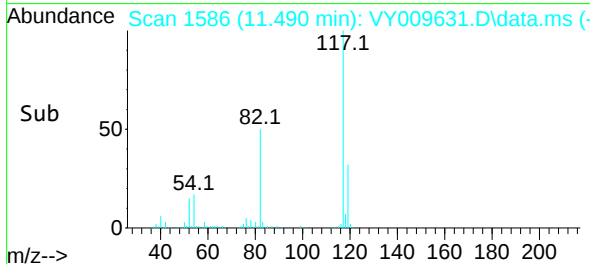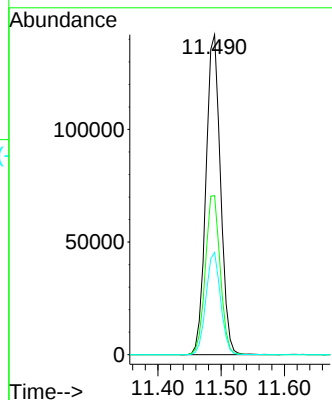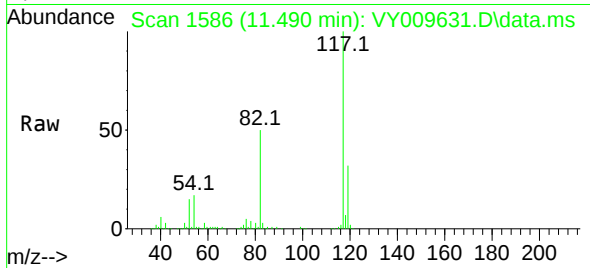

#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 13.422 min Scan# 1903  
Delta R.T. 0.000 min  
Lab File: VY009631.D  
Acq: 21 Jul 2022 14:19

Tgt Ion:152 Resp: 107383  
Ion Ratio Lower Upper  
152 100  
115 54.8 28.2 84.7  
150 155.9 0.0 347.6

