

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY072123\
 Data File : VY014746.D
 Acq On : 21 Jul 2023 14:56
 Operator : SY/MD
 Sample : 03681-15
 Misc : 4.88g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 RPTP-5-GRAB-10

Quant Time: Jul 22 05:37:26 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y071323S.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 14 02:09:50 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	210810	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	365988	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	345697	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	160930	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.142	65	129173	53.771	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	107.540%
35) Dibromofluoromethane	7.716	113	115096	49.402	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	98.800%
50) Toluene-d8	10.179	98	432484	50.351	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	100.700%
62) 4-Bromofluorobenzene	12.477	95	161662	49.085	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	98.160%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY072123\
Data File : VY014746.D
Acq On : 21 Jul 2023 14:56
Operator : SY/MD
Sample : 03681-15
Misc : 4.88g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
RPTP-5-GRAB-10

Quant Time: Jul 22 05:37:26 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y071323S.M
Quant Title : SW846 8260
QLast Update : Fri Jul 14 02:09:50 2023
Response via : Initial Calibration




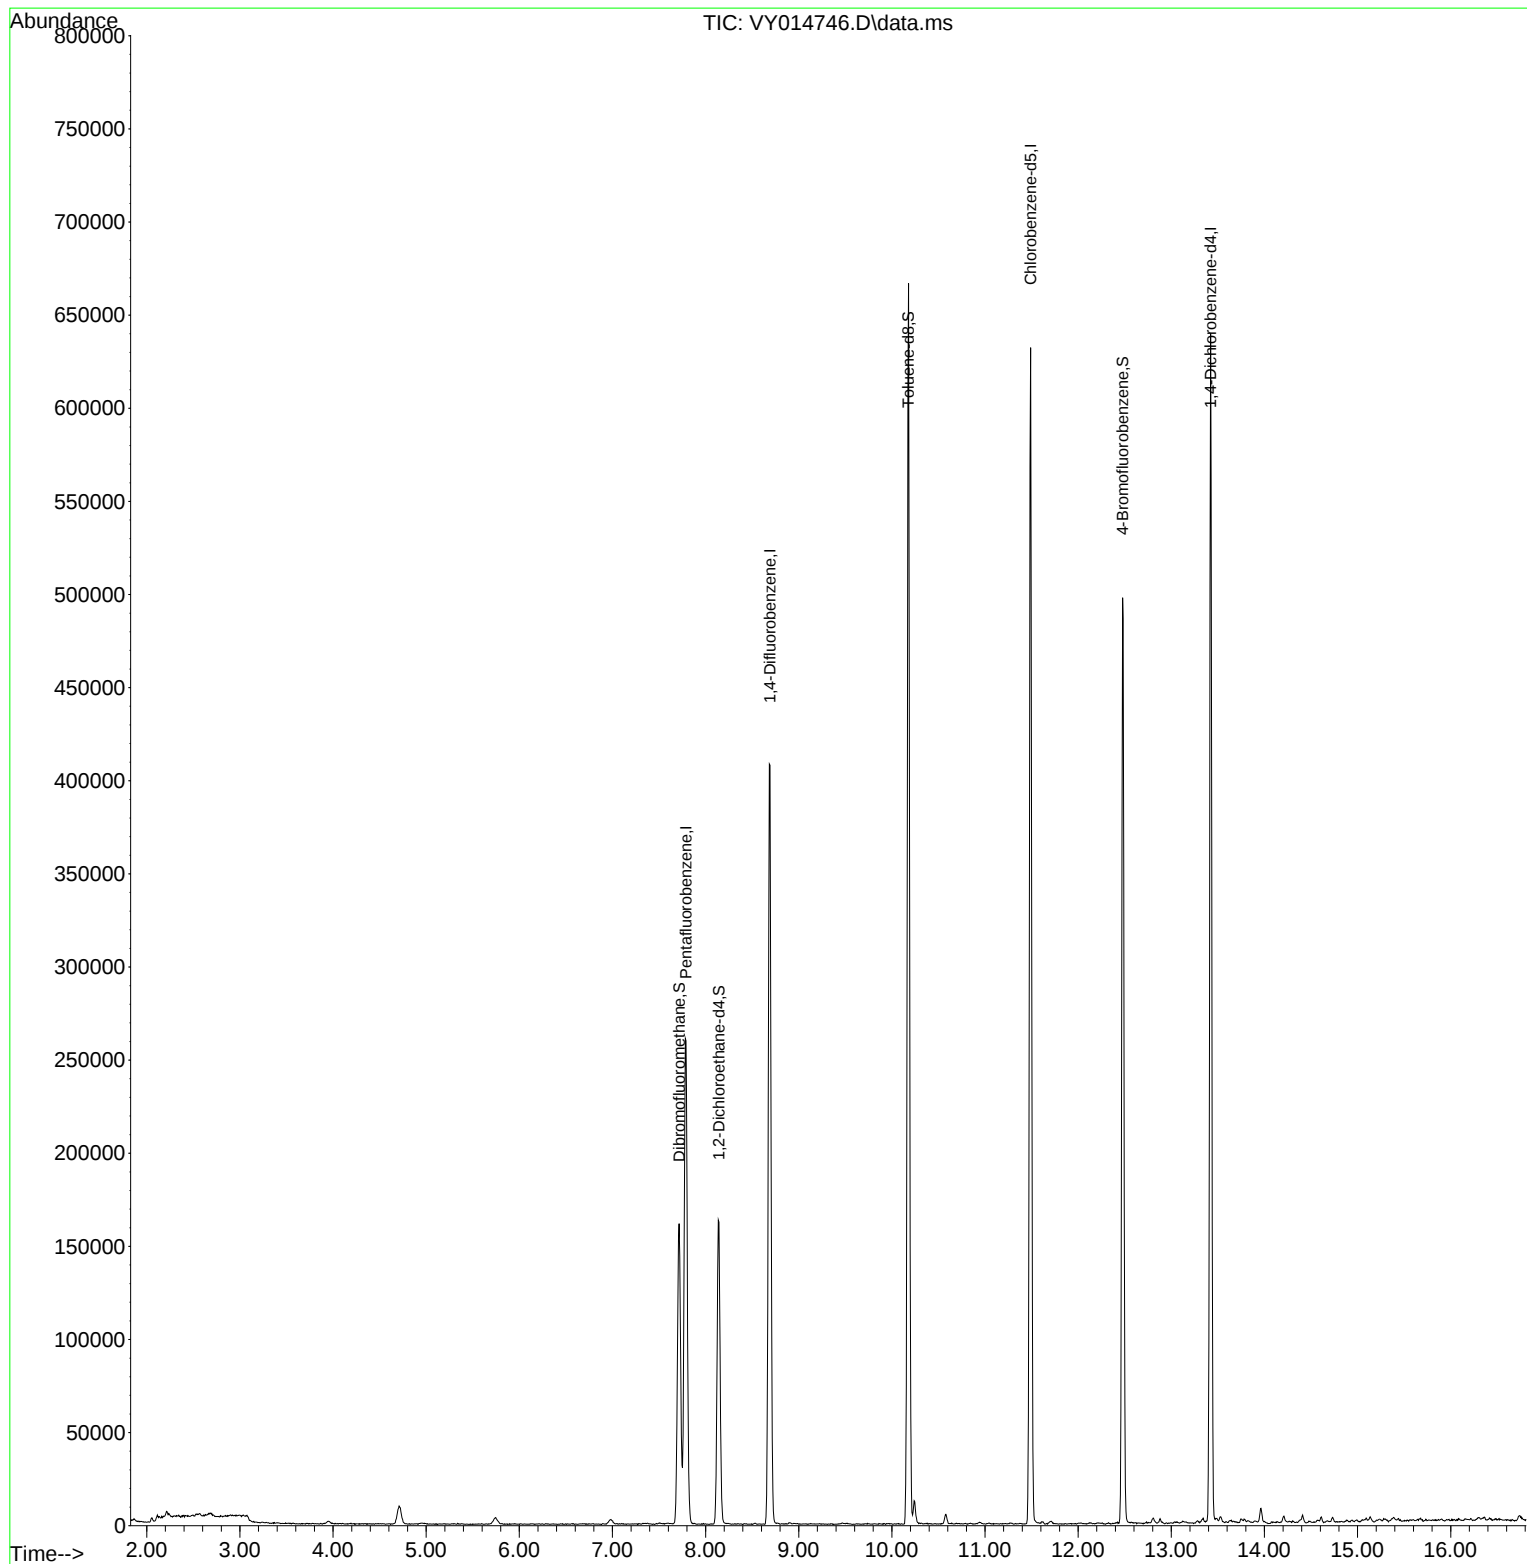


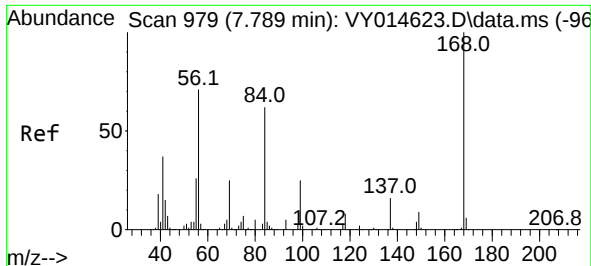

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY014746.D
Acq: 21 Jul 2023 14:56




Instrument :
MSVOA_Y
ClientSampleId :
RPTP-5-GRAB-10


Tgt Ion:168 Resp: 210810
Ion Ratio Lower Upper
168 100
99 54.5 43.4 65.0

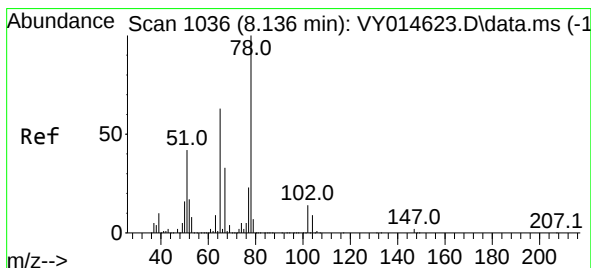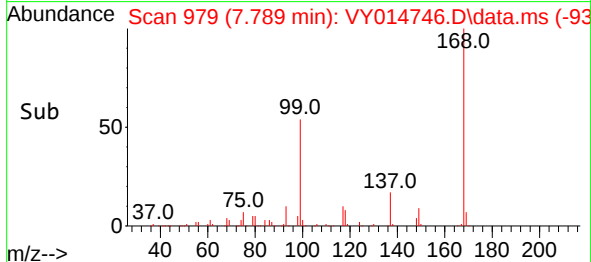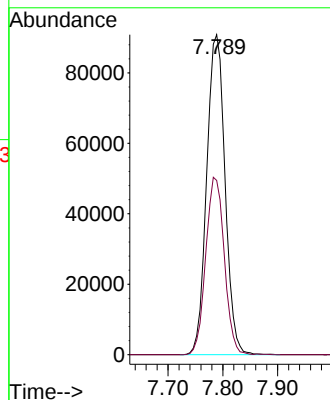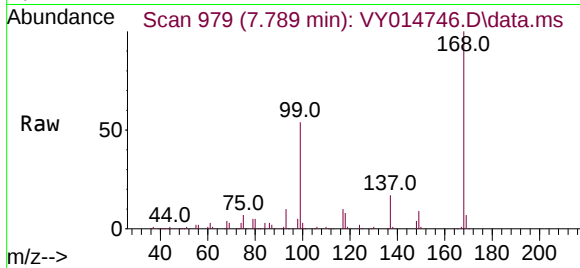

#33
1,2-Dichloroethane-d4
Concen: 53.771 ug/l
RT: 8.142 min Scan# 1037
Delta R.T. 0.006 min
Lab File: VY014746.D
Acq: 21 Jul 2023 14:56

Tgt Ion: 65 Resp: 129173
Ion Ratio Lower Upper
65 100
67 52.4 0.0 101.8

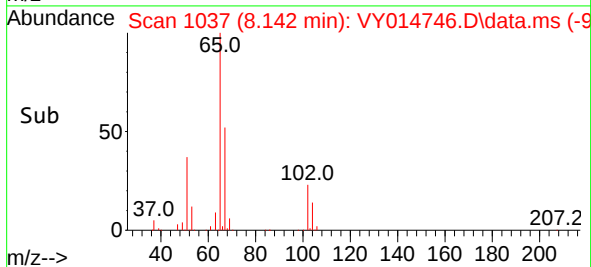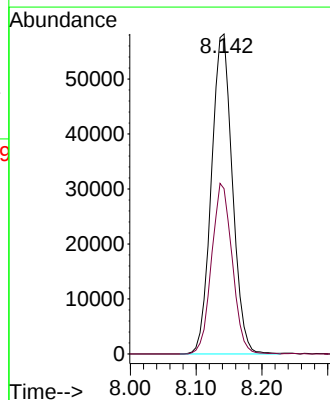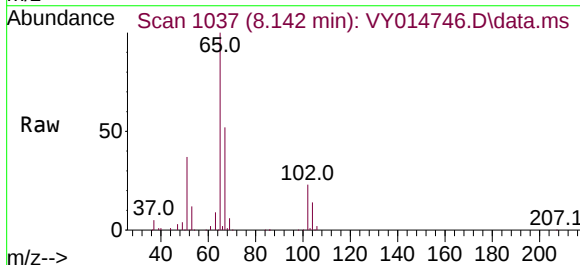

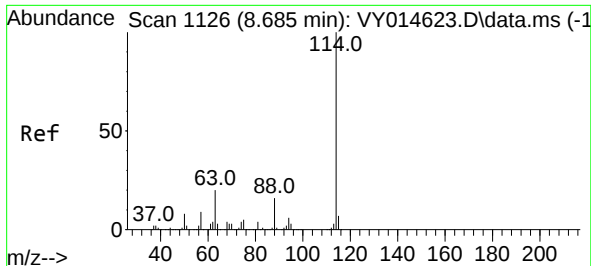

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1126

Delta R.T. 0.006 min

Lab File: VY014746.D

Acq: 21 Jul 2023 14:56

Instrument :

MSVOA_Y

ClientSampleId :

RPTP-5-GRAB-10





Tgt Ion:114 Resp: 365988

Ion Ratio Lower Upper

114 100

63 18.2 0.0 42.4

88 15.3 0.0 30.6

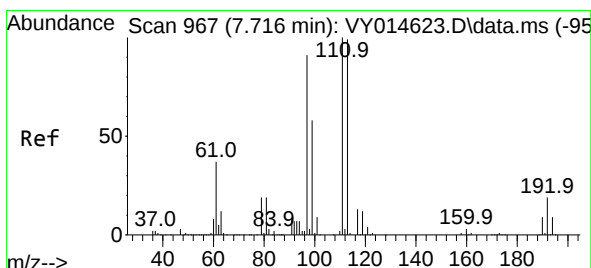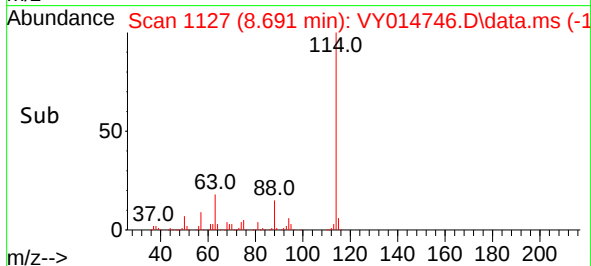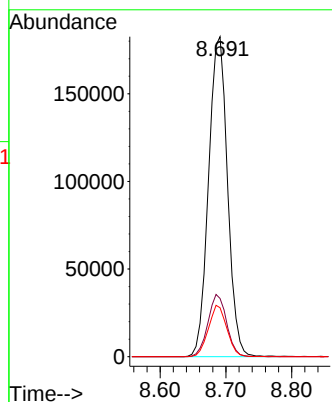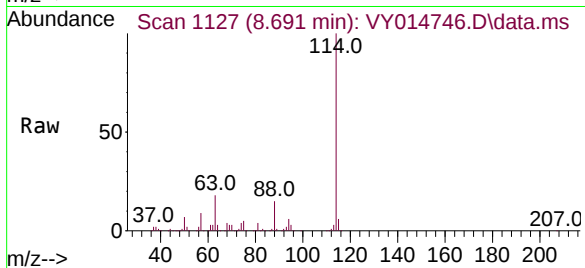

#35

Dibromofluoromethane

Concen: 49.402 ug/l

RT: 7.716 min Scan# 967

Delta R.T. -0.000 min

Lab File: VY014746.D

Acq: 21 Jul 2023 14:56




Tgt Ion:113 Resp: 115096


Ion Ratio Lower Upper

113 100

111 103.3 81.3 121.9

192 19.5 16.9 25.3

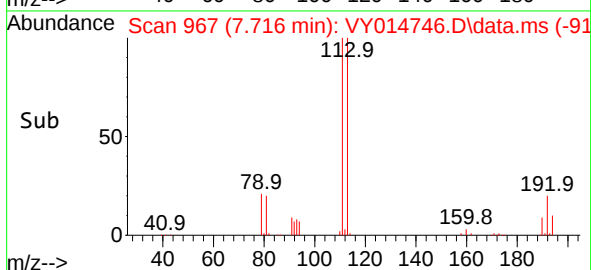
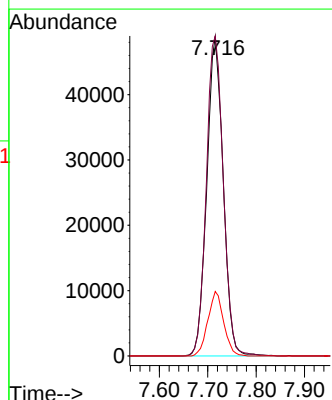
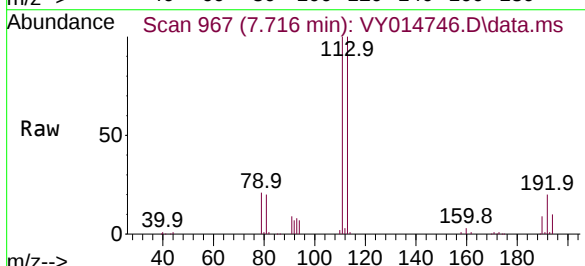


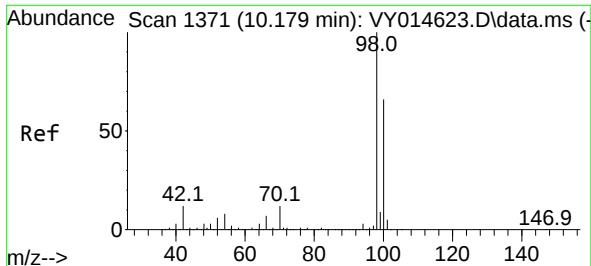

#50
Toluene-d8
Concen: 50.351 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. -0.000 min
Lab File: VY014746.D
Acq: 21 Jul 2023 14:56




Instrument :
MSVOA_Y
ClientSampleId :
RPTP-5-GRAB-10


Tgt Ion: 98 Resp: 432484
Ion Ratio Lower Upper
98 100
100 65.0 50.1 75.1

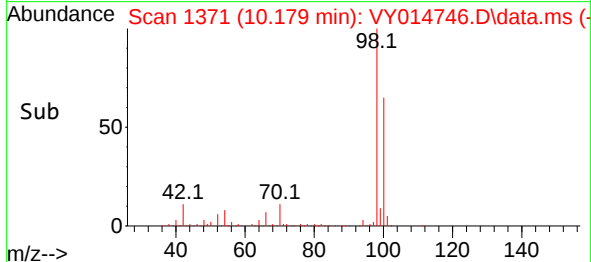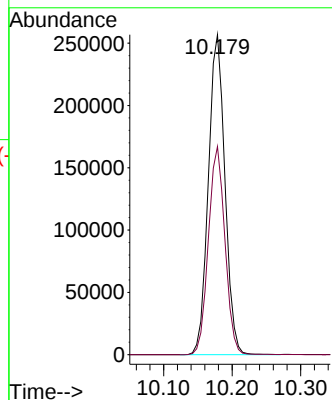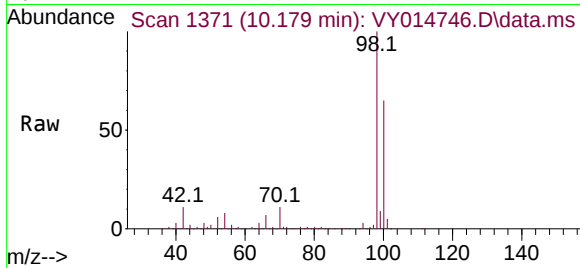

#62
4-Bromofluorobenzene
Concen: 49.085 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. -0.000 min
Lab File: VY014746.D
Acq: 21 Jul 2023 14:56

Tgt Ion: 95 Resp: 161662
Ion Ratio Lower Upper
95 100
174 80.7 0.0 178.2
176 77.7 0.0 173.8

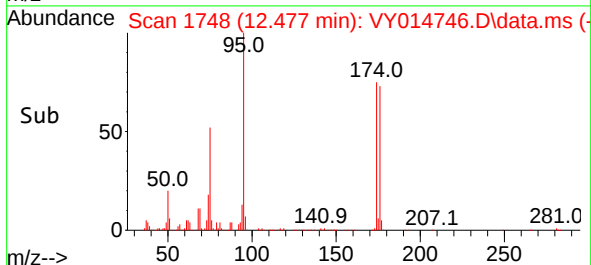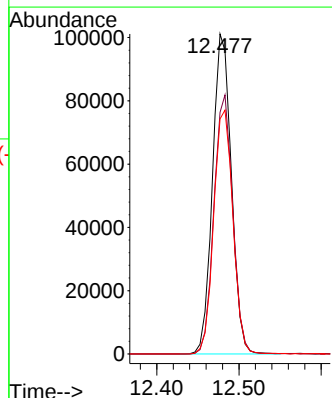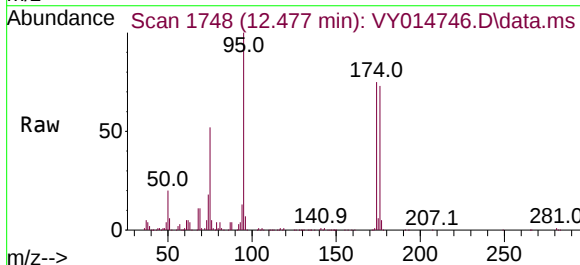

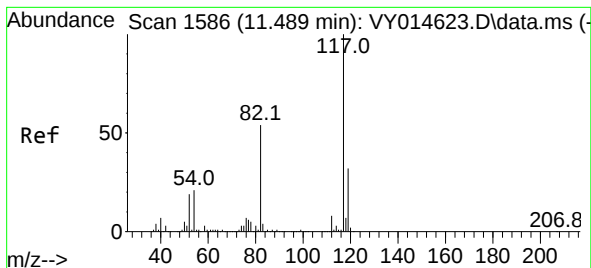

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.489 min Scan# 11

Delta R.T. 0.000 min

Lab File: VY014746.D

Acq: 21 Jul 2023 14:56

Instrument :

MSVOA_Y

ClientSampleId :

RPTP-5-GRAB-10





Tgt Ion:117 Resp: 345697

Ion Ratio Lower Upper

117 100

82 54.3 43.4 65.0

119 32.2 26.3 39.5

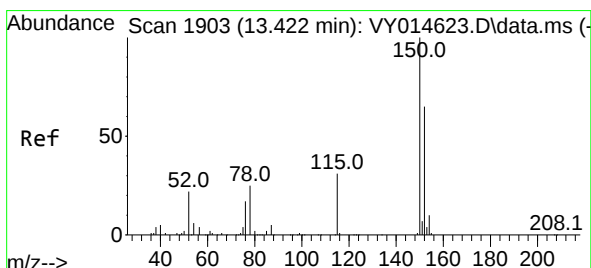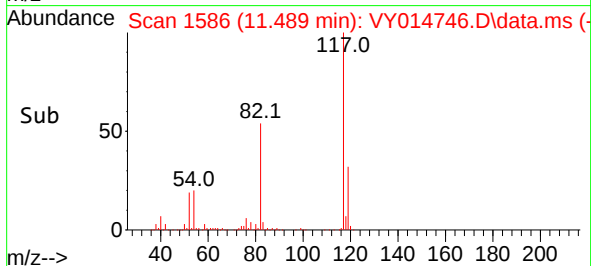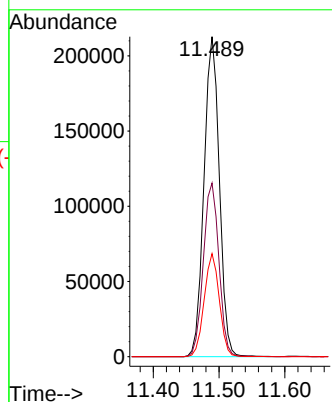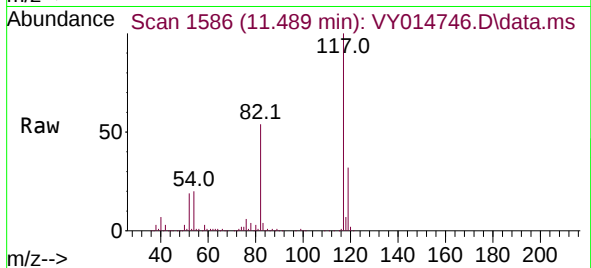

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.422 min Scan# 1903

Delta R.T. -0.000 min

Lab File: VY014746.D

Acq: 21 Jul 2023 14:56

Tgt Ion:152 Resp: 160930

Ion Ratio Lower Upper

152 100

115 60.0 28.8 86.5

150 157.0 0.0 348.8

