
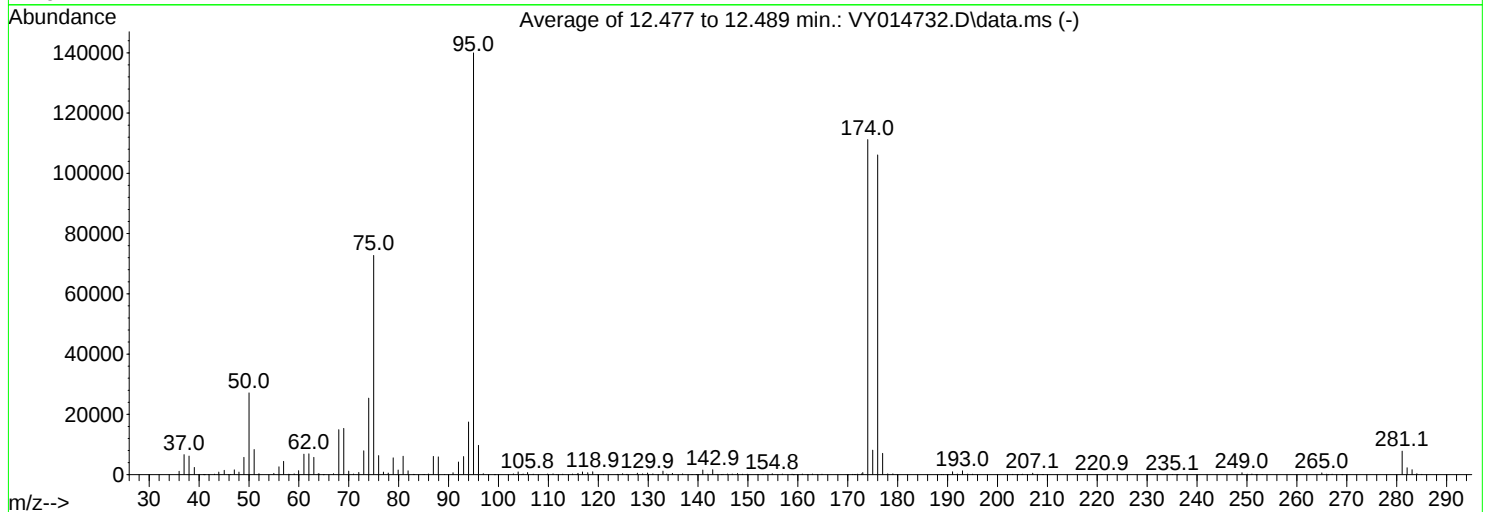


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY072123\
Data File : VY014732.D
Acq On : 21 Jul 2023 08:41
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y071323S.M
Title : SW846 8260
Last Update : Fri Jul 14 02:09:50 2023

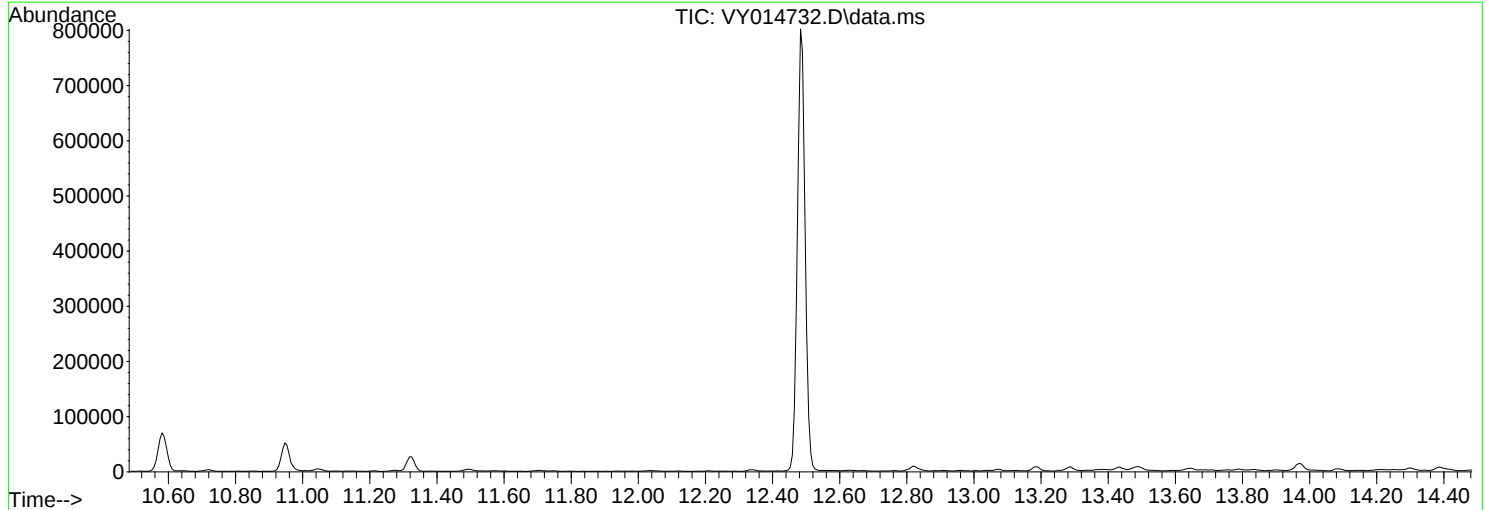

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.4	27160	PASS
75	95	30	60	52.0	72760	PASS
95	95	100	100	100.0	139989	PASS
96	95	5	9	7.0	9746	PASS
173	174	0.00	2	0.6	693	PASS
174	95	50	100	79.4	111184	PASS
175	174	5	9	7.3	8123	PASS
176	174	95	101	95.4	106112	PASS
177	176	5	9	6.7	7079	PASS