
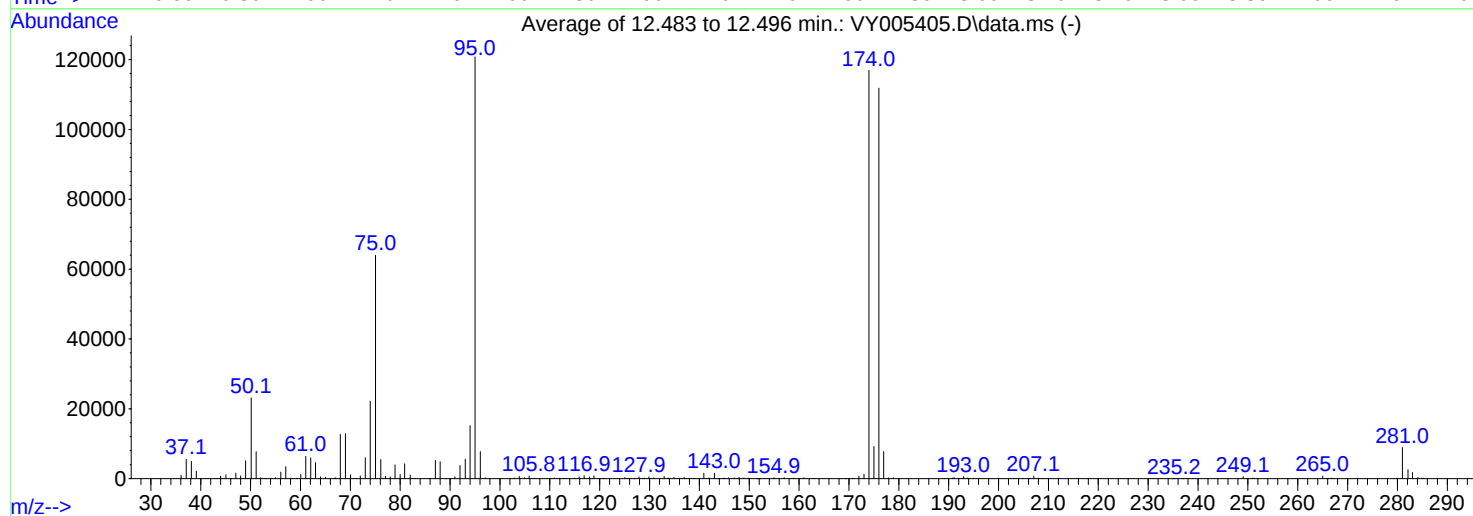


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY072221\
 Data File : VY005405.D
 Acq On : 22 Jul 2021 08:53
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y072221S.M
 Title : SW846 8260
 Last Update : Fri Jul 23 06:20:14 2021

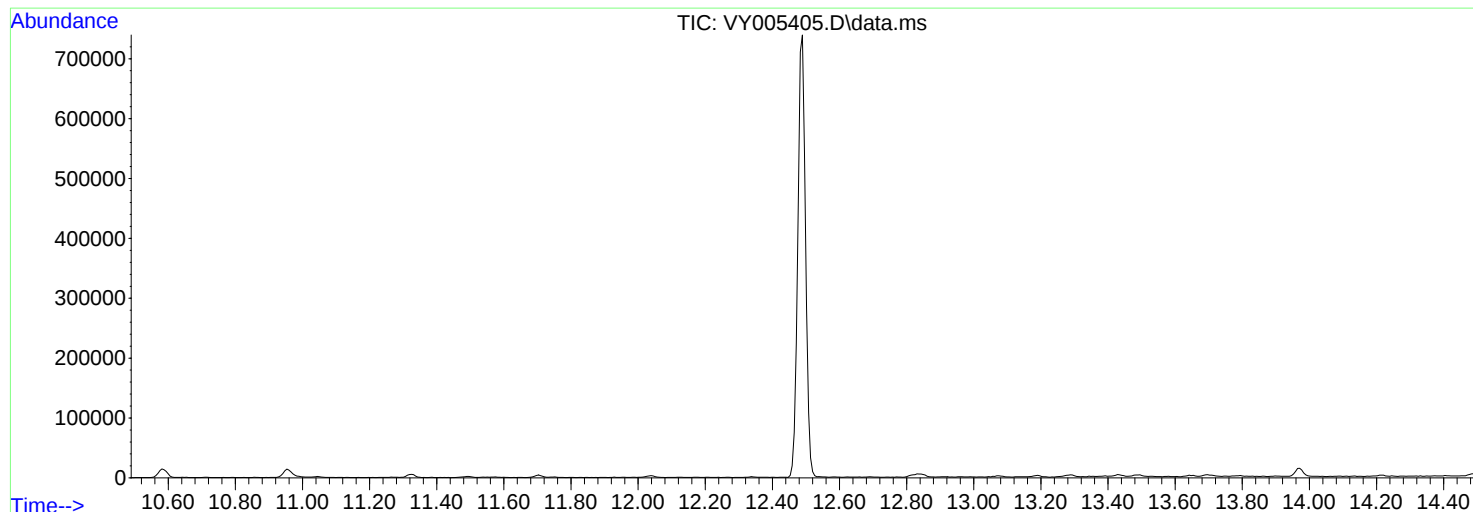

AutoFind: Scans 1749, 1750, 1751; Background Corrected with Scan 1741

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	23144	PASS
75	95	30	60	52.9	63952	PASS
95	95	100	100	100.0	120792	PASS
96	95	5	9	6.4	7727	PASS
173	174	0.00	2	1.1	1305	PASS
174	95	50	100	96.8	116925	PASS
175	174	5	9	7.9	9207	PASS
176	174	95	101	95.7	111861	PASS
177	176	5	9	6.9	7752	PASS