

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY072222\
 Data File : VY009668.D
 Acq On : 22 Jul 2022 18:33
 Operator : KP/MD
 Sample : N3836-01
 Misc : 5.53g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 TP-1

Quant Time: Jul 23 00:55:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y071822S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jul 19 04:22:09 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.783	168	174797	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	8.685	114	274833	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	257330	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	120433	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.130	65	95013	57.474	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	114.940%
35) Dibromofluoromethane	7.710	113	86602	50.017	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	100.040%
50) Toluene-d8	10.173	98	315645	47.421	ug/l	0.00
Spiked Amount	50.000	Range	78 - 125	Recovery	=	94.840%
62) 4-Bromofluorobenzene	12.477	95	103246	47.870	ug/l	0.00
Spiked Amount	50.000	Range	50 - 146	Recovery	=	95.740%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY072222\
Data File : VY009668.D
Acq On : 22 Jul 2022 18:33
Operator : KP/MD
Sample : N3836-01
Misc : 5.53g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
TP-1

Quant Time: Jul 23 00:55:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y071822S.M
Quant Title : SW846 8260
QLast Update : Tue Jul 19 04:22:09 2022
Response via : Initial Calibration




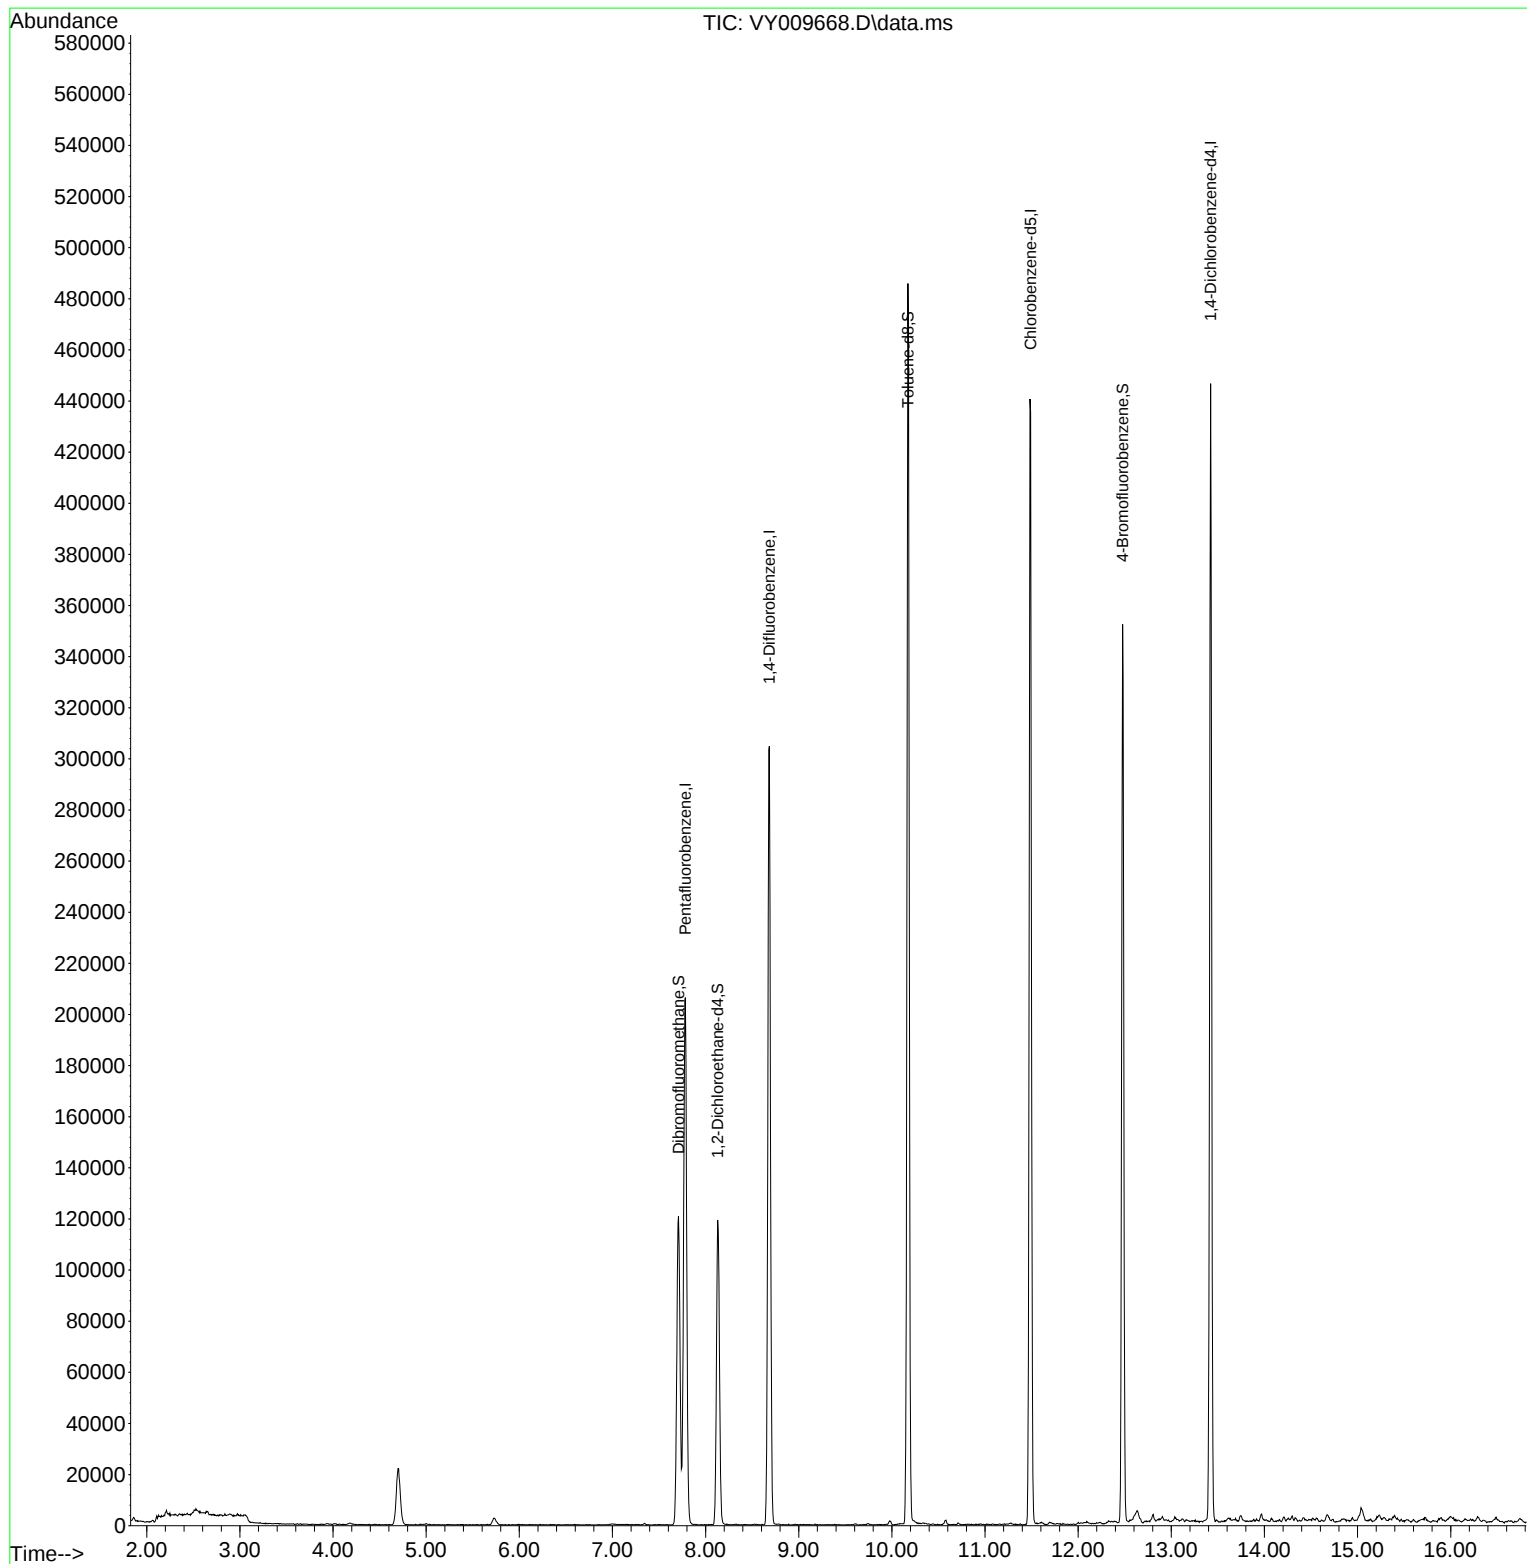


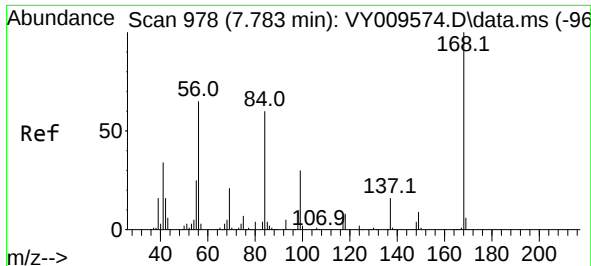

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.783 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY009668.D
Acq: 22 Jul 2022 18:33




Instrument :
MSVOA_Y
ClientSampleId :
TP-1


Tgt Ion:168 Resp: 174797
Ion Ratio Lower Upper
168 100
99 45.7 46.9 70.3#

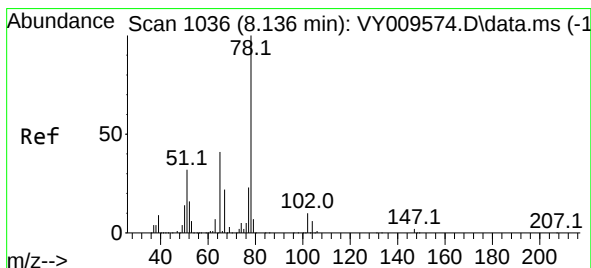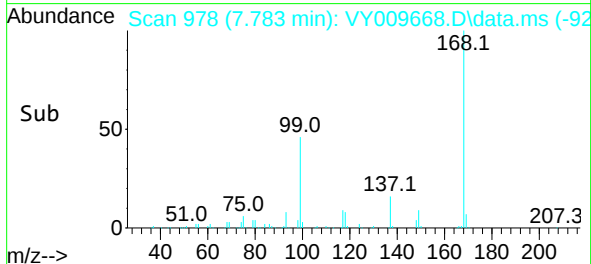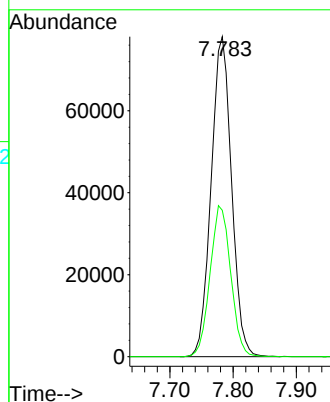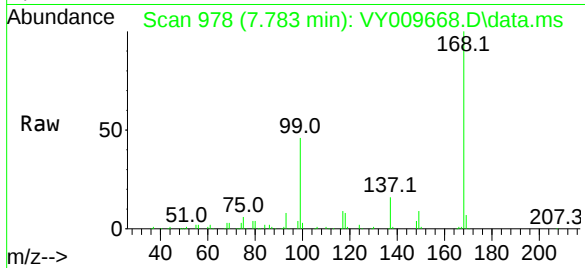

#33
1,2-Dichloroethane-d4
Concen: 57.474 ug/l
RT: 8.130 min Scan# 1035
Delta R.T. -0.006 min
Lab File: VY009668.D
Acq: 22 Jul 2022 18:33

Tgt Ion: 65 Resp: 95013
Ion Ratio Lower Upper
65 100
67 51.3 0.0 99.4

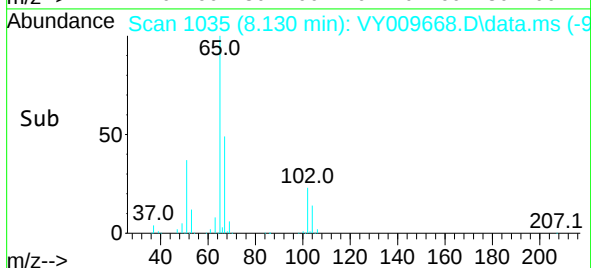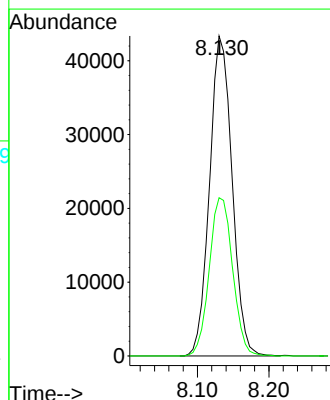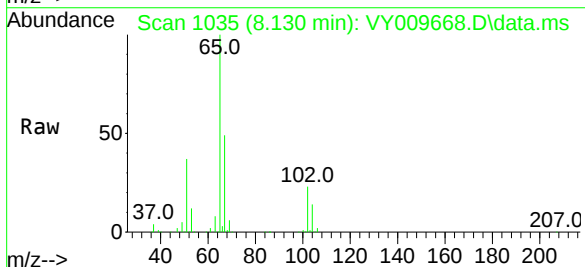

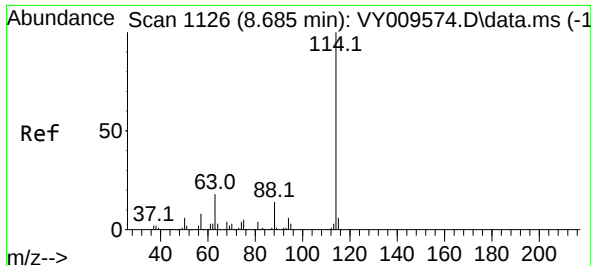

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.685 min Scan# 11

Delta R.T. -0.000 min

Lab File: VY009668.D

Acq: 22 Jul 2022 18:33

Instrument :

MSVOA_Y

ClientSampleId :

TP-1





Tgt Ion:114 Resp: 274833

Ion Ratio Lower Upper

114 100

63 16.2 0.0 43.2

88 14.5 0.0 31.8

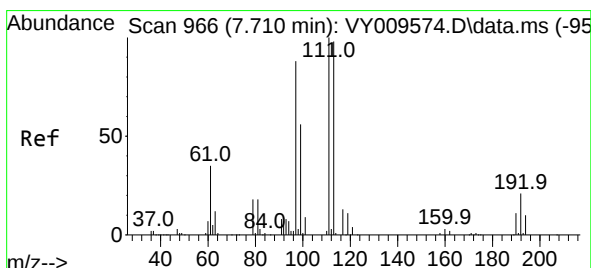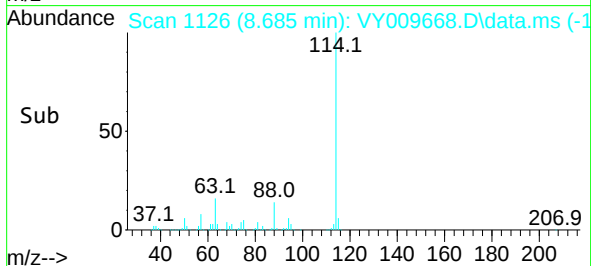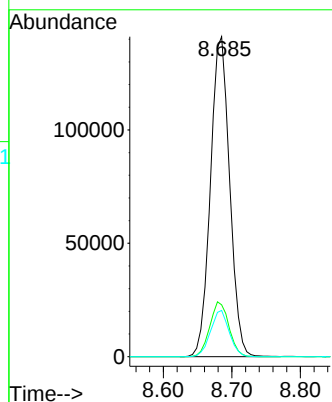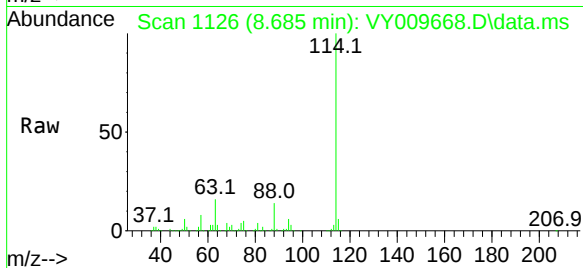

#35

Dibromofluoromethane

Concen: 50.017 ug/l

RT: 7.710 min Scan# 966

Delta R.T. -0.000 min

Lab File: VY009668.D

Acq: 22 Jul 2022 18:33




Tgt Ion:113 Resp: 86602


Ion Ratio Lower Upper

113 100

111 102.8 82.6 124.0

192 22.4 17.6 26.4


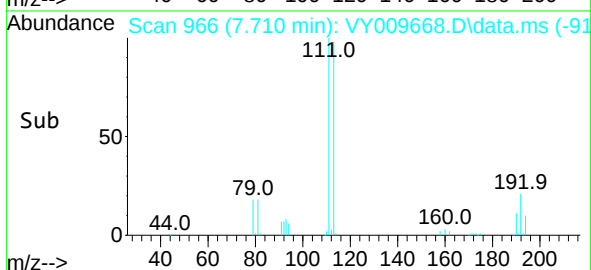
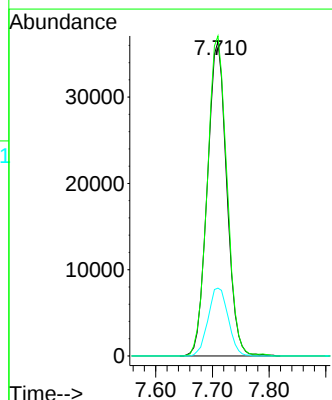
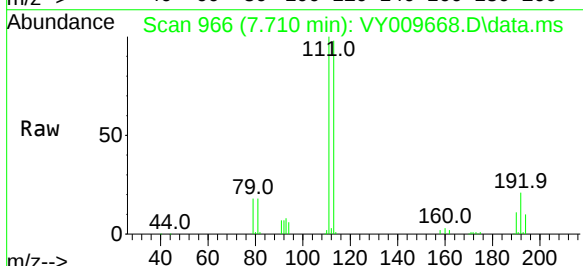


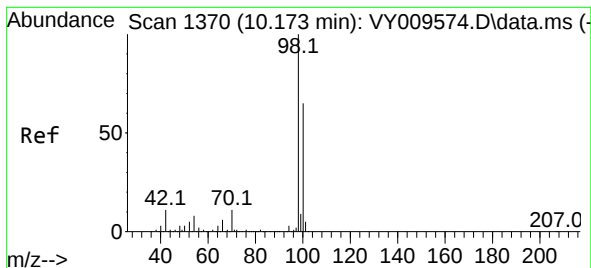

#50
Toluene-d8
Concen: 47.421 ug/l
RT: 10.173 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY009668.D
Acq: 22 Jul 2022 18:33




Instrument :
MSVOA_Y
ClientSampleId :
TP-1


Tgt Ion: 98 Resp: 315645
Ion Ratio Lower Upper
98 100
100 65.9 50.2 75.2

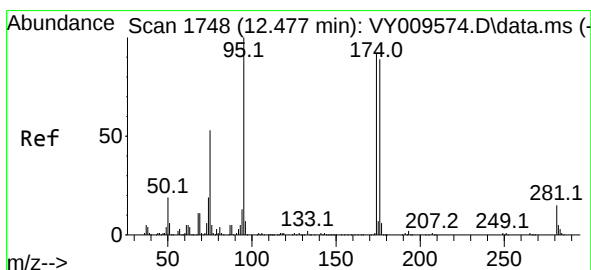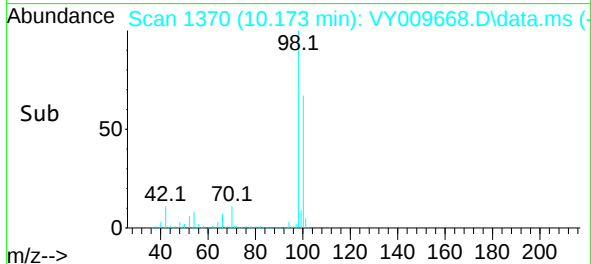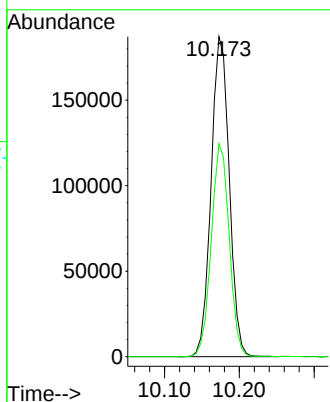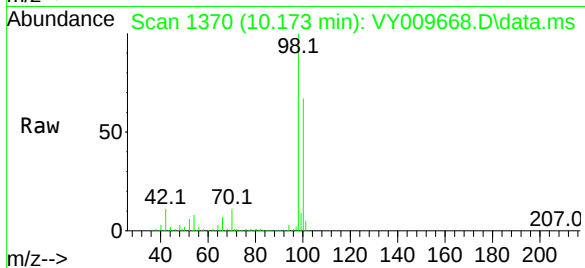

#62
4-Bromofluorobenzene
Concen: 47.870 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. -0.000 min
Lab File: VY009668.D
Acq: 22 Jul 2022 18:33

Tgt Ion: 95 Resp: 103246
Ion Ratio Lower Upper
95 100
174 97.0 0.0 177.0
176 93.6 0.0 175.8


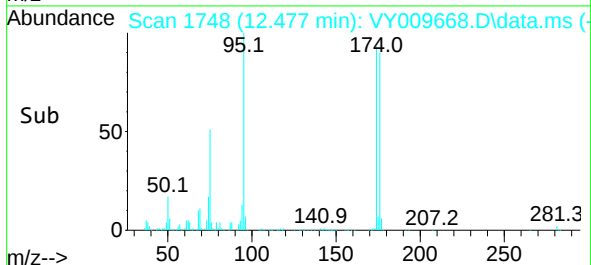
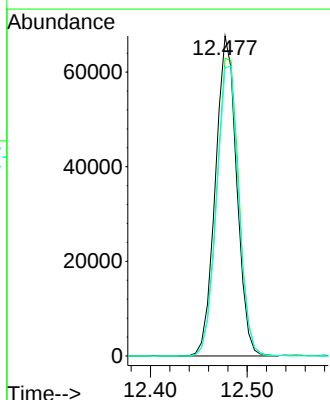
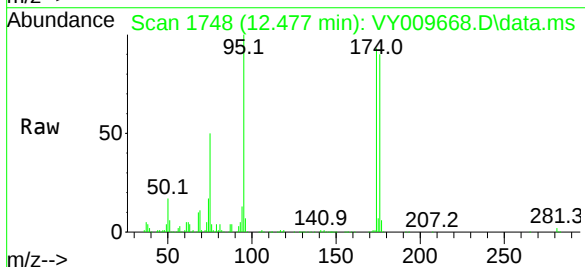


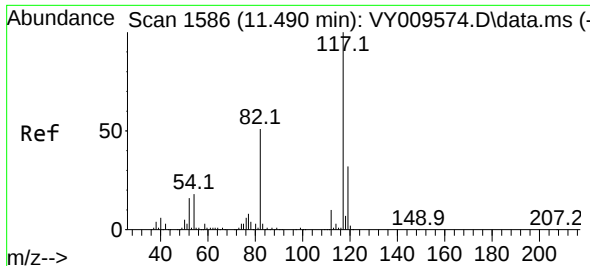

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY009668.D
Acq: 22 Jul 2022 18:33

Instrument :
MSVOA_Y
ClientSampleId :
TP-1

Tgt Ion:117 Resp: 257330
Ion Ratio Lower Upper
117 100
82 48.9 43.0 64.4
119 32.6 25.4 38.0

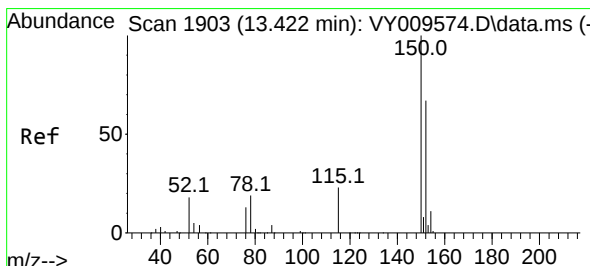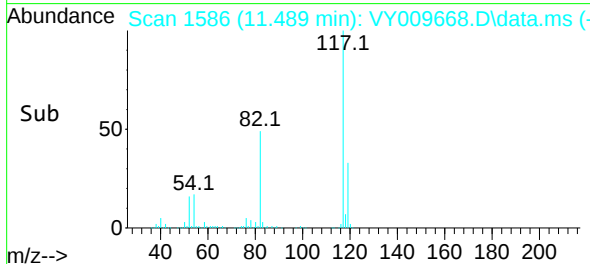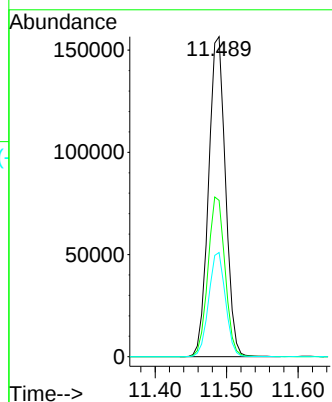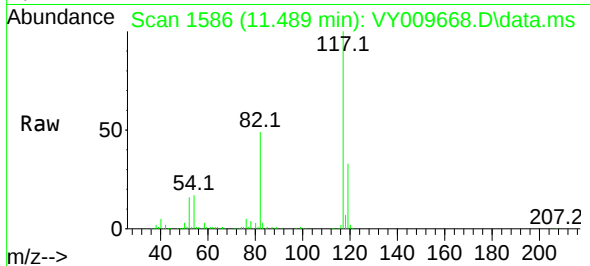

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.422 min Scan# 1903
Delta R.T. -0.000 min
Lab File: VY009668.D
Acq: 22 Jul 2022 18:33

Tgt Ion:152 Resp: 120433
Ion Ratio Lower Upper
152 100
115 54.2 28.2 84.7
150 154.8 0.0 347.6

