

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY072222\
 Data File : VY009670.D
 Acq On : 22 Jul 2022 19:21
 Operator : KP/MD
 Sample : N3839-01
 Misc : 5.97g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 ENV-DE-1-(5-10)

Quant Time: Jul 23 00:55:59 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y071822S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jul 19 04:22:09 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.783	168	176641	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	277711	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	263035	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	122648	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.130	65	95411	57.112	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	114.220%
35) Dibromofluoromethane	7.710	113	87898	50.240	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	100.480%
50) Toluene-d8	10.172	98	322237	47.910	ug/l	0.00
Spiked Amount	50.000	Range	78 - 125	Recovery	=	95.820%
62) 4-Bromofluorobenzene	12.477	95	103767	47.613	ug/l	0.00
Spiked Amount	50.000	Range	50 - 146	Recovery	=	95.220%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY072222\
Data File : VY009670.D
Acq On : 22 Jul 2022 19:21
Operator : KP/MD
Sample : N3839-01
Misc : 5.97g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
ENV-DE-1-(5-10)

Quant Time: Jul 23 00:55:59 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y071822S.M
Quant Title : SW846 8260
QLast Update : Tue Jul 19 04:22:09 2022
Response via : Initial Calibration




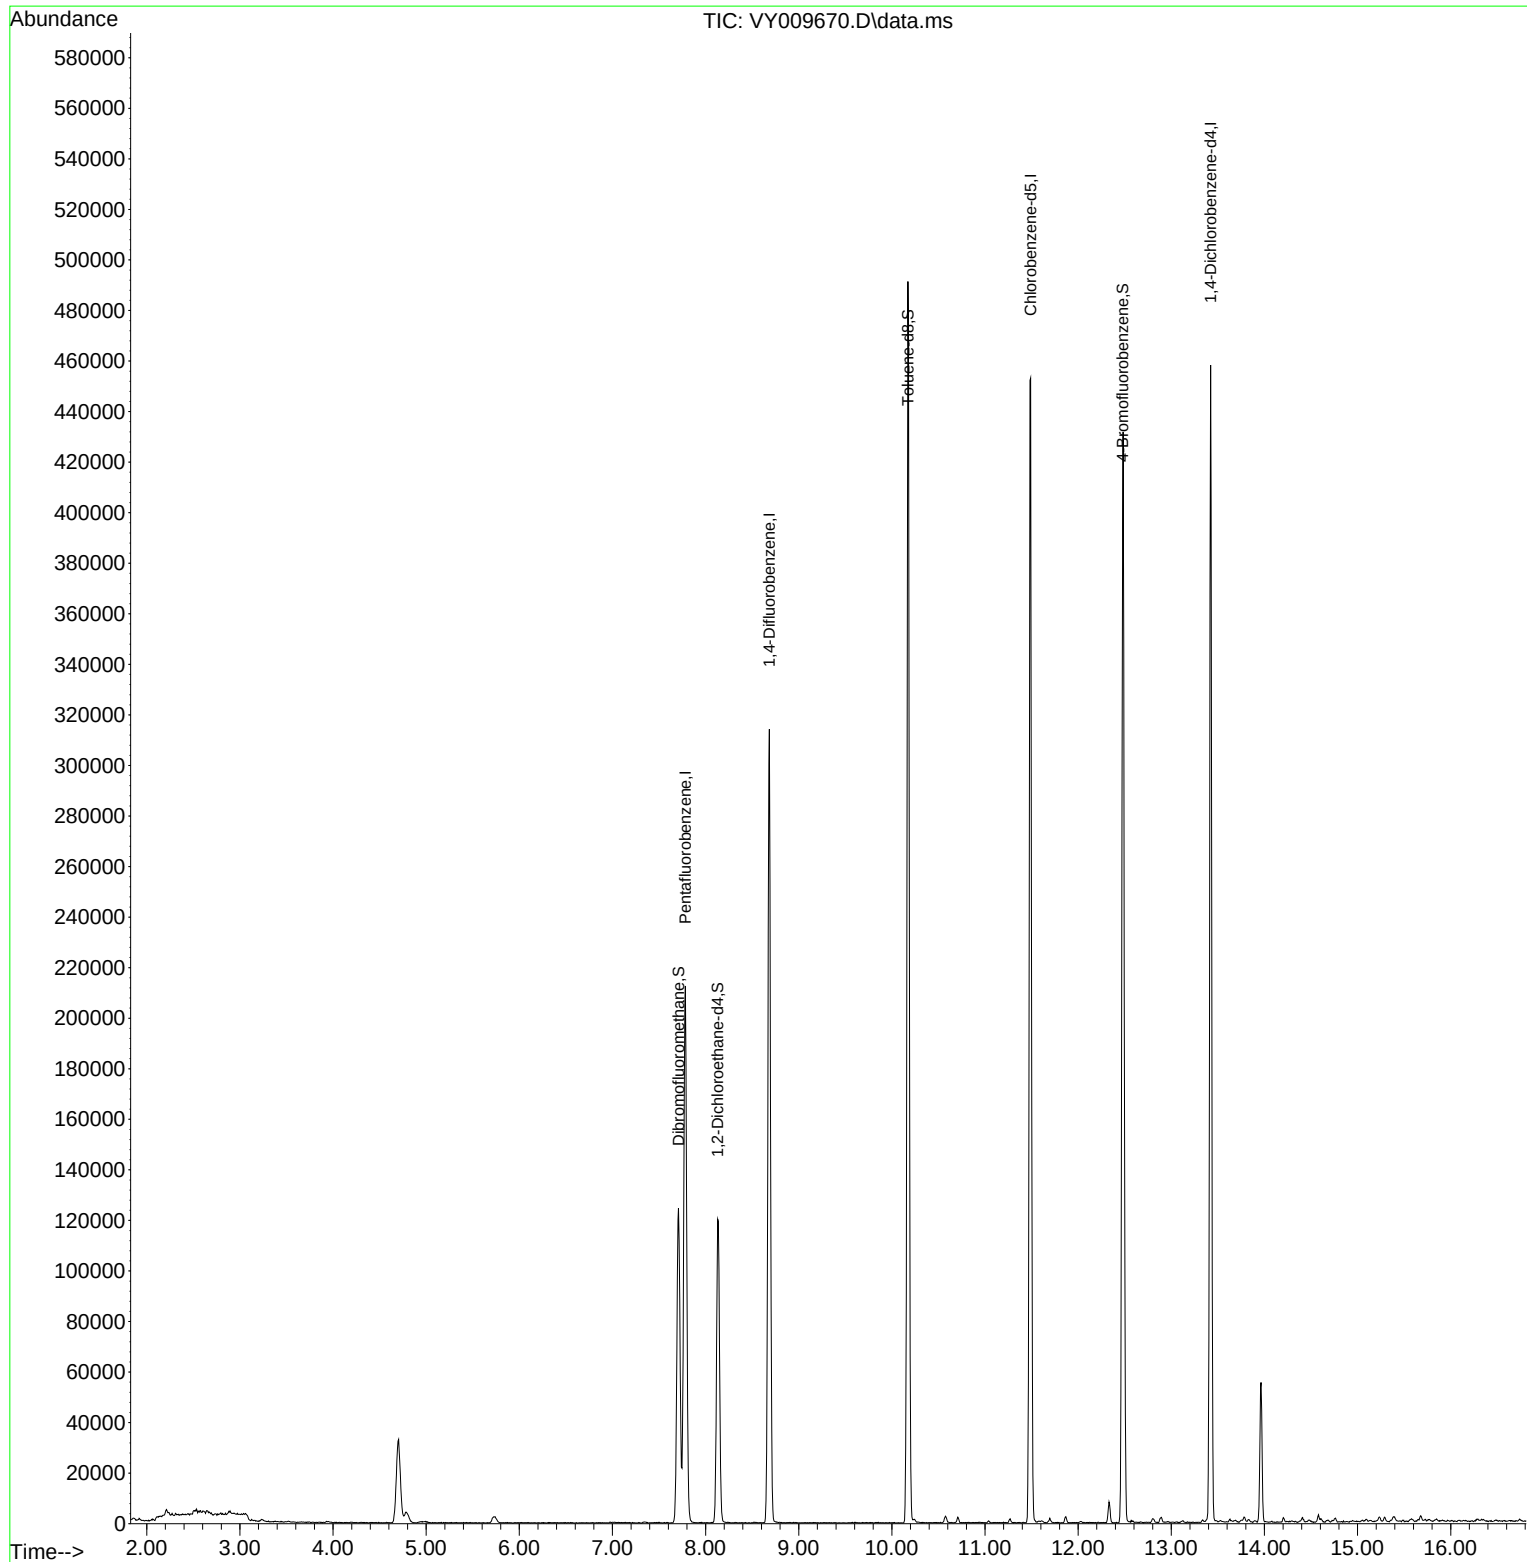


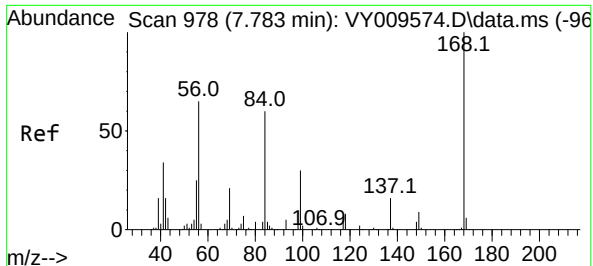

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.783 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY009670.D
Acq: 22 Jul 2022 19:21




Instrument :
MSVOA_Y
ClientSampleId :
ENV-DE-1-(5-10)


Tgt Ion:168 Resp: 176641
Ion Ratio Lower Upper
168 100
99 46.9 46.9 70.3

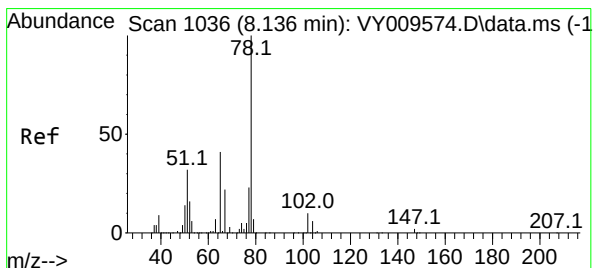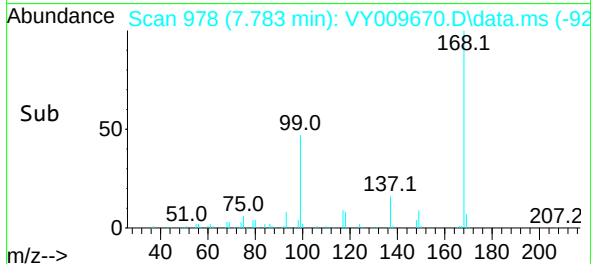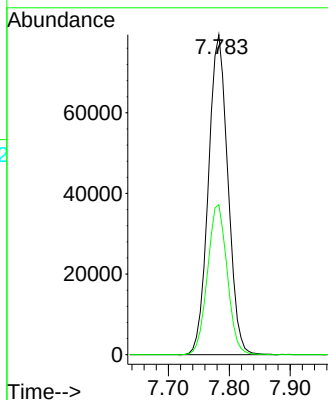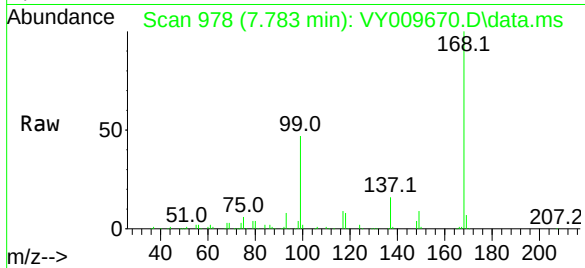

#33
1,2-Dichloroethane-d4
Concen: 57.112 ug/l
RT: 8.130 min Scan# 1035
Delta R.T. -0.006 min
Lab File: VY009670.D
Acq: 22 Jul 2022 19:21

Tgt Ion: 65 Resp: 95411
Ion Ratio Lower Upper
65 100
67 52.5 0.0 99.4


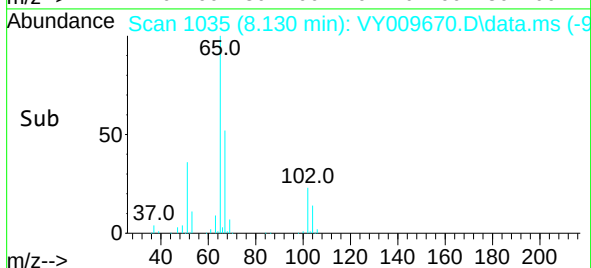
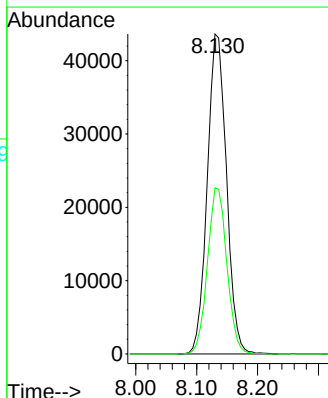
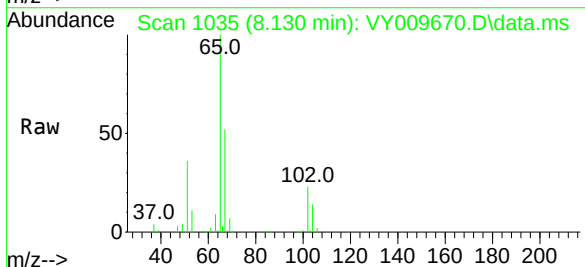


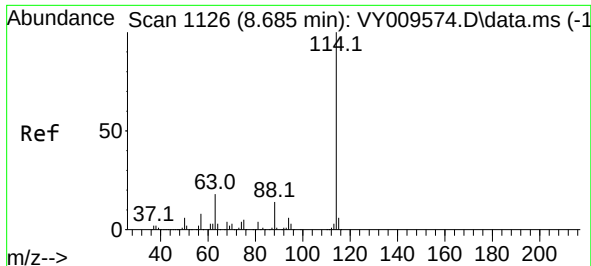

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.685 min Scan# 1126
Delta R.T. -0.000 min
Lab File: VY009670.D
Acq: 22 Jul 2022 19:21




Instrument :
MSVOA_Y
ClientSampleId :
ENV-DE-1-(5-10)


Tgt Ion:114 Resp: 277711
Ion Ratio Lower Upper
114 100
63 17.1 0.0 43.2
88 14.0 0.0 31.8

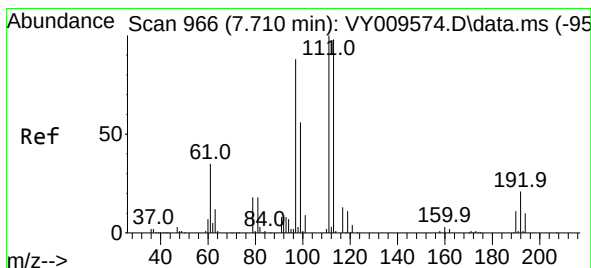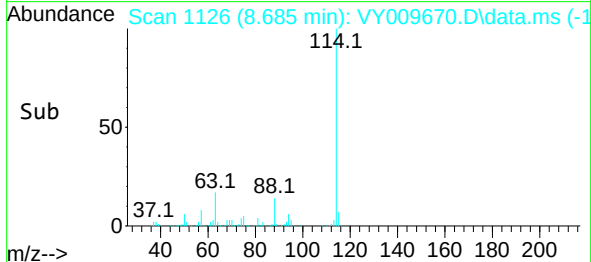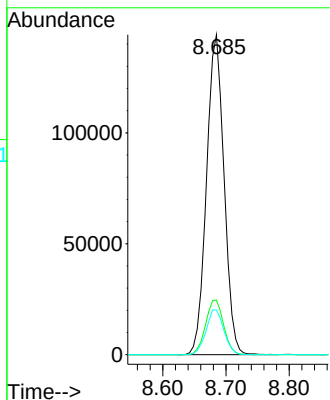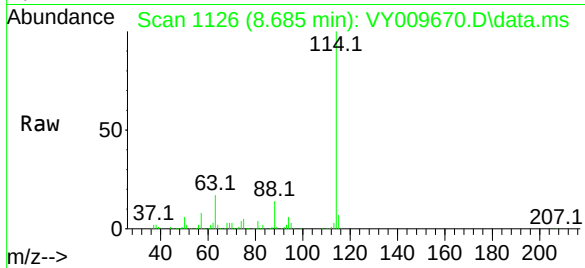

#35
Dibromofluoromethane
Concen: 50.240 ug/l
RT: 7.710 min Scan# 966
Delta R.T. -0.000 min
Lab File: VY009670.D
Acq: 22 Jul 2022 19:21

Tgt Ion:113 Resp: 87898
Ion Ratio Lower Upper
113 100
111 102.8 82.6 124.0
192 22.6 17.6 26.4


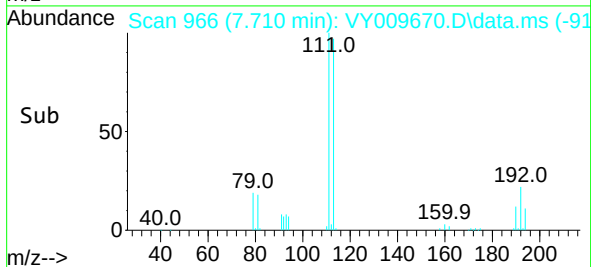
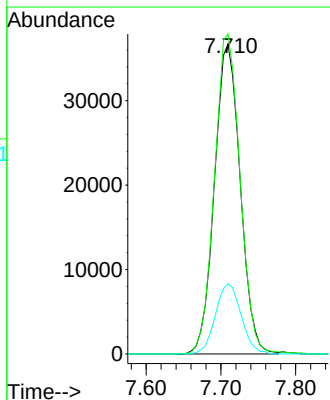
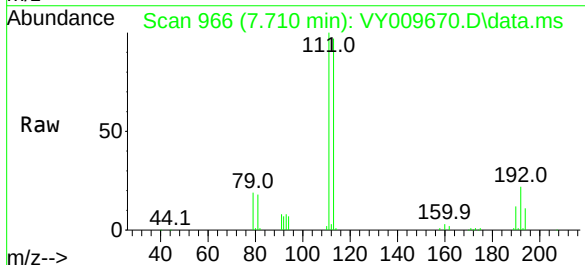


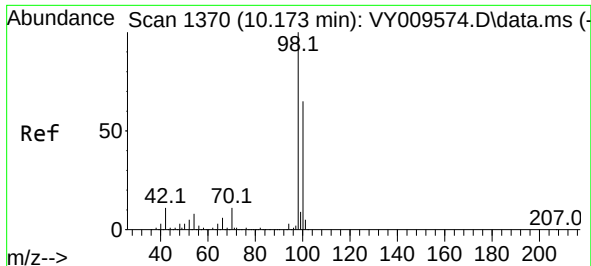

#50
Toluene-d8
Concen: 47.910 ug/l
RT: 10.172 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY009670.D
Acq: 22 Jul 2022 19:21




Instrument :
MSVOA_Y
ClientSampleId :
ENV-DE-1-(5-10)


Tgt Ion: 98 Resp: 322237
Ion Ratio Lower Upper
98 100
100 64.4 50.2 75.2

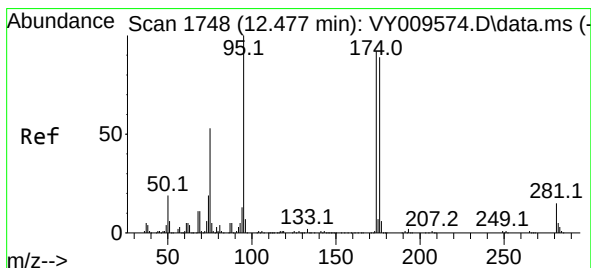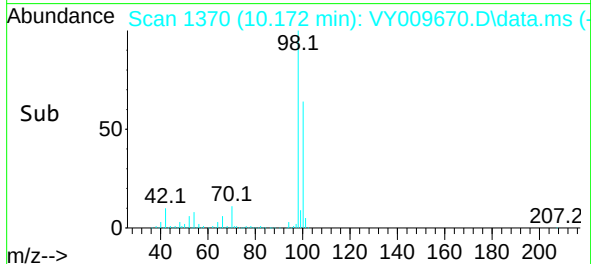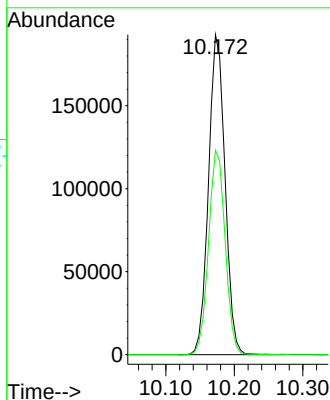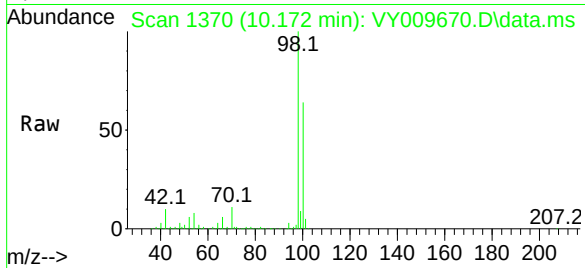

#62
4-Bromofluorobenzene
Concen: 47.613 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. -0.000 min
Lab File: VY009670.D
Acq: 22 Jul 2022 19:21

Tgt Ion: 95 Resp: 103767
Ion Ratio Lower Upper
95 100
174 98.5 0.0 177.0
176 94.8 0.0 175.8


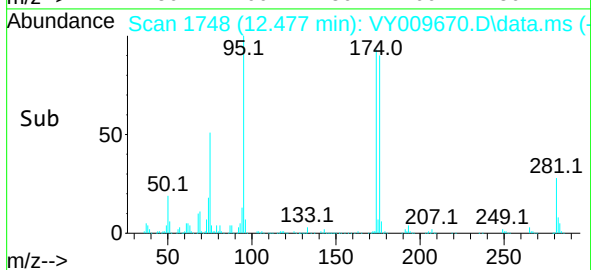
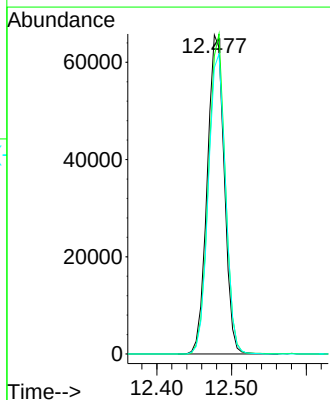
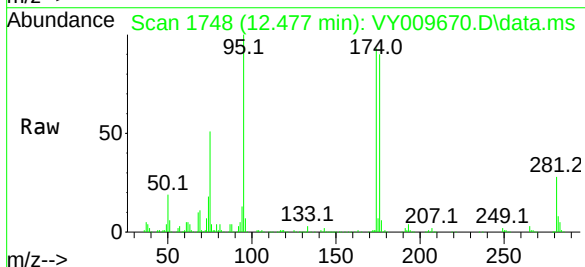


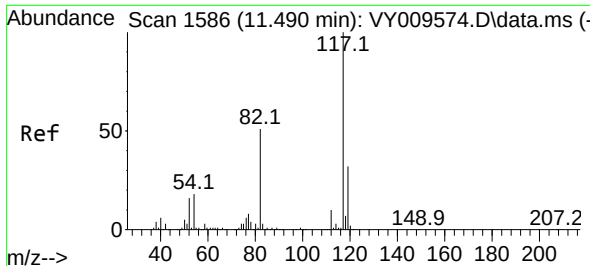

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY009670.D
Acq: 22 Jul 2022 19:21

Instrument :
MSVOA_Y
ClientSampleId :
ENV-DE-1-(5-10)

Tgt Ion:117 Resp: 263035
Ion Ratio Lower Upper
117 100
82 49.0 43.0 64.4
119 32.2 25.4 38.0

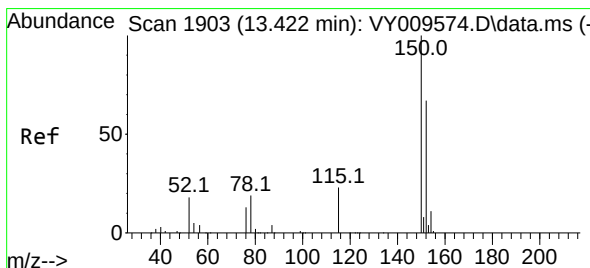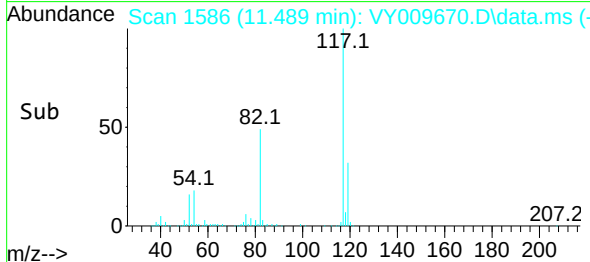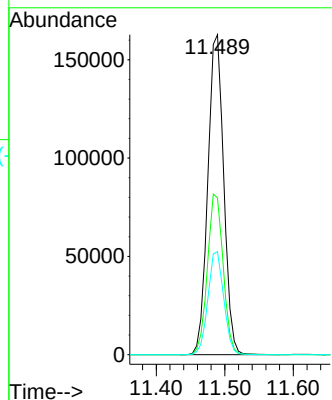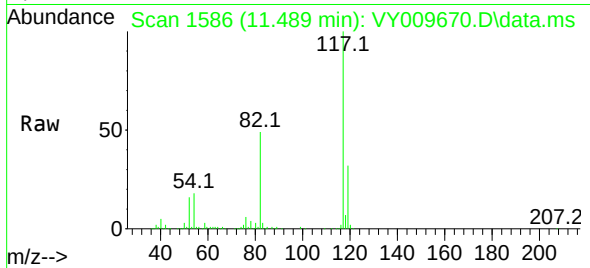

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.422 min Scan# 1903
Delta R.T. -0.000 min
Lab File: VY009670.D
Acq: 22 Jul 2022 19:21

Tgt Ion:152 Resp: 122648
Ion Ratio Lower Upper
152 100
115 54.4 28.2 84.7
150 156.3 0.0 347.6

