
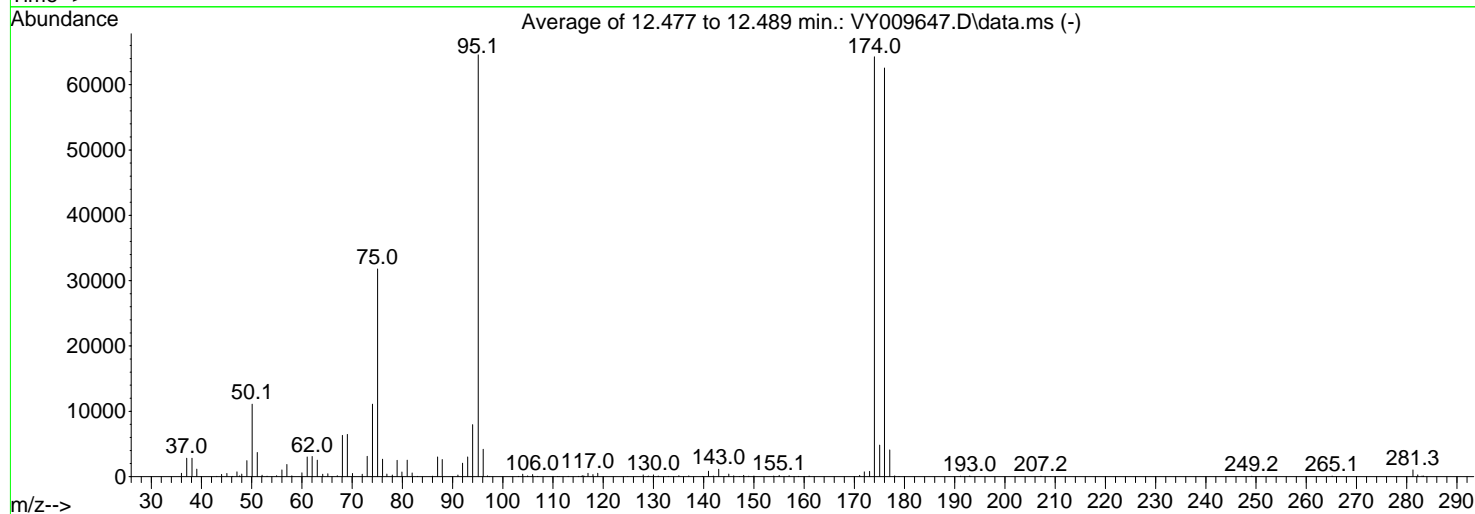


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY072222\  
 Data File : VY009647.D  
 Acq On : 22 Jul 2022 08:42  
 Operator : KP/MD  
 Sample : BFB  
 Misc : 5.00g/5.0mL/MSVOA\_Y/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_Y  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y071822S.M  
 Title : SW846 8260  
 Last Update : Tue Jul 19 04:22:09 2022

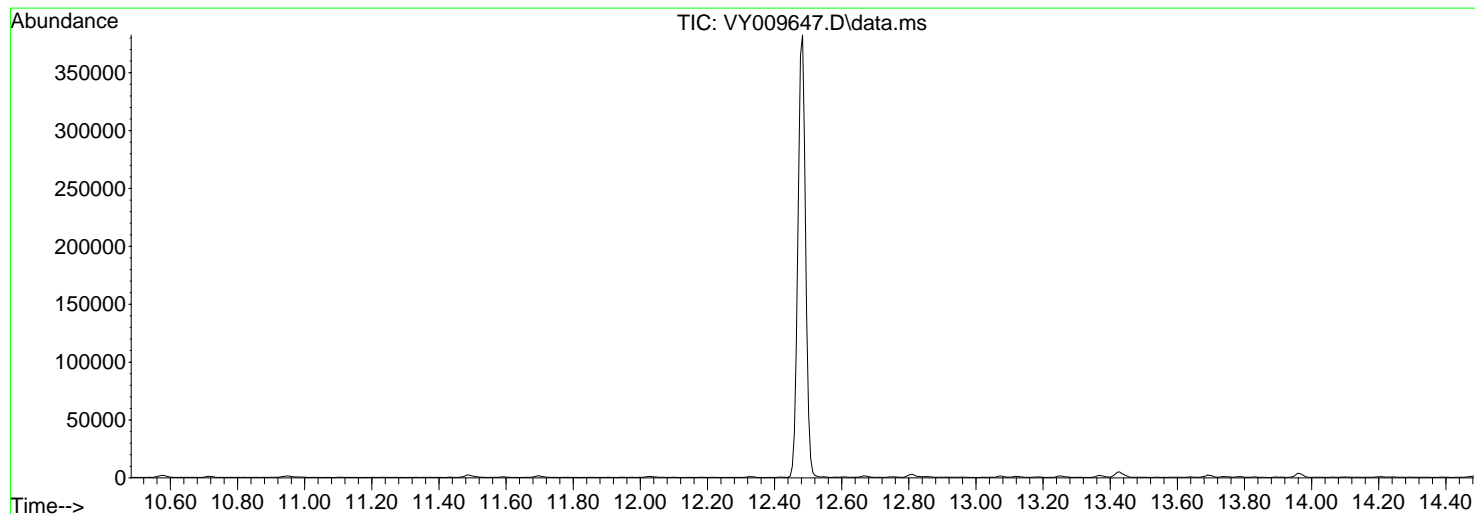

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1739

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	11103	PASS
75	95	30	60	49.3	31803	PASS
95	95	100	100	100.0	64568	PASS
96	95	5	9	6.5	4188	PASS
173	174	0.00	2	1.3	823	PASS
174	95	50	100	99.5	64277	PASS
175	174	5	9	7.5	4817	PASS
176	174	95	101	97.3	62555	PASS
177	176	5	9	6.5	4092	PASS