

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY072522\
 Data File : VY009681.D
 Acq On : 25 Jul 2022 13:04
 Operator : KP/MD
 Sample : N3858-01
 Misc : 4.39g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 SB-A

Quant Time: Jul 26 05:56:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y071822S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jul 19 04:22:09 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.783	168	169202	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	264218	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	258647	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	127700	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.130	65	87151	54.461	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 108.920%	
35) Dibromofluoromethane	7.710	113	83821	50.356	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 100.720%	
50) Toluene-d8	10.173	98	309379	48.347	ug/l	0.00
Spiked Amount	50.000	Range	78 - 125	Recovery	= 96.700%	
62) 4-Bromofluorobenzene	12.477	95	106428	51.328	ug/l	0.00
Spiked Amount	50.000	Range	50 - 146	Recovery	= 102.660%	
Target Compounds						
2) Dichlorodifluoromethane	1.900	85	8394	5.654	ug/l	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY072522\
Data File : VY009681.D
Acq On : 25 Jul 2022 13:04
Operator : KP/MD
Sample : N3858-01
Misc : 4.39g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
SB-A

Quant Time: Jul 26 05:56:11 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y071822S.M
Quant Title : SW846 8260
QLast Update : Tue Jul 19 04:22:09 2022
Response via : Initial Calibration




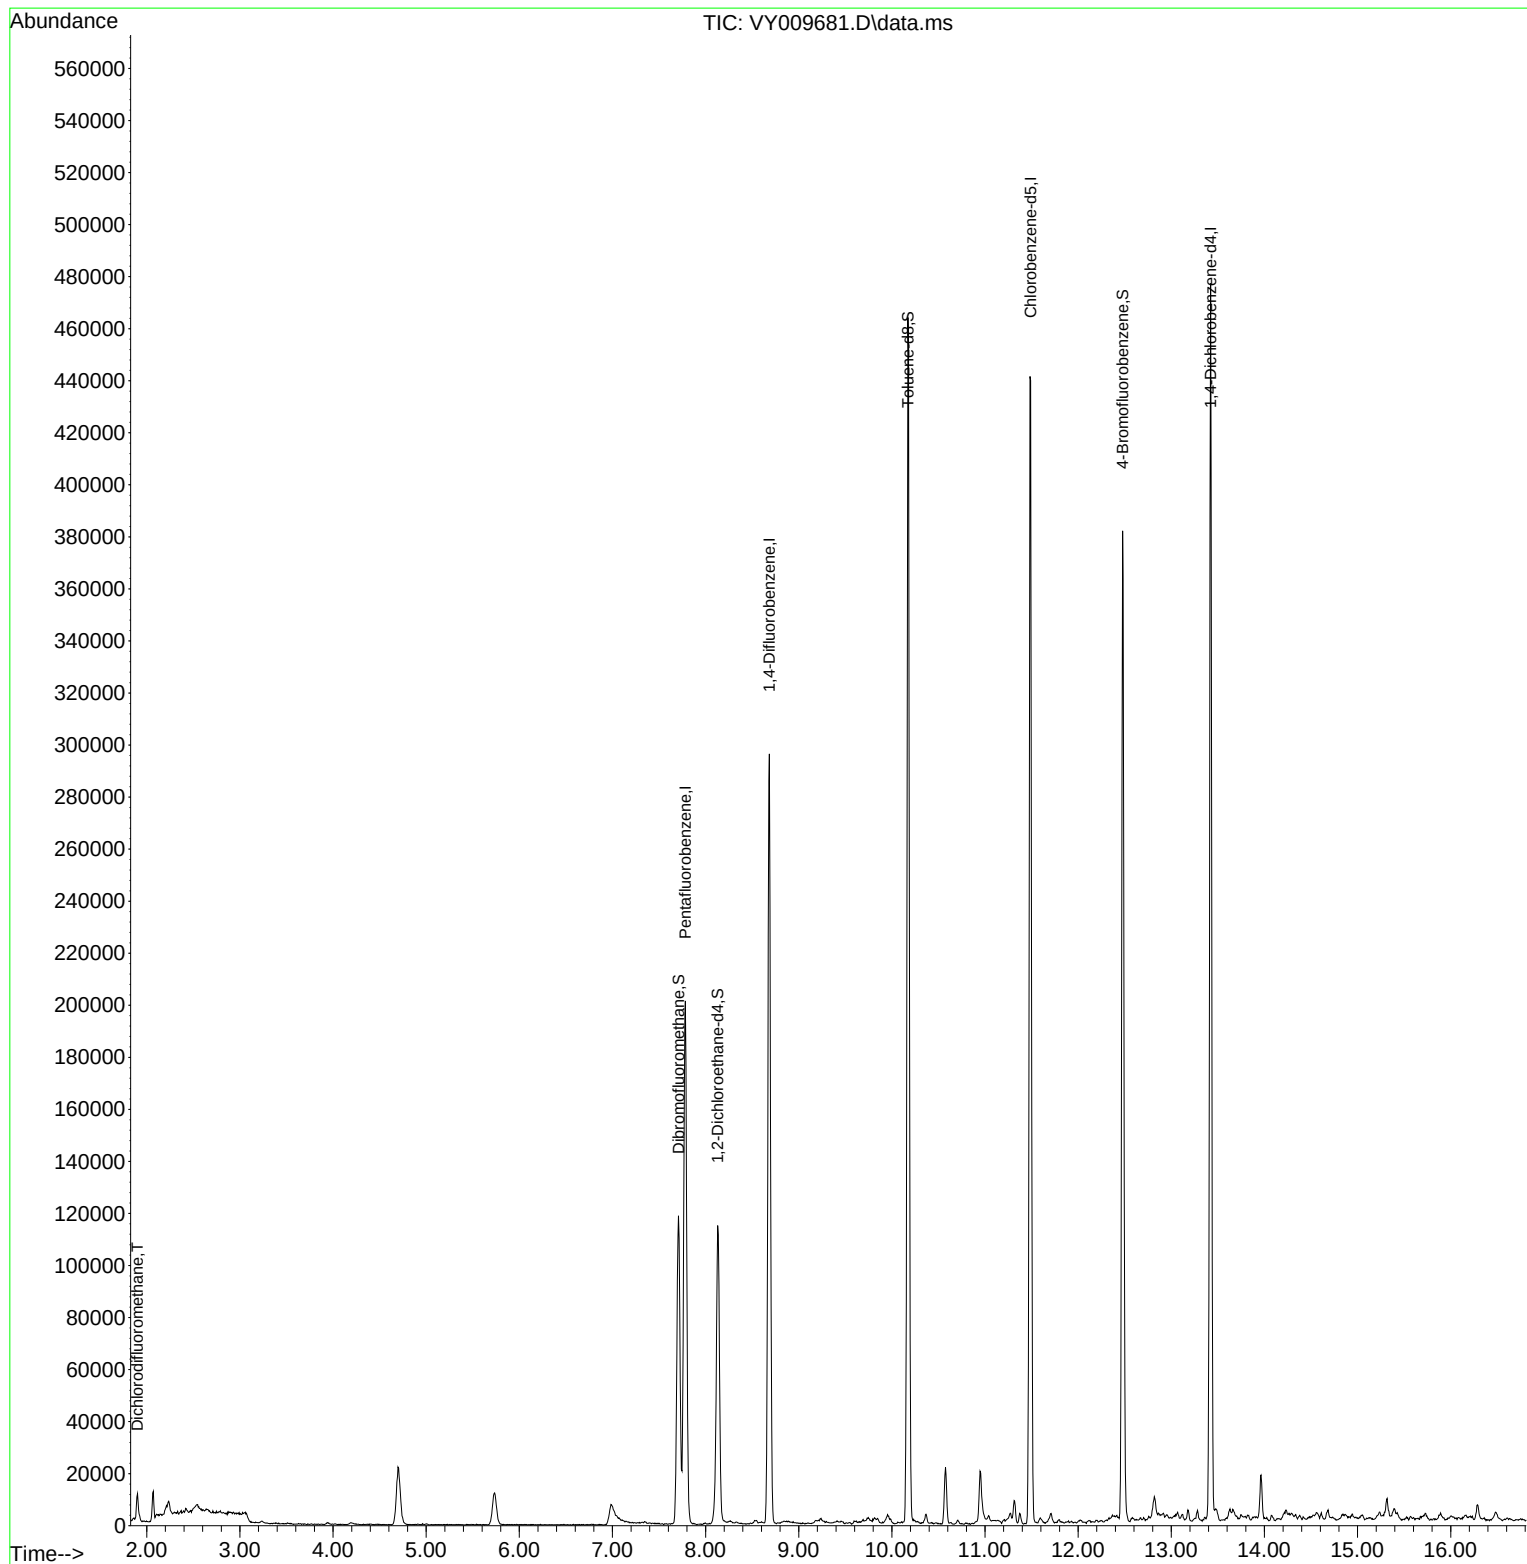


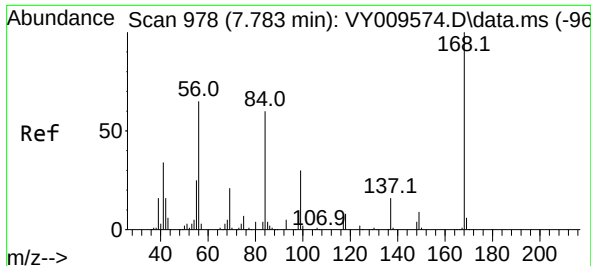

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.783 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY009681.D
Acq: 25 Jul 2022 13:04




Instrument :
MSVOA_Y
ClientSampleId :
SB-A


Tgt Ion:168 Resp: 169202
Ion Ratio Lower Upper
168 100
99 47.3 46.9 70.3

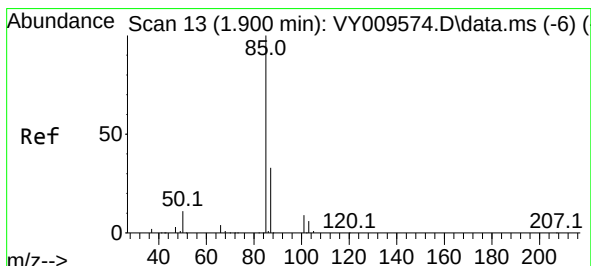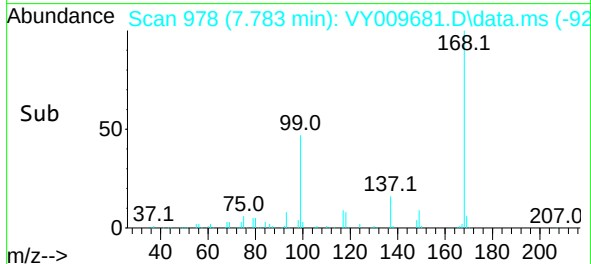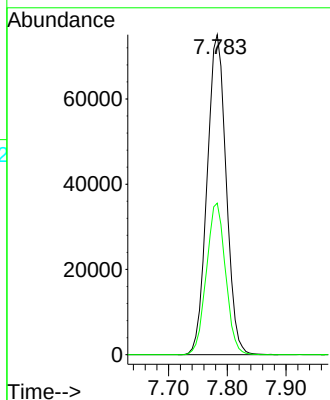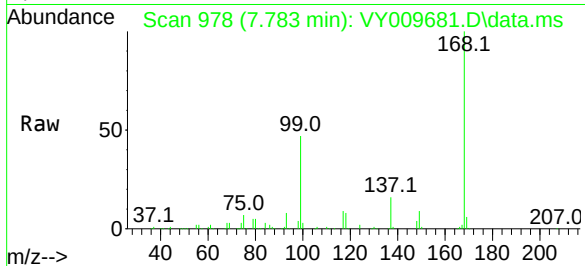

#2
Dichlorodifluoromethane
Concen: 5.654 ug/l
RT: 1.900 min Scan# 13
Delta R.T. -0.000 min
Lab File: VY009681.D
Acq: 25 Jul 2022 13:04

Tgt Ion: 85 Resp: 8394
Ion Ratio Lower Upper
85 100
87 31.4 16.1 48.2

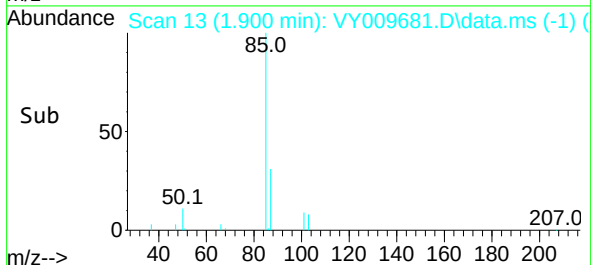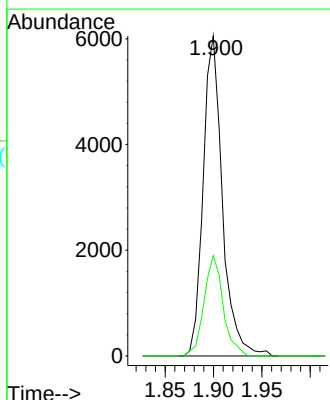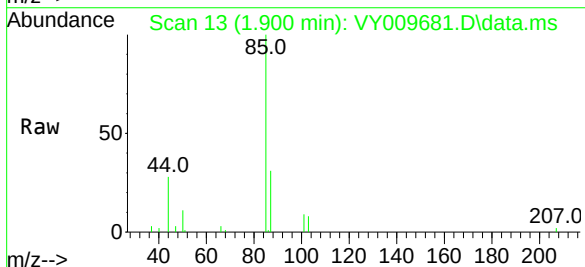

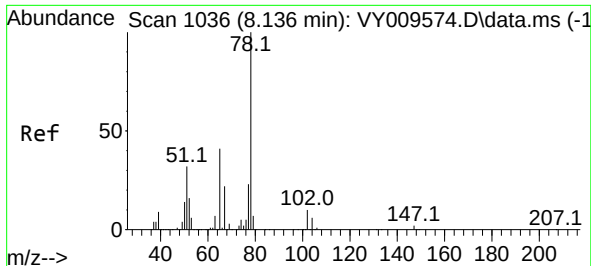

#33

1,2-Dichloroethane-d4

Concen: 54.461 ug/l

RT: 8.130 min Scan# 1

Delta R.T. -0.006 min

Lab File: VY009681.D

Acq: 25 Jul 2022 13:04

Instrument :

MSVOA_Y

ClientSampleId :





SB-A

Tgt Ion: 65 Resp: 87151

Ion Ratio Lower Upper

65 100

67 52.4 0.0 99.4

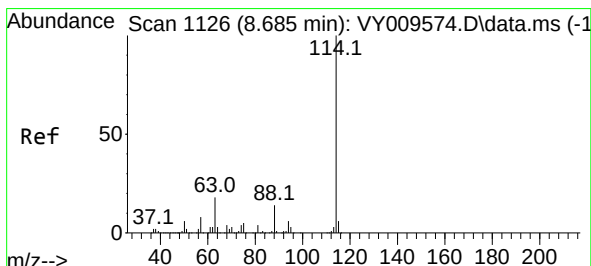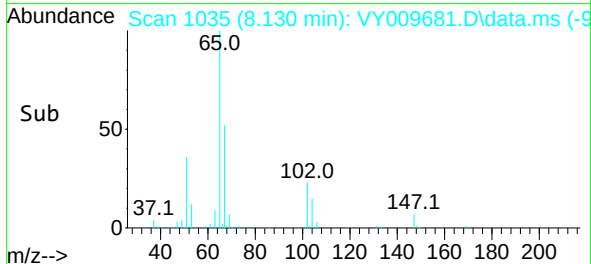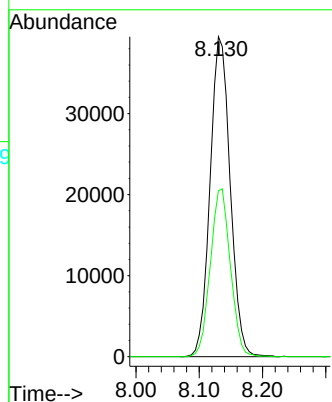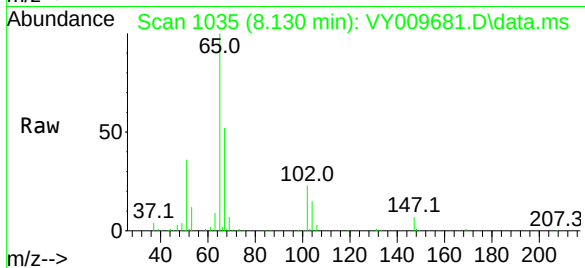

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.685 min Scan# 1126

Delta R.T. -0.000 min

Lab File: VY009681.D

Acq: 25 Jul 2022 13:04




Tgt Ion: 114 Resp: 264218


Ion Ratio Lower Upper

114 100

63 16.3 0.0 43.2

88 13.8 0.0 31.8


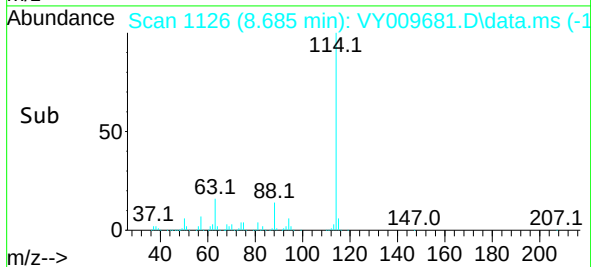
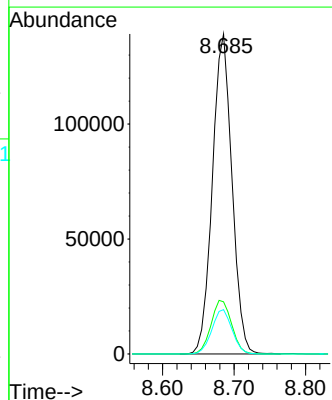
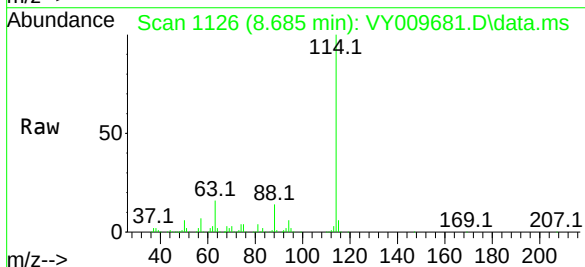


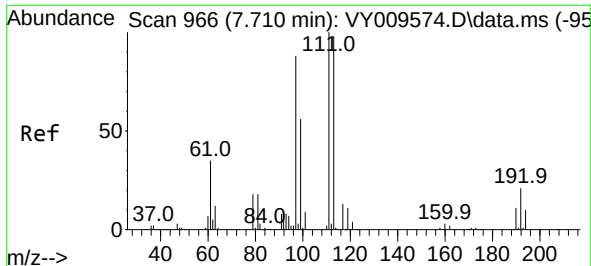

#35
Dibromofluoromethane
Concen: 50.356 ug/l
RT: 7.710 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY009681.D
Acq: 25 Jul 2022 13:04




Instrument :
MSVOA_Y
ClientSampleId :
SB-A


Tgt Ion:113 Resp: 83821
Ion Ratio Lower Upper
113 100
111 102.4 82.6 124.0
192 22.5 17.6 26.4

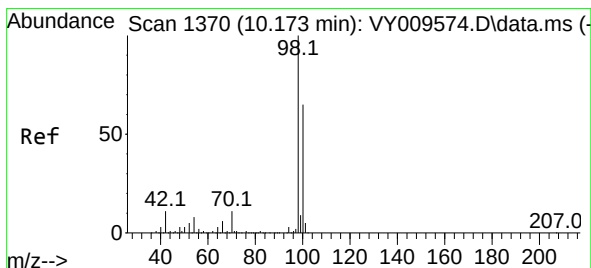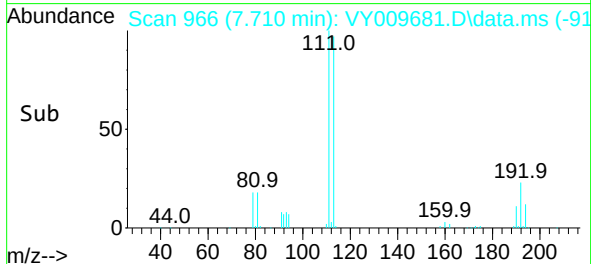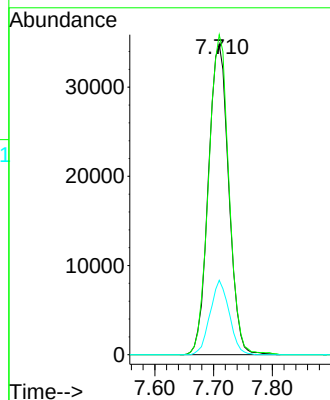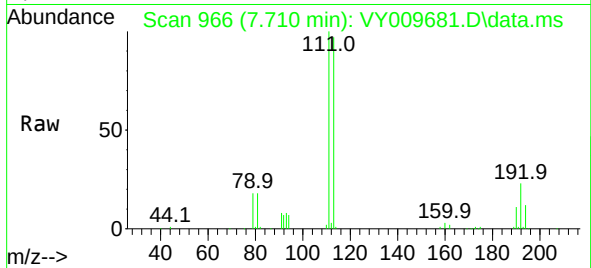

#50
Toluene-d8
Concen: 48.347 ug/l
RT: 10.173 min Scan# 1370
Delta R.T. -0.000 min
Lab File: VY009681.D
Acq: 25 Jul 2022 13:04

Tgt Ion: 98 Resp: 309379
Ion Ratio Lower Upper
98 100
100 65.0 50.2 75.2


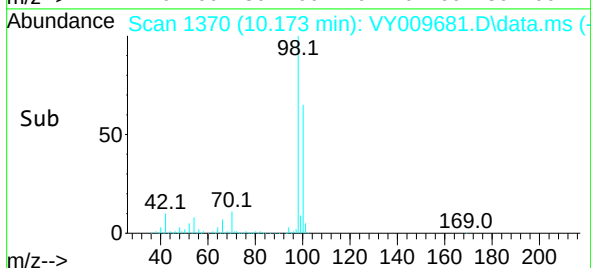
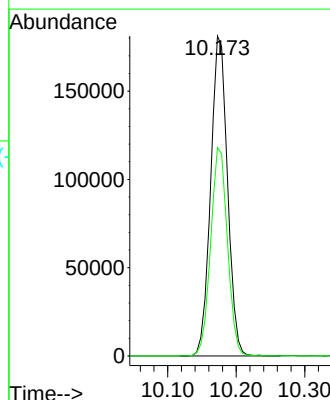
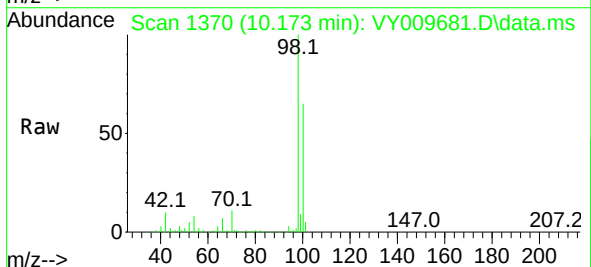


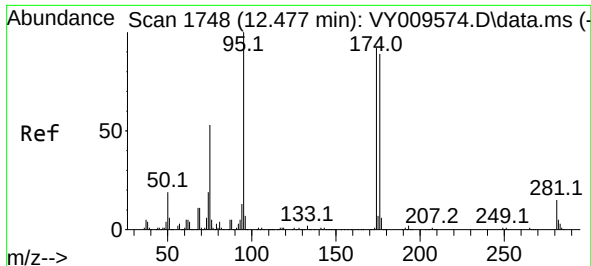

#62
4-Bromofluorobenzene
Concen: 51.328 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. -0.000 min
Lab File: VY009681.D
Acq: 25 Jul 2022 13:04




Instrument :
MSVOA_Y
ClientSampleId :
SB-A


Tgt Ion: 95 Resp: 106428
Ion Ratio Lower Upper
95 100
174 97.5 0.0 177.0
176 94.6 0.0 175.8

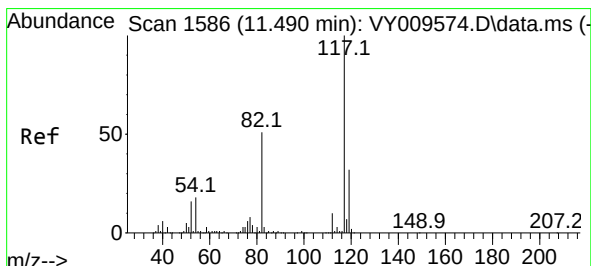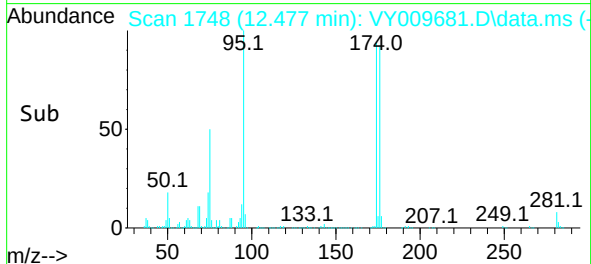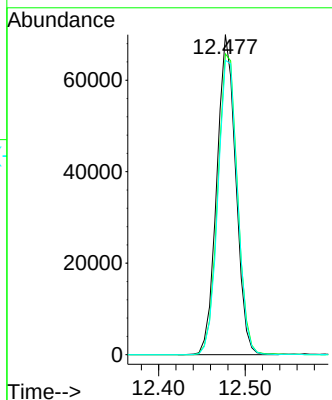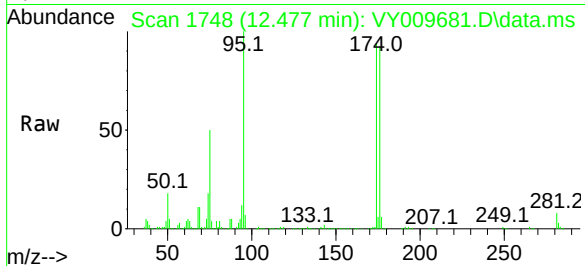

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 1586
Delta R.T. -0.000 min
Lab File: VY009681.D
Acq: 25 Jul 2022 13:04

Tgt Ion: 117 Resp: 258647
Ion Ratio Lower Upper
117 100
82 49.5 43.0 64.4
119 31.7 25.4 38.0

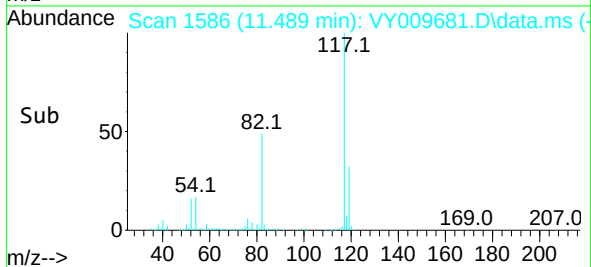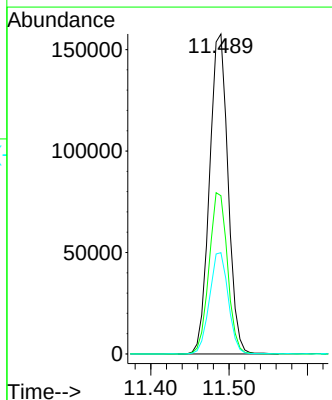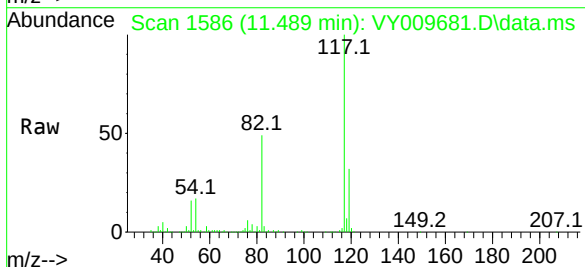

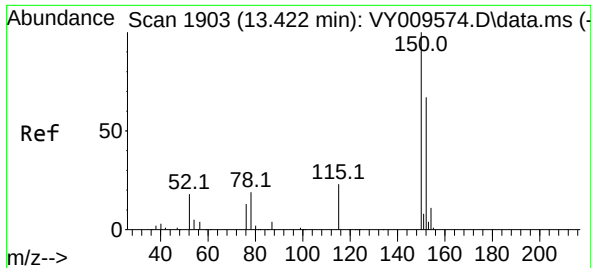

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.422 min Scan# 1903

Delta R.T. -0.000 min

Lab File: VY009681.D


Acq: 25 Jul 2022 13:04

Instrument :

MSVOA_Y

ClientSampleId :

SB-A

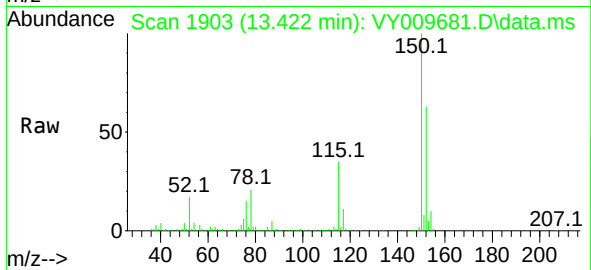

Tgt Ion:152 Resp: 127700

Ion Ratio Lower Upper

152 100

115 54.3 28.2 84.7

150 158.0 0.0 347.6

