


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY072522\
Data File : VY009673.D
Acq On : 25 Jul 2022 09:07
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y071822S.M
Title : SW846 8260
Last Update : Tue Jul 19 04:22:09 2022

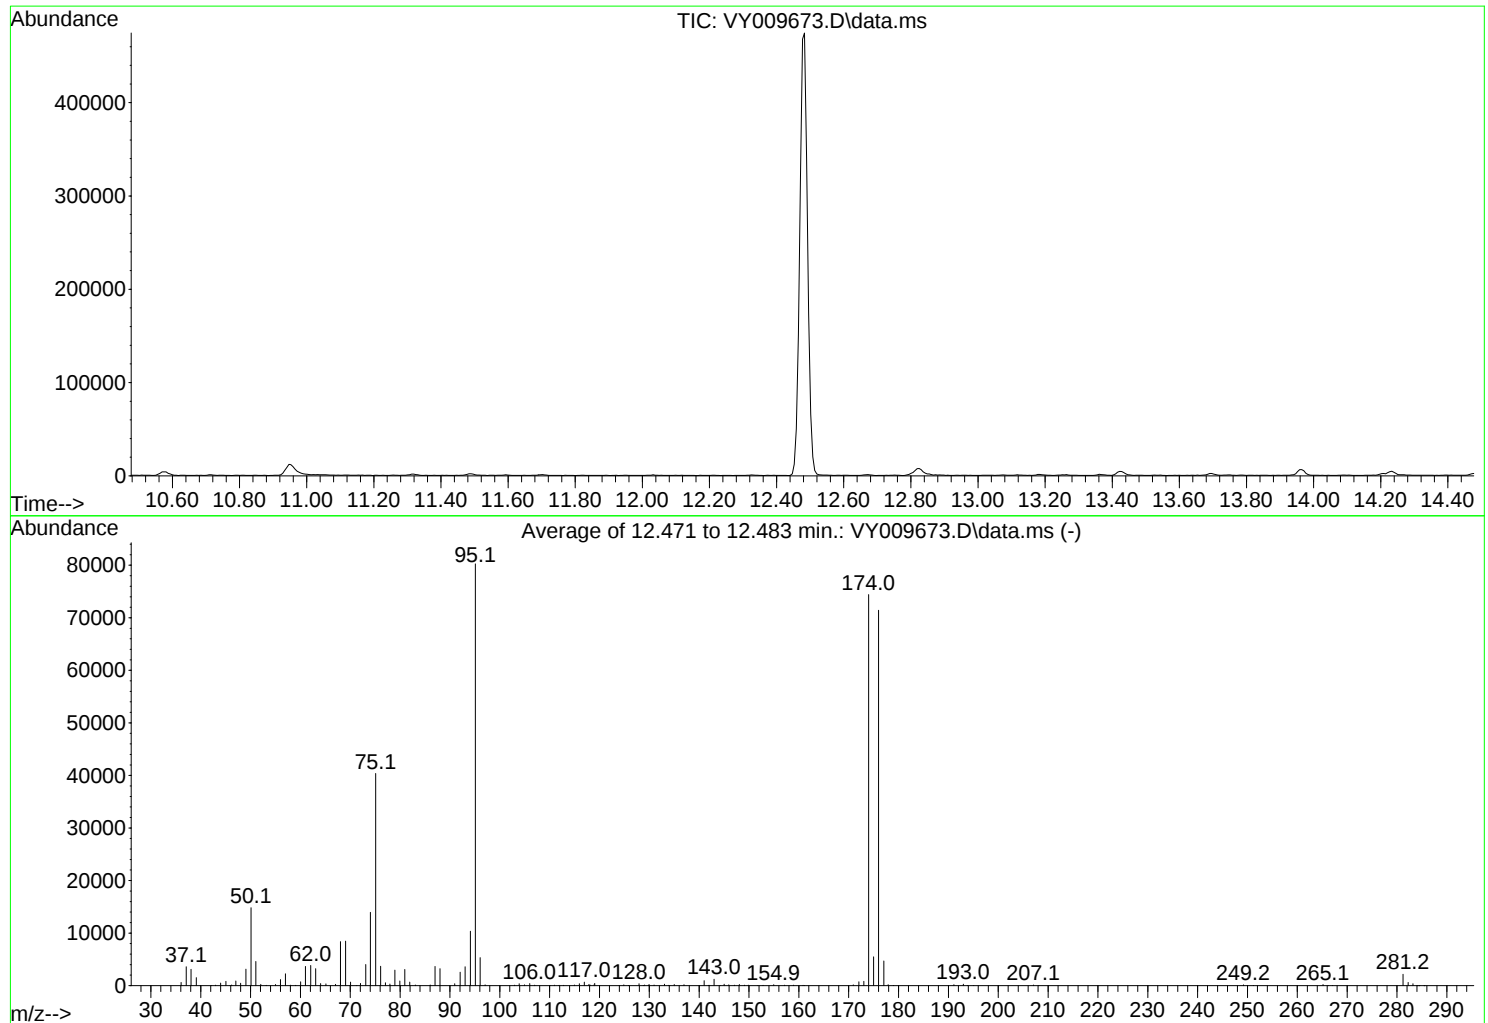

AutoFind: Scans 1747, 1748, 1749; Background Corrected with Scan 1739

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	14839	PASS
75	95	30	60	50.3	40389	PASS
95	95	100	100	100.0	80264	PASS
96	95	5	9	6.7	5343	PASS
173	174	0.00	2	1.1	810	PASS
174	95	50	100	92.7	74403	PASS
175	174	5	9	7.4	5476	PASS
176	174	95	101	96.0	71416	PASS
177	176	5	9	6.6	4692	PASS