

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY072523\
 Data File : VY014805.D
 Acq On : 25 Jul 2023 16:33
 Operator : SY/MD
 Sample : 03742-06
 Misc : 5.10g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 DUP-02

Quant Time: Jul 26 01:20:13 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y071323S.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 14 02:09:50 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	168588	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	299533	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	287766	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	139260	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	109442	56.968	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	113.940%
35) Dibromofluoromethane	7.716	113	95625	50.151	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	100.300%
50) Toluene-d8	10.179	98	355898	50.627	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	101.260%
62) 4-Bromofluorobenzene	12.477	95	132841	49.283	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	98.560%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY072523\
Data File : VY014805.D
Acq On : 25 Jul 2023 16:33
Operator : SY/MD
Sample : 03742-06
Misc : 5.10g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
DUP-02

Quant Time: Jul 26 01:20:13 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y071323S.M
Quant Title : SW846 8260
QLast Update : Fri Jul 14 02:09:50 2023
Response via : Initial Calibration




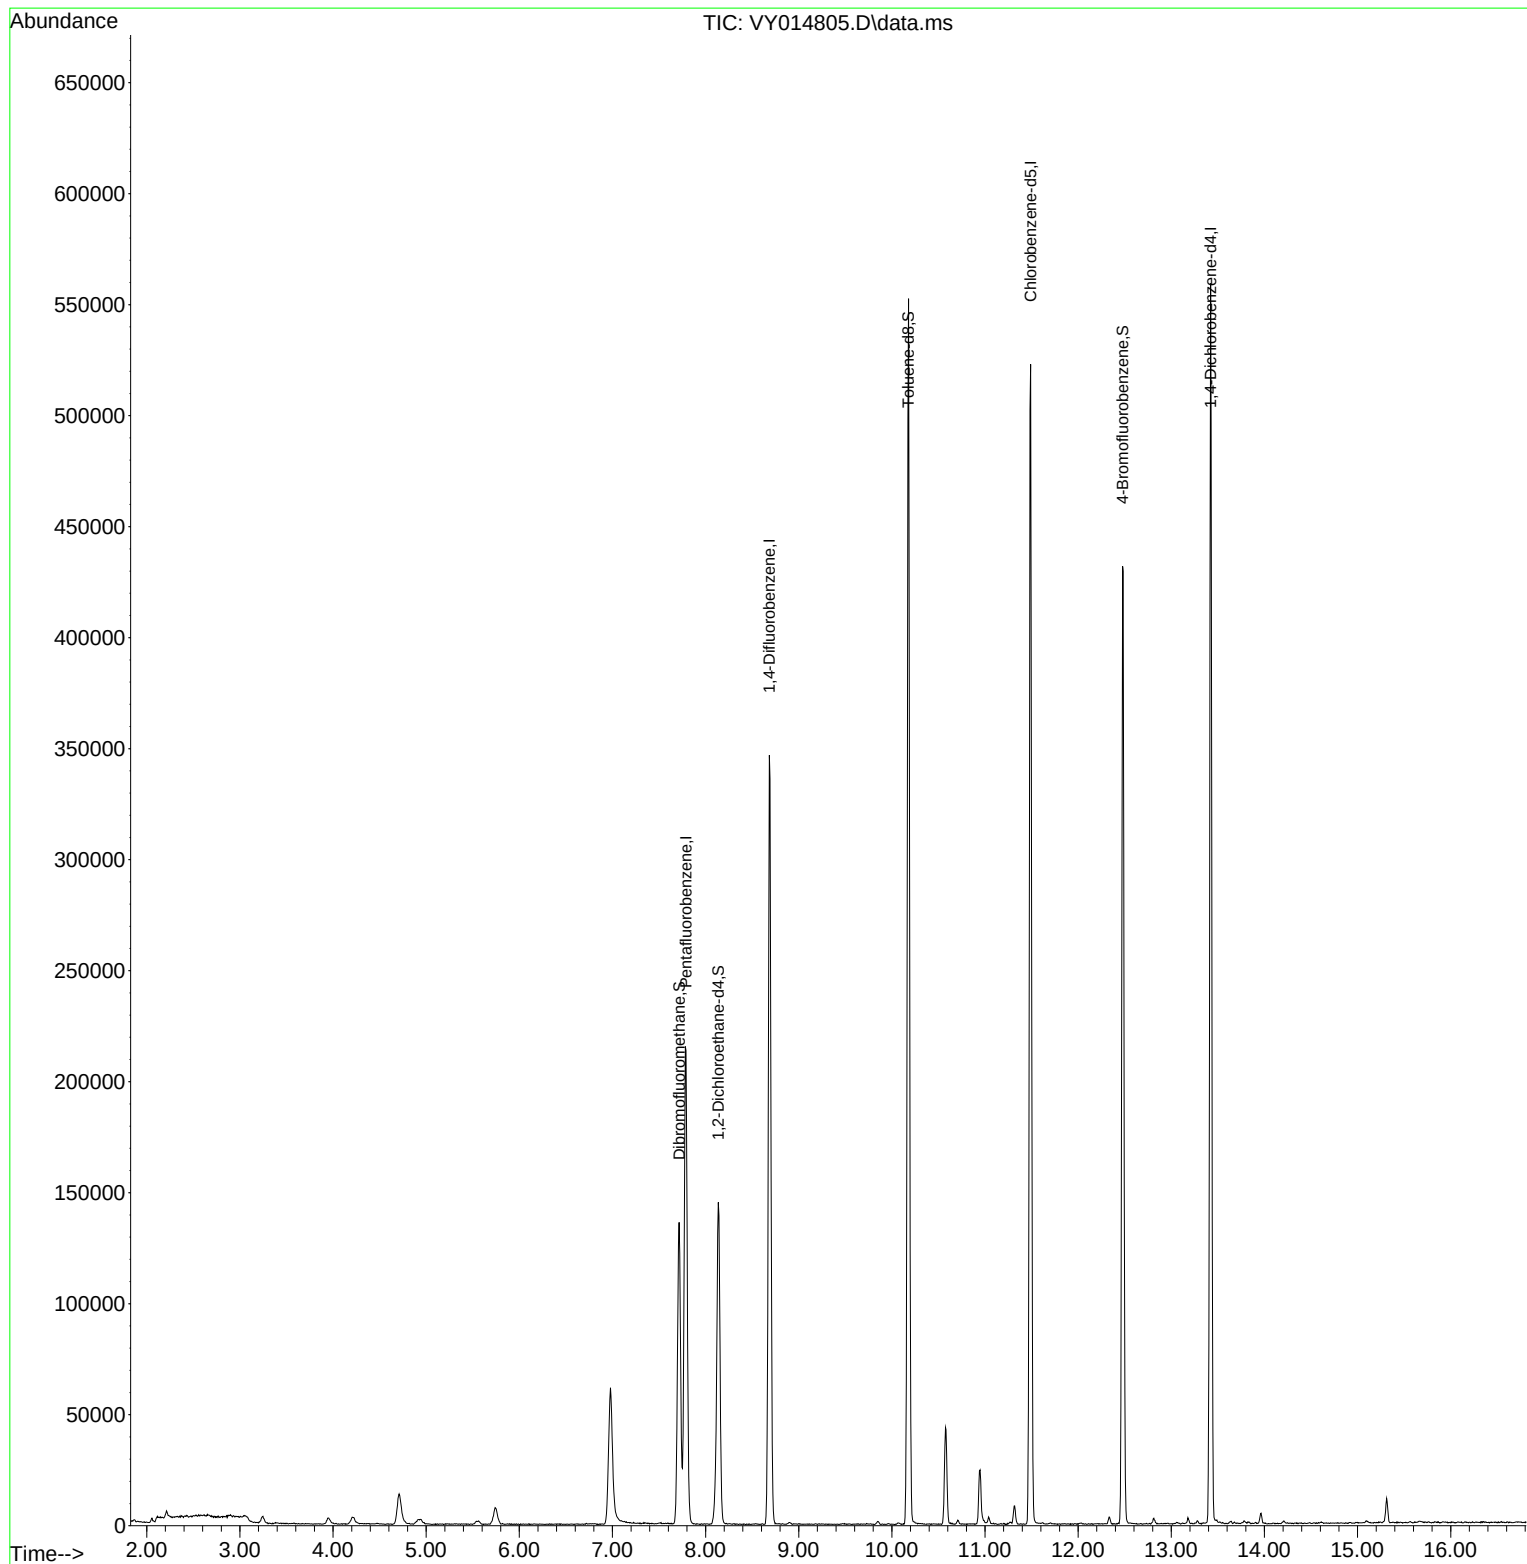


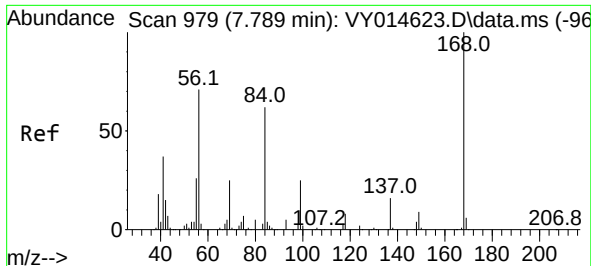

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY014805.D
Acq: 25 Jul 2023 16:33




Instrument :
MSVOA_Y
ClientSampleId :
DUP-02


Tgt Ion:168 Resp: 168588
Ion Ratio Lower Upper
168 100
99 56.3 43.4 65.0

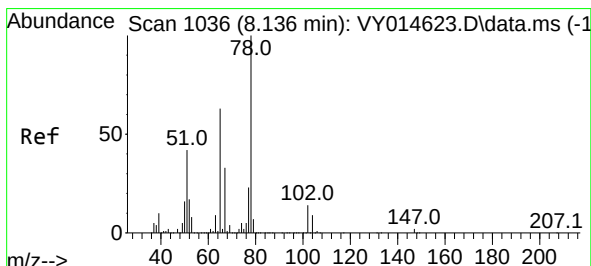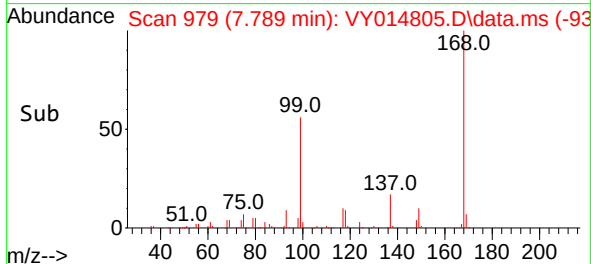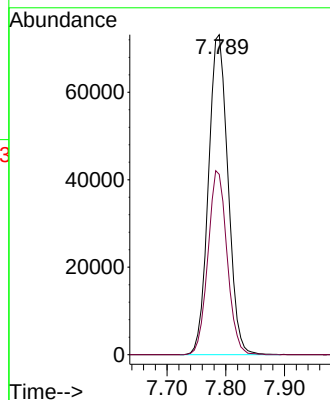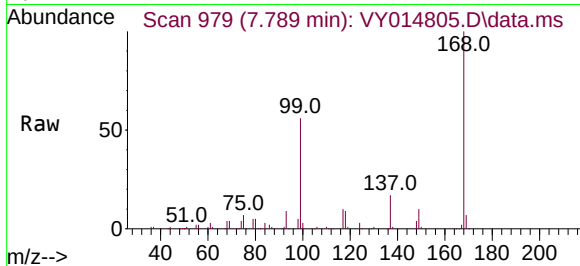

#33
1,2-Dichloroethane-d4
Concen: 56.968 ug/l
RT: 8.136 min Scan# 1036
Delta R.T. 0.000 min
Lab File: VY014805.D
Acq: 25 Jul 2023 16:33

Tgt Ion: 65 Resp: 109442
Ion Ratio Lower Upper
65 100
67 53.0 0.0 101.8


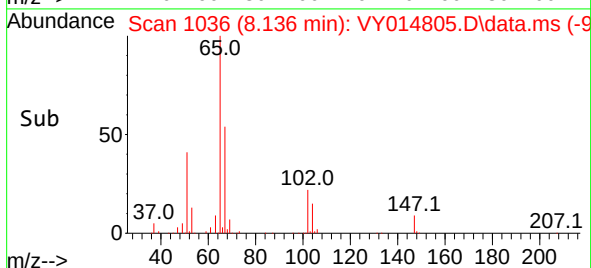
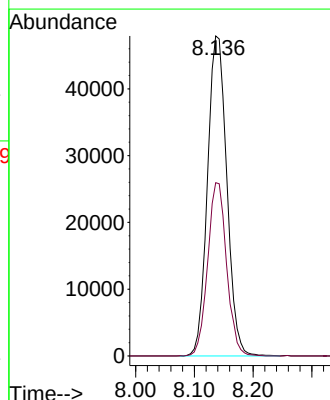
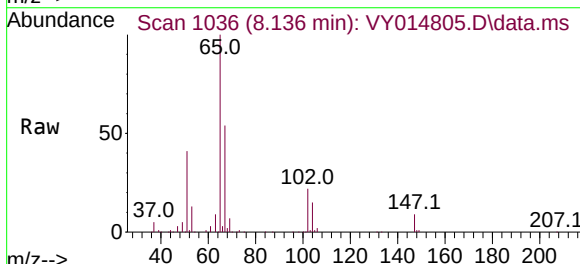


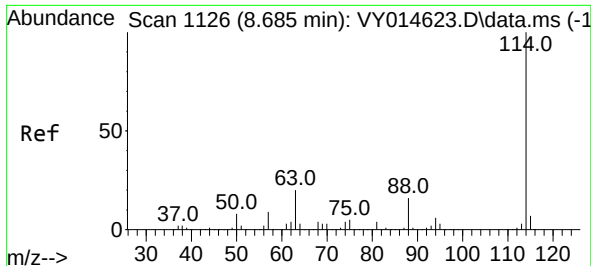

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.685 min Scan# 1126
Delta R.T. 0.000 min
Lab File: VY014805.D
Acq: 25 Jul 2023 16:33




Instrument :
MSVOA_Y
ClientSampleId :
DUP-02


Tgt Ion:114 Resp: 299533
Ion Ratio Lower Upper
114 100
63 19.6 0.0 42.4
88 15.0 0.0 30.6

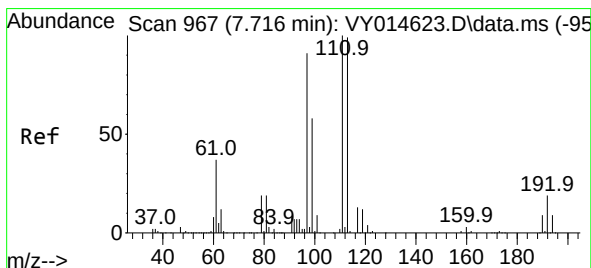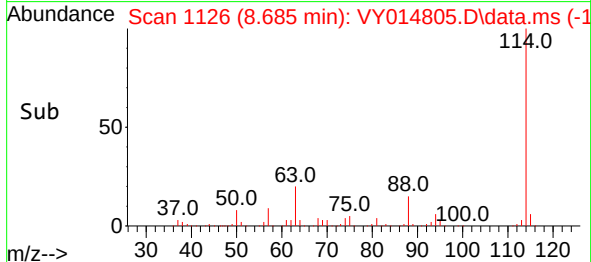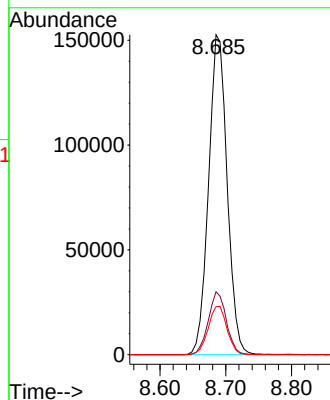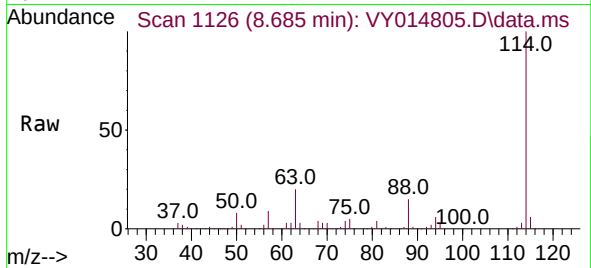

#35
Dibromofluoromethane
Concen: 50.151 ug/l
RT: 7.716 min Scan# 967
Delta R.T. -0.000 min
Lab File: VY014805.D
Acq: 25 Jul 2023 16:33

Tgt Ion:113 Resp: 95625
Ion Ratio Lower Upper
113 100
111 101.9 81.3 121.9
192 19.2 16.9 25.3


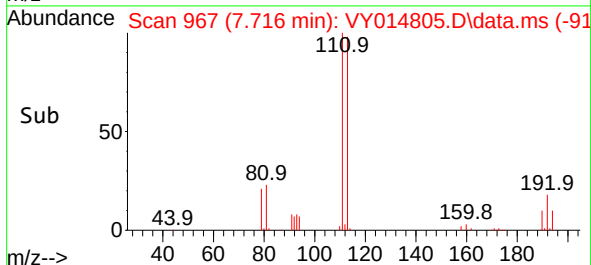
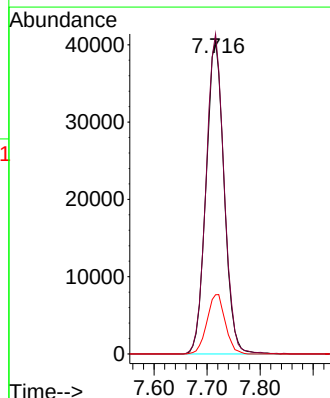
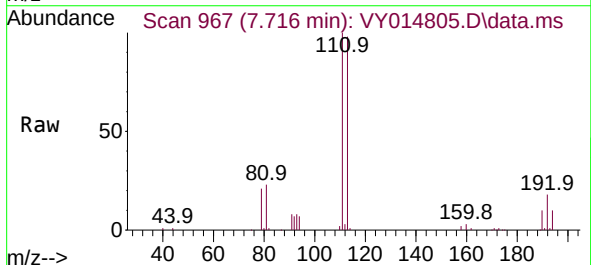


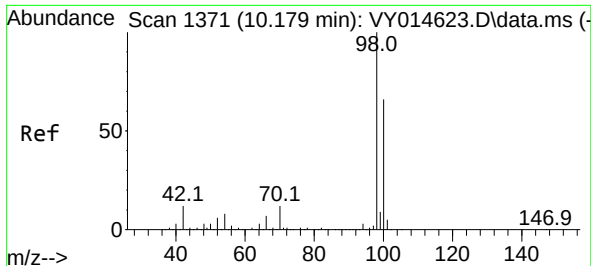

#50
Toluene-d8
Concen: 50.627 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. -0.000 min
Lab File: VY014805.D
Acq: 25 Jul 2023 16:33




Instrument :
MSVOA_Y
ClientSampleId :
DUP-02


Tgt Ion: 98 Resp: 355898
Ion Ratio Lower Upper
98 100
100 65.0 50.1 75.1

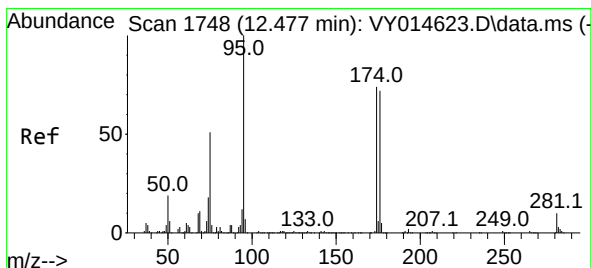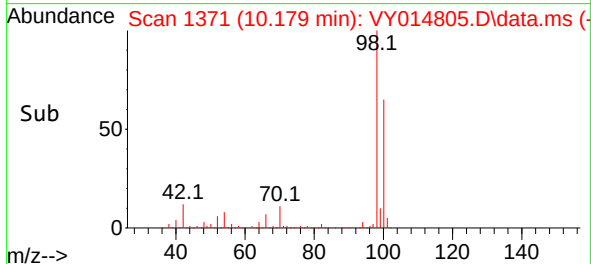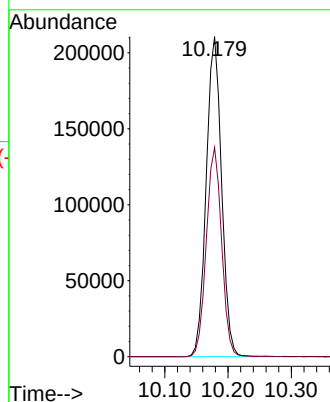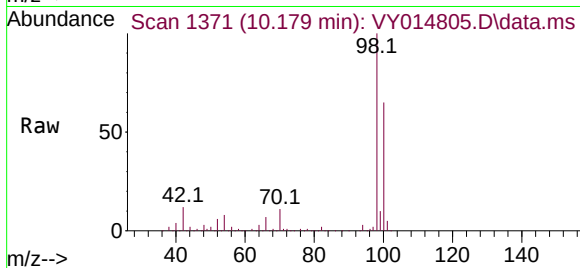

#62
4-Bromofluorobenzene
Concen: 49.283 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. 0.000 min
Lab File: VY014805.D
Acq: 25 Jul 2023 16:33

Tgt Ion: 95 Resp: 132841
Ion Ratio Lower Upper
95 100
174 82.9 0.0 178.2
176 80.4 0.0 173.8


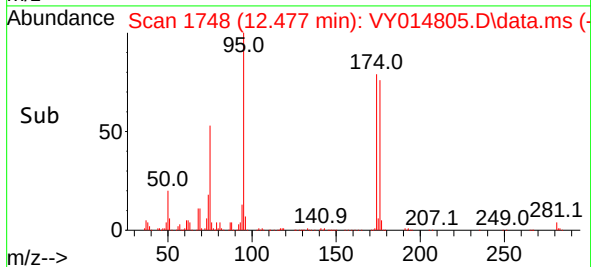
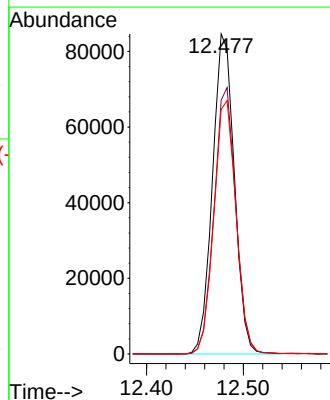
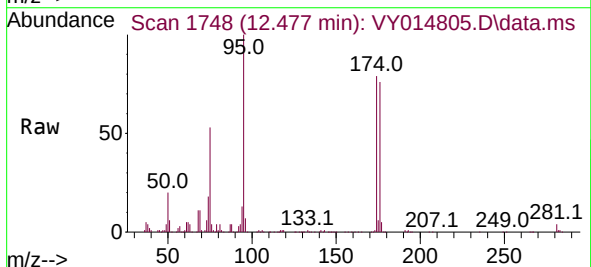


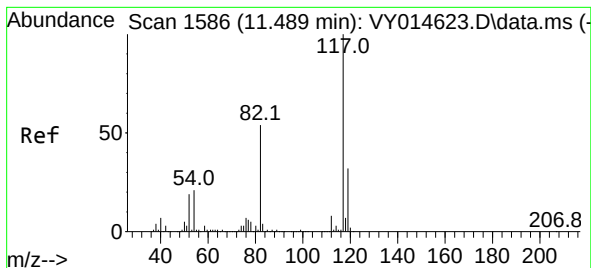

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY014805.D
Acq: 25 Jul 2023 16:33

Instrument :
MSVOA_Y
ClientSampleId :
DUP-02

Tgt Ion:117 Resp: 287766
Ion Ratio Lower Upper
117 100
82 52.8 43.4 65.0
119 31.9 26.3 39.5

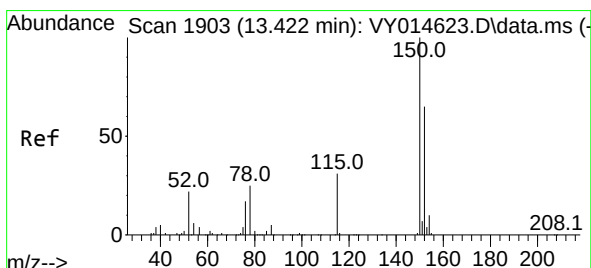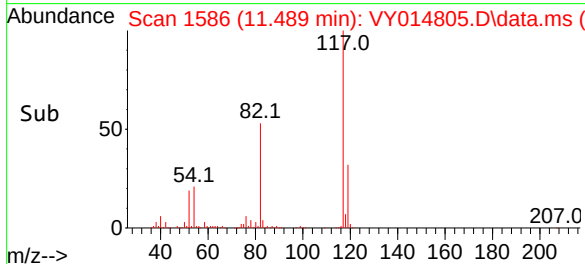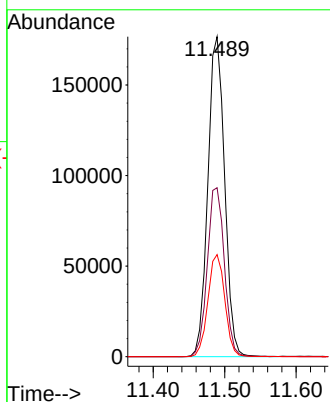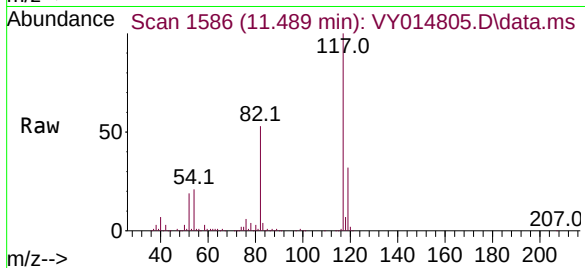

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.422 min Scan# 1903
Delta R.T. 0.000 min
Lab File: VY014805.D
Acq: 25 Jul 2023 16:33

Tgt Ion:152 Resp: 139260
Ion Ratio Lower Upper
152 100
115 59.4 28.8 86.5
150 157.2 0.0 348.8

