

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY072523\
 Data File : VY014824.D
 Acq On : 26 Jul 2023 00:48
 Operator : SY/MD
 Sample : 03741-05
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 B-P24B

Quant Time: Jul 26 03:34:37 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y071323S.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 14 02:09:50 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.795	168	144478	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.697	114	251514	50.000	ug/l	0.01
63) Chlorobenzene-d5	11.496	117	233851	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	108125	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.149	65	86418	52.490	ug/l	0.01
Spiked Amount	50.000	Range	50 - 163	Recovery	=	104.980%
35) Dibromofluoromethane	7.722	113	78174	48.826	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	97.660%
50) Toluene-d8	10.185	98	297262	50.359	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	100.720%
62) 4-Bromofluorobenzene	12.483	95	105530	46.625	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	93.260%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY072523\
Data File : VY014824.D
Acq On : 26 Jul 2023 00:48
Operator : SY/MD
Sample : 03741-05
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
B-P24B

Quant Time: Jul 26 03:34:37 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y071323S.M
Quant Title : SW846 8260
QLast Update : Fri Jul 14 02:09:50 2023
Response via : Initial Calibration




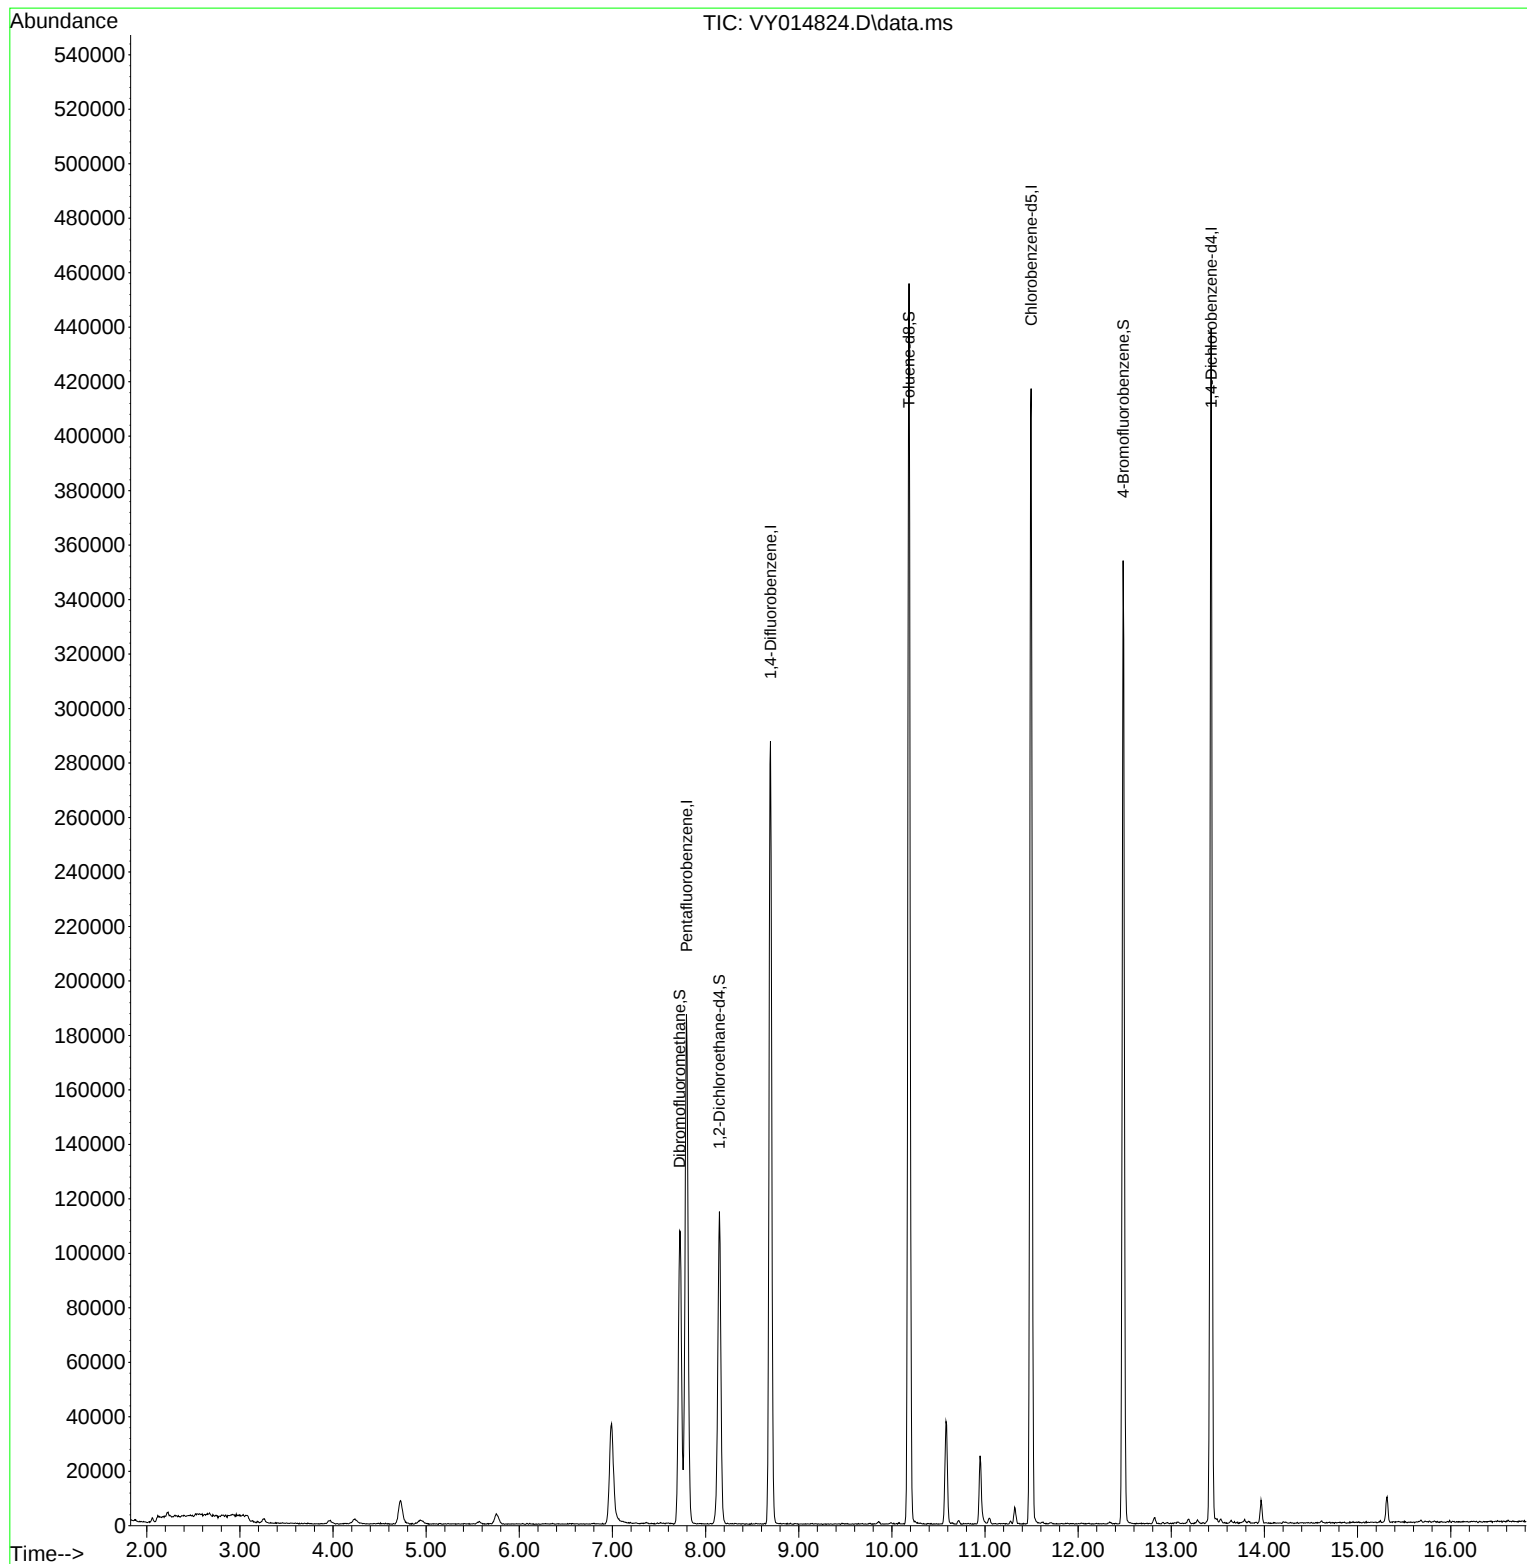




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.795 min Scan# 91
Delta R.T. 0.006 min
Lab File: VY014824.D
Acq: 26 Jul 2023 00:48




Instrument :
MSVOA_Y
ClientSampleId :
B-P24B


Tgt Ion:168 Resp: 144478
Ion Ratio Lower Upper
168 100
99 58.1 43.4 65.0

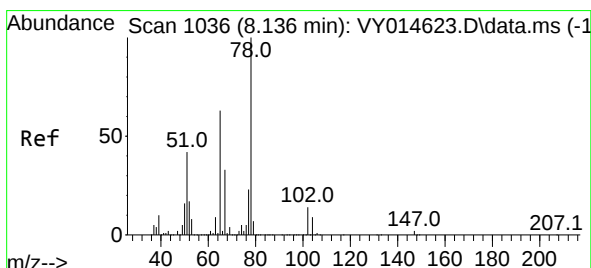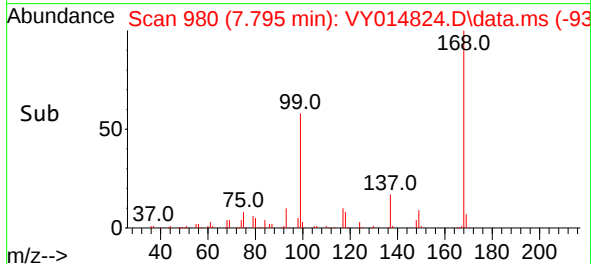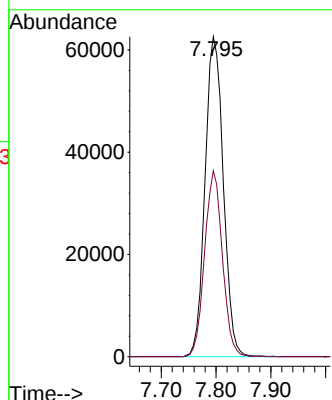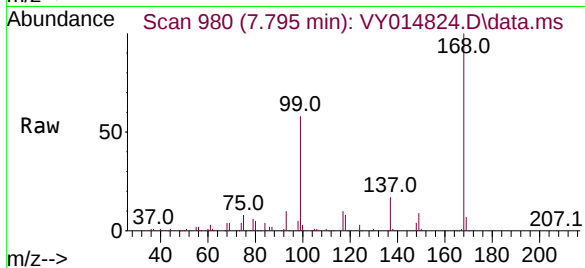

#33
1,2-Dichloroethane-d4
Concen: 52.490 ug/l
RT: 8.149 min Scan# 1038
Delta R.T. 0.013 min
Lab File: VY014824.D
Acq: 26 Jul 2023 00:48

Tgt Ion: 65 Resp: 86418
Ion Ratio Lower Upper
65 100
67 51.7 0.0 101.8

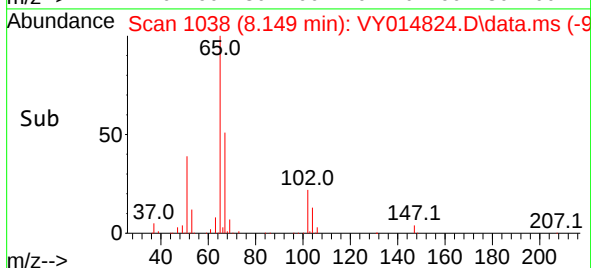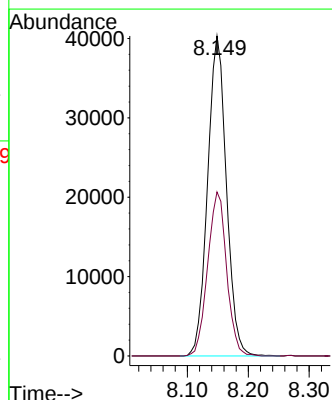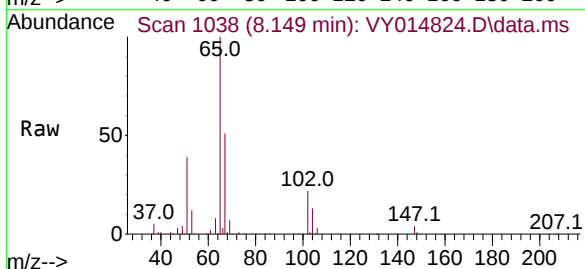

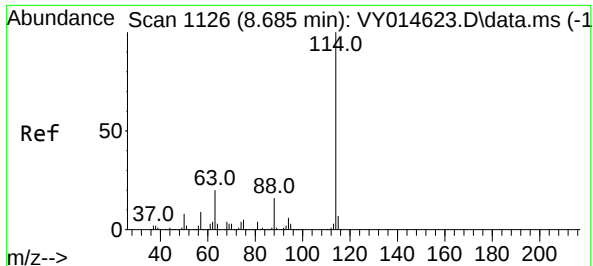

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.697 min Scan# 1128

Delta R.T. 0.012 min

Lab File: VY014824.D

Acq: 26 Jul 2023 00:48

Instrument :

MSVOA_Y

ClientSampleId :

B-P24B





Tgt Ion:114 Resp: 251514

Ion Ratio Lower Upper

114 100

63 18.5 0.0 42.4

88 14.7 0.0 30.6

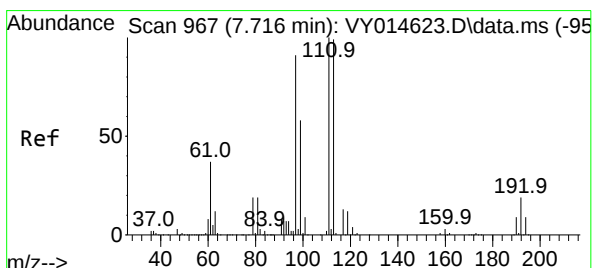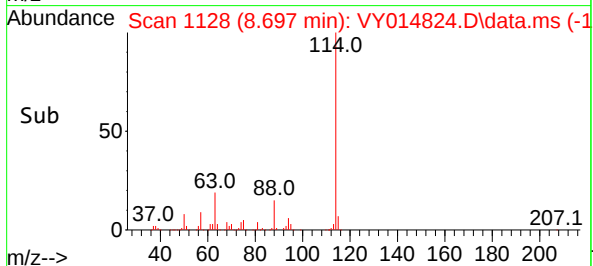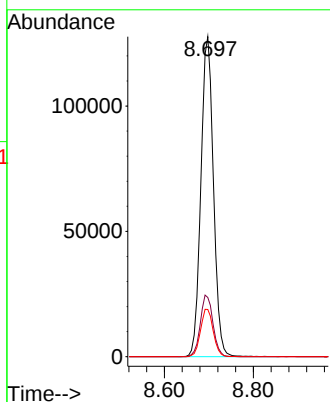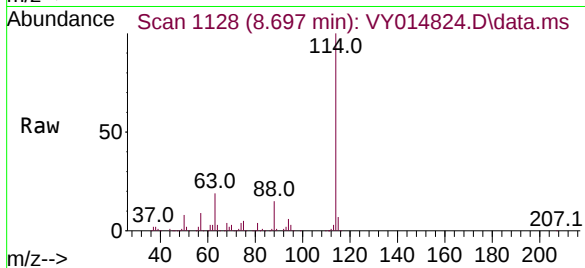

#35

Dibromofluoromethane

Concen: 48.826 ug/l

RT: 7.722 min Scan# 968

Delta R.T. 0.006 min

Lab File: VY014824.D

Acq: 26 Jul 2023 00:48




Tgt Ion:113 Resp: 78174


Ion Ratio Lower Upper

113 100

111 101.7 81.3 121.9

192 19.8 16.9 25.3


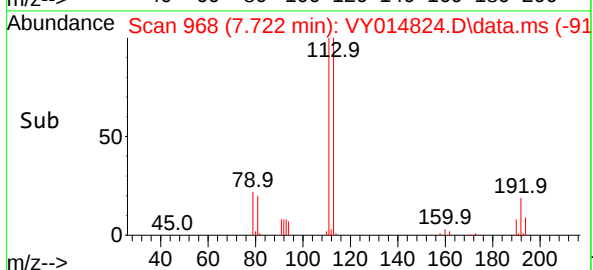
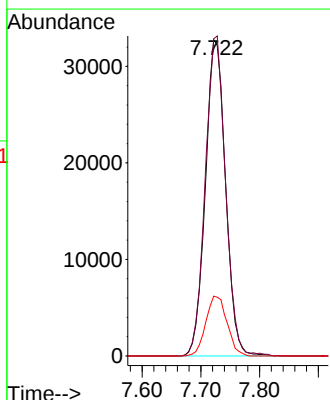
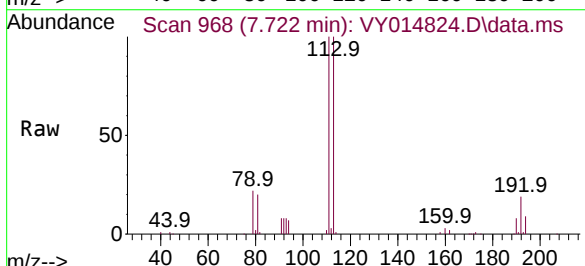


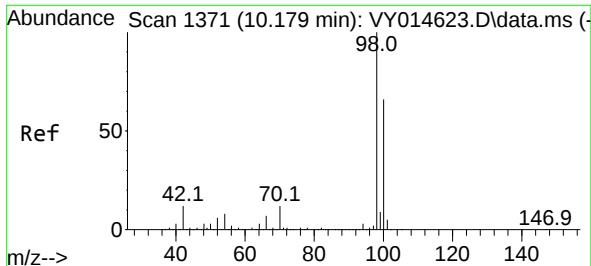

#50
Toluene-d8
Concen: 50.359 ug/l
RT: 10.185 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY014824.D
Acq: 26 Jul 2023 00:48




Instrument :
MSVOA_Y
ClientSampleId :
B-P24B


Tgt Ion: 98 Resp: 297262
Ion Ratio Lower Upper
98 100
100 65.1 50.1 75.1

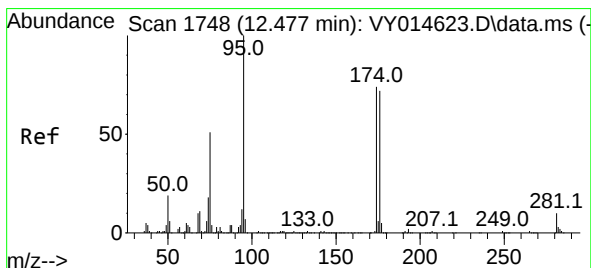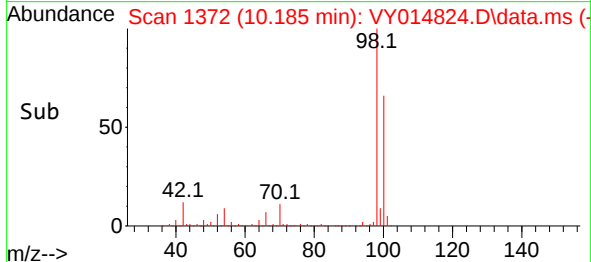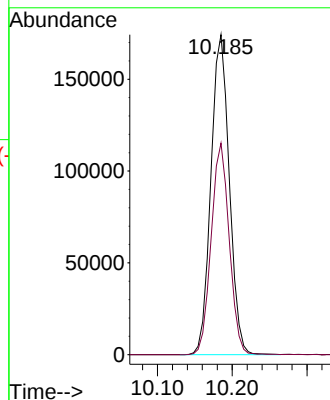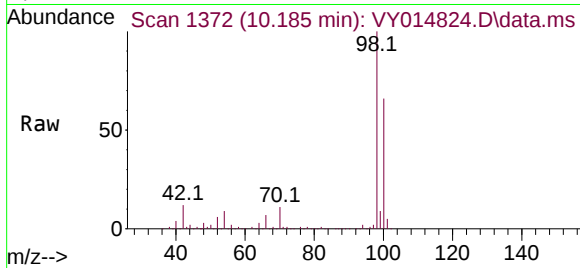

#62
4-Bromofluorobenzene
Concen: 46.625 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.006 min
Lab File: VY014824.D
Acq: 26 Jul 2023 00:48

Tgt Ion: 95 Resp: 105530
Ion Ratio Lower Upper
95 100
174 80.9 0.0 178.2
176 79.1 0.0 173.8

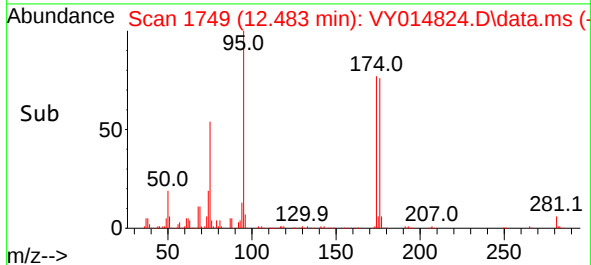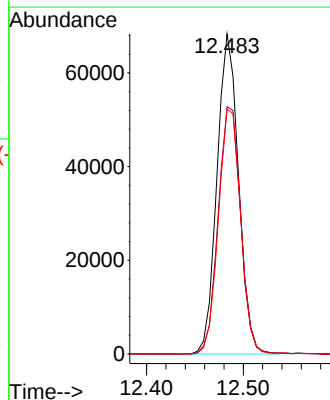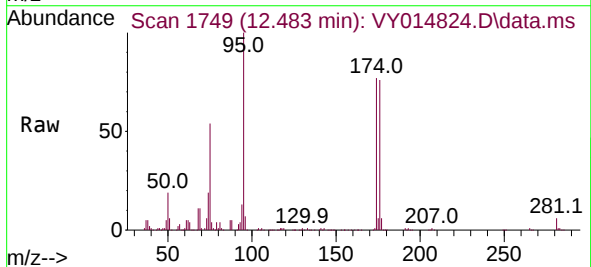

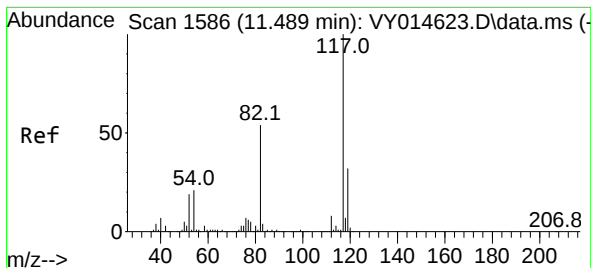

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.496 min Scan# 11

Delta R.T. 0.007 min

Lab File: VY014824.D

Acq: 26 Jul 2023 00:48

Instrument :

MSVOA_Y

ClientSampleId :

B-P24B





Tgt Ion:117 Resp: 233851

Ion Ratio Lower Upper

117 100

82 53.9 43.4 65.0

119 31.8 26.3 39.5

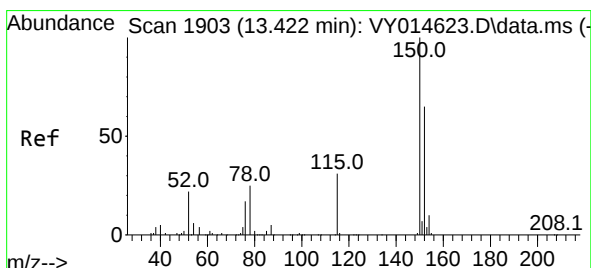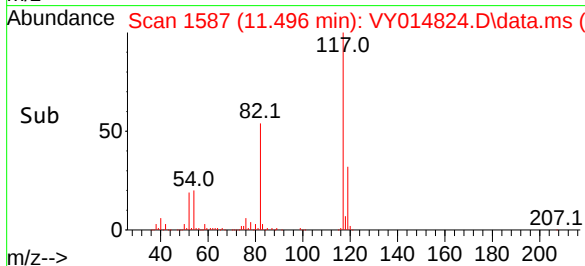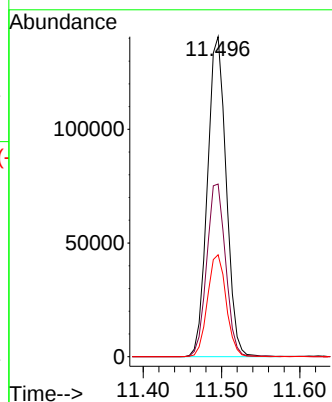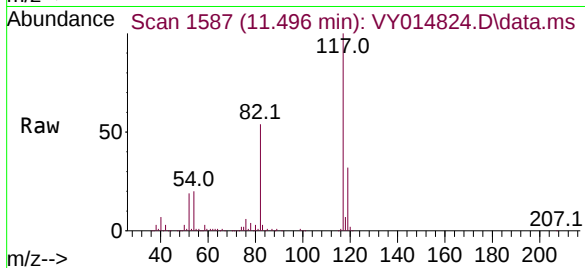

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.428 min Scan# 1904

Delta R.T. 0.006 min

Lab File: VY014824.D

Acq: 26 Jul 2023 00:48

Tgt Ion:152 Resp: 108125

Ion Ratio Lower Upper

152 100

115 59.0 28.8 86.5

150 157.1 0.0 348.8

